

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041422\
 Data File : PL074082.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 00:05
 Operator : AR\AJ
 Sample : N2368-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 E14ST-EB3-041122-0-5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/18/2022
 Supervised By :mohammad ahmed 04/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 02:20:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.637	5.491	4101738	18148099	12.695	10.179
28) SA Decachlor...	10.410	11.333	5290405	17017100	10.173	9.634m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041422\
Data File : PL074082.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 00:05
Operator : AR\AJ
Sample : N2368-02
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
E14ST-EB3-041122-0-5


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/18/2022
Supervised By : mohammad ahmed 04/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 02:20:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

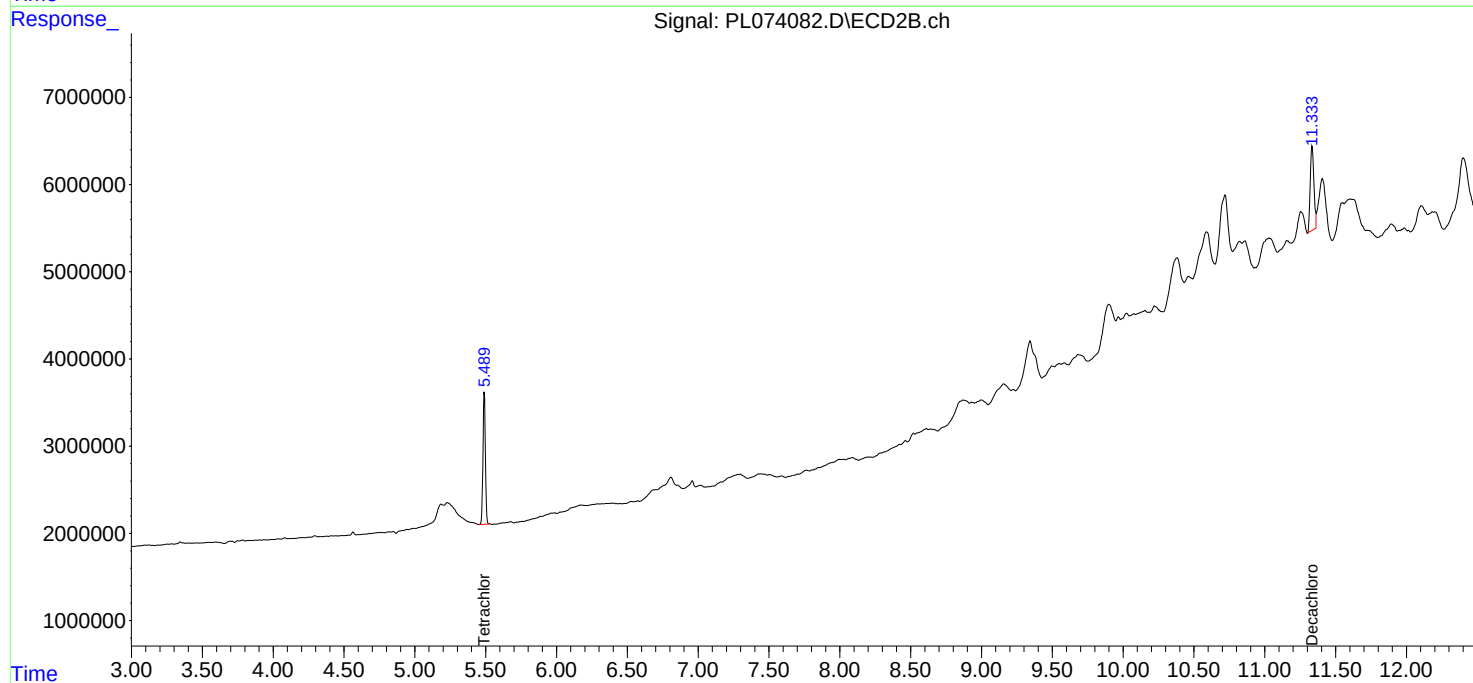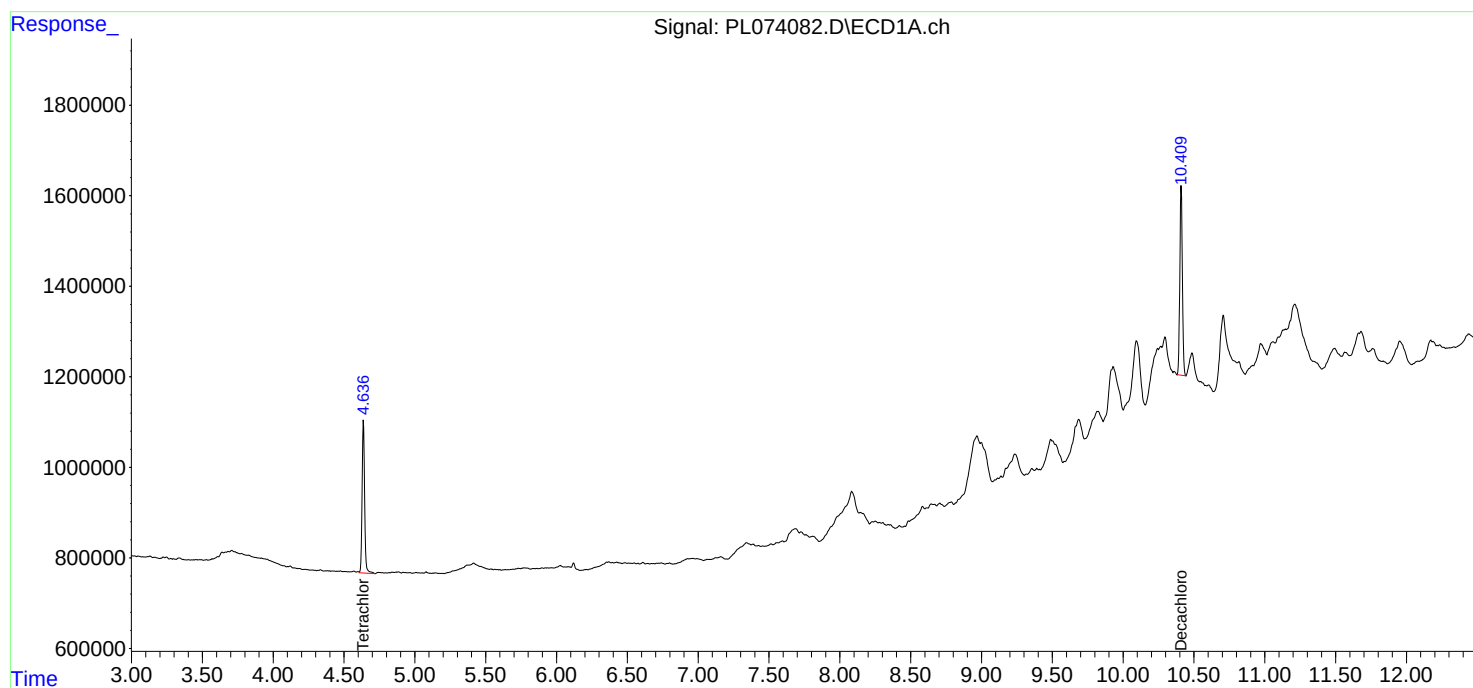

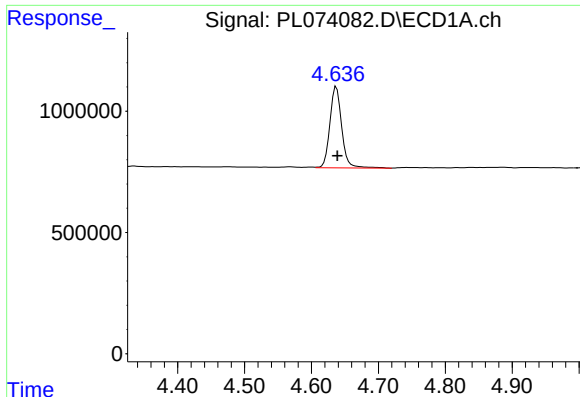


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: -0.002 min
Response: 4101738
Conc: 12.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
E14ST-EB3-041122-0-5


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/18/2022
Supervised By :mohammad ahmed 04/18/2022

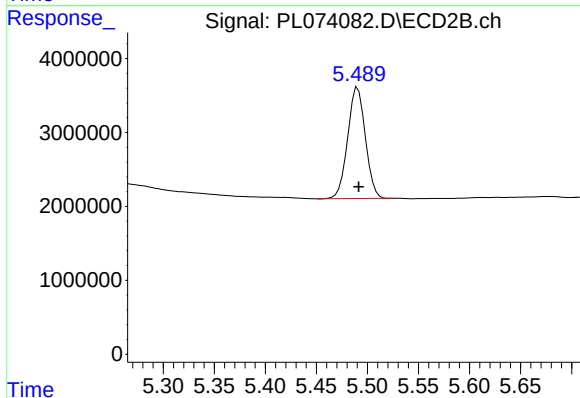


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 18148099
Conc: 10.18 ng/ml

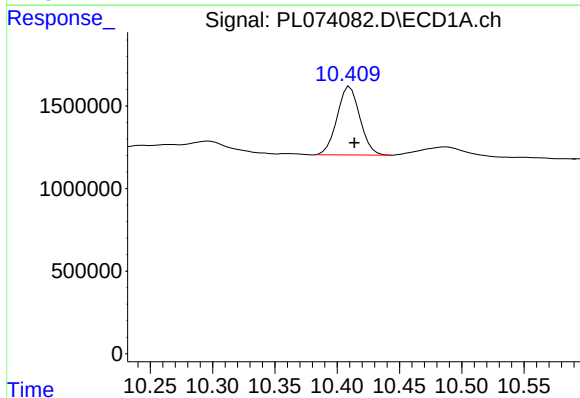

#28 Decachlorobiphenyl

R.T.: 10.410 min
Delta R.T.: -0.004 min
Response: 5290405
Conc: 10.17 ng/ml

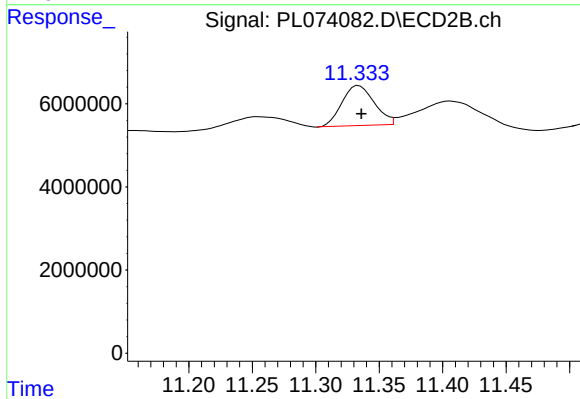

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: -0.004 min
Response: 17017100
Conc: 9.63 ng/ml m