

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041425\
 Data File : PL095204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2025 14:54
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 17:50:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 14 17:48:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.767	53333275	69846365	19.441	18.770
28)	SA Decachlor...	9.051	7.898	46940938	82318367	19.496	18.713
Target Compounds							
9)	A Endosulfan I	6.064	5.086	29095682	36899467	9.390	8.500
10)	B gamma-Chl...	5.935	4.966	34016323	42989623	10.183	8.925
12)	B 4,4'-DDE	6.188	5.219	63918962	90012412	19.548	18.695
13)	MA Dieldrin	6.340	5.350	63174279	87432357	19.172	18.215
19)	B Endosulfa...	7.155	6.323	50654072	77236274	19.713	18.493
20)	A Methoxychlor	7.498	6.599	116.4E6	203.3E6	86.920	90.518
21)	B Endrin ke...	7.640	6.828	54337070	90325290	18.823	17.914
25)	Chlordane-3	5.935	4.966	34016323	42989623	69.390	85.243



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041425\
Data File : PL095204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2025 14:54
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 17:50:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
Quant Title : GC Extractables
QLast Update : Mon Apr 14 17:48:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

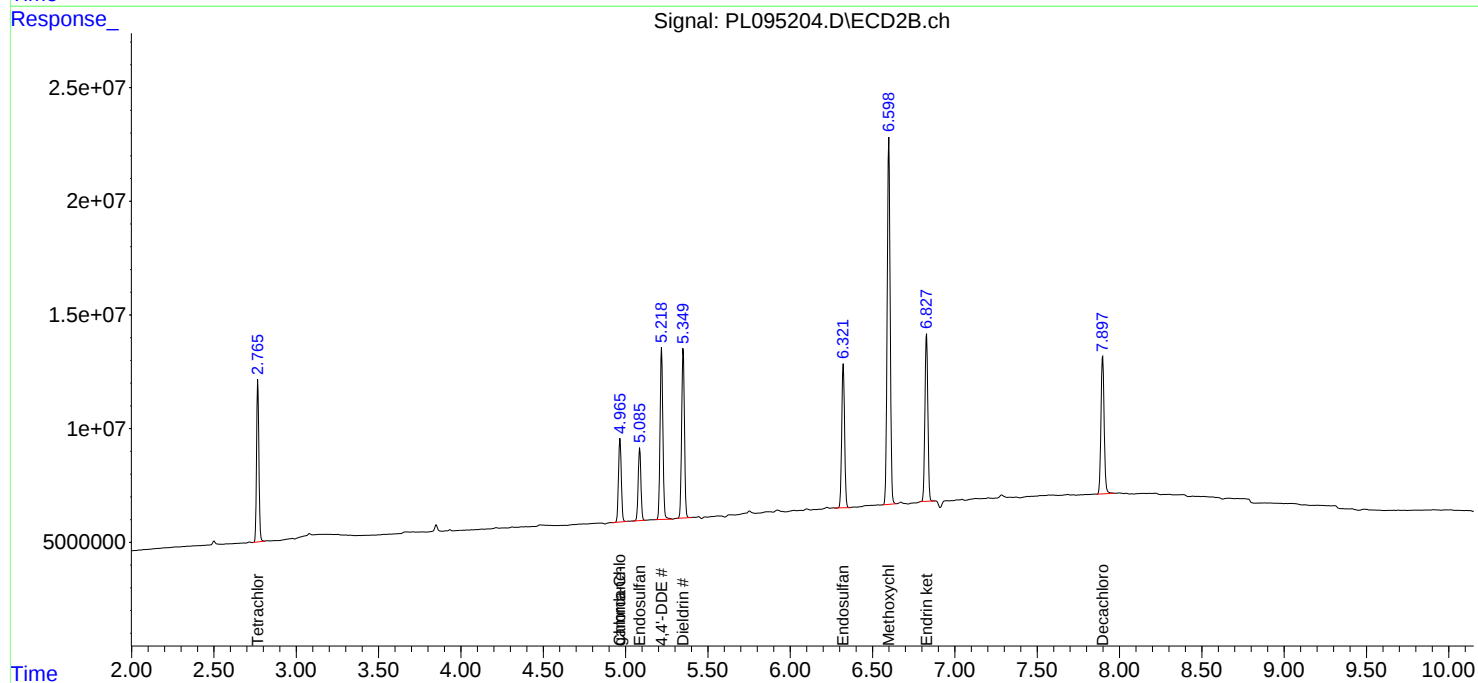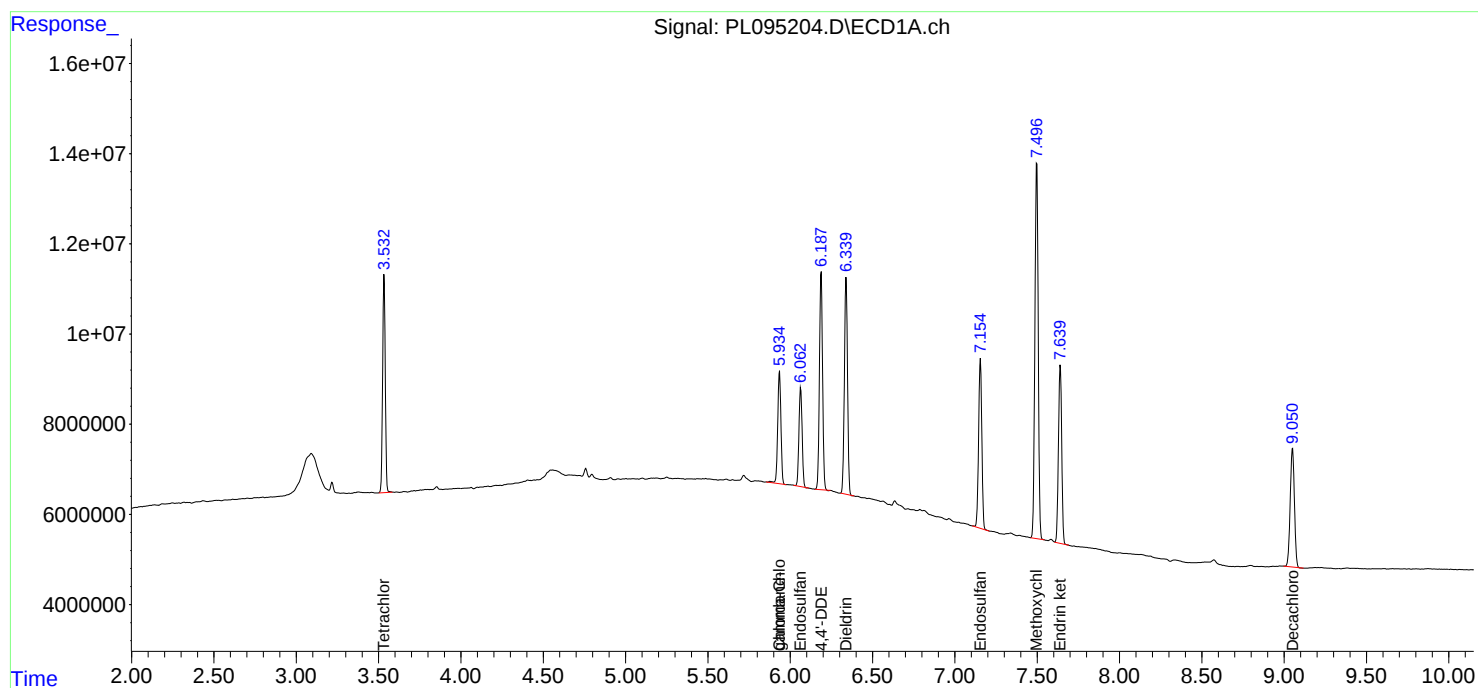


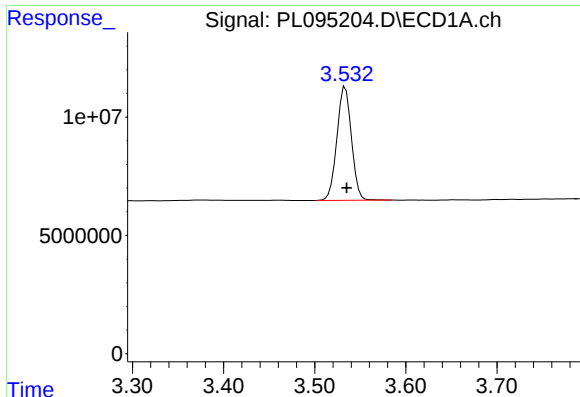

#1 Tetrachloro-m-xylene


R.T.: 3.534 min
Delta R.T.: -0.001 min
Response: 53333275
Conc: 19.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

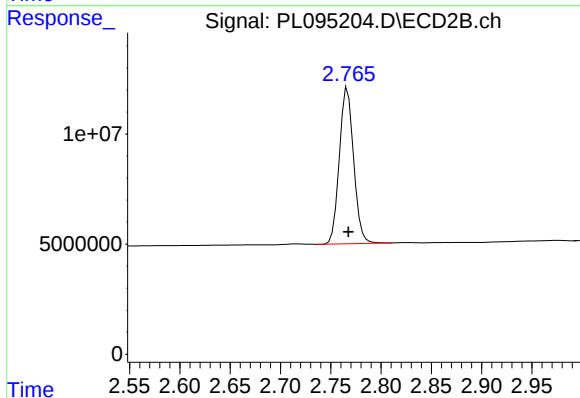


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 69846365
Conc: 18.77 ng/ml

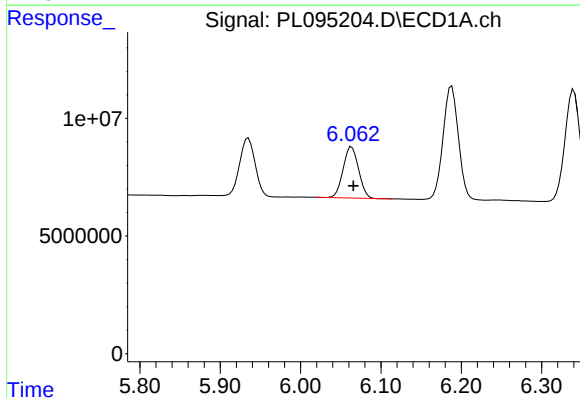


#9 Endosulfan I

R.T.: 6.064 min
Delta R.T.: -0.002 min
Response: 29095682
Conc: 9.39 ng/ml

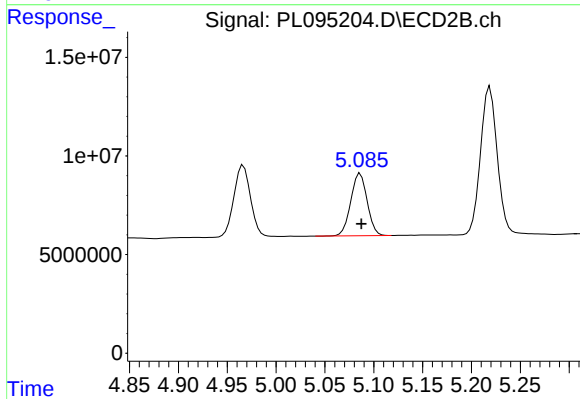

#9 Endosulfan I


R.T.: 5.086 min
Delta R.T.: -0.001 min
Response: 36899467
Conc: 8.50 ng/ml

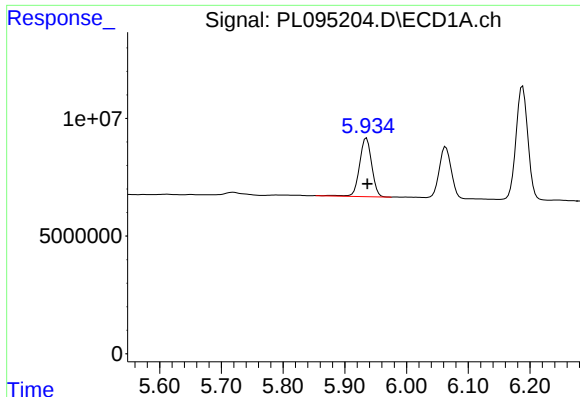

#10 gamma-Chlordane


R.T.: 5.935 min
Delta R.T.: -0.002 min
Response: 34016323
Conc: 10.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

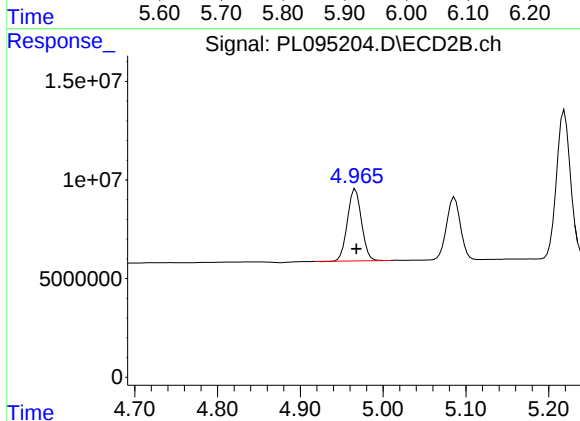


#10 gamma-Chlordane

R.T.: 4.966 min
Delta R.T.: -0.001 min
Response: 42989623
Conc: 8.93 ng/ml

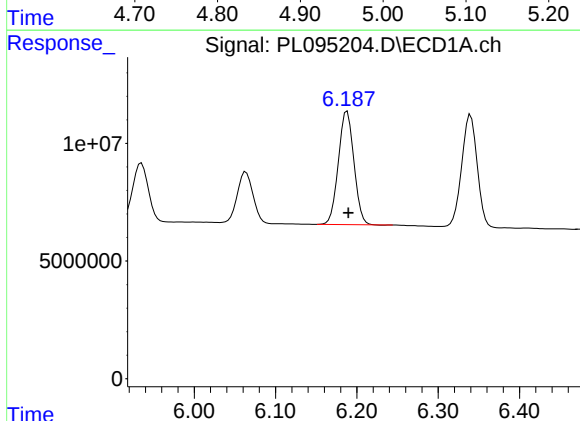


#12 4,4'-DDE

R.T.: 6.188 min
Delta R.T.: -0.002 min
Response: 63918962
Conc: 19.55 ng/ml

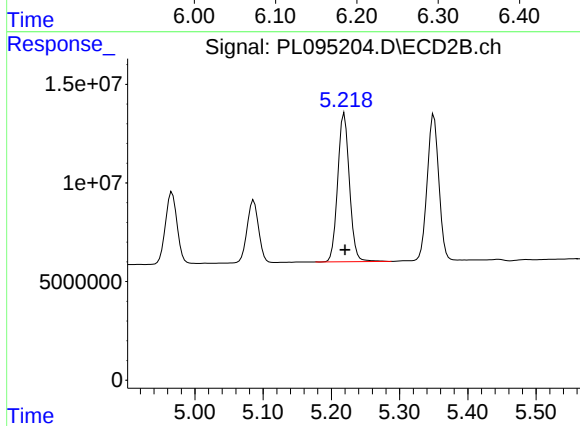

#12 4,4'-DDE


R.T.: 5.219 min
Delta R.T.: -0.001 min
Response: 90012412
Conc: 18.70 ng/ml

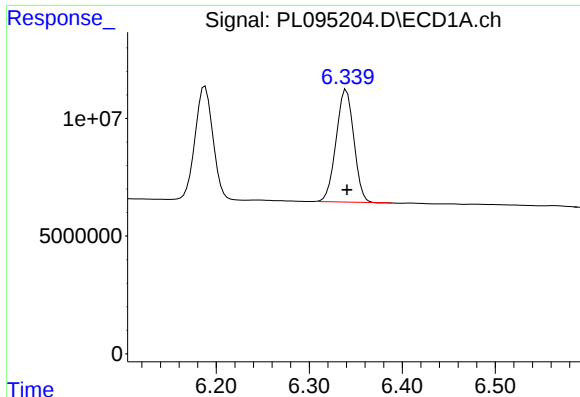

#13 Dieldrin


R.T.: 6.340 min
Delta R.T.: 0.000 min
Response: 63174279
Conc: 19.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

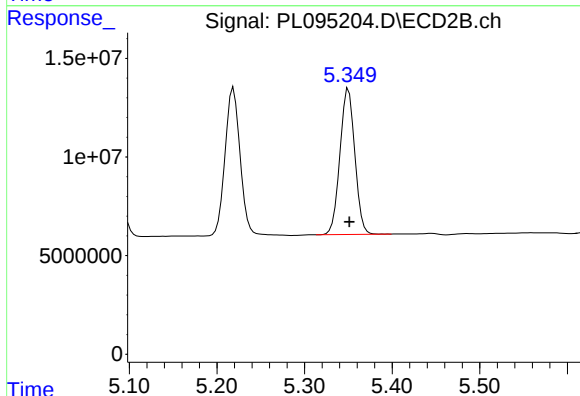


#13 Dieldrin

R.T.: 5.350 min
Delta R.T.: -0.001 min
Response: 87432357
Conc: 18.21 ng/ml

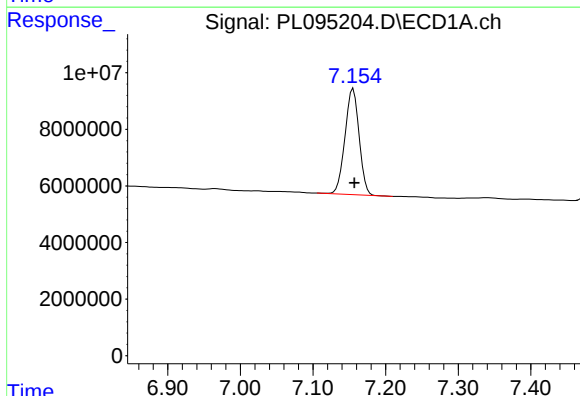


#19 Endosulfan Sulfate

R.T.: 7.155 min
Delta R.T.: -0.002 min
Response: 50654072
Conc: 19.71 ng/ml

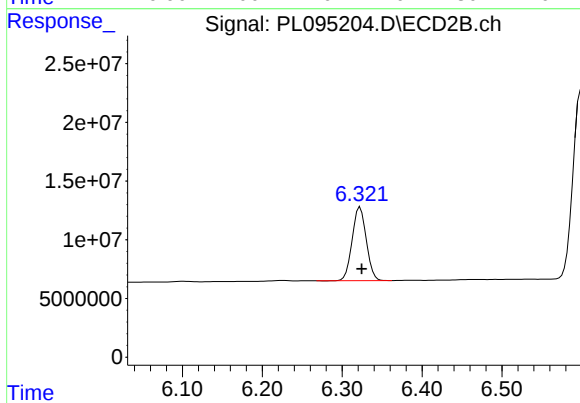

#19 Endosulfan Sulfate


R.T.: 6.323 min
Delta R.T.: -0.002 min
Response: 77236274
Conc: 18.49 ng/ml

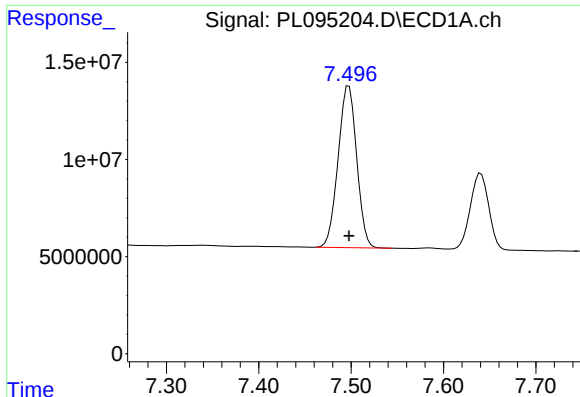

#20 Methoxychlor


R.T.: 7.498 min
Delta R.T.: 0.000 min
Response: 116424037
Conc: 86.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

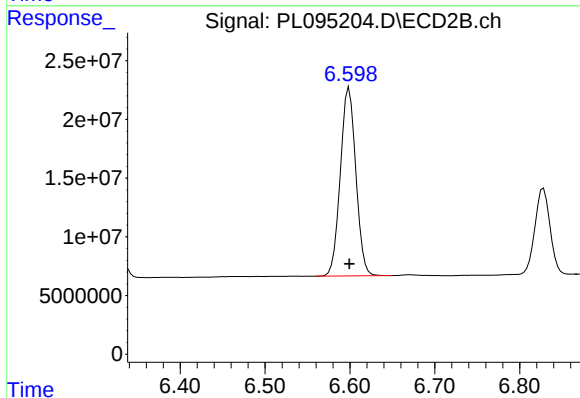


#20 Methoxychlor

R.T.: 6.599 min
Delta R.T.: 0.000 min
Response: 203274853
Conc: 90.52 ng/ml

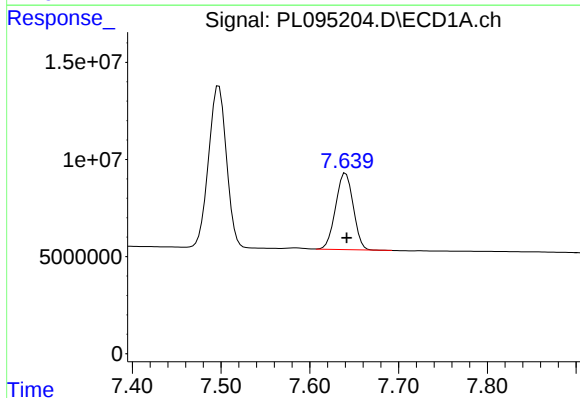


#21 Endrin ketone

R.T.: 7.640 min
Delta R.T.: -0.001 min
Response: 54337070
Conc: 18.82 ng/ml

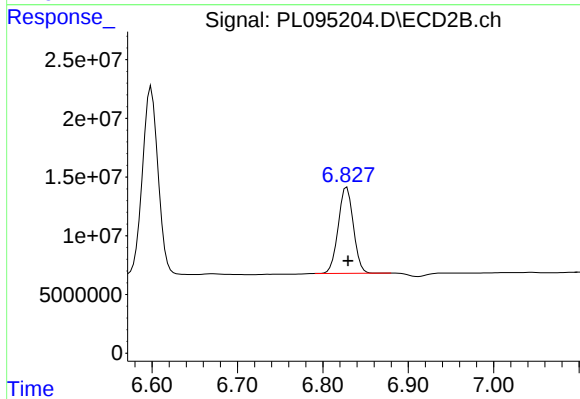

#21 Endrin ketone


R.T.: 6.828 min
Delta R.T.: -0.001 min
Response: 90325290
Conc: 17.91 ng/ml

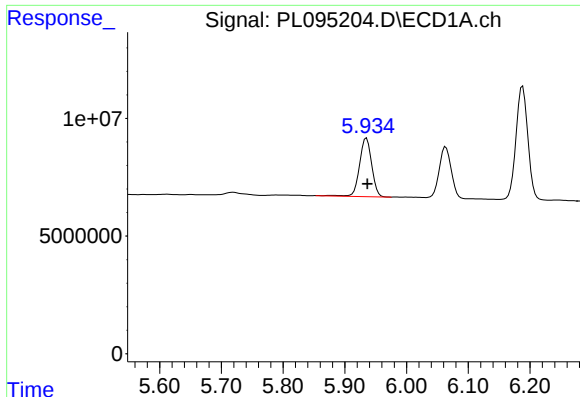

#25 Chlordane-3


R.T.: 5.935 min
Delta R.T.: -0.001 min
Response: 34016323
Conc: 69.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

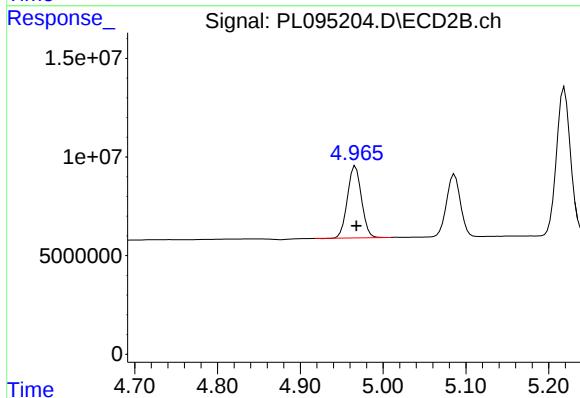


#25 Chlordane-3

R.T.: 4.966 min
Delta R.T.: -0.001 min
Response: 42989623
Conc: 85.24 ng/ml

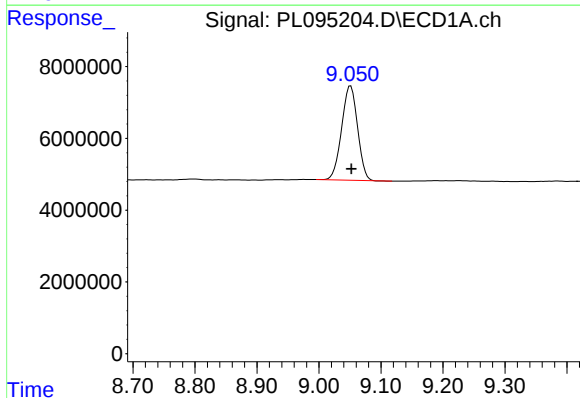

#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: -0.001 min
Response: 46940938
Conc: 19.50 ng/ml

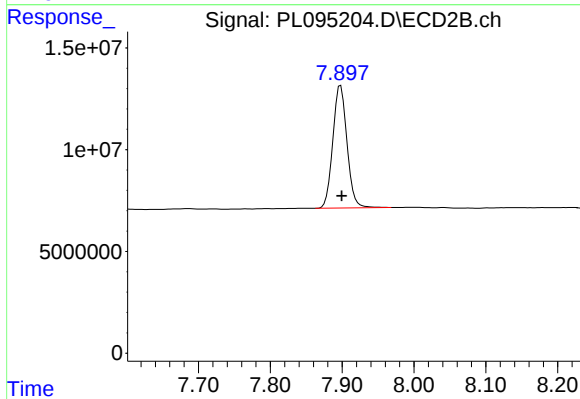

#28 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.002 min
Response: 82318367
Conc: 18.71 ng/ml