

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041425\
 Data File : PL095211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2025 16:43
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 17:42:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 14 17:38:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.767	193.3E6	340.8E6	74.552	74.741
28)	SA Decachlor...	9.055	7.900	164.5E6	315.5E6	73.959	74.244
Target Compounds							
23)	Chlordane-1	4.697	3.763	92734683	110.4E6	743.532	745.360
24)	Chlordane-2	5.227	4.339	94833248	126.2E6	745.762	745.158
25)	Chlordane-3	5.939	4.969	341.7E6	376.1E6	741.540	745.928
26)	Chlordane-4	6.020	5.032	404.6E6	369.1E6	743.989	742.623
27)	Chlordane-5	6.870	5.927	78499871	138.6E6	743.367	745.084



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041425\
Data File : PL095211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2025 16:43
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 17:42:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
Quant Title : GC Extractables
QLast Update : Mon Apr 14 17:38:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

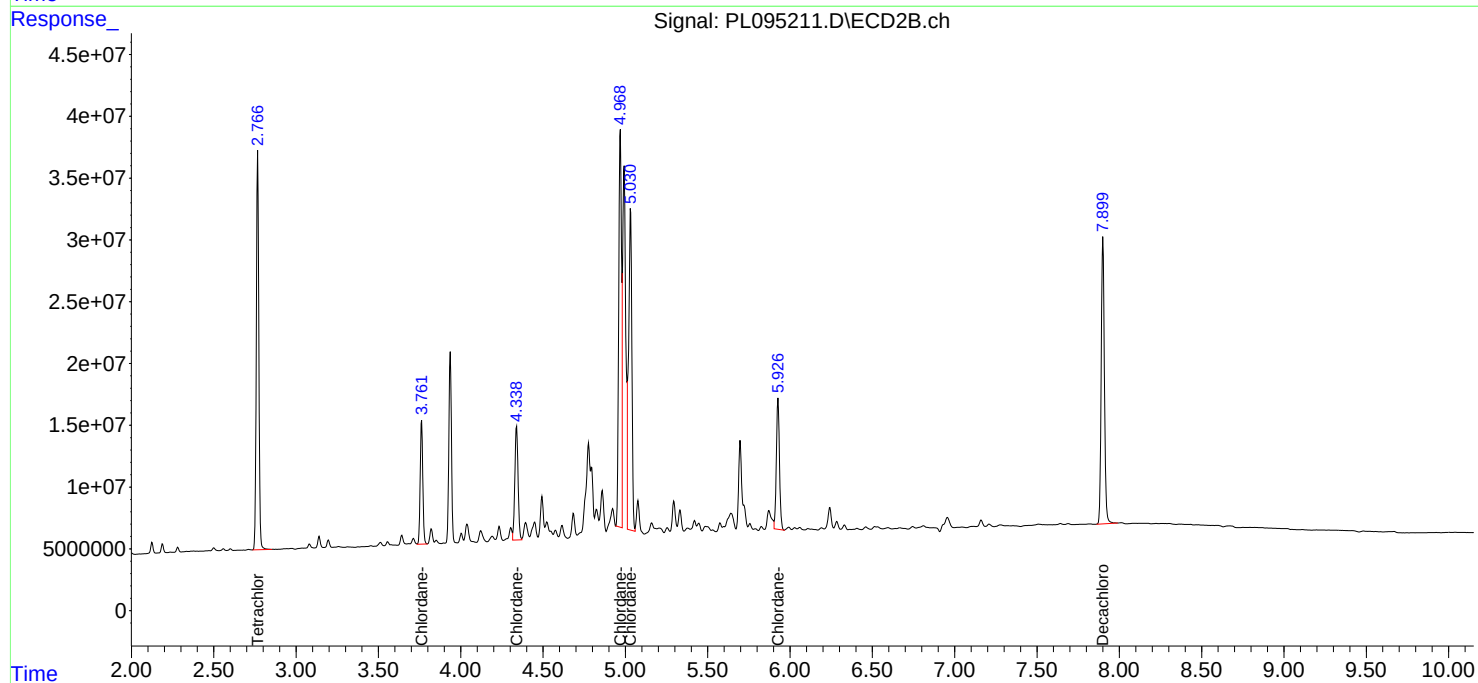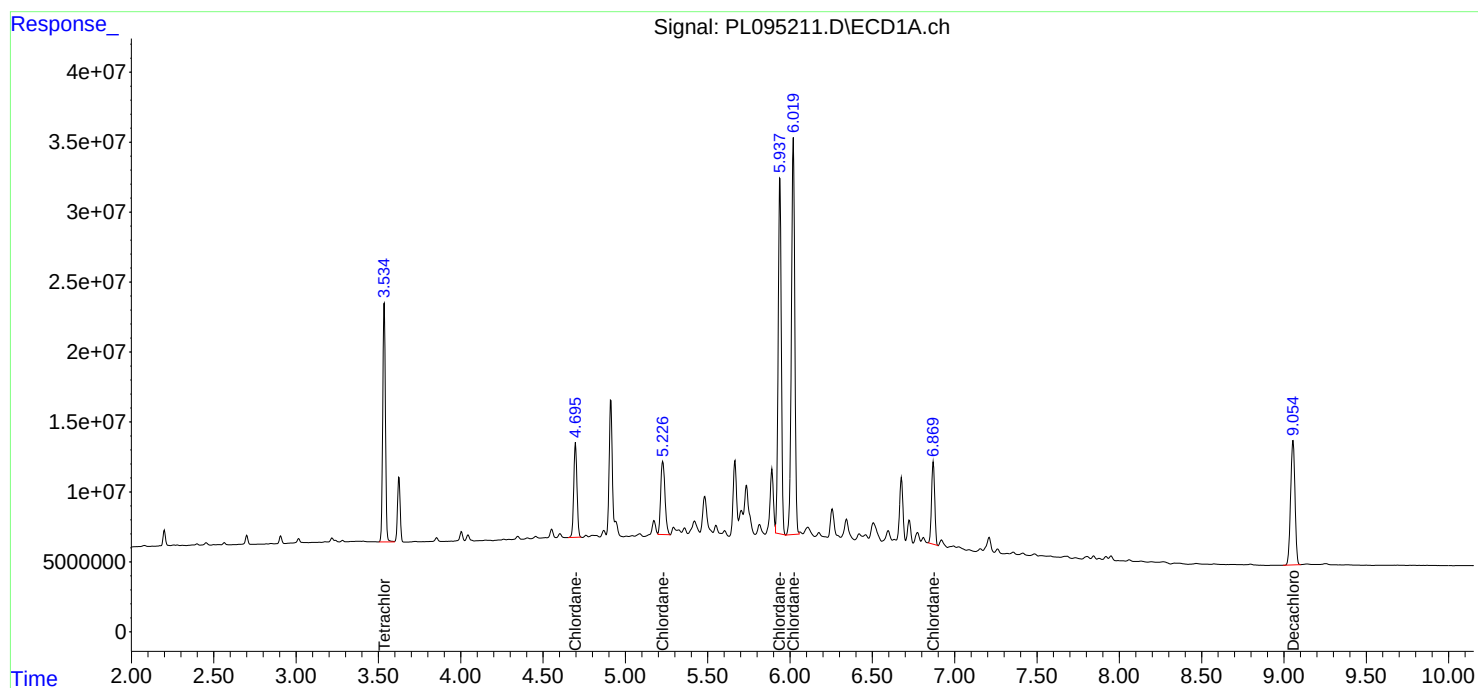


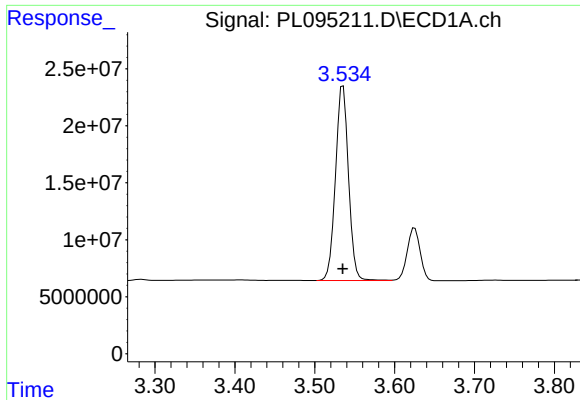

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 193293769
Conc: 74.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

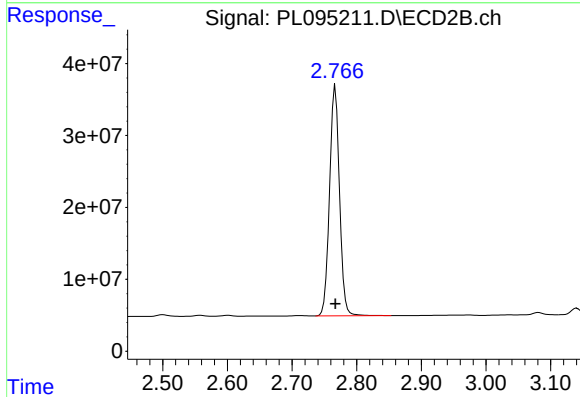


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 340751748
Conc: 74.74 ng/ml

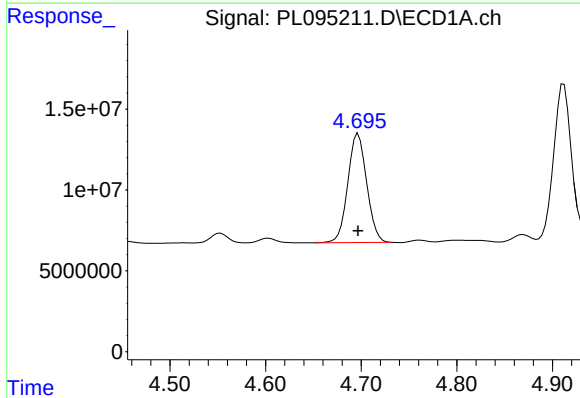


#23 Chlordane-1

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 92734683
Conc: 743.53 ng/ml

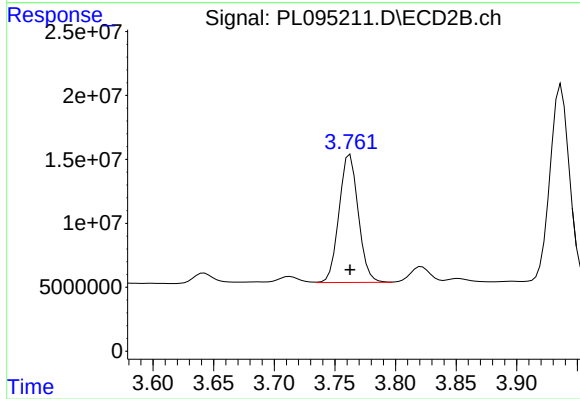

#23 Chlordane-1


R.T.: 3.763 min
Delta R.T.: 0.000 min
Response: 110412945
Conc: 745.36 ng/ml

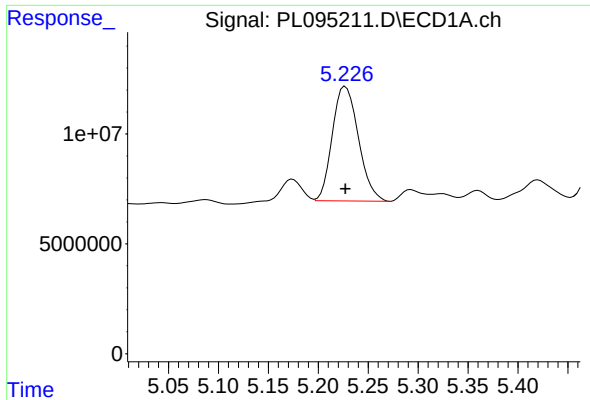

#24 Chlordane-2


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 94833248
Conc: 745.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

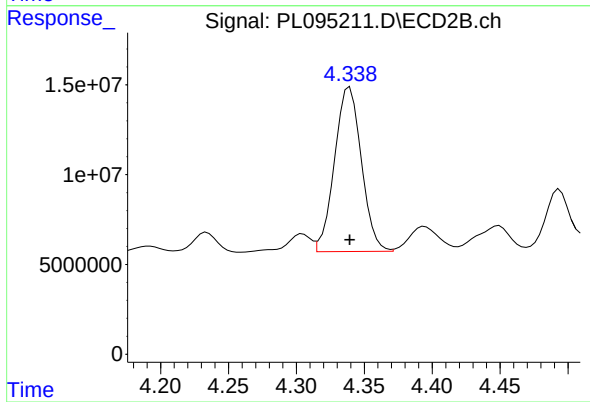


#24 Chlordane-2

R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 126241352
Conc: 745.16 ng/ml

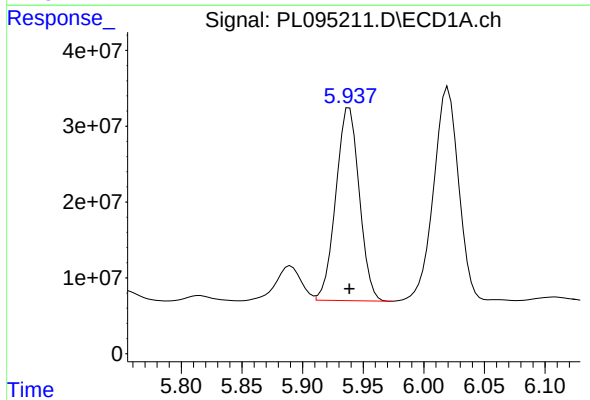


#25 Chlordane-3

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 341722603
Conc: 741.54 ng/ml

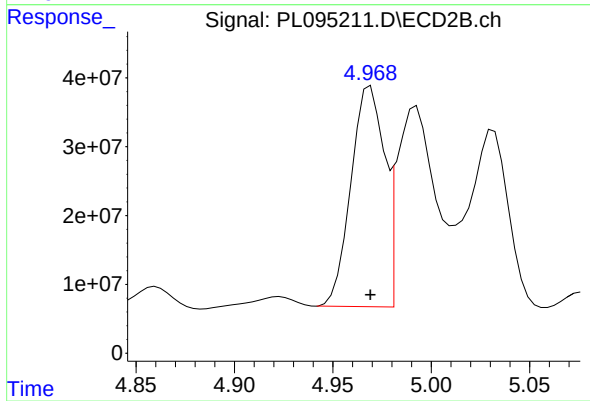

#25 Chlordane-3


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 376107052
Conc: 745.93 ng/ml

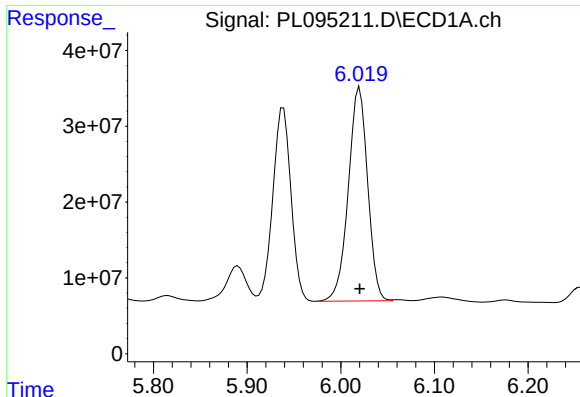

#26 Chlordane-4


R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 404608535
Conc: 743.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

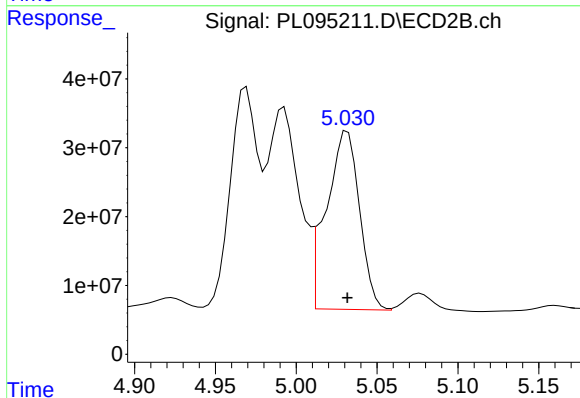


#26 Chlordane-4

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 369065404
Conc: 742.62 ng/ml

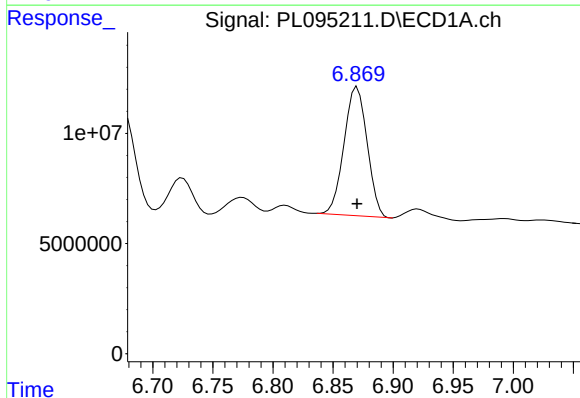


#27 Chlordane-5

R.T.: 6.870 min
Delta R.T.: 0.000 min
Response: 78499871
Conc: 743.37 ng/ml

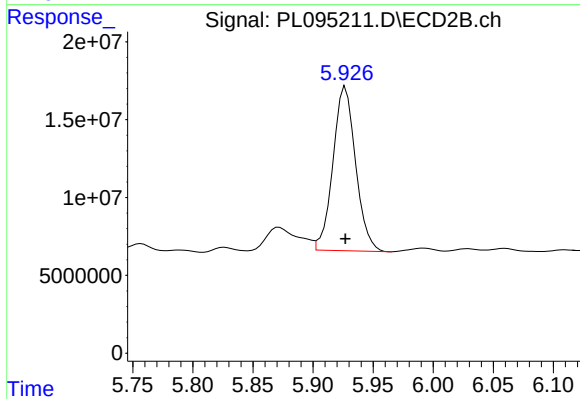

#27 Chlordane-5


R.T.: 5.927 min
Delta R.T.: 0.000 min
Response: 138612732
Conc: 745.08 ng/ml

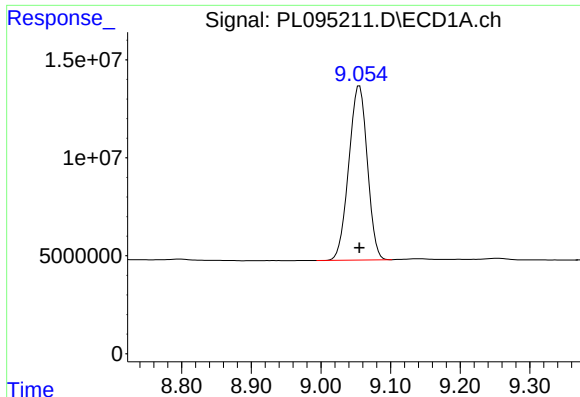

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 164525785
Conc: 73.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

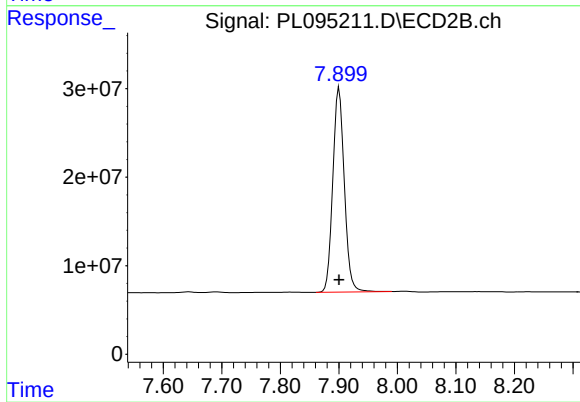

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 315490653
Conc: 74.24 ng/ml