

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041425\
 Data File : PL095212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2025 16:56
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 17:38:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 14 17:38:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.767	131.6E6	226.3E6	50.000	50.000
28)	SA Decachlor...	9.053	7.900	114.9E6	213.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.696	3.762	63778810	73851411	500.000	500.000
24)	Chlordane-2	5.226	4.338	65091212	85236842	500.000	500.000
25)	Chlordane-3	5.937	4.968	234.1E6	249.3E6	500.000	500.000
26)	Chlordane-4	6.019	5.030	275.1E6	247.7E6	500.000	500.000
27)	Chlordane-5	6.869	5.926	53962240	91780125	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041425\
Data File : PL095212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2025 16:56
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 17:38:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
Quant Title : GC Extractables
QLast Update : Mon Apr 14 17:38:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

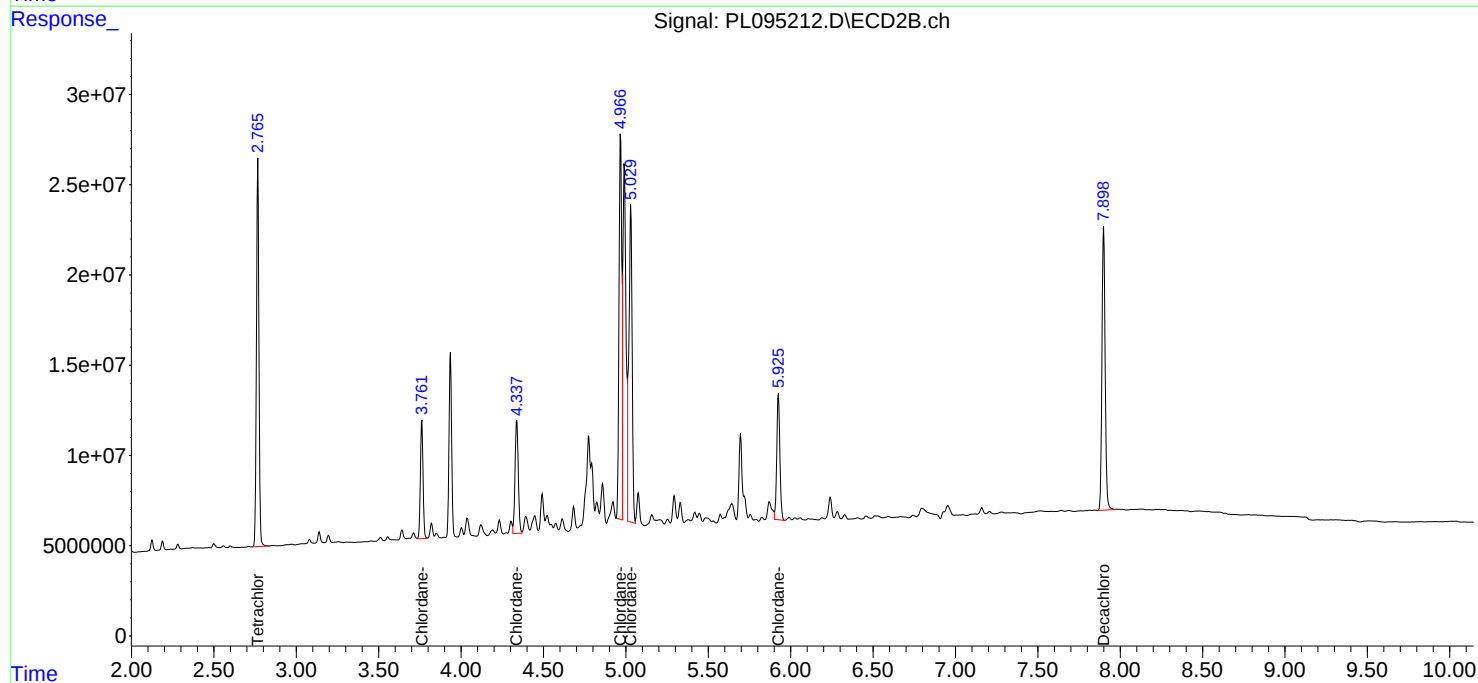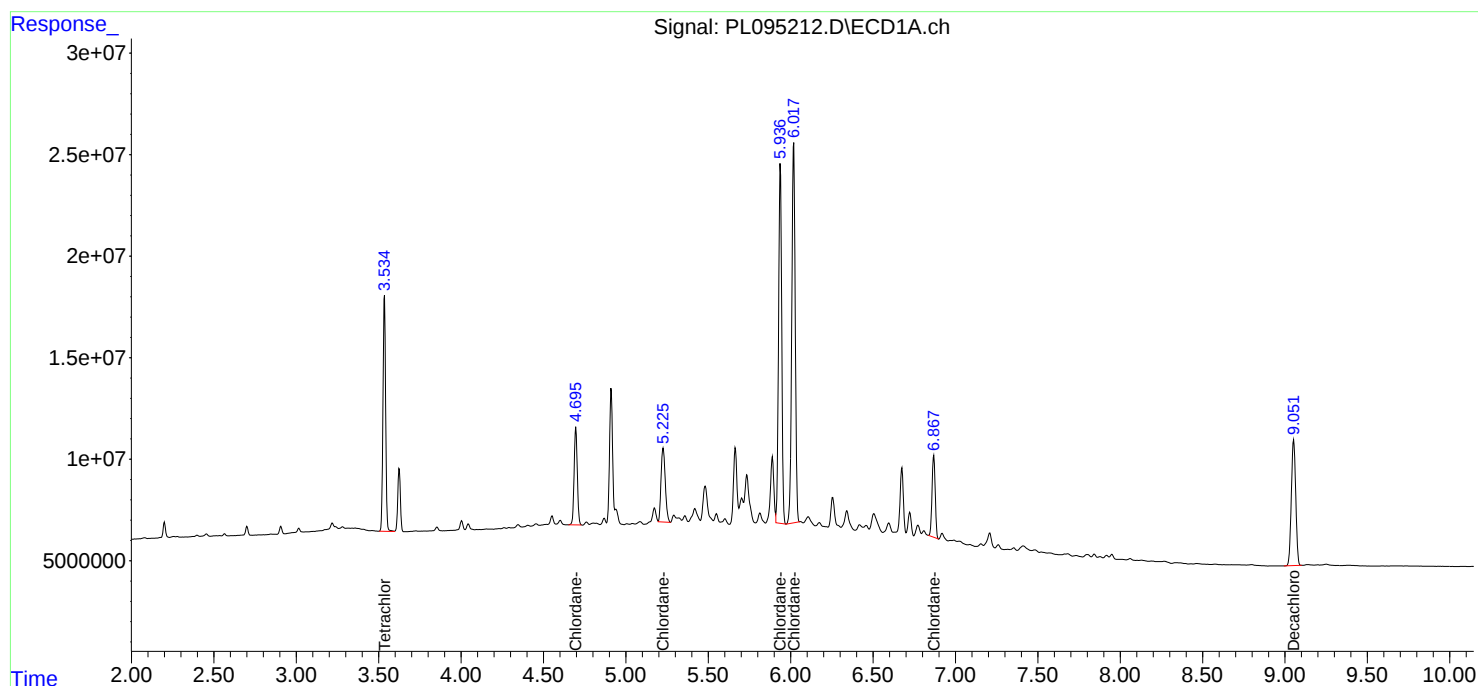


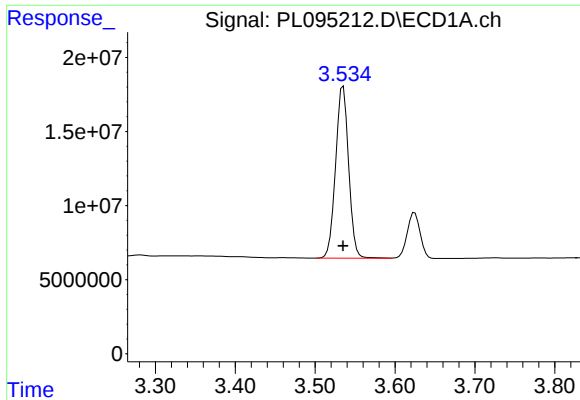

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 131631332
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

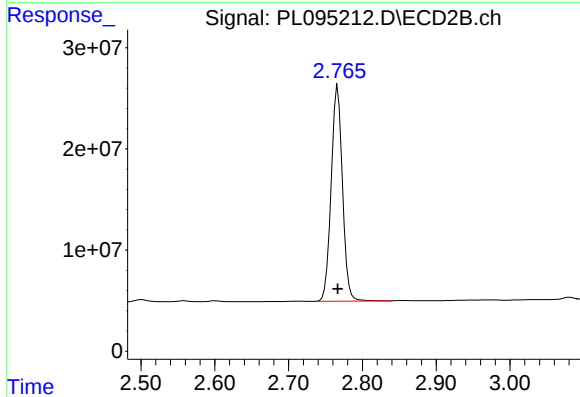


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 226258033
Conc: 50.00 ng/ml

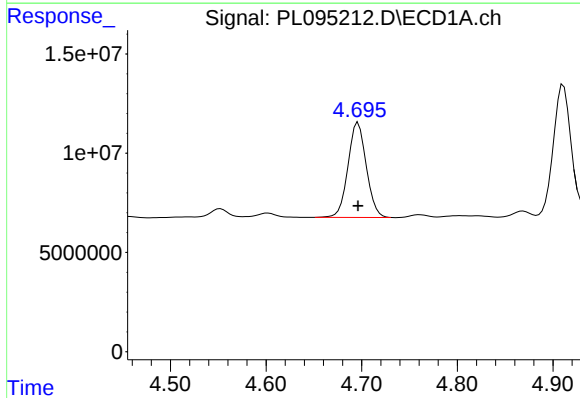


#23 Chlordane-1

R.T.: 4.696 min
Delta R.T.: 0.000 min
Response: 63778810
Conc: 500.00 ng/ml

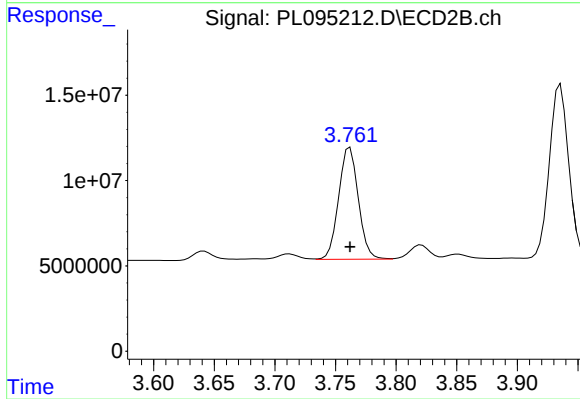

#23 Chlordane-1


R.T.: 3.762 min
Delta R.T.: 0.000 min
Response: 73851411
Conc: 500.00 ng/ml

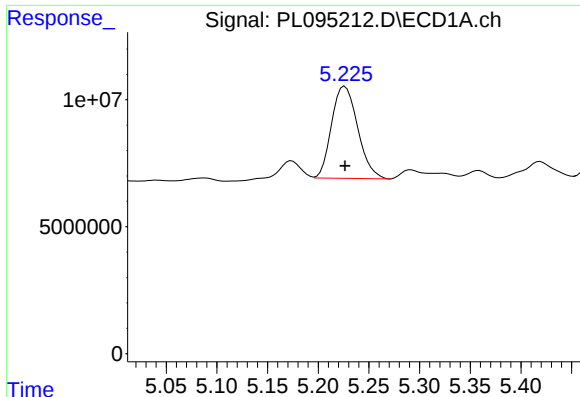

#24 Chlordane-2


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 65091212
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

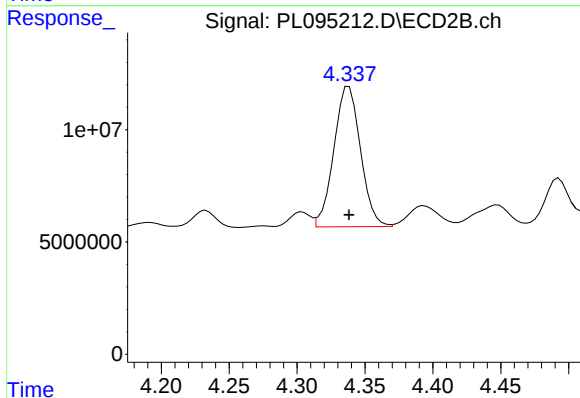


#24 Chlordane-2

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 85236842
Conc: 500.00 ng/ml

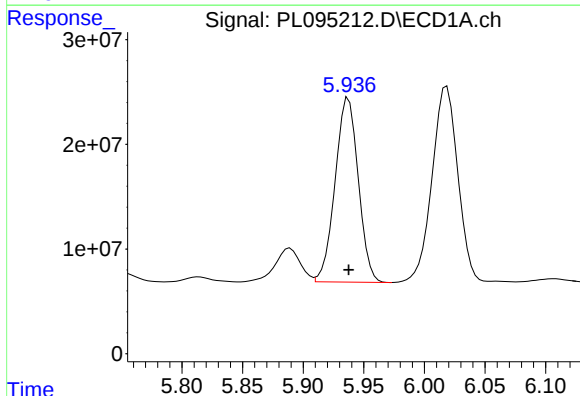


#25 Chlordane-3

R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 234100337
Conc: 500.00 ng/ml

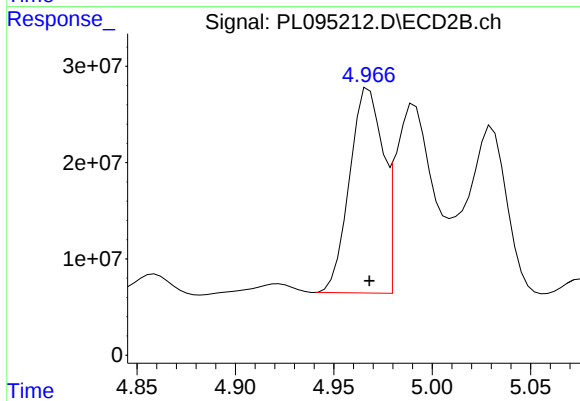

#25 Chlordane-3


R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 249300977
Conc: 500.00 ng/ml

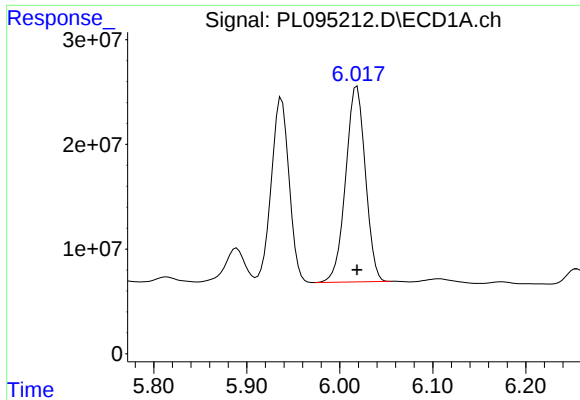

#26 Chlordane-4


R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 275065678
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

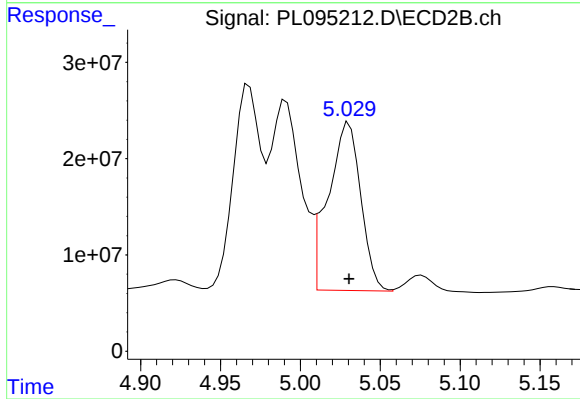


#26 Chlordane-4

R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 247732635
Conc: 500.00 ng/ml

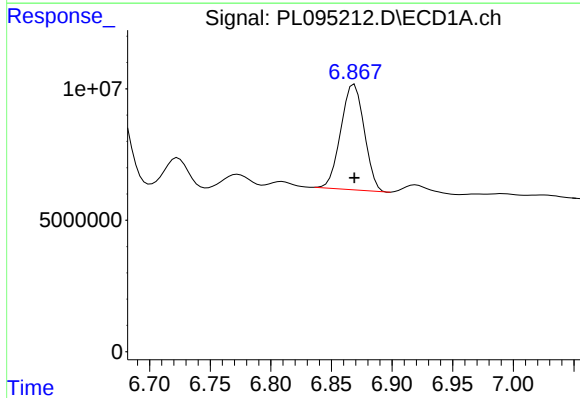


#27 Chlordane-5

R.T.: 6.869 min
Delta R.T.: 0.000 min
Response: 53962240
Conc: 500.00 ng/ml

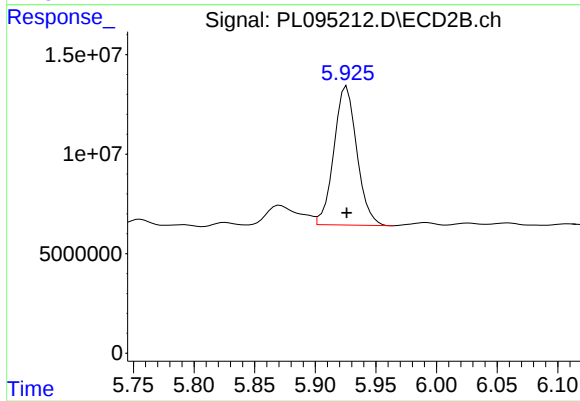

#27 Chlordane-5


R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 91780125
Conc: 500.00 ng/ml

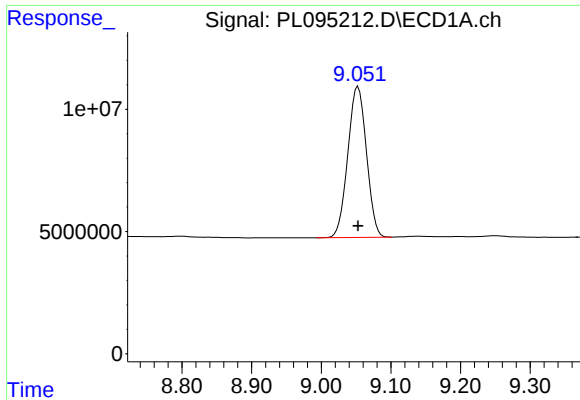

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 114860022
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

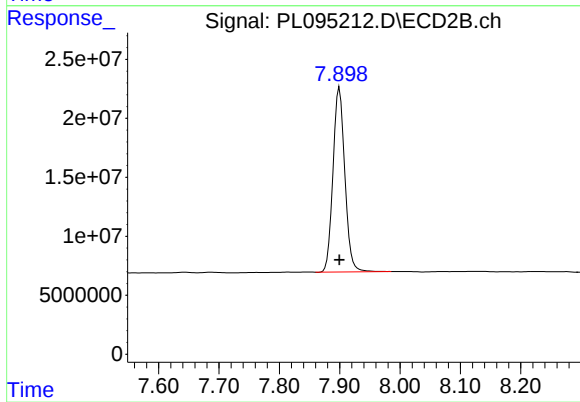

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 213541247
Conc: 50.00 ng/ml