

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041425\
 Data File : PL095213.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2025 17:10
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 17:44:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 14 17:38:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.766	67985395	112.0E6	25.905	24.666
28)	SA Decachlor...	9.053	7.900	60361027	109.8E6	26.567	25.632
Target Compounds							
23)	Chlordane-1	4.696	3.762	32512242	36105290	257.924	245.271
24)	Chlordane-2	5.226	4.338	33790990	42416105	261.615	250.275
25)	Chlordane-3	5.937	4.968	121.0E6	122.2E6	259.273	244.240
26)	Chlordane-4	6.019	5.030	143.9E6	122.5E6	260.783	247.417
27)	Chlordane-5	6.869	5.926	27795039	45619478	259.778	246.396



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041425\
Data File : PL095213.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2025 17:10
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 17:44:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
Quant Title : GC Extractables
QLast Update : Mon Apr 14 17:38:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

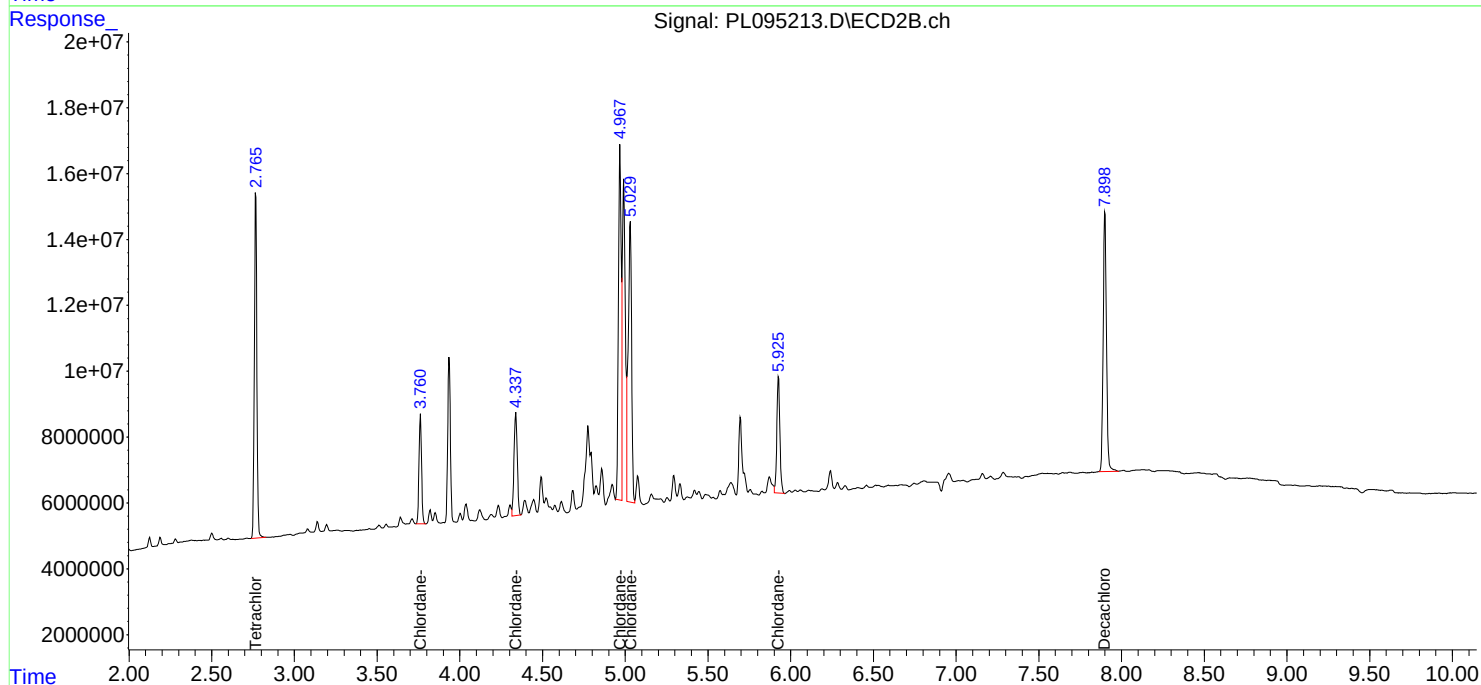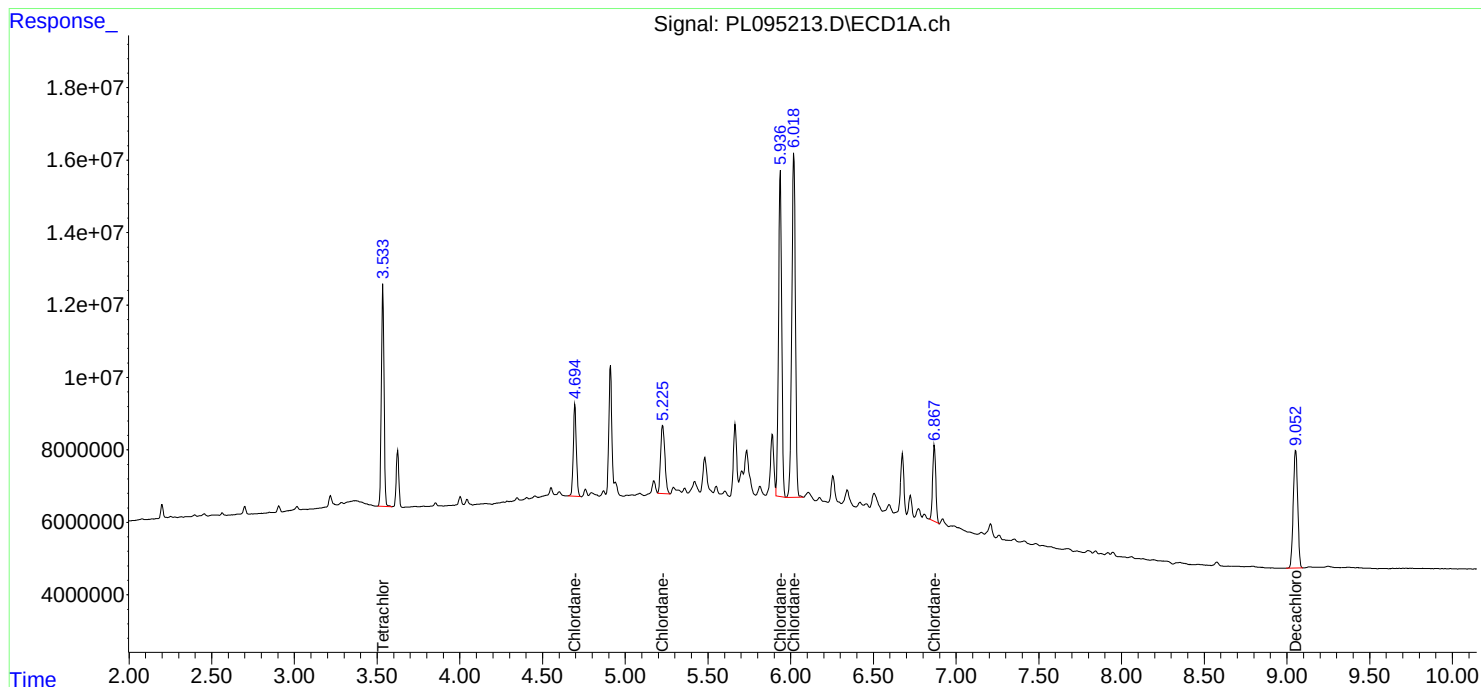


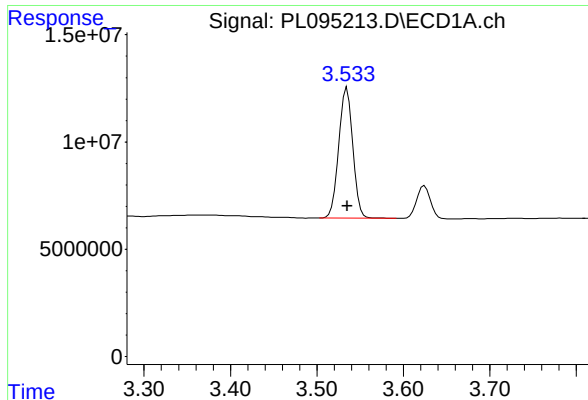

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 67985395
Conc: 25.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

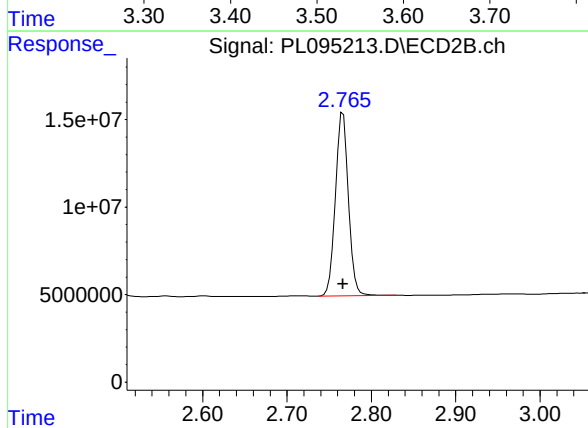


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 111953866
Conc: 24.67 ng/ml

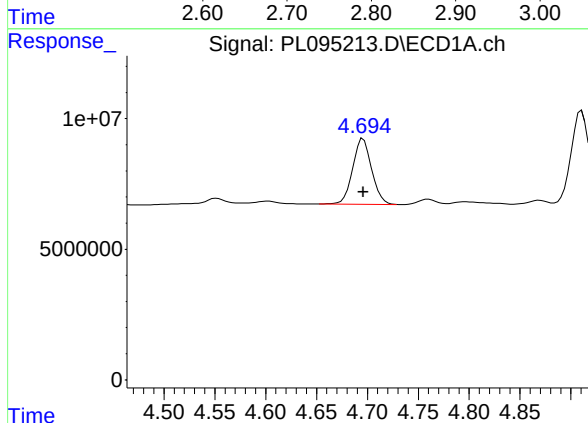


#23 Chlordane-1

R.T.: 4.696 min
Delta R.T.: 0.000 min
Response: 32512242
Conc: 257.92 ng/ml

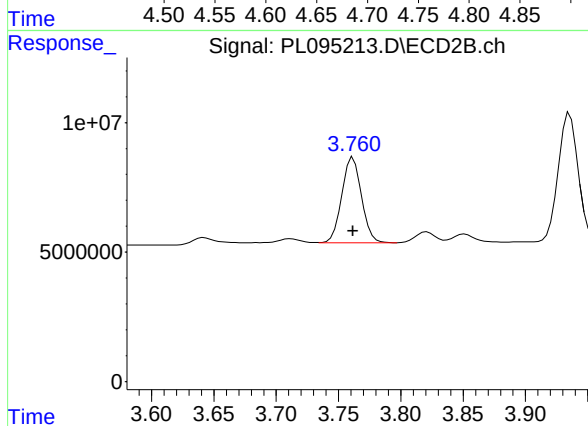

#23 Chlordane-1


R.T.: 3.762 min
Delta R.T.: 0.000 min
Response: 36105290
Conc: 245.27 ng/ml

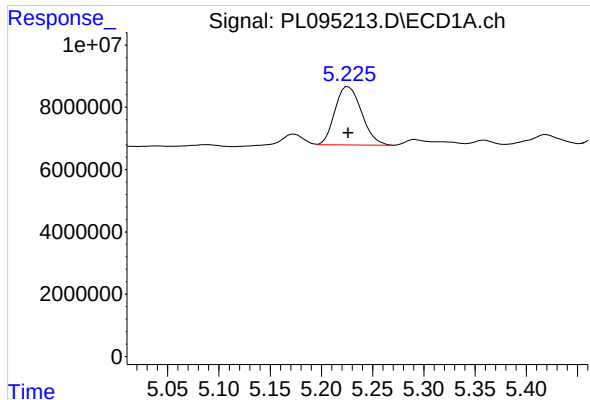

#24 Chlordane-2


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 33790990
Conc: 261.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

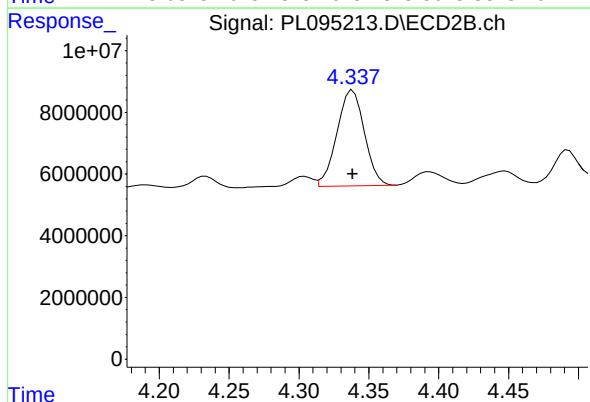


#24 Chlordane-2

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 42416105
Conc: 250.28 ng/ml

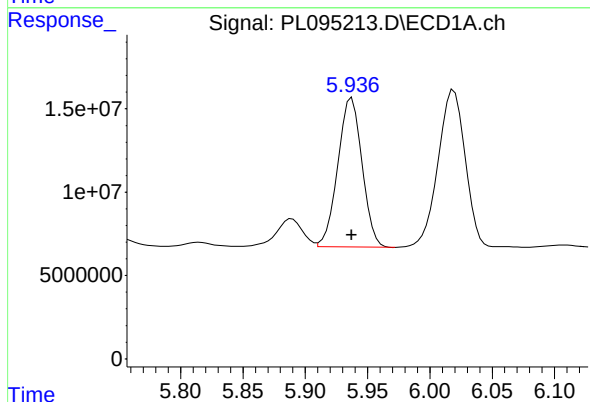


#25 Chlordane-3

R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 120976377
Conc: 259.27 ng/ml

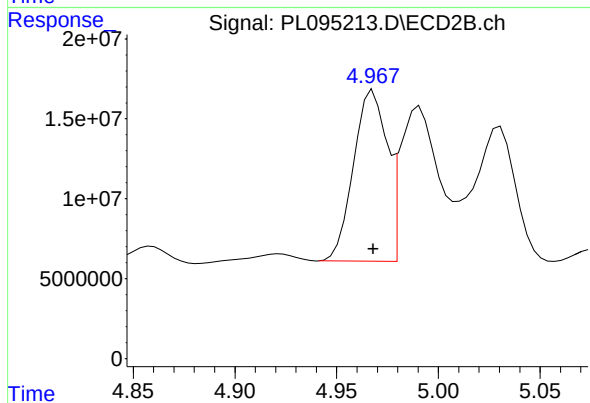

#25 Chlordane-3


R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 122210710
Conc: 244.24 ng/ml

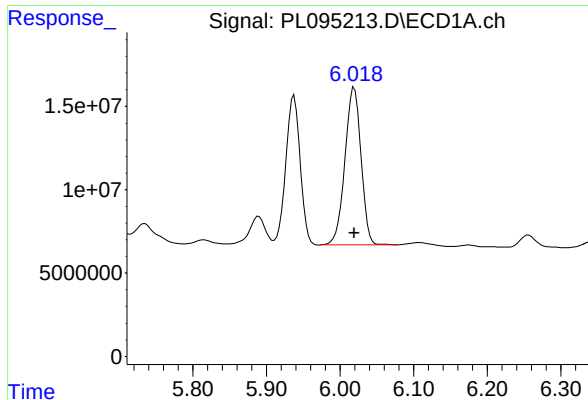

#26 Chlordane-4


R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 143892025
Conc: 260.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

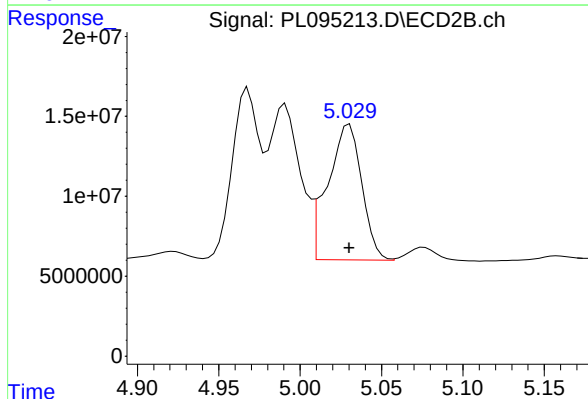


#26 Chlordane-4

R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 122537796
Conc: 247.42 ng/ml

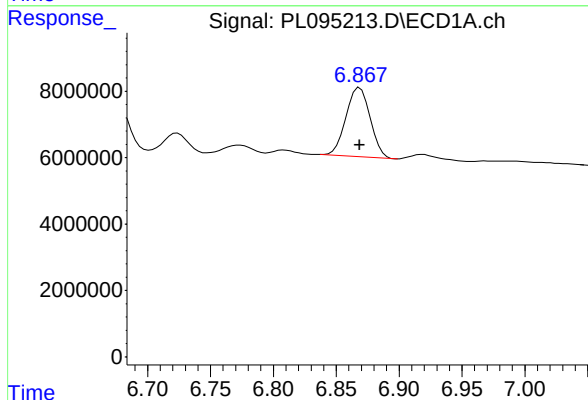


#27 Chlordane-5

R.T.: 6.869 min
Delta R.T.: 0.000 min
Response: 27795039
Conc: 259.78 ng/ml

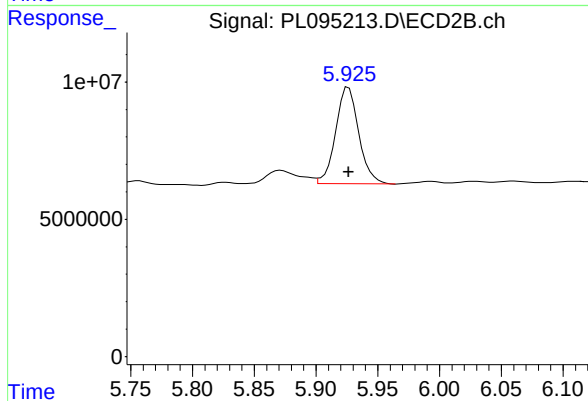

#27 Chlordane-5


R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 45619478
Conc: 246.40 ng/ml

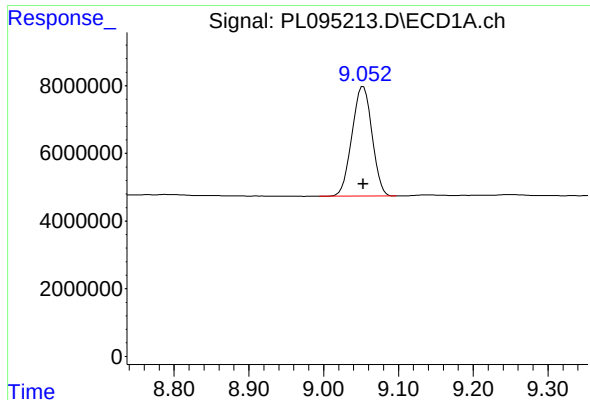

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 60361027
Conc: 26.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

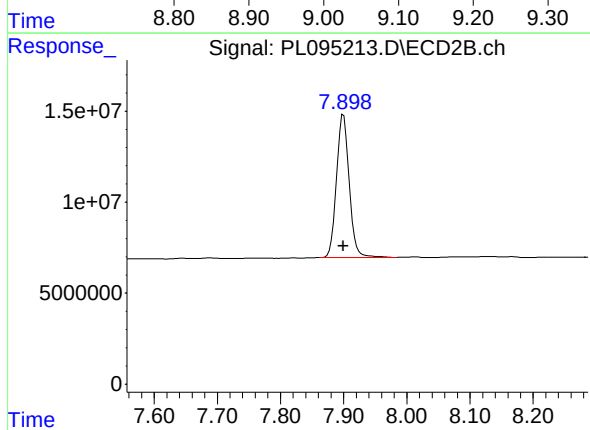

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 109844836
Conc: 25.63 ng/ml