

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041519\
 Data File : PL047364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2019 11:29
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:41:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

20) A	Methoxychlor	6.774	0.000	21980170	0	5.172	N.D.	#
23)	Chlordane-1	4.229f	0.000	13711463	0	40.772	N.D.	#
24)	Chlordane-2	4.703	0.000	4482311	0	11.814	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041519\
Data File : PL047364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2019 11:29
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:41:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

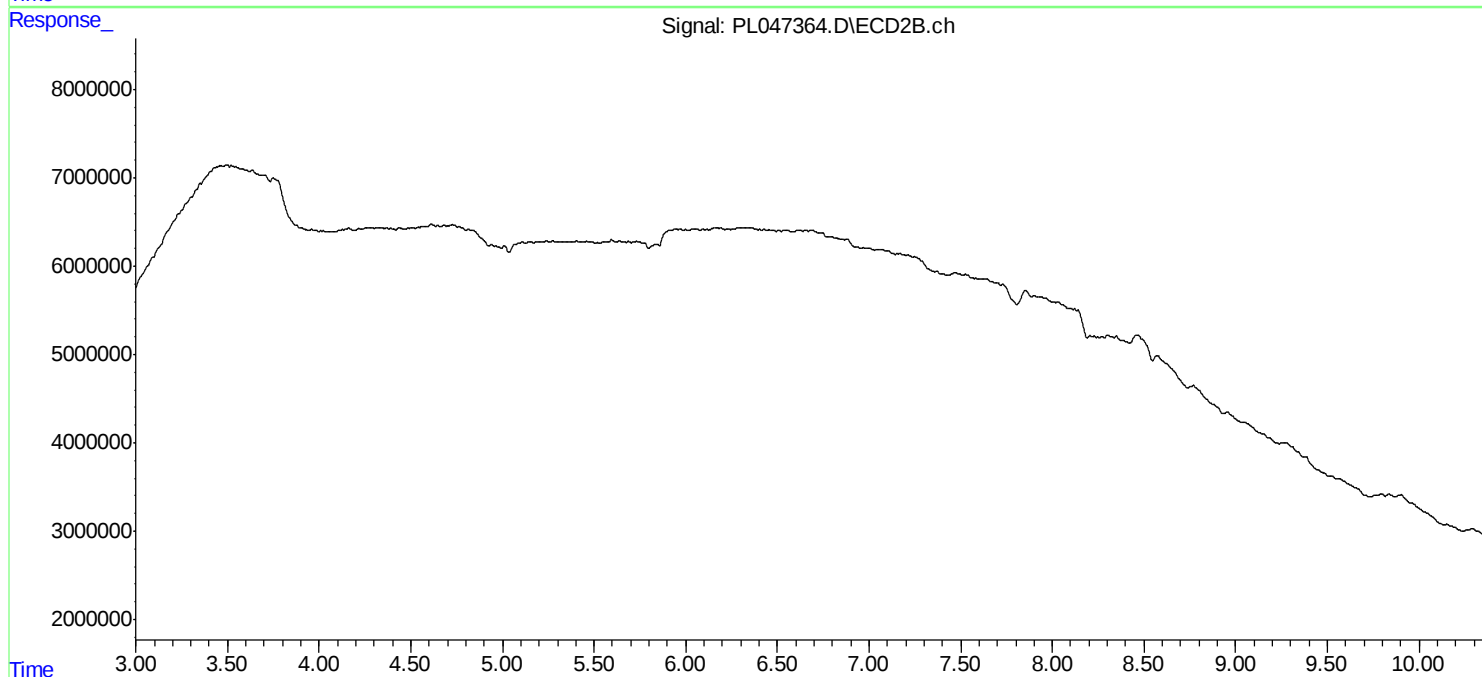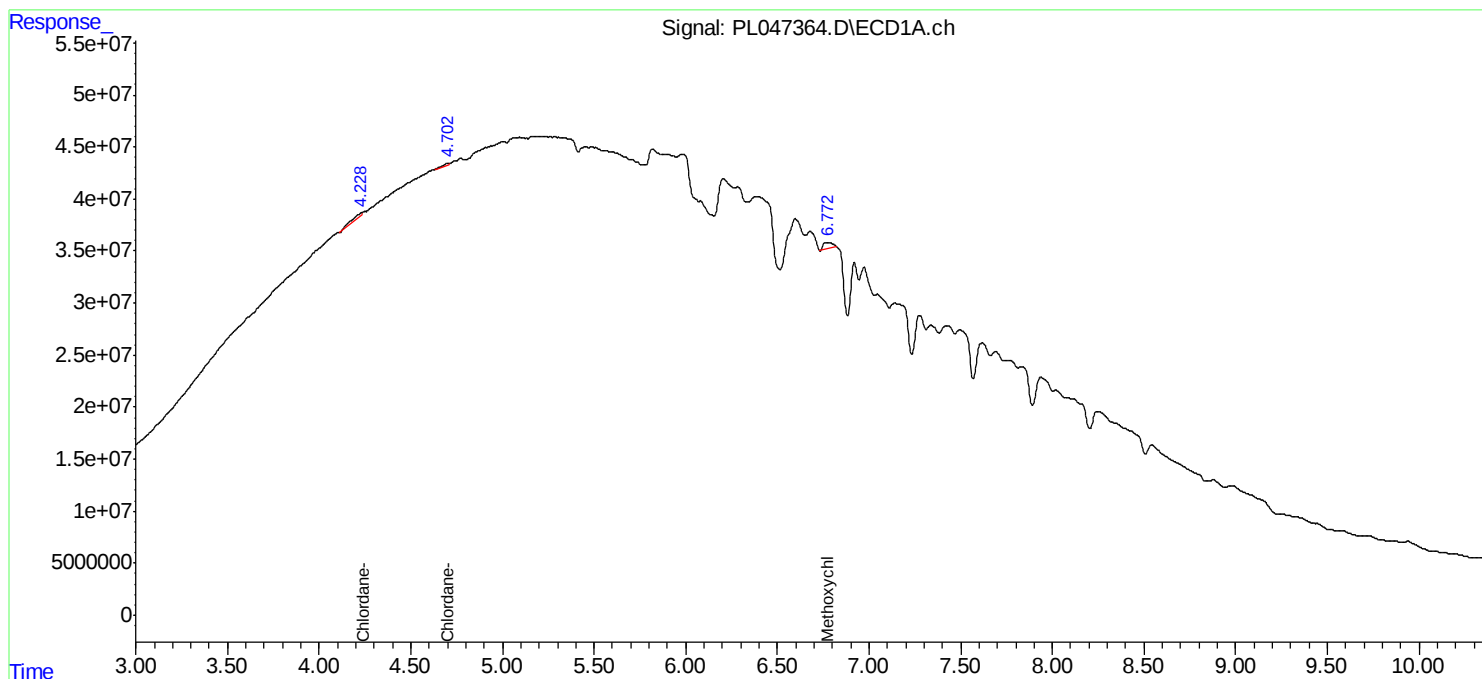


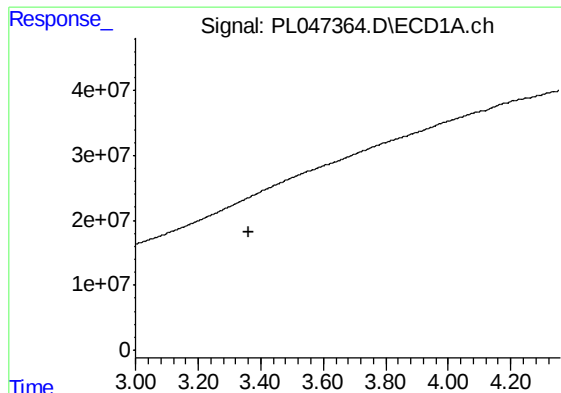

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

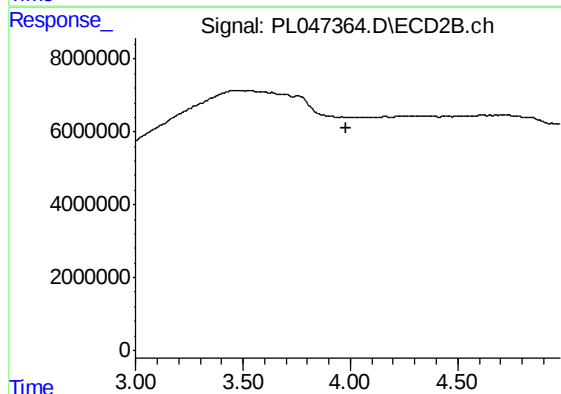


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.981 min
Response: 0
Conc: N.D.

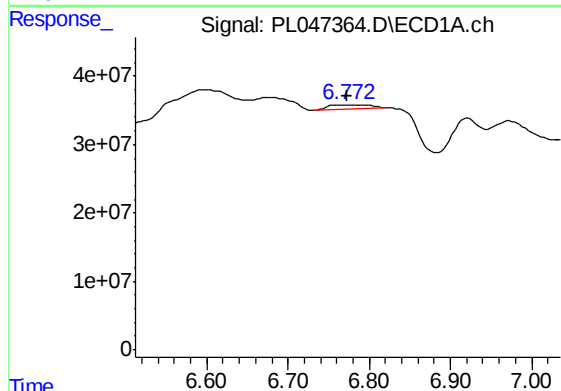


#20 Methoxychlor

R.T.: 6.774 min
Delta R.T.: 0.000 min
Response: 21980170
Conc: 5.17 ng/ml

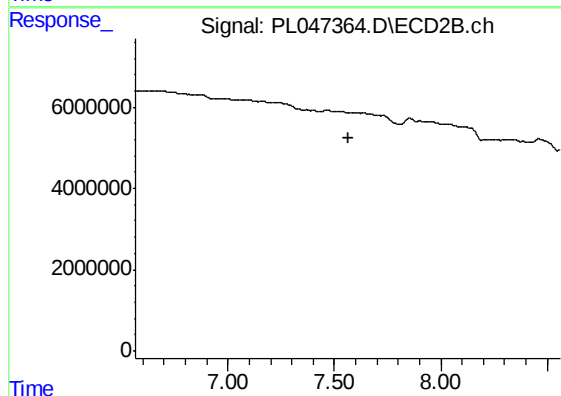

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.565 min
Response: 0
Conc: N.D.

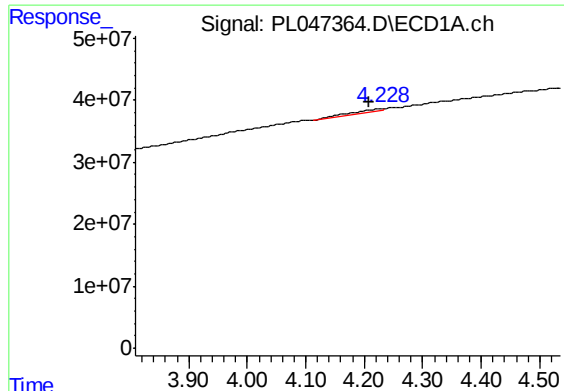

#23 Chlordane-1


R.T.: 4.229 min
Delta R.T.: 0.021 min
Response: 13711463
Conc: 40.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

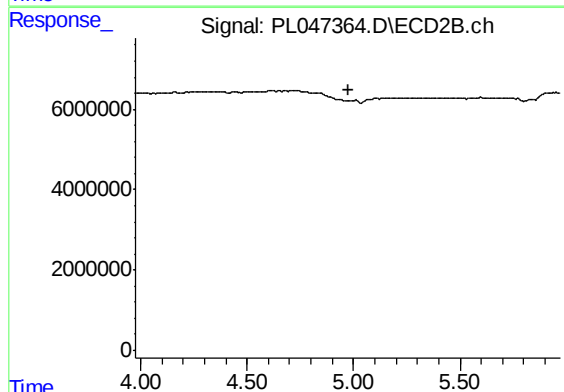


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

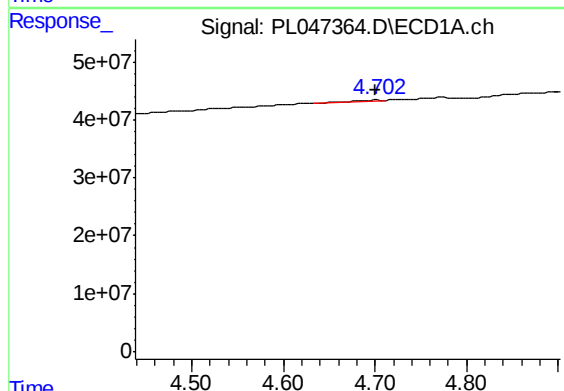


#24 Chlordane-2

R.T.: 4.703 min
Delta R.T.: 0.002 min
Response: 4482311
Conc: 11.81 ng/ml

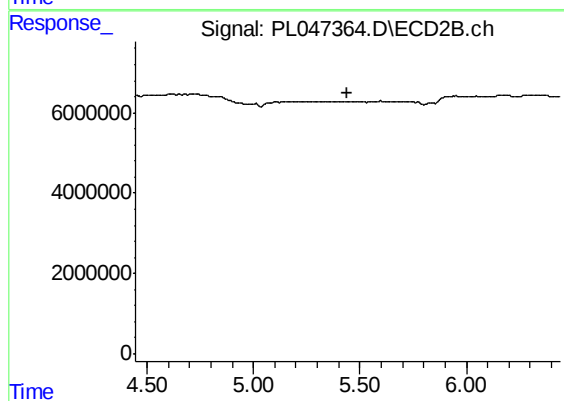

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.443 min
Response: 0
Conc: N.D.

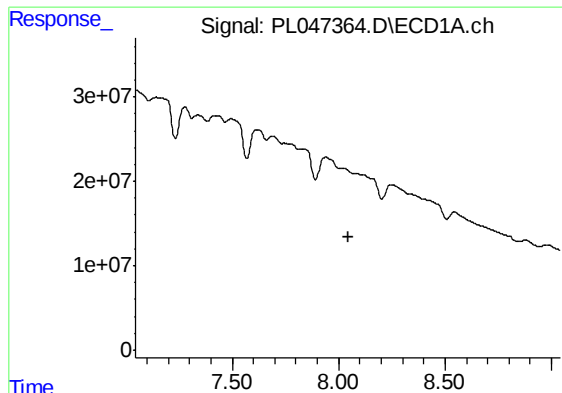

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.044 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

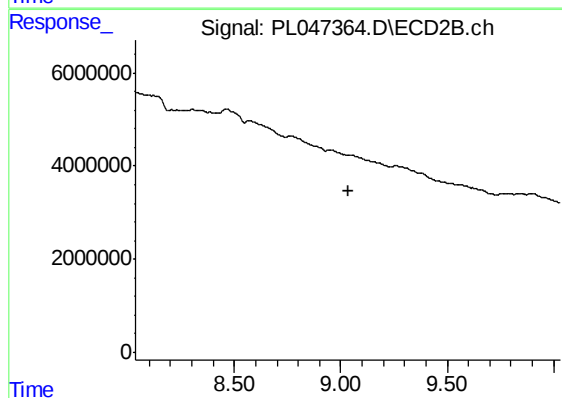

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.035 min
Response: 0
Conc: N.D.