

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041519\
 Data File : PL047405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2019 22:00
 Operator : AJ\SJ
 Sample : K2397-08
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:51:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	3.976	155.9E6	48557640	21.432	21.208
28)	SA Decachlor...	8.034	9.030	160.1E6	49010913	19.036	21.139
Target Compounds							
6)	B beta-BHC	0.000	4.826	0	208640	N.D.	0.157 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041519\
Data File : PL047405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2019 22:00
Operator : AJ\SJ
Sample : K2397-08
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:51:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

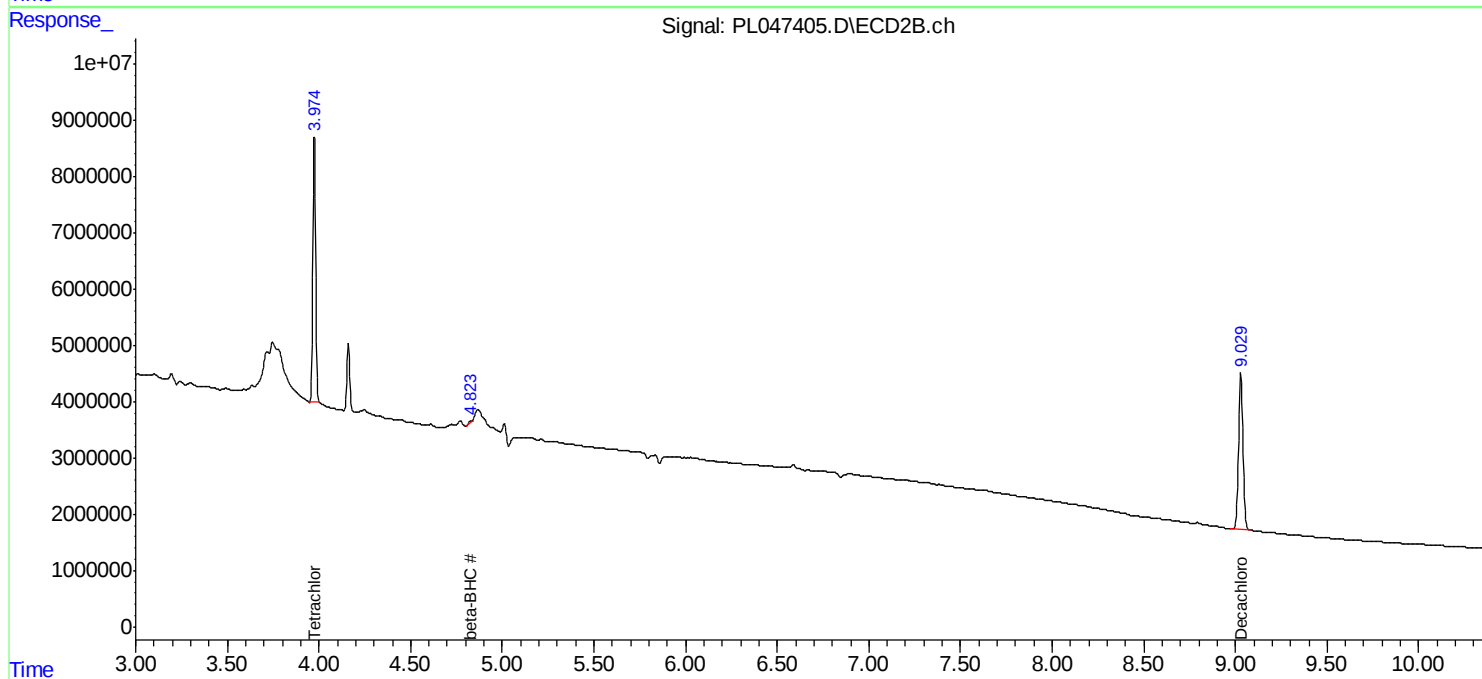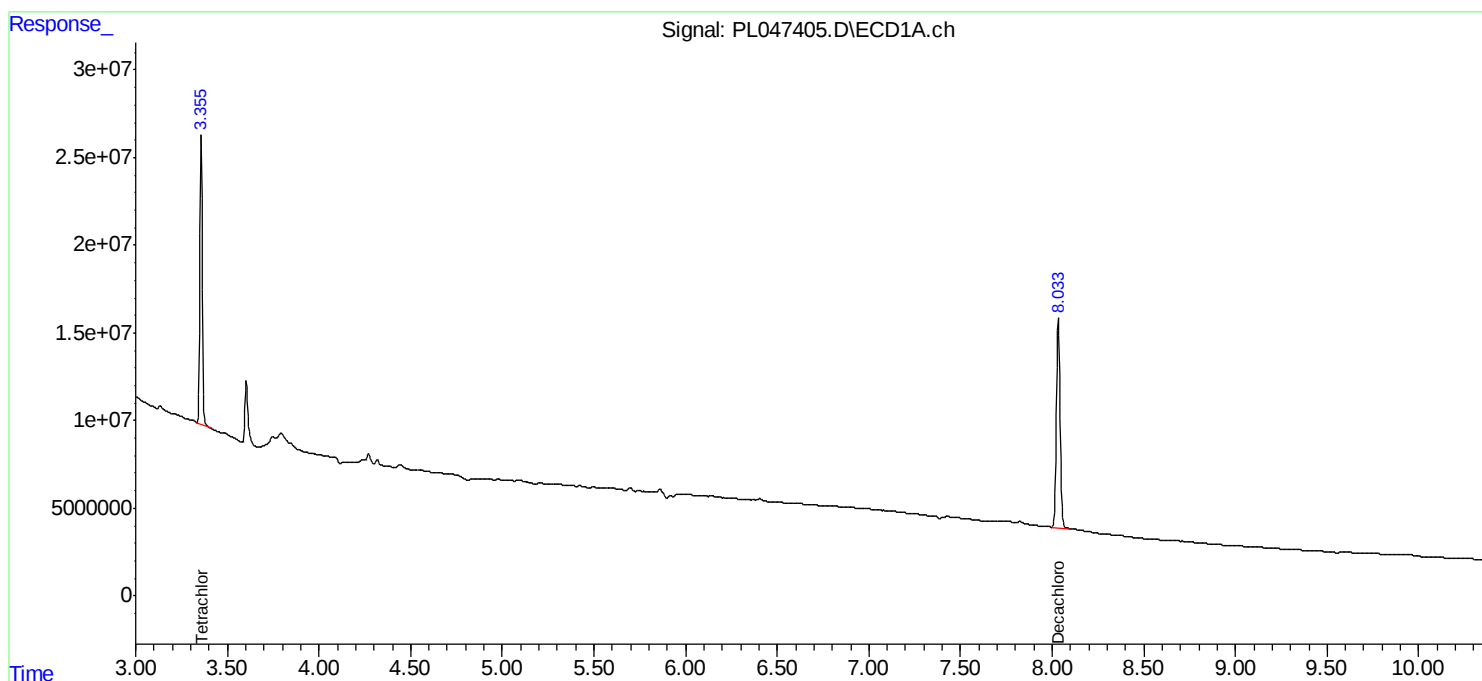


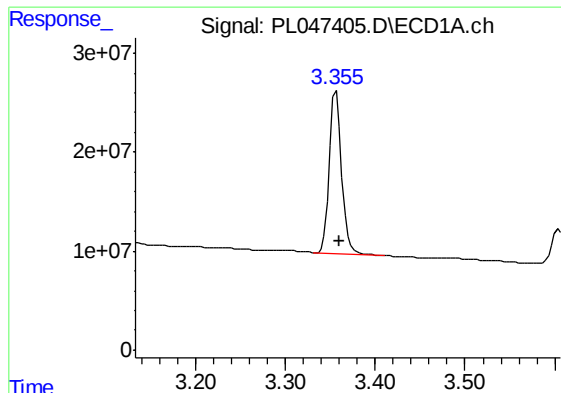

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 155913732
Conc: 21.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-D

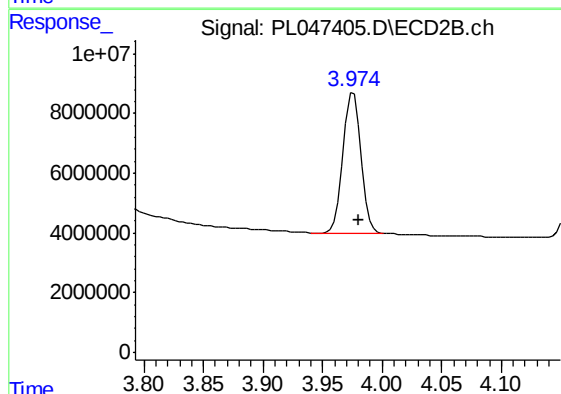


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 48557640
Conc: 21.21 ng/ml

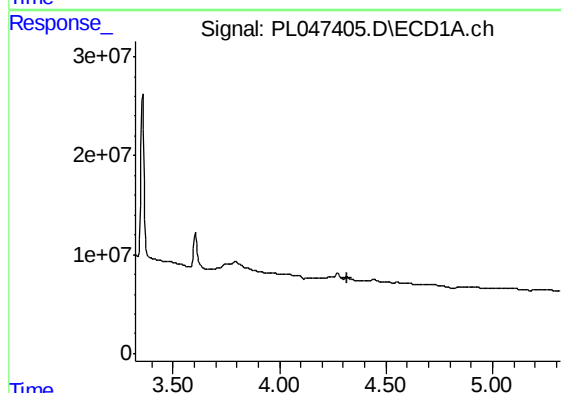


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.321 min
Response: 0
Conc: N.D.

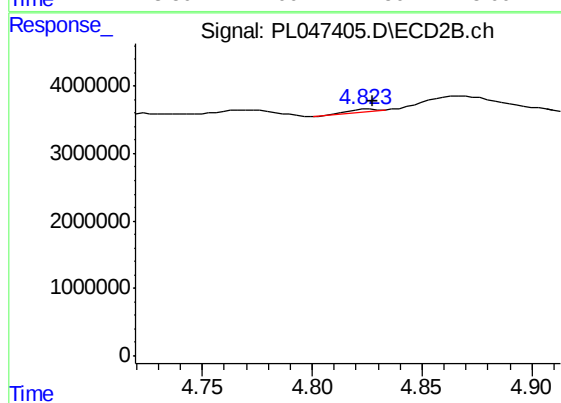

#6 beta-BHC


R.T.: 4.826 min
Delta R.T.: -0.002 min
Response: 208640
Conc: 0.16 ng/ml

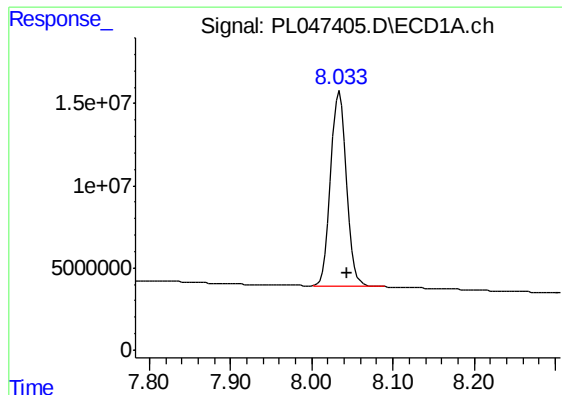

#28 Decachlorobiphenyl

R.T.: 8.034 min
Delta R.T.: -0.010 min
Response: 160110964
Conc: 19.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-D

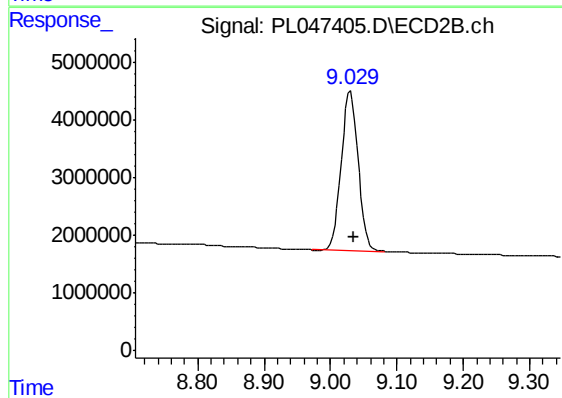

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.005 min
Response: 49010913
Conc: 21.14 ng/ml