

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
 Data File : PL058014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2020 16:48
 Operator : AJ\MA
 Sample : PB128246TB
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 00:50:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.955	204.2E6	39852750	20.253	18.364
28)	SA Decachlor...	8.204	8.977	185.9E6	41661060	18.030	18.651
Target Compounds							
2)	A alpha-BHC	3.886	0.000	3250641	0	0.187	N.D. #
4)	MA Heptachlor	0.000	5.136	0	2021240	N.D.	0.602 #
6)	B beta-BHC	4.440	0.000	245133	0	0.039	N.D. #
8)	B Heptachlo...	0.000	5.787f	0	5378103	N.D.	1.992 #
14)	MA Endrin	6.010	0.000	6465366	0	0.554	N.D. #
15)	B Endosulfa...	0.000	6.867	0	311701	N.D.	0.120 #
19)	B Endosulfa...	6.674	0.000	514562	0	0.051	N.D. #
23)	Chlordane-1	4.352f	0.000	2265754	0	6.126	N.D. #
24)	Chlordane-2	4.848f	0.000	677730	0	1.679	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
Data File : PL058014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2020 16:48
Operator : AJ\MA
Sample : PB128246TB
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 00:50:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

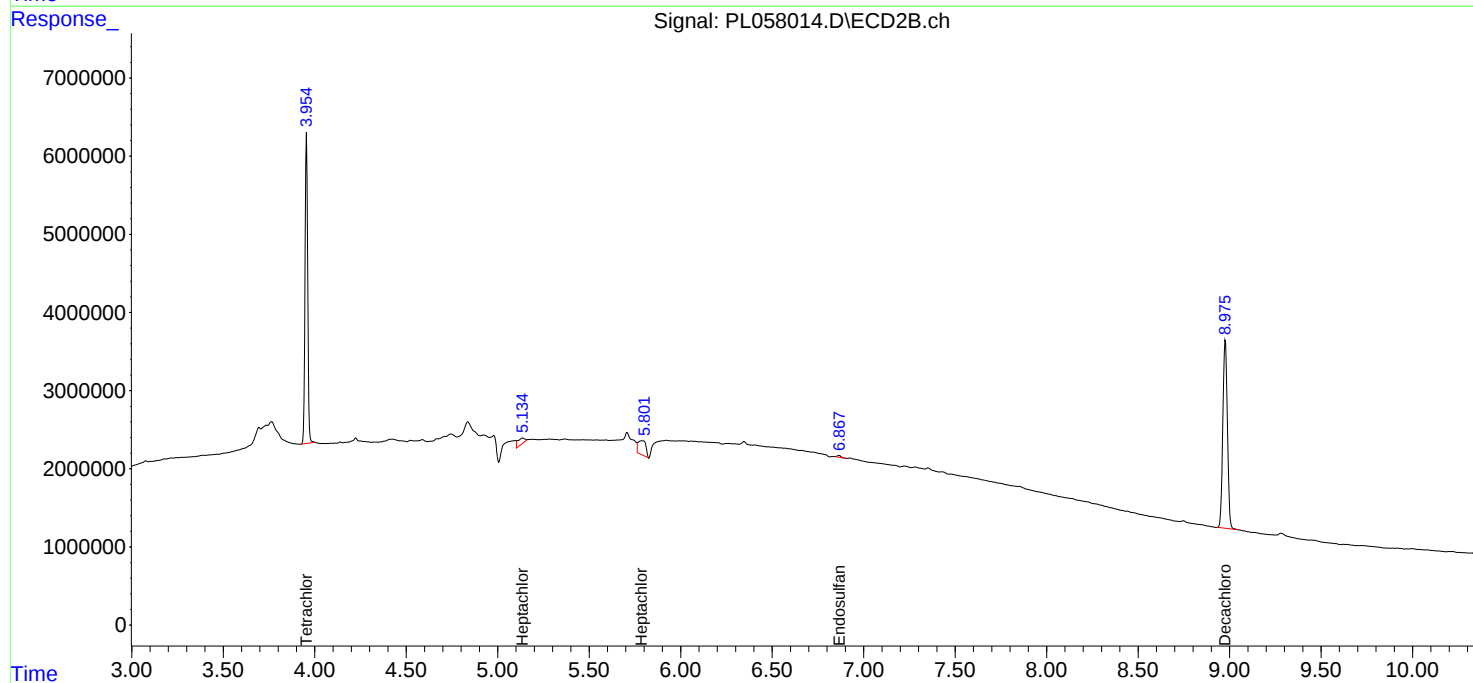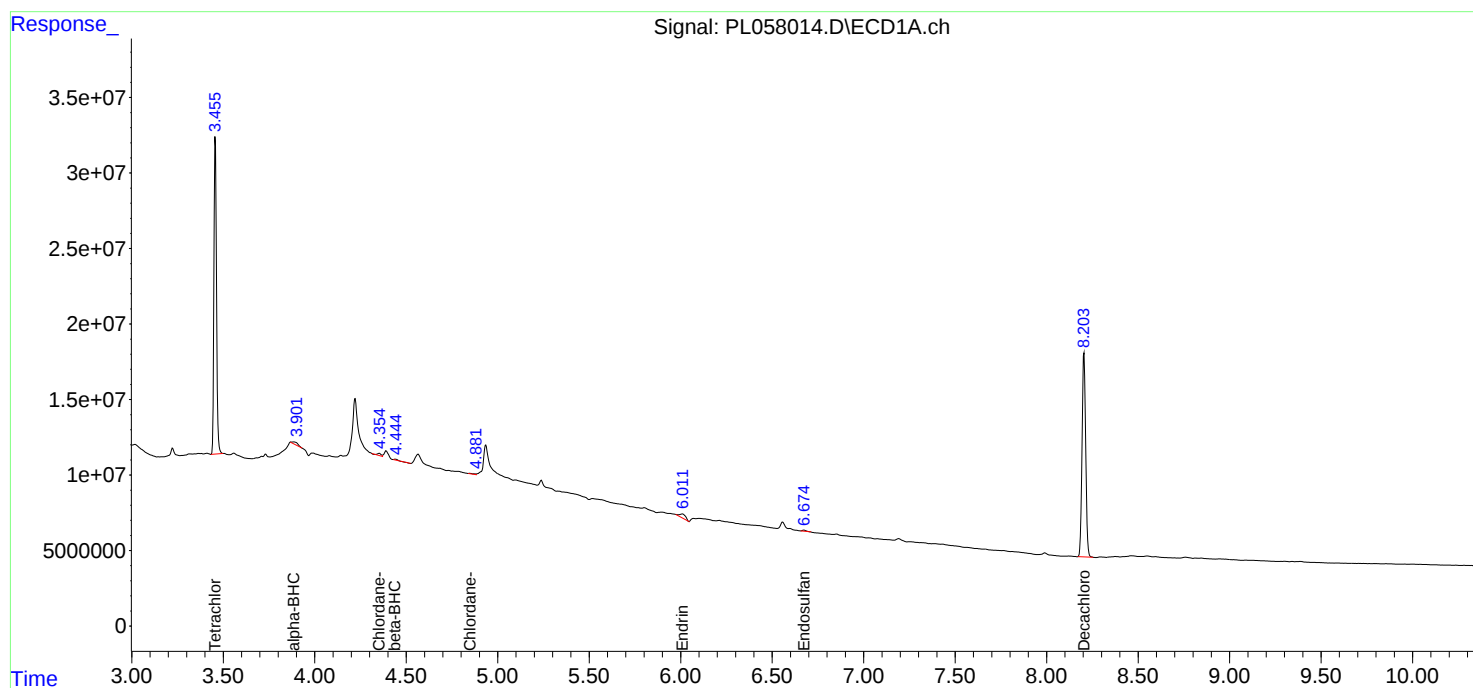


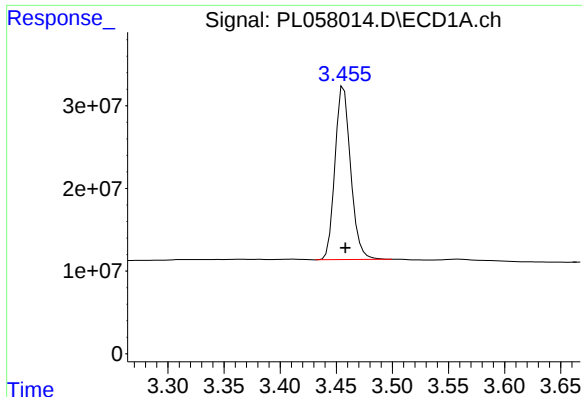

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 204169168
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

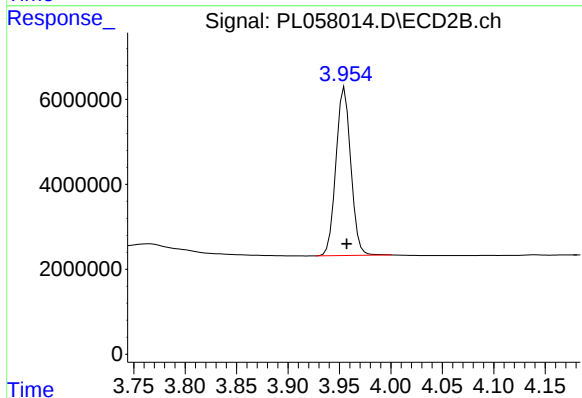


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 39852750
Conc: 18.36 ng/ml

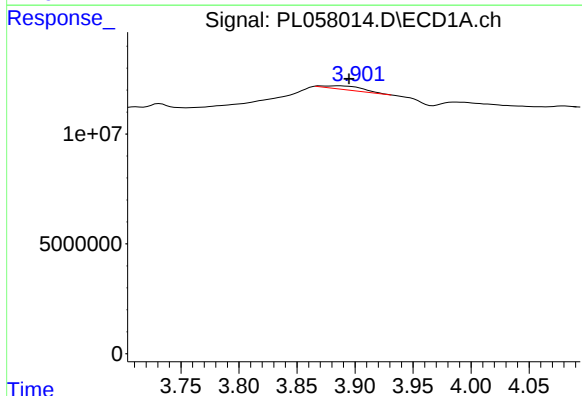


#2 alpha-BHC

R.T.: 3.886 min
Delta R.T.: -0.009 min
Response: 3250641
Conc: 0.19 ng/ml

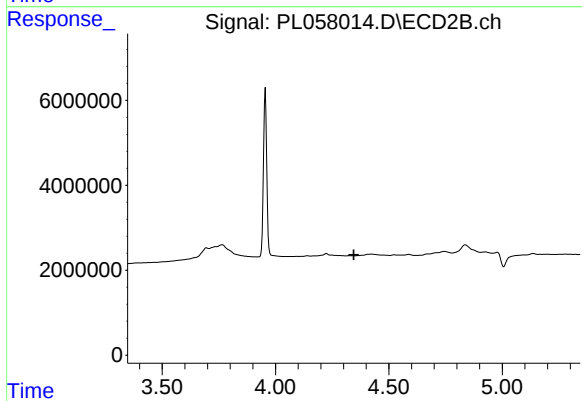

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

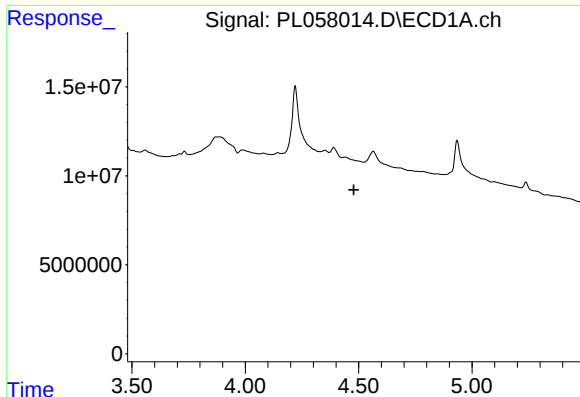

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

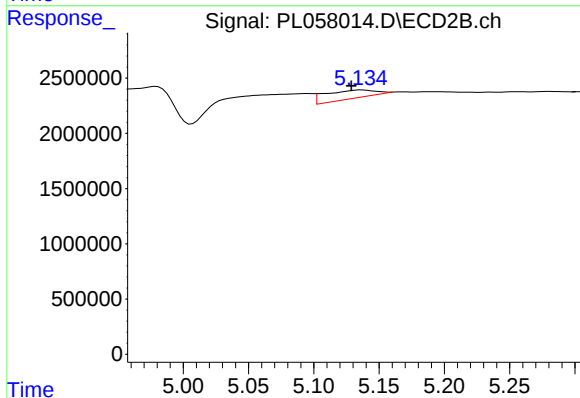


#4 Heptachlor

R.T.: 5.136 min
Delta R.T.: 0.008 min
Response: 2021240
Conc: 0.60 ng/ml

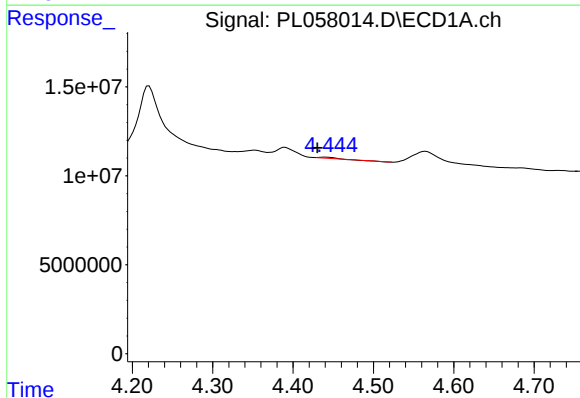


#6 beta-BHC

R.T.: 4.440 min
Delta R.T.: 0.009 min
Response: 245133
Conc: 0.04 ng/ml

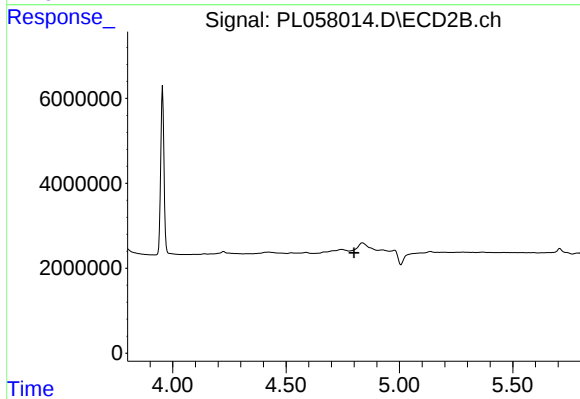

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

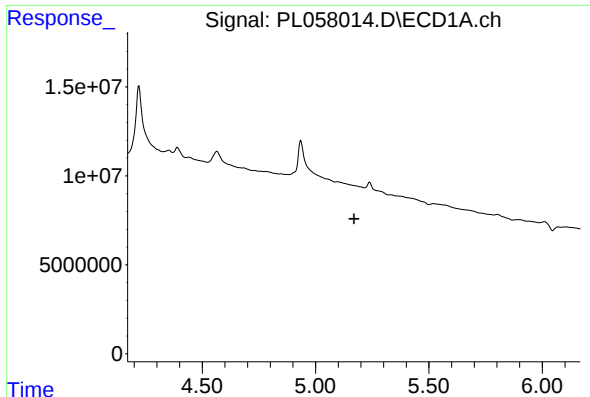

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

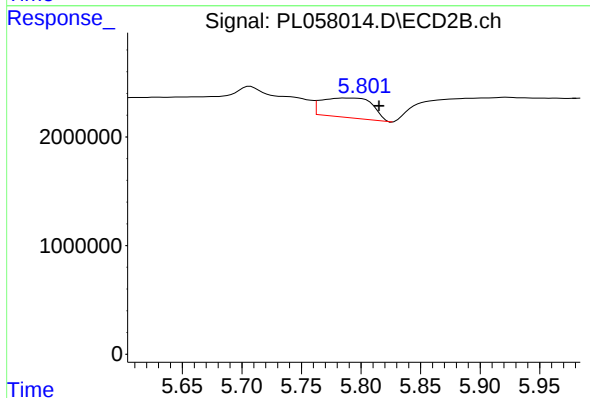


#8 Heptachlor epoxide

R.T.: 5.787 min
Delta R.T.: -0.028 min
Response: 5378103
Conc: 1.99 ng/ml

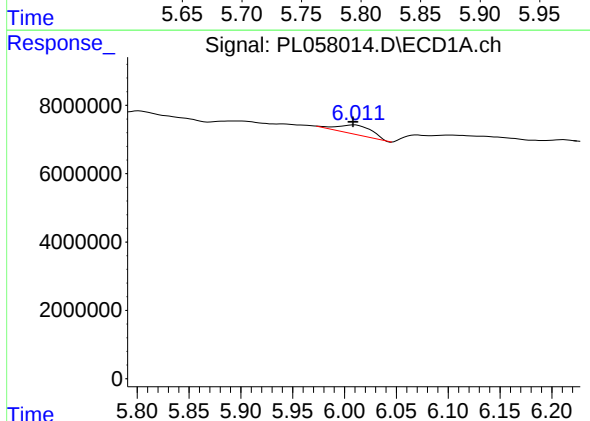


#14 Endrin

R.T.: 6.010 min
Delta R.T.: 0.001 min
Response: 6465366
Conc: 0.55 ng/ml

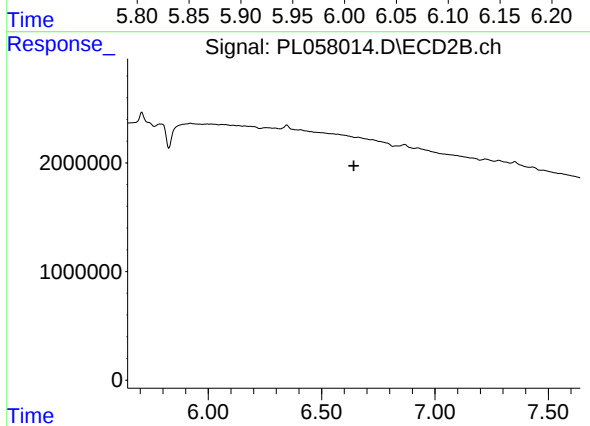

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.642 min
Response: 0
Conc: N.D.

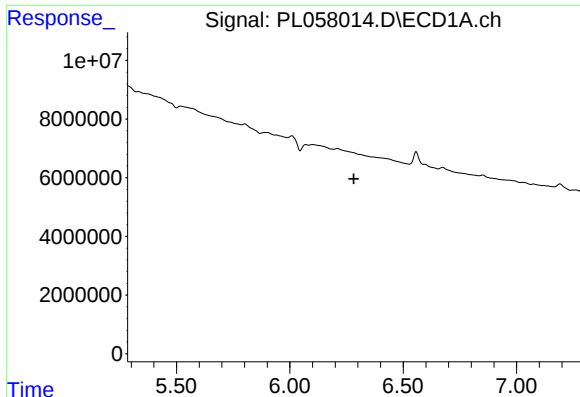

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

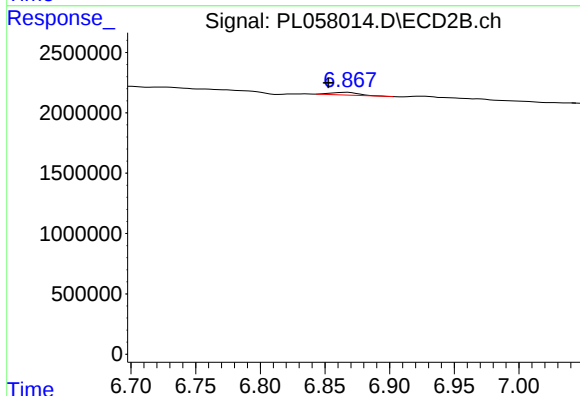


#15 Endosulfan II

R.T.: 6.867 min
Delta R.T.: 0.015 min
Response: 311701
Conc: 0.12 ng/ml

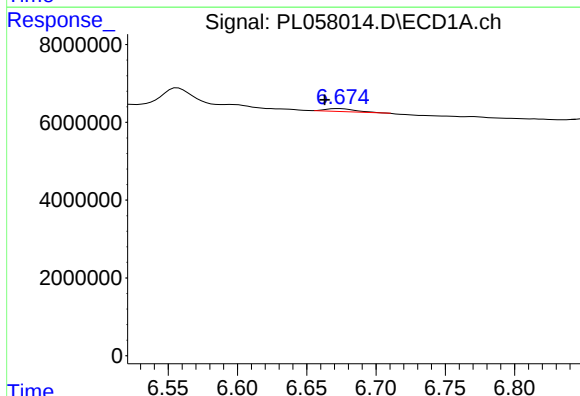


#19 Endosulfan Sulfate

R.T.: 6.674 min
Delta R.T.: 0.011 min
Response: 514562
Conc: 0.05 ng/ml

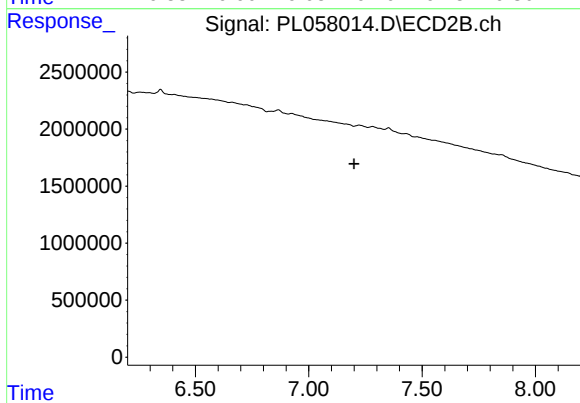

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

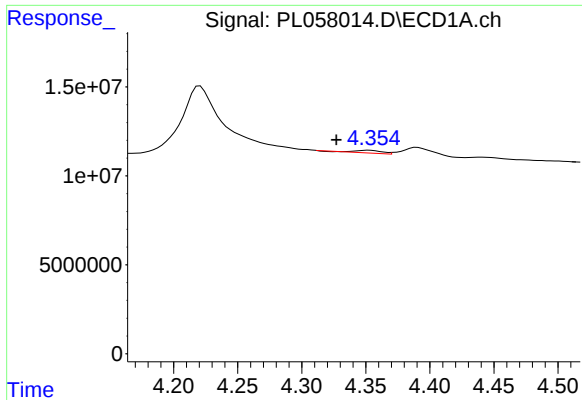

#23 Chlordane-1


R.T.: 4.352 min
Delta R.T.: 0.025 min
Response: 2265754
Conc: 6.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

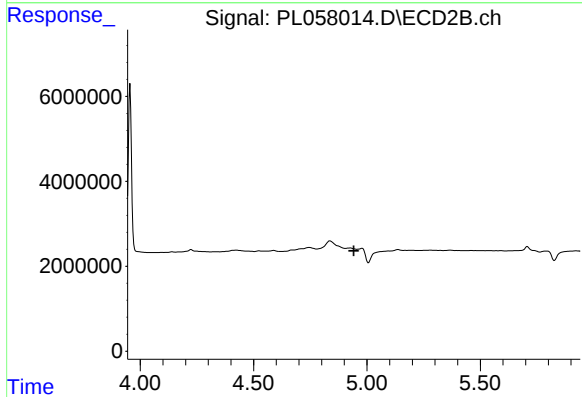


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

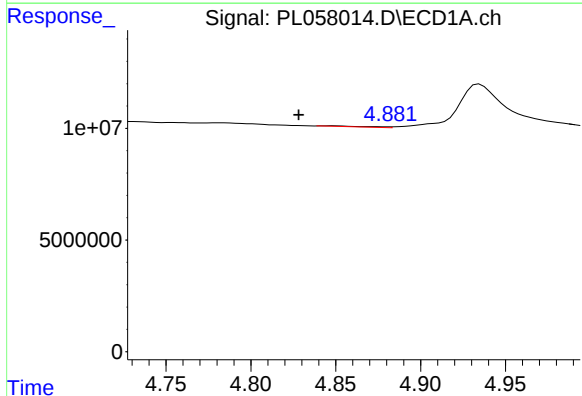


#24 Chlordane-2

R.T.: 4.848 min
Delta R.T.: 0.020 min
Response: 677730
Conc: 1.68 ng/ml

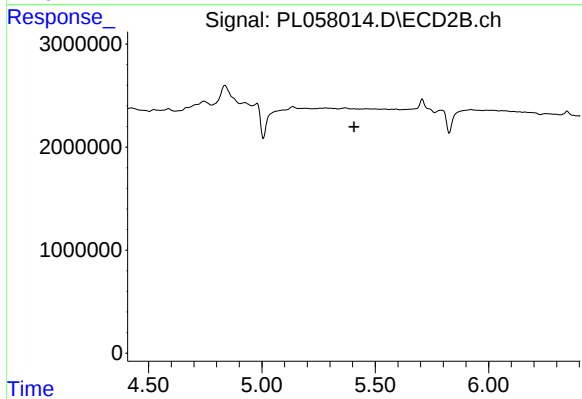

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

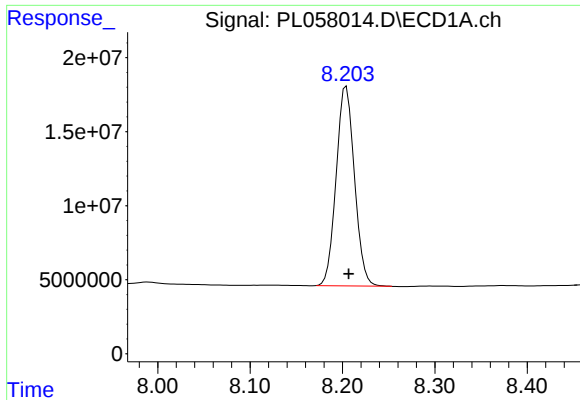

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 185858998
Conc: 18.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

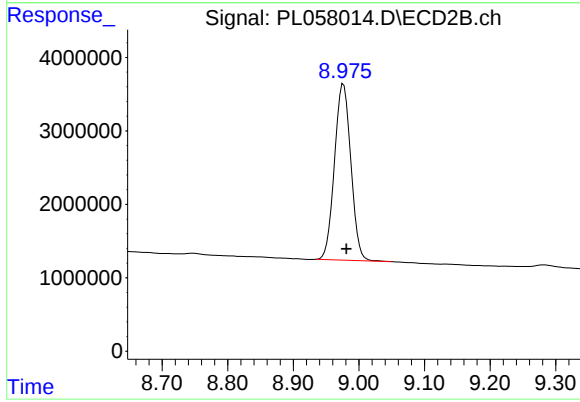

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 41661060
Conc: 18.65 ng/ml