

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
 Data File : PL058016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2020 17:16
 Operator : AJ\MA
 Sample : PB128227BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 00:50:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	213.1E6	42247202	21.136	19.467
28)	SA Decachlor...	8.204	8.977	190.4E6	43713670	18.472	19.569
Target Compounds							
2)	A alpha-BHC	3.896	0.000	6522956	0	0.375	N.D. #
4)	MA Heptachlor	0.000	5.139	0	8789752	N.D.	2.619 #
8)	B Heptachlo...	0.000	5.798f	0	4357673	N.D.	1.614 #
13)	MA Dieldrin	5.764	0.000	500858	0	0.039	N.D. #
14)	MA Endrin	6.008	0.000	2738078	0	0.235	N.D. #
15)	B Endosulfa...	0.000	6.866	0	250579	N.D.	0.097 #
23)	Chlordane-1	4.353f	0.000	3135702	0	8.478	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
Data File : PL058016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2020 17:16
Operator : AJ\MA
Sample : PB128227BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 00:50:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

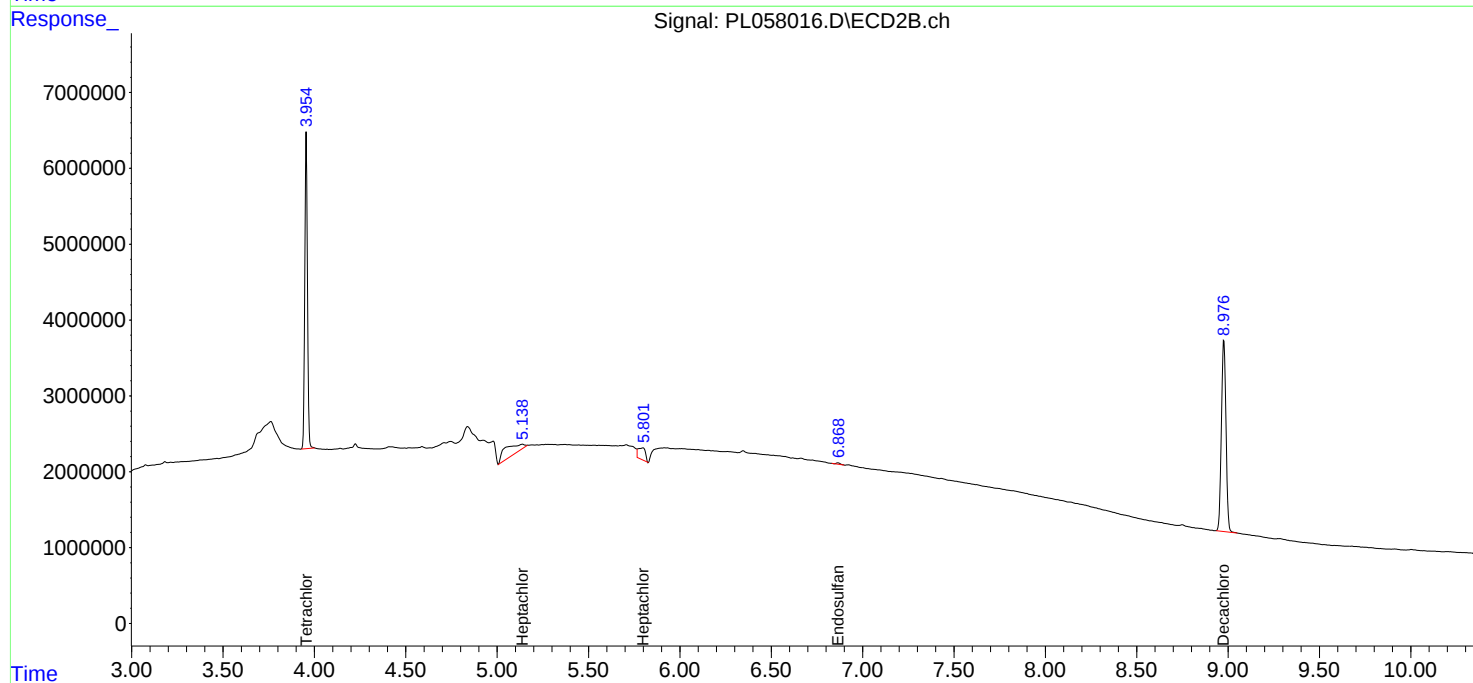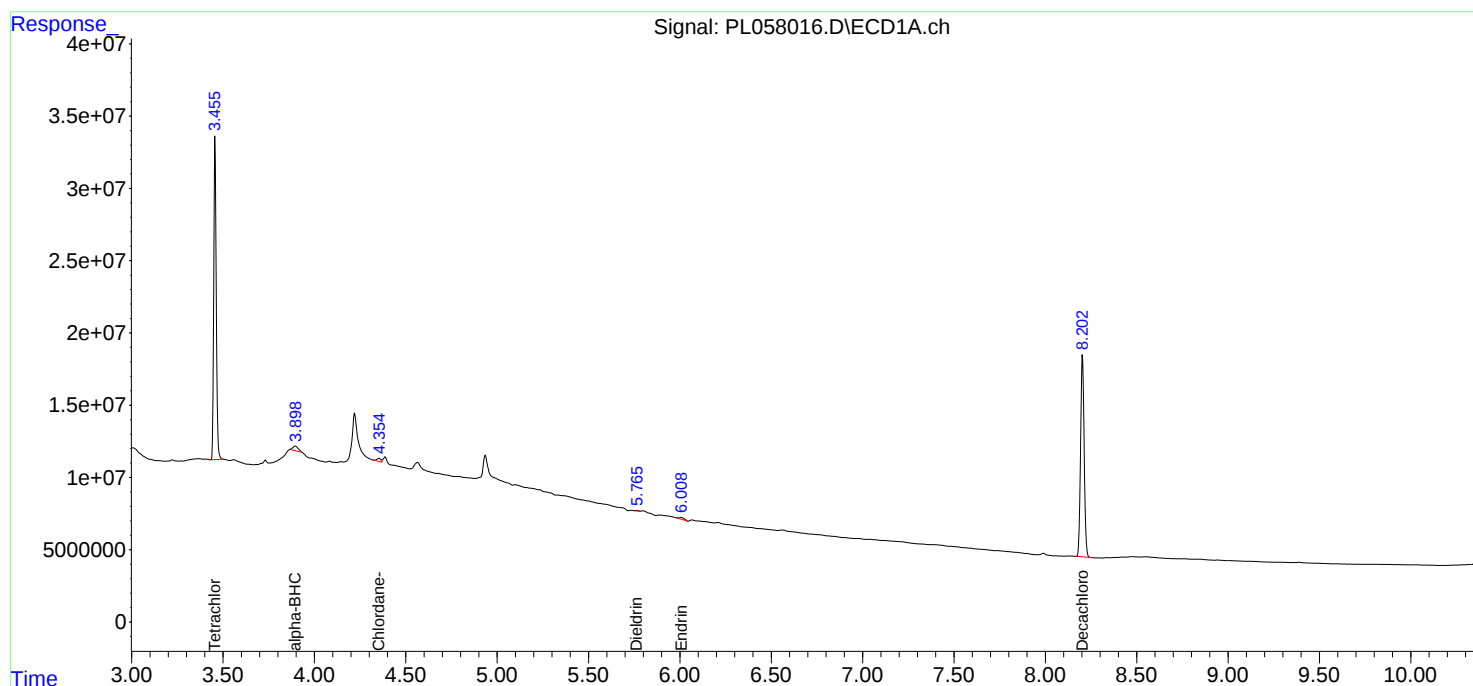

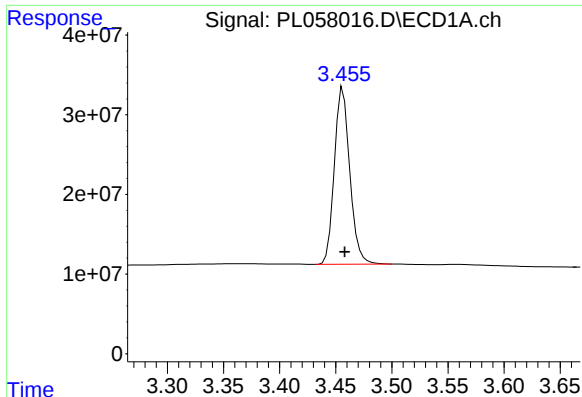


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 213070091
Conc: 21.14 ng/ml

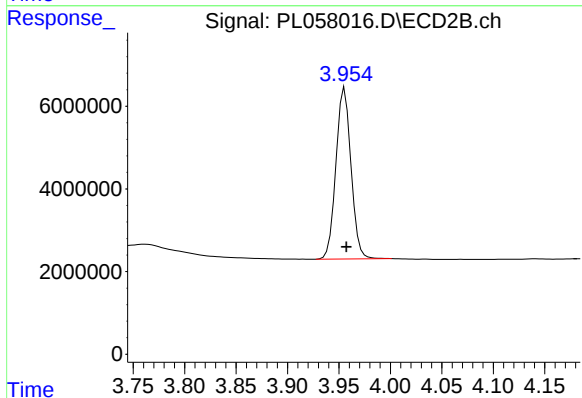


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.002 min
Response: 42247202
Conc: 19.47 ng/ml

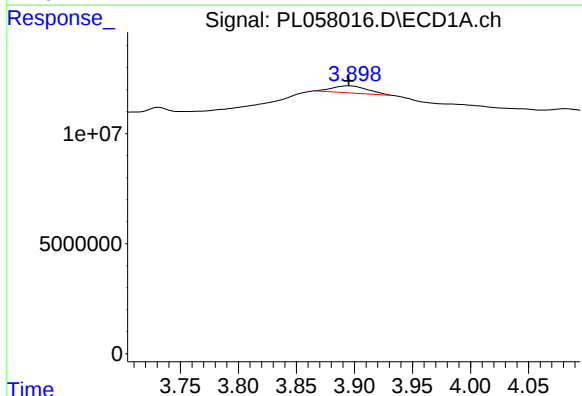


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 6522956
Conc: 0.38 ng/ml

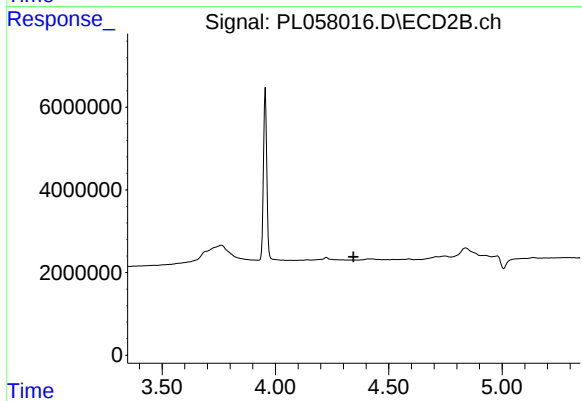


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

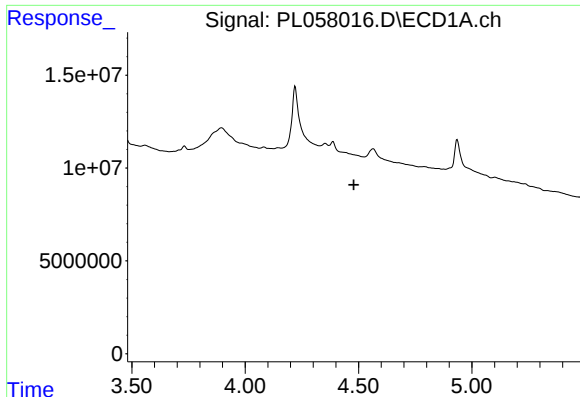


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

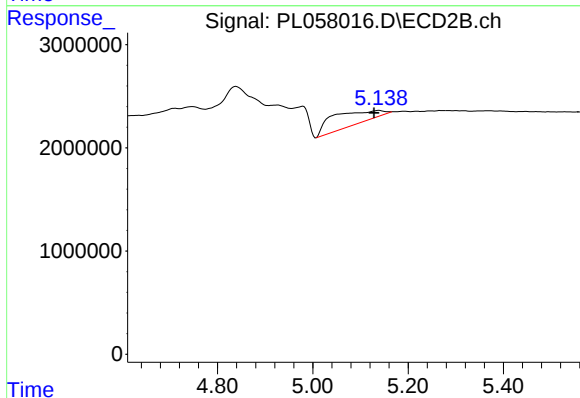


#4 Heptachlor

R.T.: 5.139 min
Delta R.T.: 0.010 min
Response: 8789752
Conc: 2.62 ng/ml

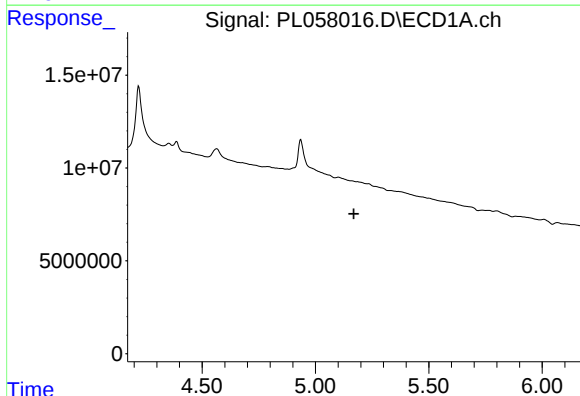


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

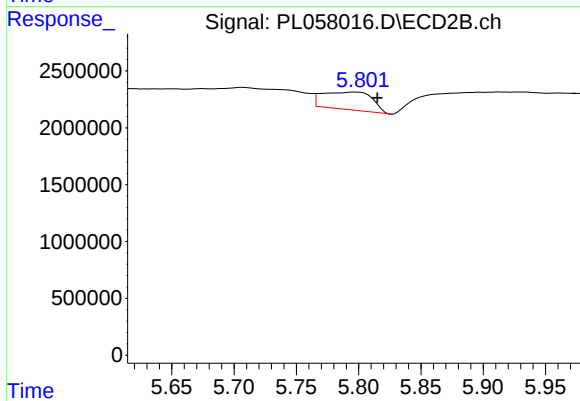


#8 Heptachlor epoxide

R.T.: 5.798 min
Delta R.T.: -0.017 min
Response: 4357673
Conc: 1.61 ng/ml

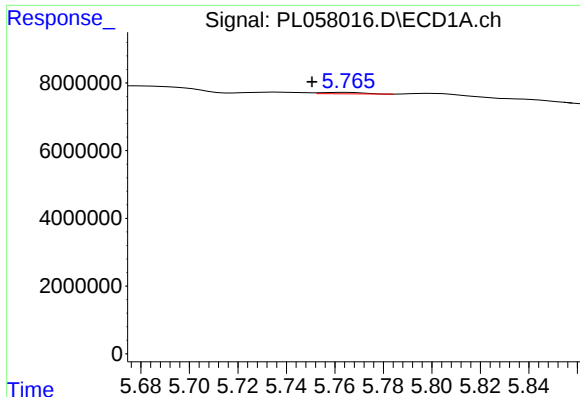


#13 Dieldrin

R.T.: 5.764 min
Delta R.T.: 0.013 min
Response: 500858
Conc: 0.04 ng/ml

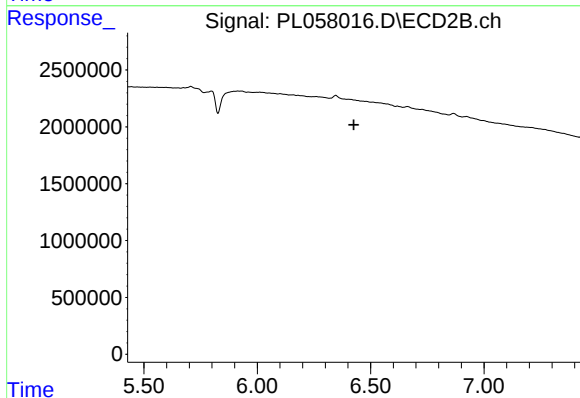


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.425 min
Response: 0
Conc: N.D.

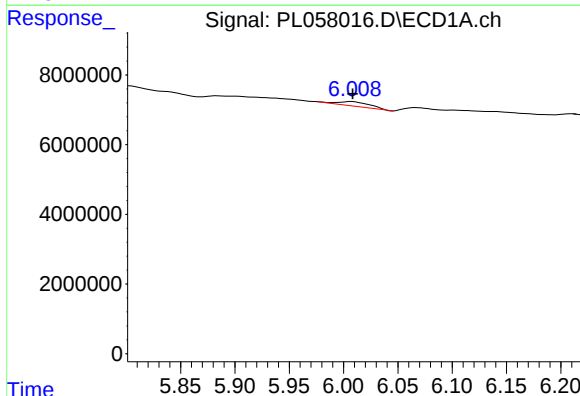


#14 Endrin

R.T.: 6.008 min
Delta R.T.: 0.000 min
Response: 2738078
Conc: 0.23 ng/ml

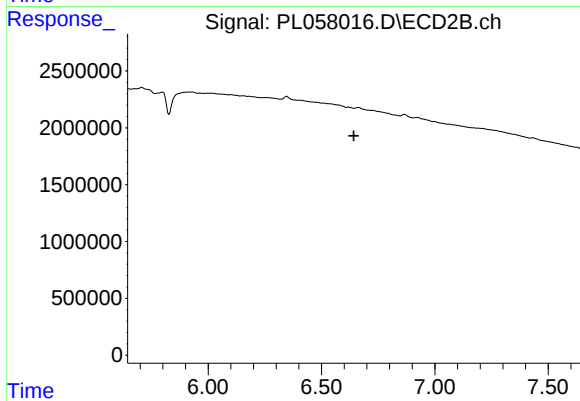


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.642 min
Response: 0
Conc: N.D.

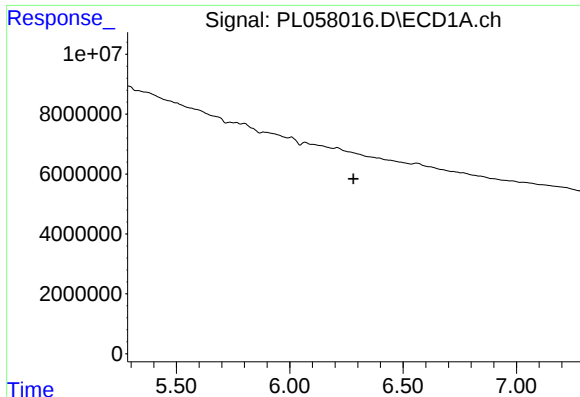


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

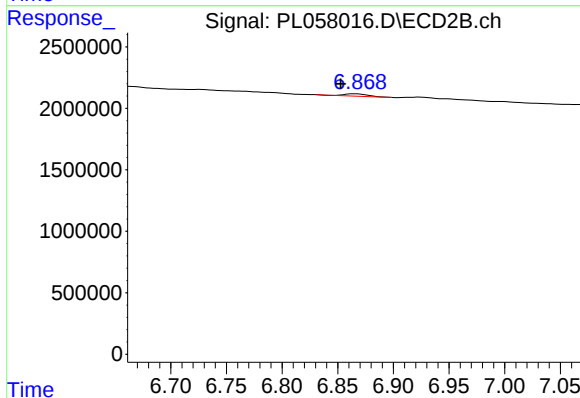


#15 Endosulfan II

R.T.: 6.866 min
Delta R.T.: 0.013 min
Response: 250579
Conc: 0.10 ng/ml

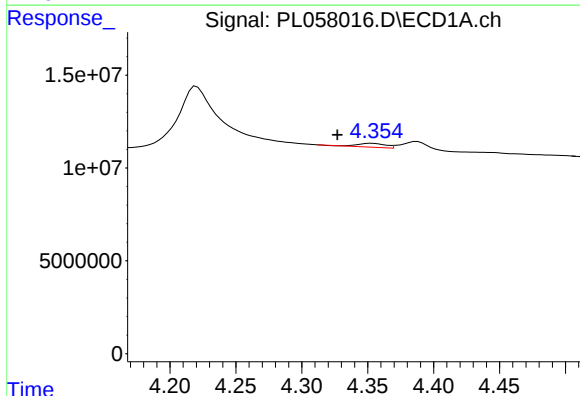


#23 Chlordane-1

R.T.: 4.353 min
Delta R.T.: 0.026 min
Response: 3135702
Conc: 8.48 ng/ml

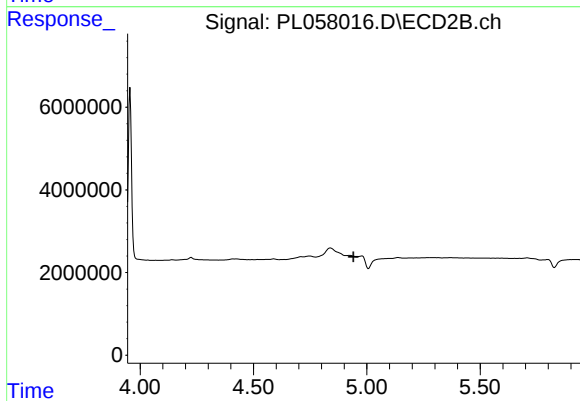


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

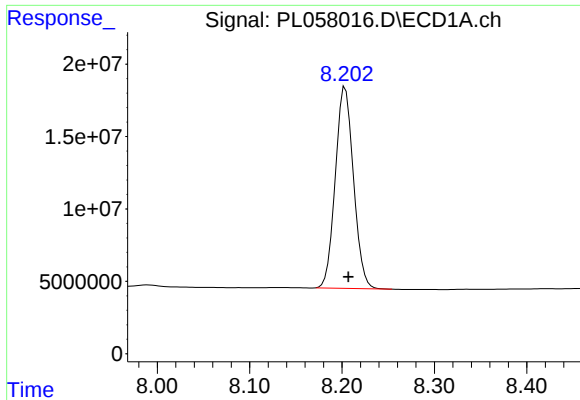

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 190417252
Conc: 18.47 ng/ml

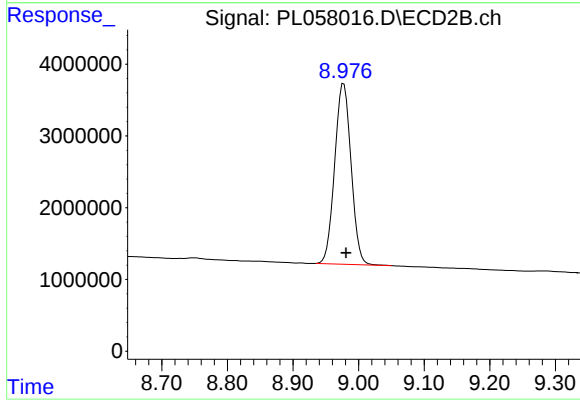

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.003 min
Response: 43713670
Conc: 19.57 ng/ml