

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
 Data File : PL058018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2020 17:44
 Operator : AJ\MA
 Sample : L2243-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 00:51:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	95838590	20202750	9.507	9.309
28)	SA Decachlor...	8.203	8.977	103.3E6	23699804	10.021	10.610
Target Compounds							
2)	A alpha-BHC	3.890	0.000	4202681	0	0.242	N.D. #
4)	MA Heptachlor	0.000	5.135	0	6423560	N.D.	1.914 #
12)	B 4,4'-DDE	5.613	0.000	419621	0	0.032	N.D. #
17)	MA 4,4'-DDT	6.366	0.000	1069031	0	0.105	N.D. #
24)	Chlordane-2	4.855f	0.000	1722326	0	4.266	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
Data File : PL058018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2020 17:44
Operator : AJ\MA
Sample : L2243-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 00:51:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

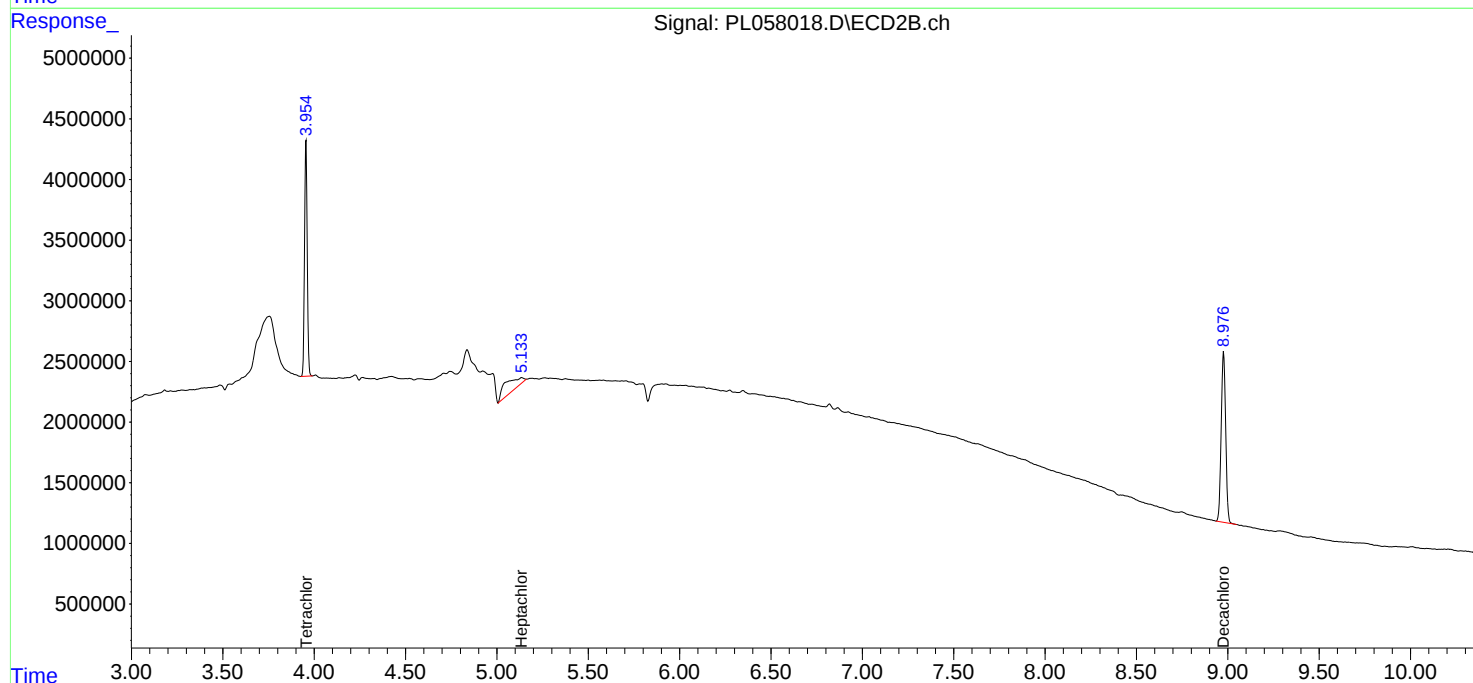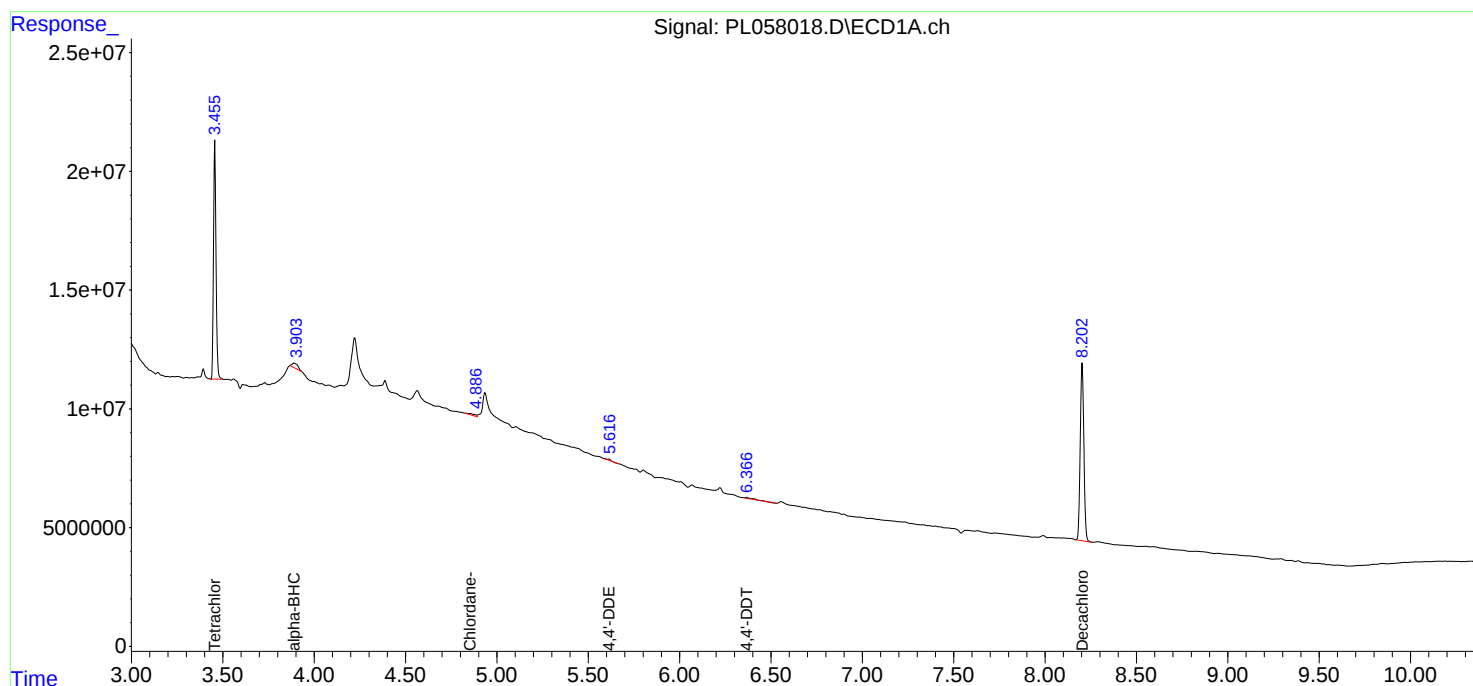


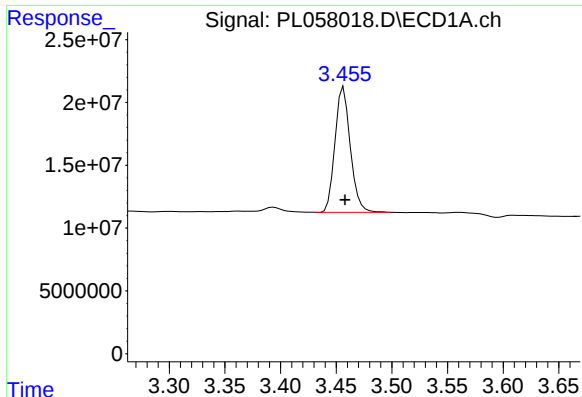

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 95838590
Conc: 9.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

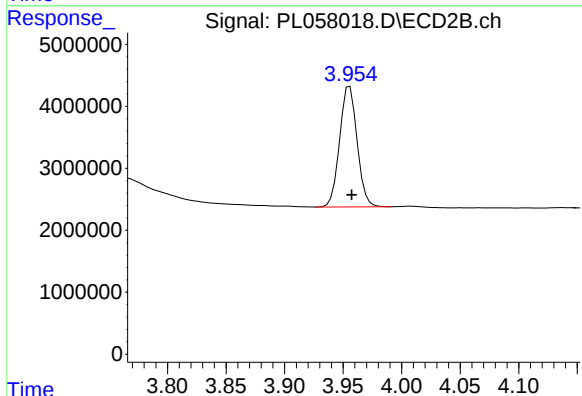


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.002 min
Response: 20202750
Conc: 9.31 ng/ml

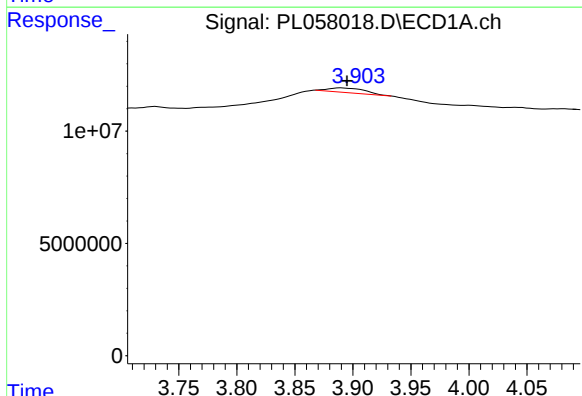


#2 alpha-BHC

R.T.: 3.890 min
Delta R.T.: -0.005 min
Response: 4202681
Conc: 0.24 ng/ml

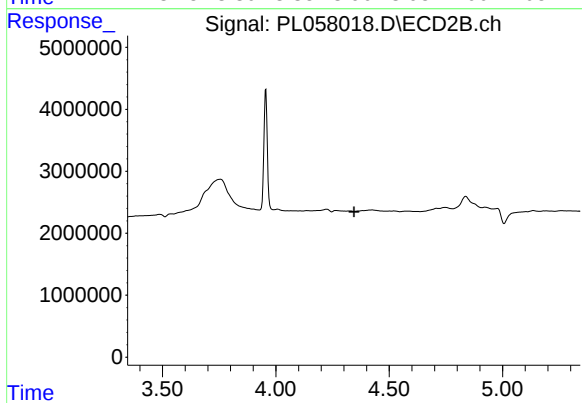

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

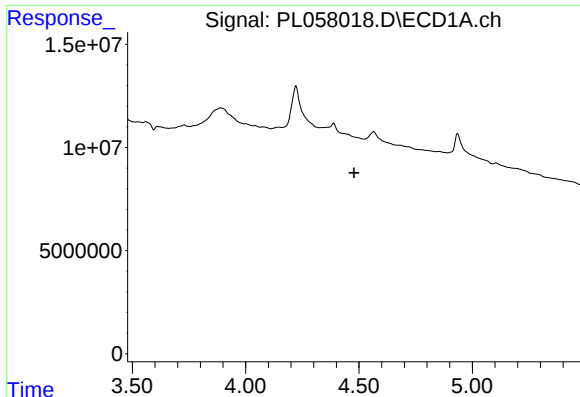

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

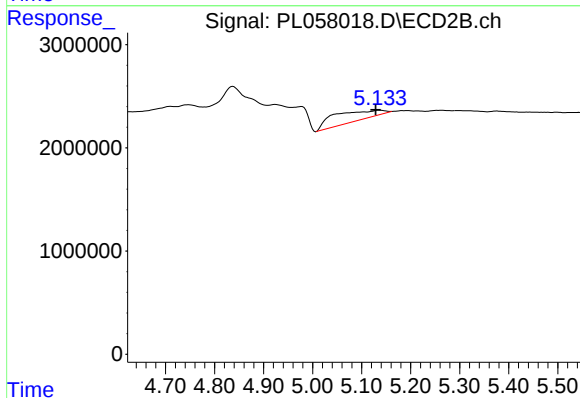


#4 Heptachlor

R.T.: 5.135 min
Delta R.T.: 0.006 min
Response: 6423560
Conc: 1.91 ng/ml

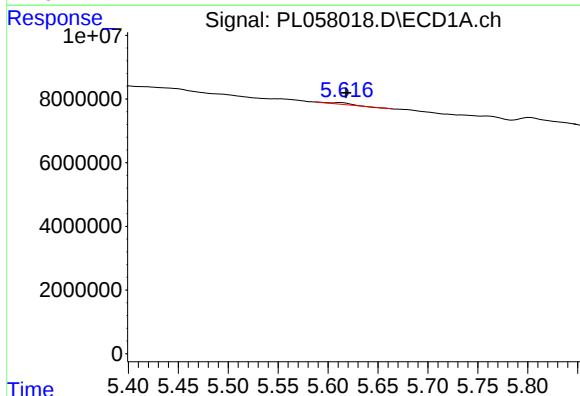


#12 4,4'-DDE

R.T.: 5.613 min
Delta R.T.: -0.005 min
Response: 419621
Conc: 0.03 ng/ml

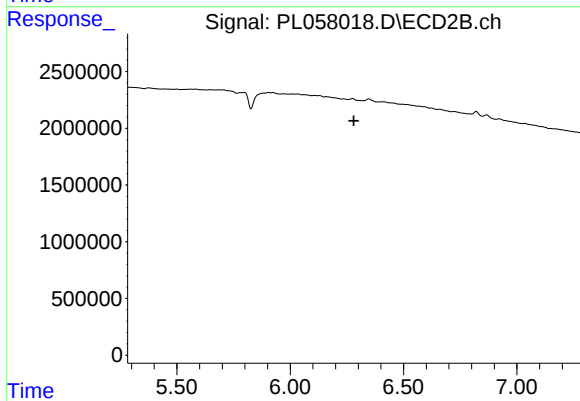

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.280 min
Response: 0
Conc: N.D.

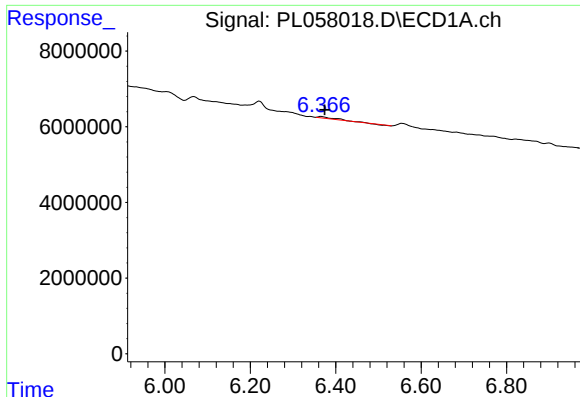

#17 4,4'-DDT


R.T.: 6.366 min
Delta R.T.: -0.008 min
Response: 1069031
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

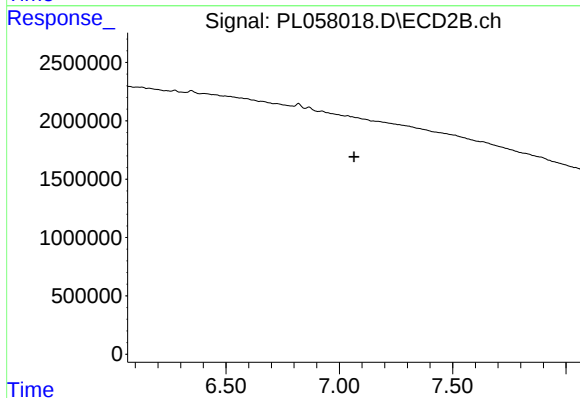


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.066 min
Response: 0
Conc: N.D.

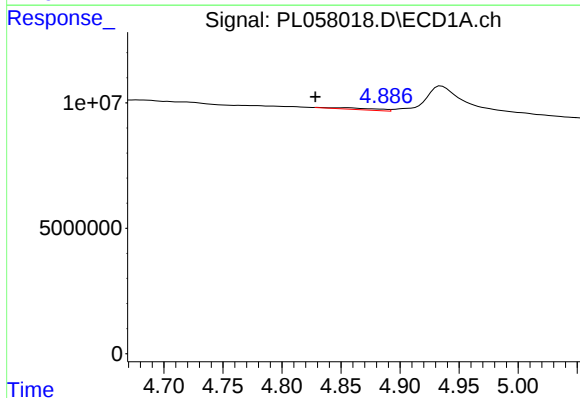


#24 Chlordane-2

R.T.: 4.855 min
Delta R.T.: 0.026 min
Response: 1722326
Conc: 4.27 ng/ml

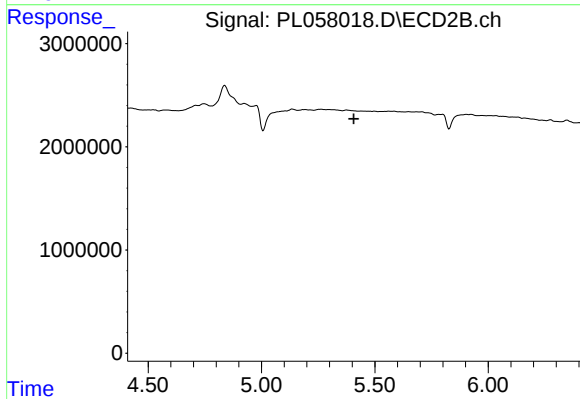

#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

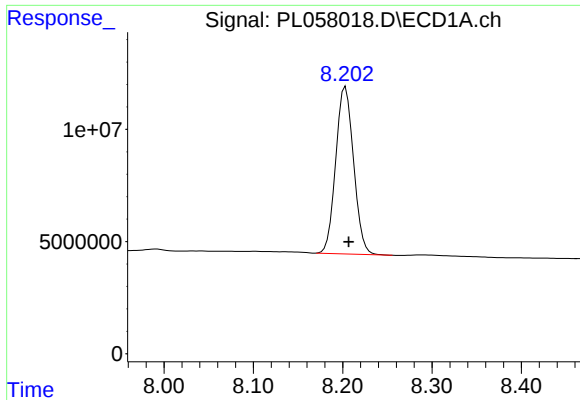

#28 Decachlorobiphenyl


R.T.: 8.203 min

Delta R.T.: -0.003 min

Response: 103303227

Conc: 10.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

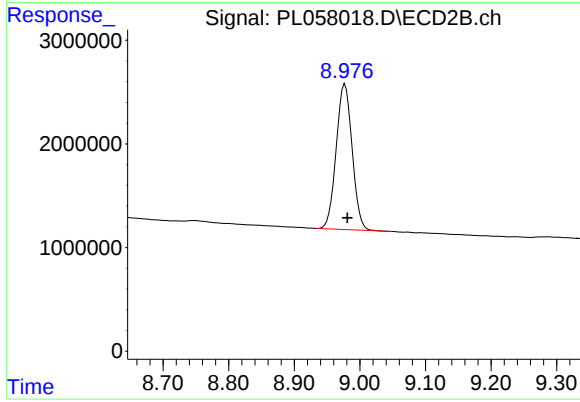

#28 Decachlorobiphenyl

R.T.: 8.977 min

Delta R.T.: -0.004 min

Response: 23699804

Conc: 10.61 ng/ml