

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
 Data File : PL058019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2020 17:58
 Operator : AJ\MA
 Sample : L2243-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 00:51:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.955	85297493	18191708	8.461	8.383
28)	SA Decachlor...	8.204	8.977	100.8E6	23405111	9.781	10.478
Target Compounds							
2)	A alpha-BHC	3.890	0.000	4401043	0	0.253	N.D. #
4)	MA Heptachlor	0.000	5.136	0	2024792	N.D.	0.603 #
12)	B 4,4'-DDE	5.615	6.275	1774290	364590	0.135	0.123
13)	MA Dieldrin	5.757	6.416	2577625	349153	0.198	0.114 #
14)	MA Endrin	6.004	0.000	3522046	0	0.302	N.D. #
15)	B Endosulfa...	0.000	6.867	0	275587	N.D.	0.106 #
16)	A 4,4'-DDD	0.000	6.769	0	374335	N.D.	0.164 #
17)	MA 4,4'-DDT	6.369	0.000	1969562	0	0.194	N.D. #
18)	B Endrin al...	6.462	0.000	1043229	0	0.112	N.D. #
19)	B Endosulfa...	6.653	0.000	1216640	0	0.120	N.D. #
20)	A Methoxychlor	6.901f	0.000	4213983	0	0.764	N.D. #
21)	B Endrin ke...	7.174f	0.000	1510424	0	0.136	N.D. #
22)	Mirex	7.335	0.000	462481	0	0.056	N.D. #
24)	Chlordane-2	4.856f	0.000	3046842	0	7.547	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
Data File : PL058019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2020 17:58
Operator : AJ\MA
Sample : L2243-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 00:51:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

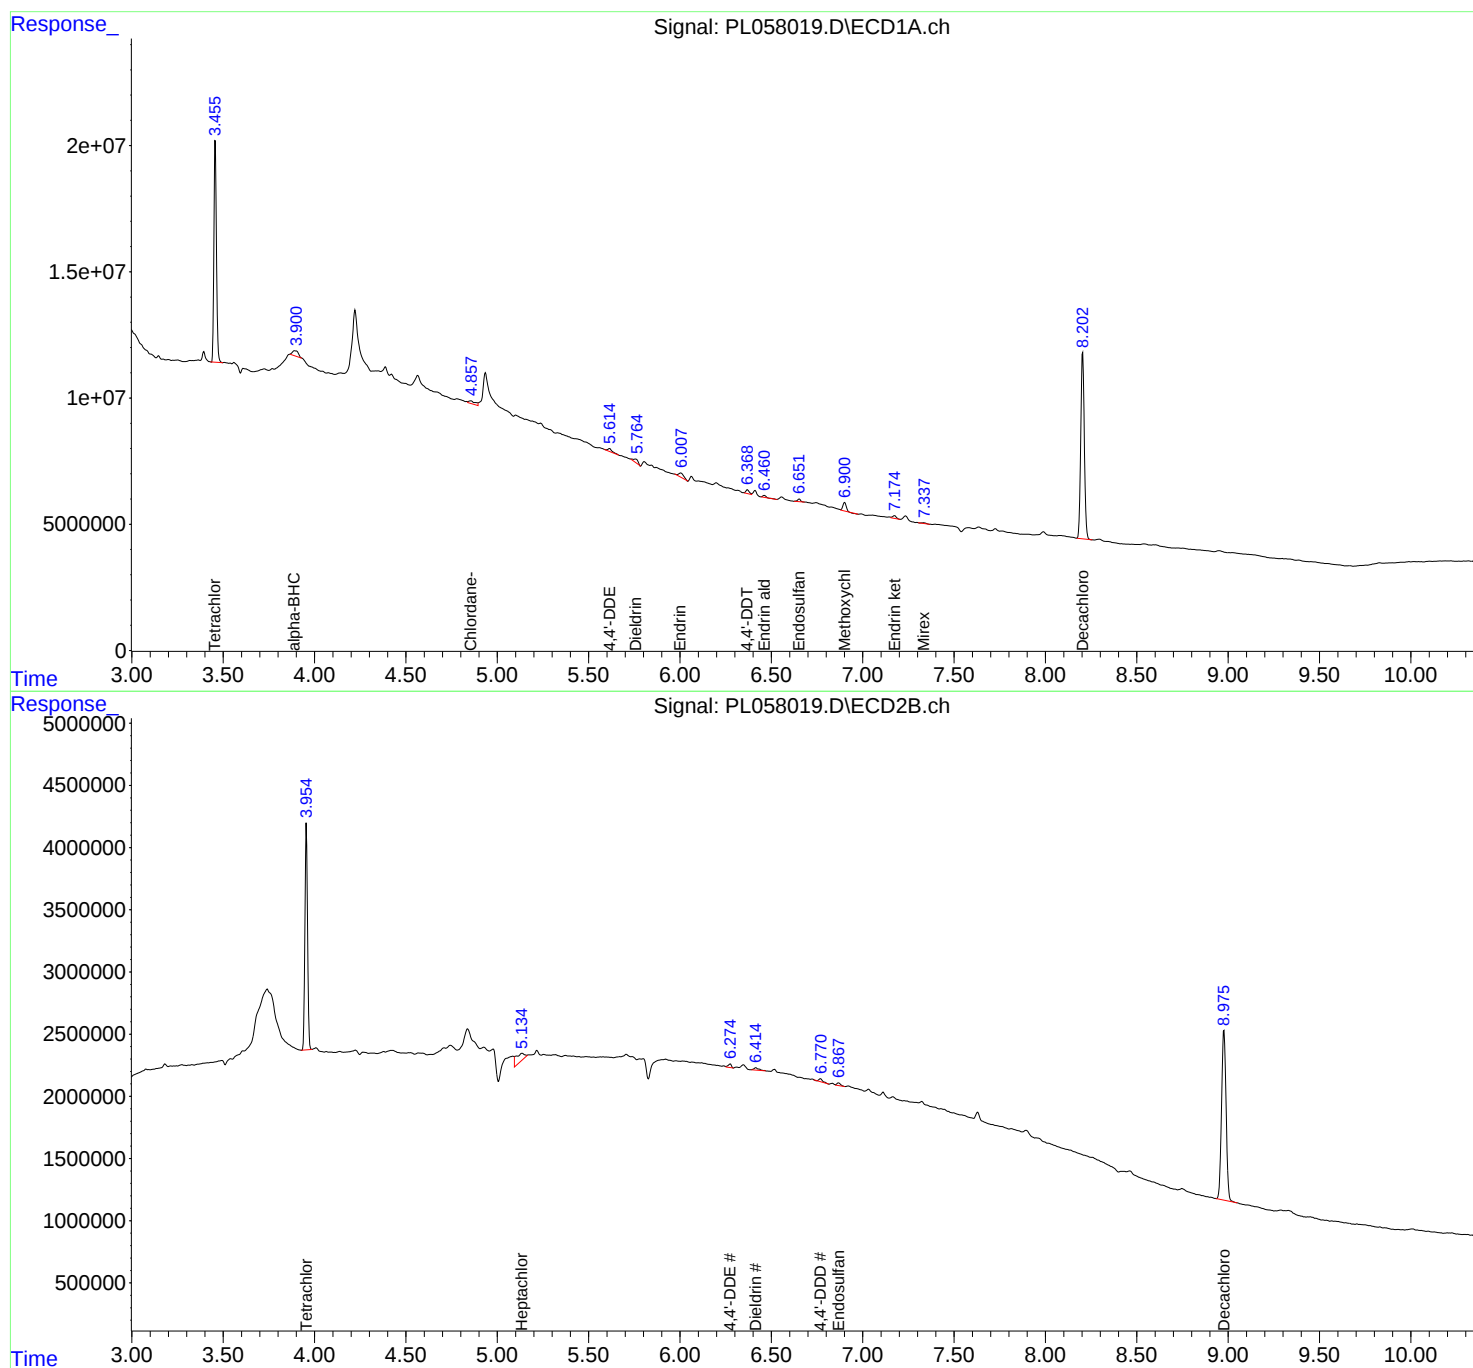

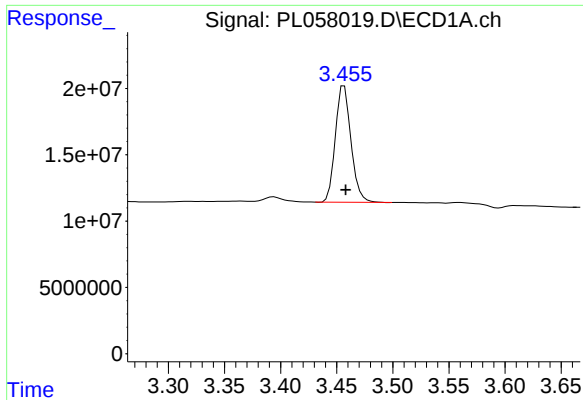


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 85297493
Conc: 8.46 ng/ml

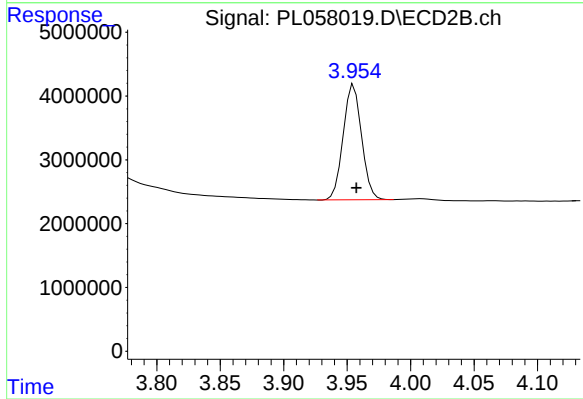


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 18191708
Conc: 8.38 ng/ml

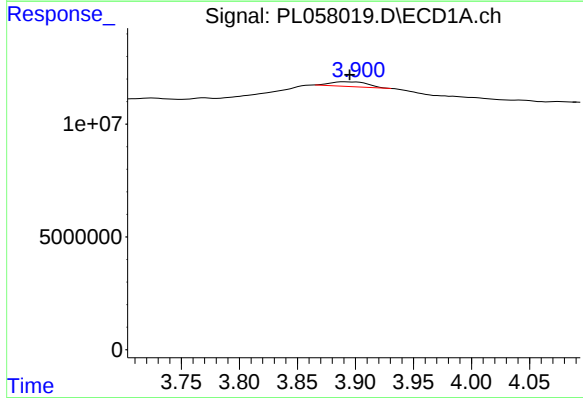


#2 alpha-BHC

R.T.: 3.890 min
Delta R.T.: -0.005 min
Response: 4401043
Conc: 0.25 ng/ml

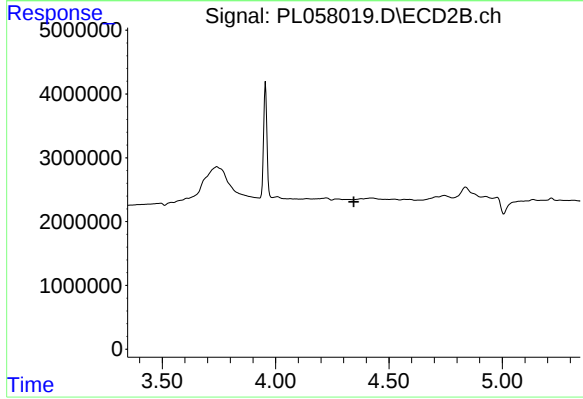


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

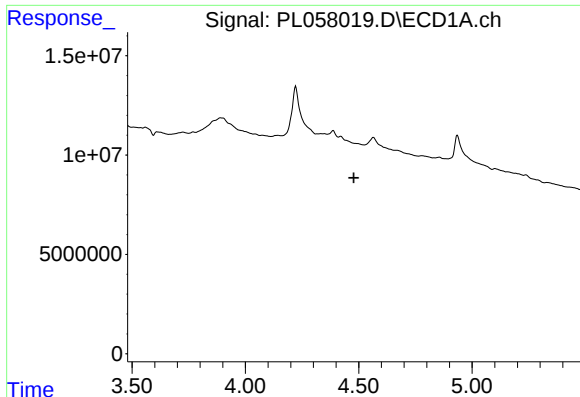


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

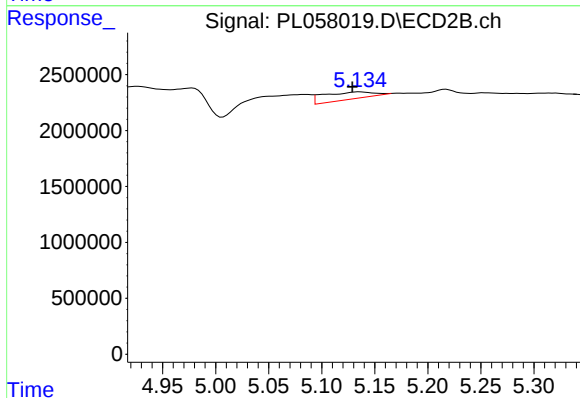


#4 Heptachlor

R.T.: 5.136 min
Delta R.T.: 0.007 min
Response: 2024792
Conc: 0.60 ng/ml

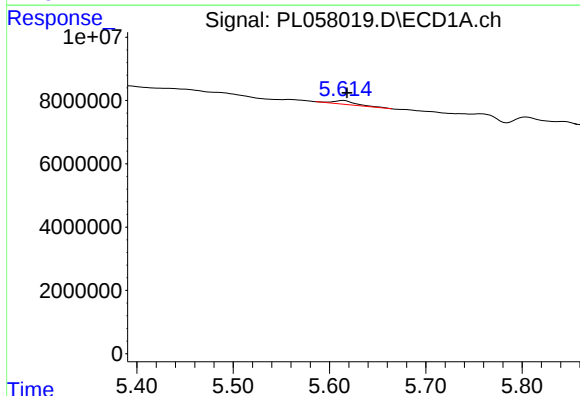


#12 4,4'-DDE

R.T.: 5.615 min
Delta R.T.: -0.004 min
Response: 1774290
Conc: 0.14 ng/ml

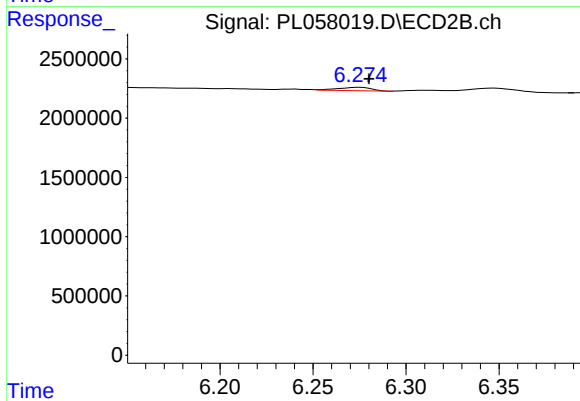


#12 4,4'-DDE

R.T.: 6.275 min
Delta R.T.: -0.005 min
Response: 364590
Conc: 0.12 ng/ml

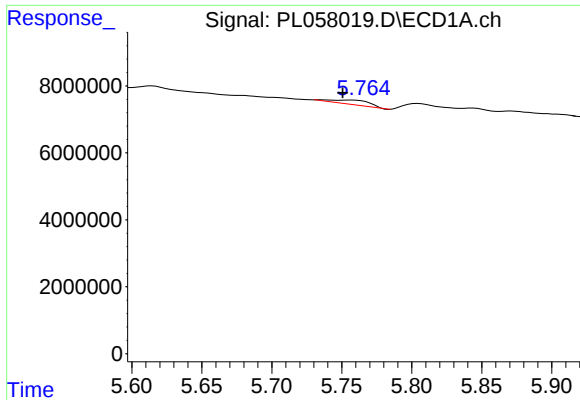


#13 Dieldrin

R.T.: 5.757 min
Delta R.T.: 0.006 min
Response: 2577625
Conc: 0.20 ng/ml

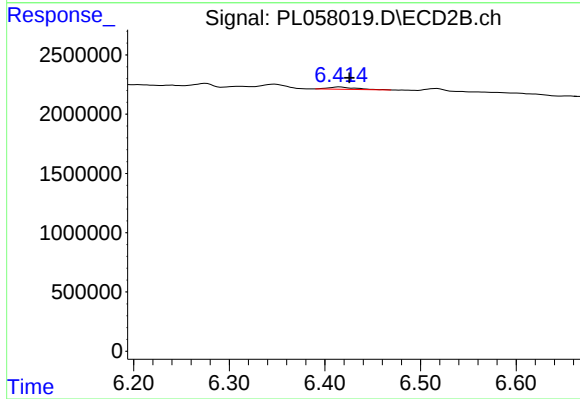


#13 Dieldrin

R.T.: 6.416 min
Delta R.T.: -0.010 min
Response: 349153
Conc: 0.11 ng/ml

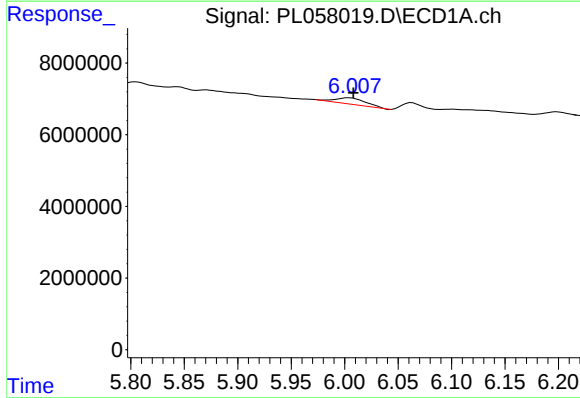


#14 Endrin

R.T.: 6.004 min
Delta R.T.: -0.005 min
Response: 3522046
Conc: 0.30 ng/ml

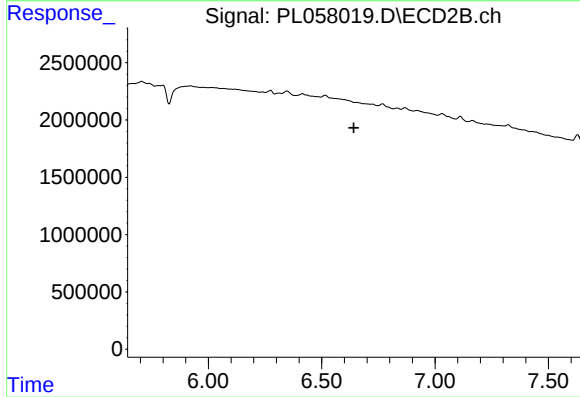


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.642 min
Response: 0
Conc: N.D.

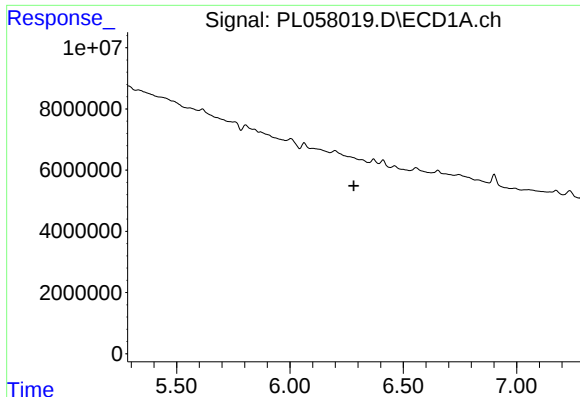


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

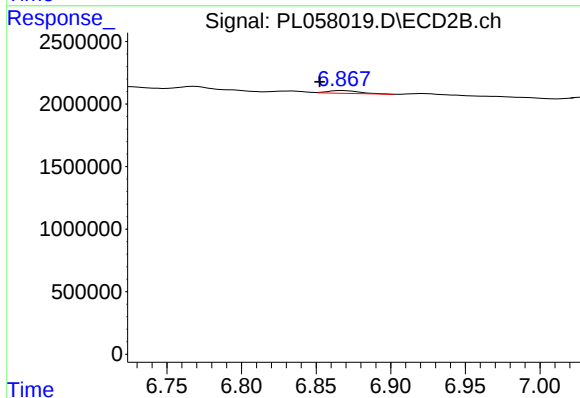


#15 Endosulfan II

R.T.: 6.867 min
Delta R.T.: 0.015 min
Response: 275587
Conc: 0.11 ng/ml

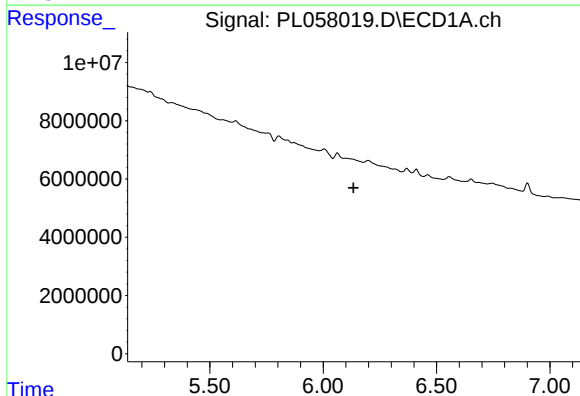


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.134 min
Response: 0
Conc: N.D.

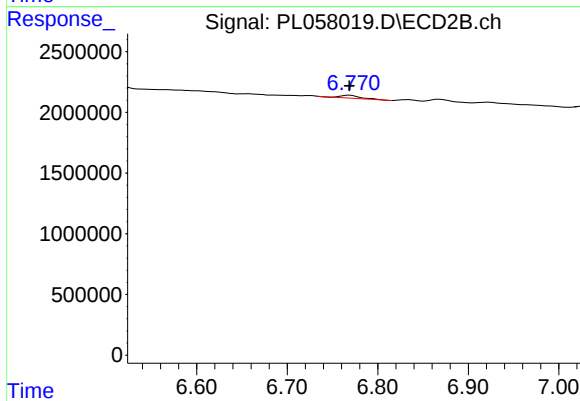


#16 4,4'-DDD

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 374335
Conc: 0.16 ng/ml

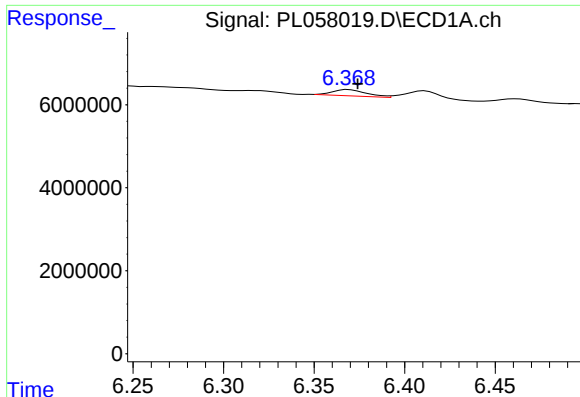


#17 4,4'-DDT

R.T.: 6.369 min
Delta R.T.: -0.005 min
Response: 1969562
Conc: 0.19 ng/ml

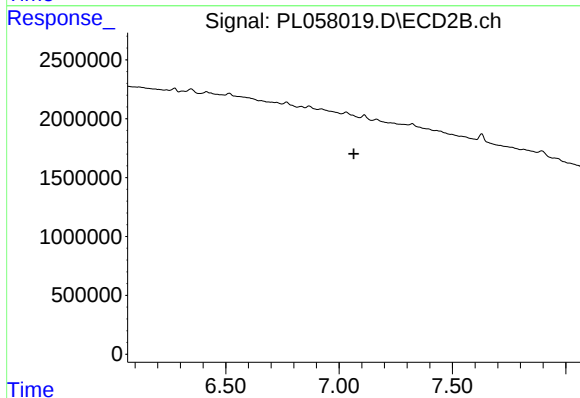


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.066 min
Response: 0
Conc: N.D.

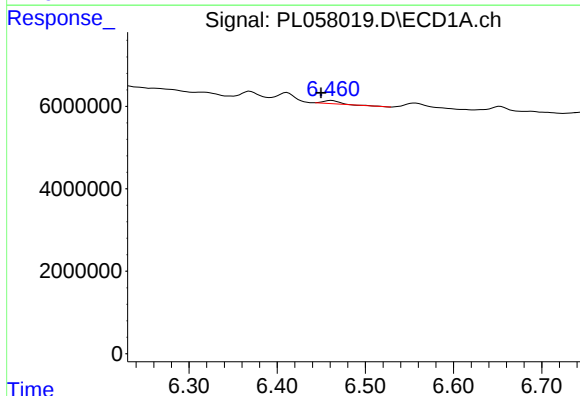


#18 Endrin aldehyde

R.T.: 6.462 min
Delta R.T.: 0.012 min
Response: 1043229
Conc: 0.11 ng/ml

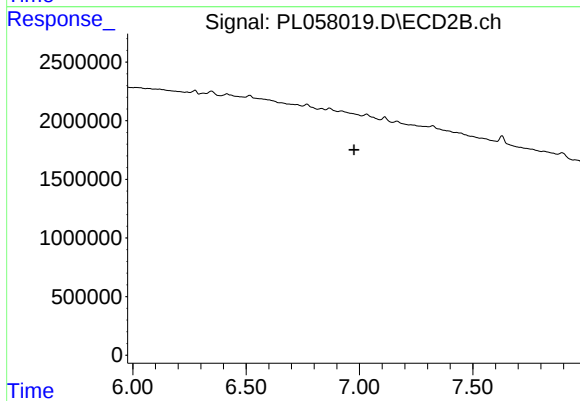


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

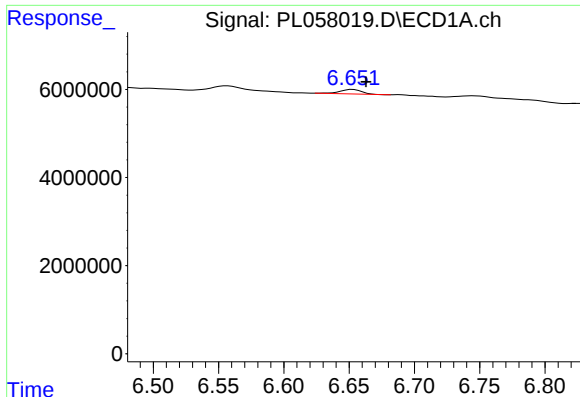


#19 Endosulfan Sulfate

R.T.: 6.653 min
Delta R.T.: -0.010 min
Response: 1216640
Conc: 0.12 ng/ml

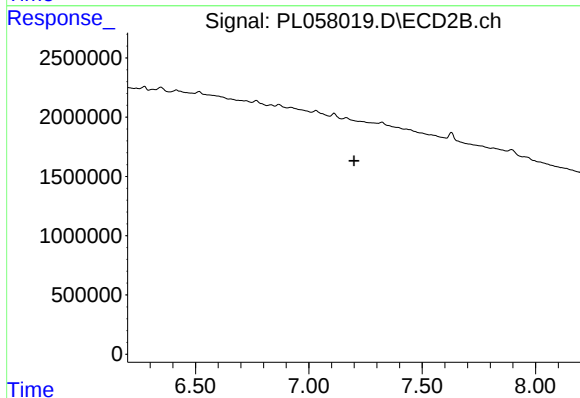


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

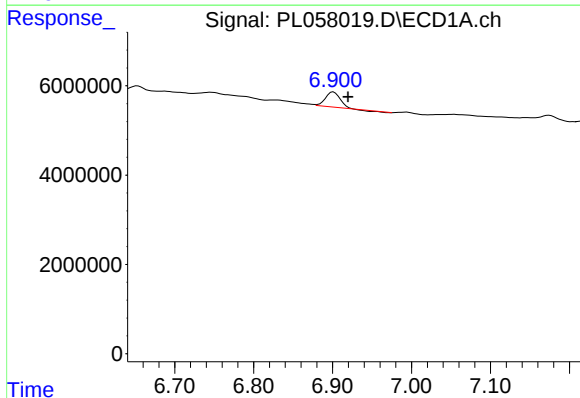


#20 Methoxychlor

R.T.: 6.901 min
Delta R.T.: -0.019 min
Response: 4213983
Conc: 0.76 ng/ml

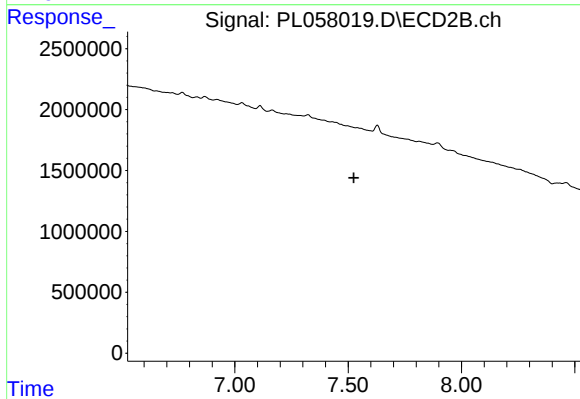


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.525 min
Response: 0
Conc: N.D.

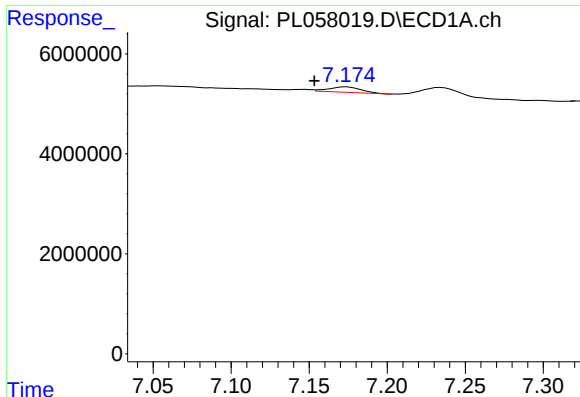


#21 Endrin ketone

R.T.: 7.174 min
Delta R.T.: 0.021 min
Response: 1510424
Conc: 0.14 ng/ml

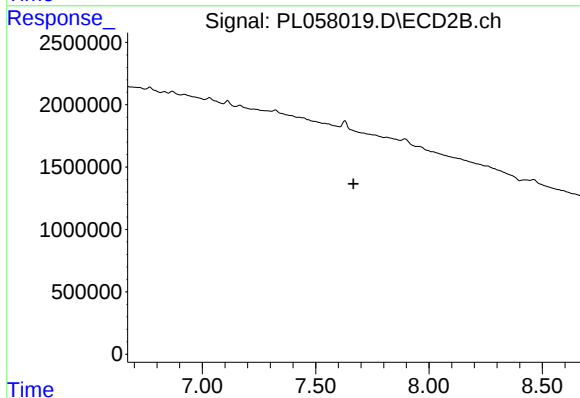


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.667 min
Response: 0
Conc: N.D.

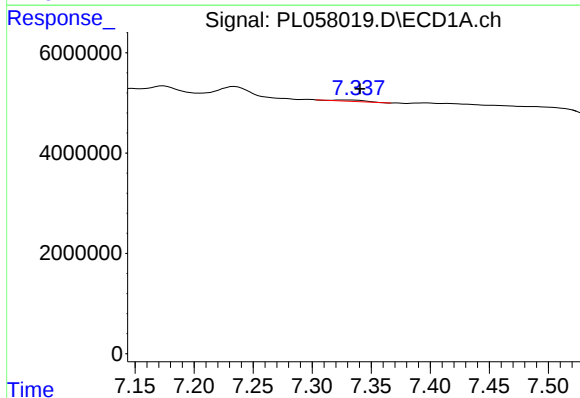


#22 Mirex

R.T.: 7.335 min
Delta R.T.: -0.006 min
Response: 462481
Conc: 0.06 ng/ml

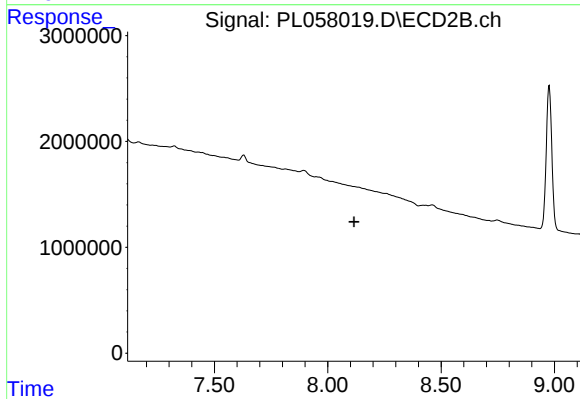


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.117 min
Response: 0
Conc: N.D.

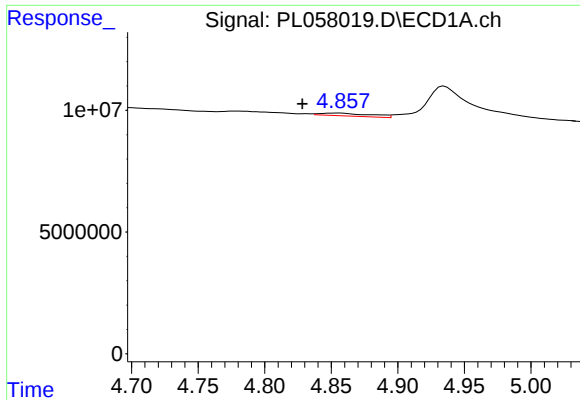


#24 Chlordane-2

R.T.: 4.856 min
Delta R.T.: 0.028 min
Response: 3046842
Conc: 7.55 ng/ml

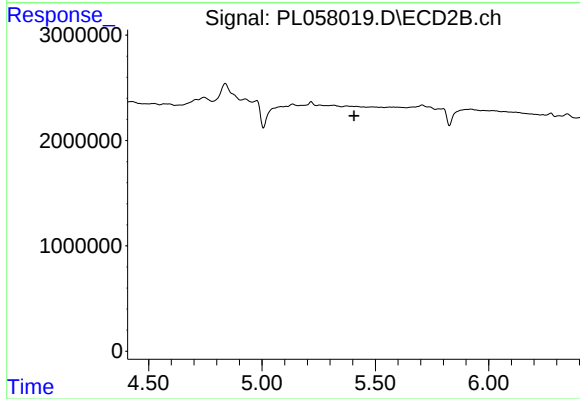


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

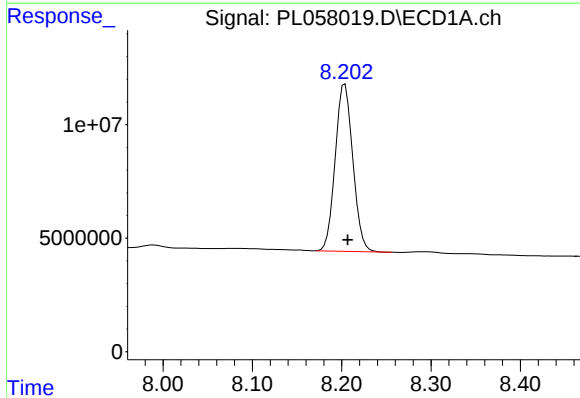

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 100824999
Conc: 9.78 ng/ml

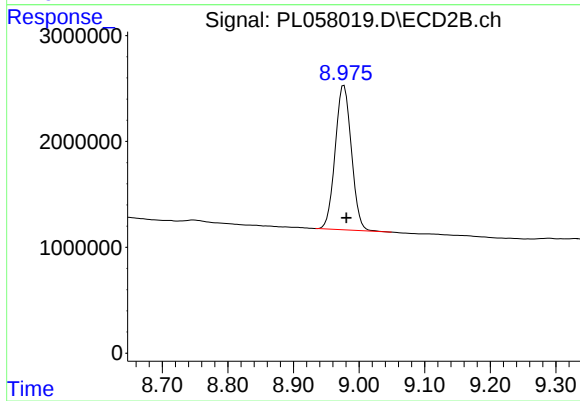

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 23405111
Conc: 10.48 ng/ml