

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
 Data File : PL058021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2020 18:27
 Operator : AJ\MA
 Sample : L2244-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 00:52:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.955	80158313	17241445	7.951	7.945
28)	SA Decachlor...	8.203	8.977	80451645	18907639	7.804	8.464
Target Compounds							
2)	A alpha-BHC	3.899	0.000	3672933	0	0.211	N.D. #
4)	MA Heptachlor	0.000	5.137	0	6264610	N.D.	1.867 #
14)	MA Endrin	6.005	0.000	2488328	0	0.213	N.D. #
15)	B Endosulfa...	0.000	6.868f	0	170457	N.D.	0.066 #
18)	B Endrin al...	0.000	6.960f	0	4904612	N.D.	2.208 #
23)	Chlordane-1	4.345f	0.000	1718692	0	4.647	N.D. #
24)	Chlordane-2	4.838	0.000	679309	0	1.683	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
Data File : PL058021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2020 18:27
Operator : AJ\MA
Sample : L2244-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 00:52:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

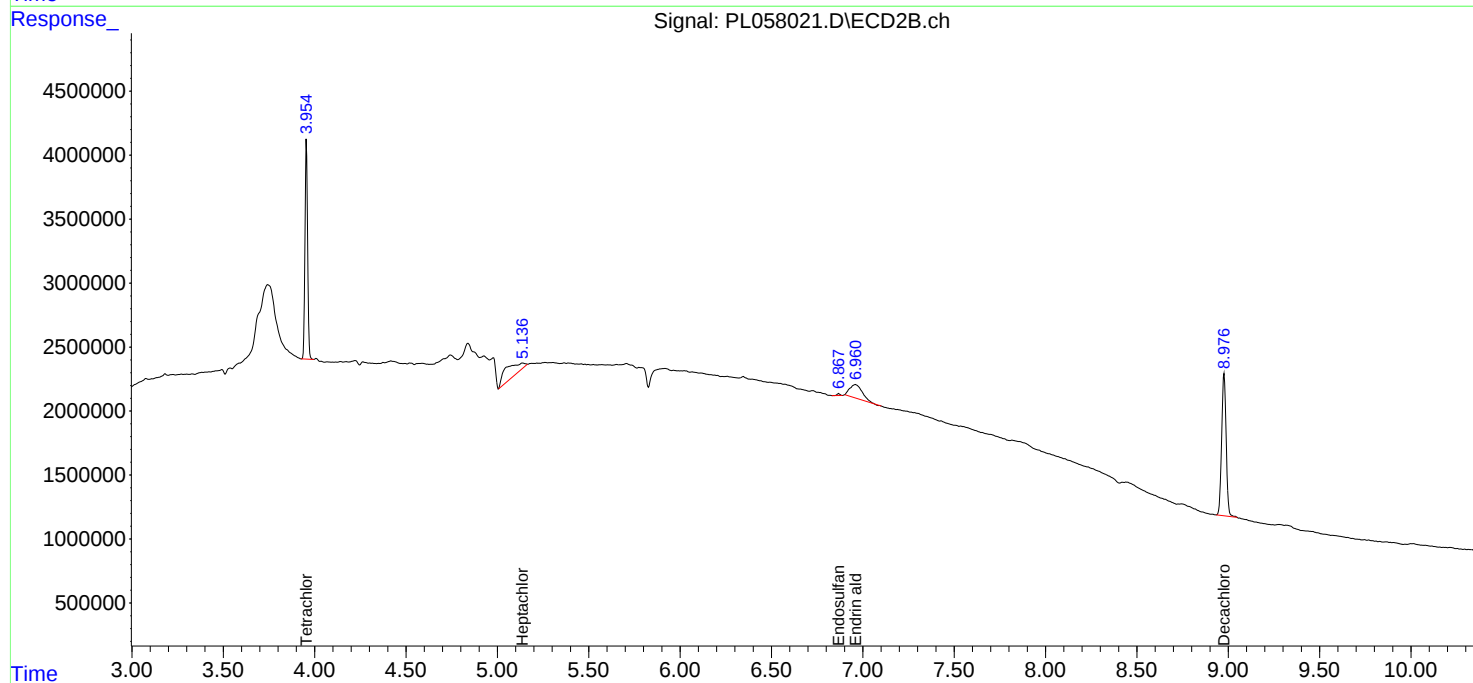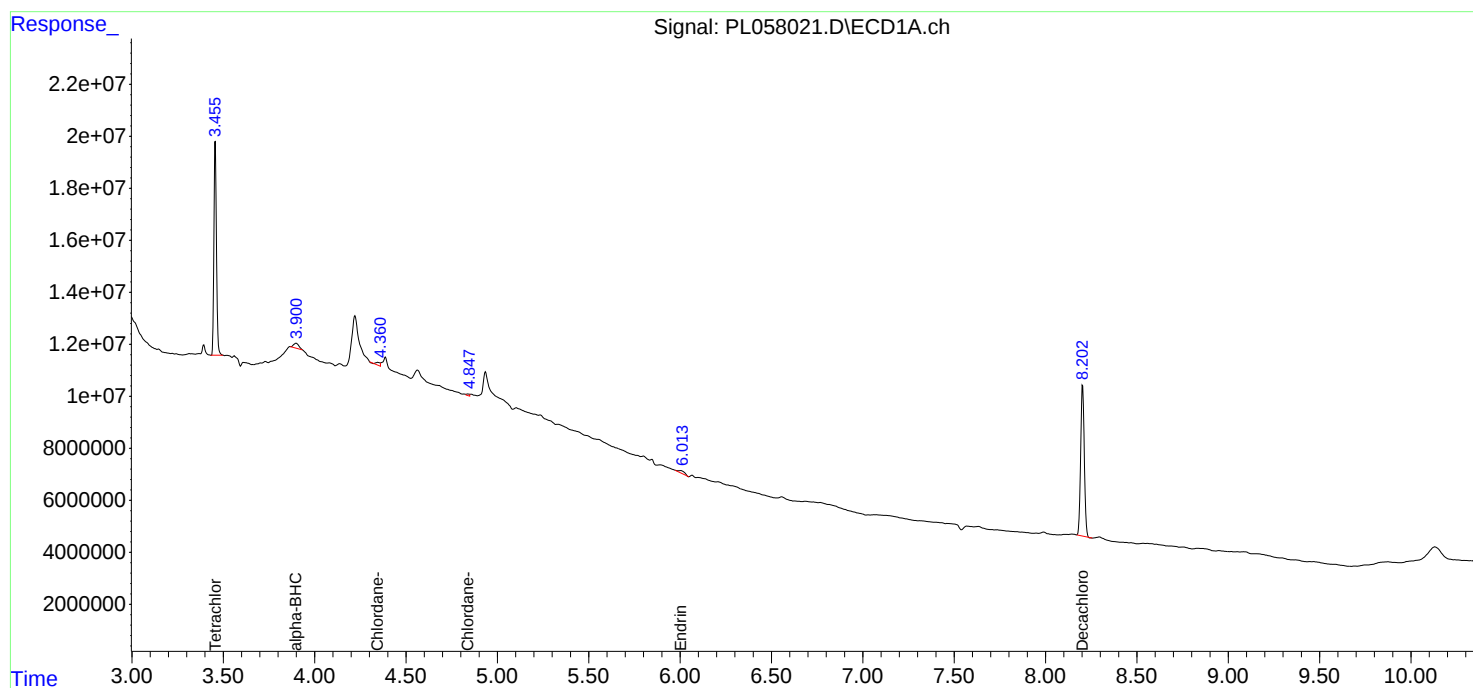

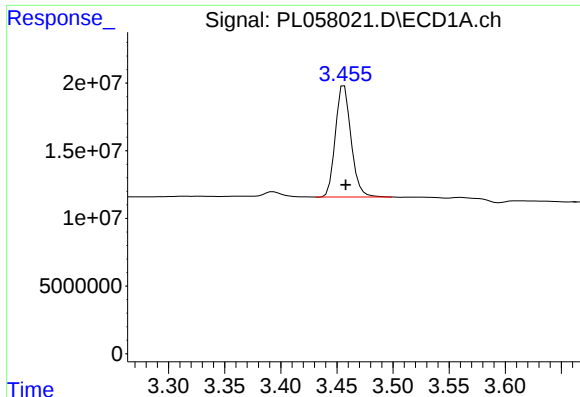


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 80158313
Conc: 7.95 ng/ml

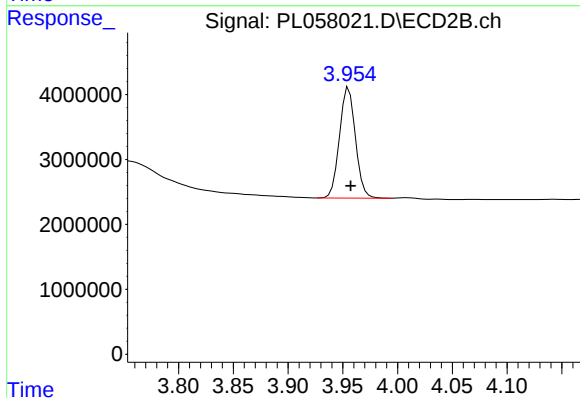


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 17241445
Conc: 7.94 ng/ml

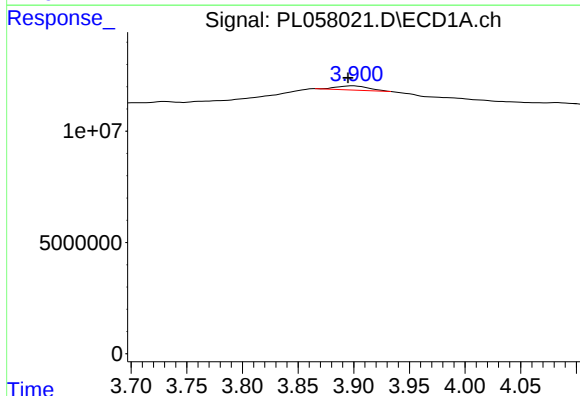


#2 alpha-BHC

R.T.: 3.899 min
Delta R.T.: 0.004 min
Response: 3672933
Conc: 0.21 ng/ml

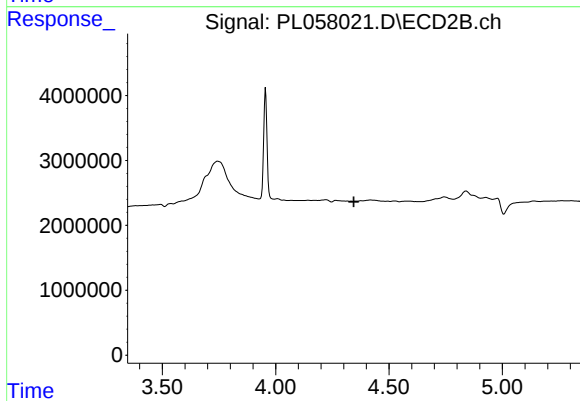


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

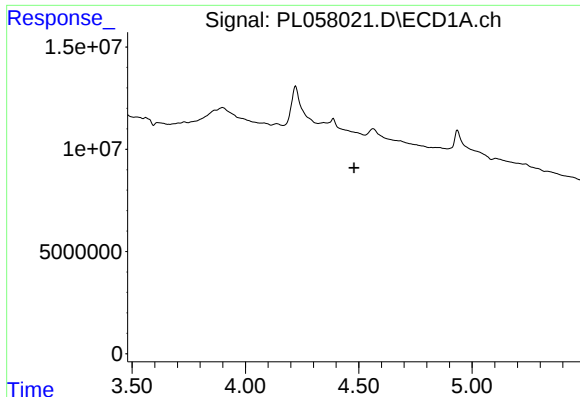


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

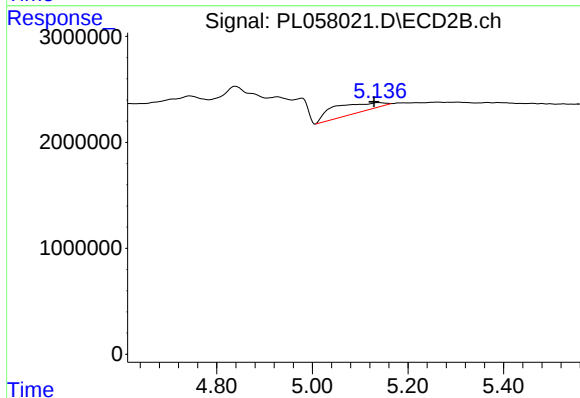


#4 Heptachlor

R.T.: 5.137 min
Delta R.T.: 0.008 min
Response: 6264610
Conc: 1.87 ng/ml

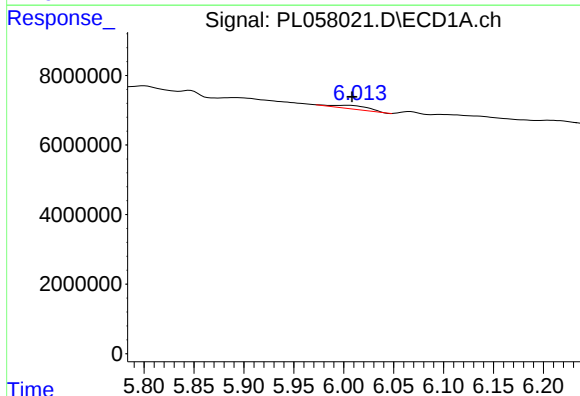


#14 Endrin

R.T.: 6.005 min
Delta R.T.: -0.004 min
Response: 2488328
Conc: 0.21 ng/ml

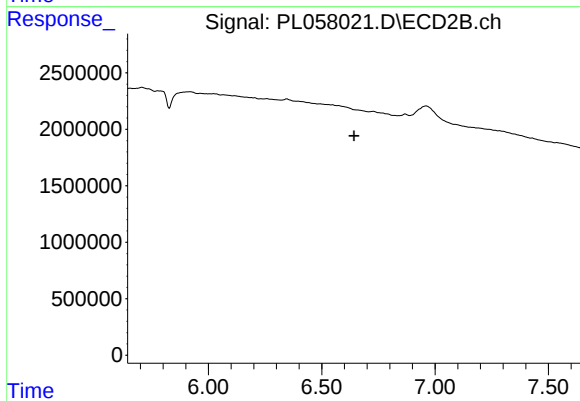


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

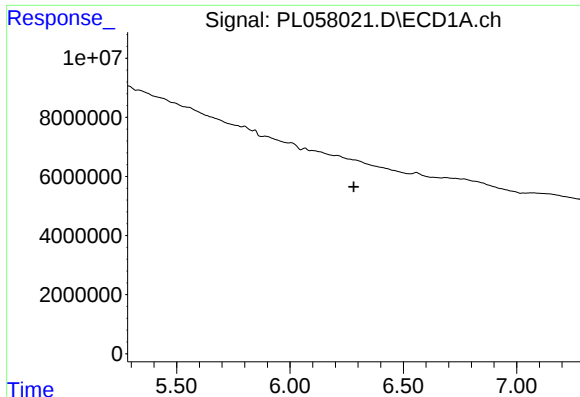


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

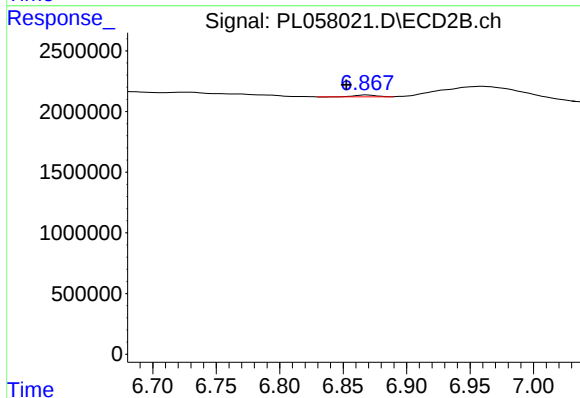


#15 Endosulfan II

R.T.: 6.868 min
Delta R.T.: 0.016 min
Response: 170457
Conc: 0.07 ng/ml

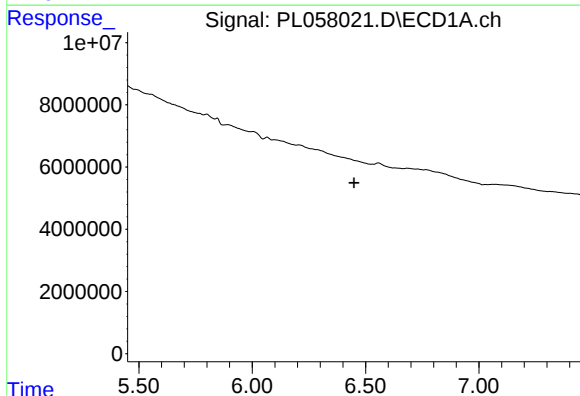


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.450 min
Response: 0
Conc: N.D.

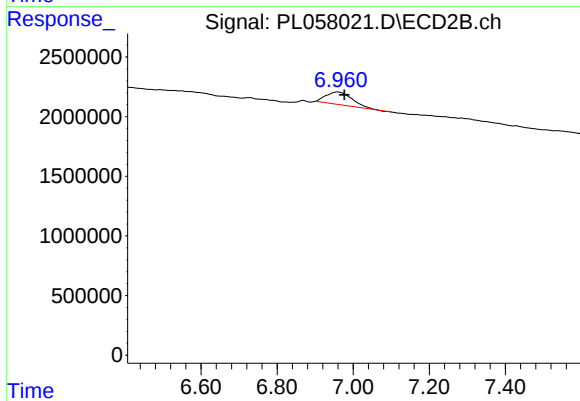


#18 Endrin aldehyde

R.T.: 6.960 min
Delta R.T.: -0.017 min
Response: 4904612
Conc: 2.21 ng/ml

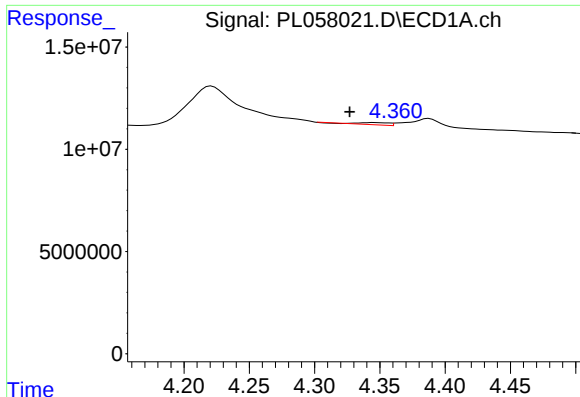


#23 Chlordane-1

R.T.: 4.345 min
Delta R.T.: 0.018 min
Response: 1718692
Conc: 4.65 ng/ml

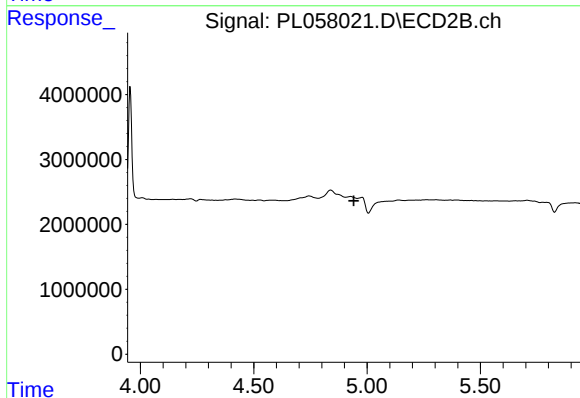


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

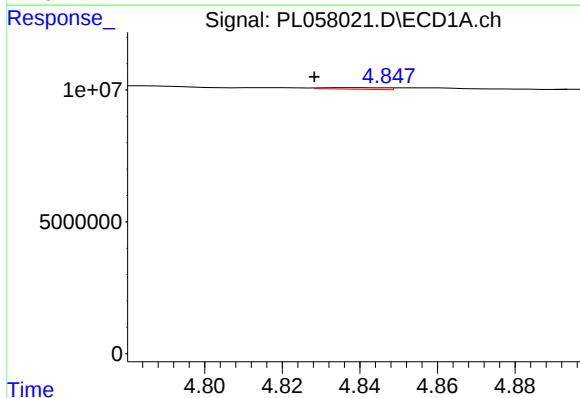


#24 Chlordane-2

R.T.: 4.838 min
Delta R.T.: 0.010 min
Response: 679309
Conc: 1.68 ng/ml

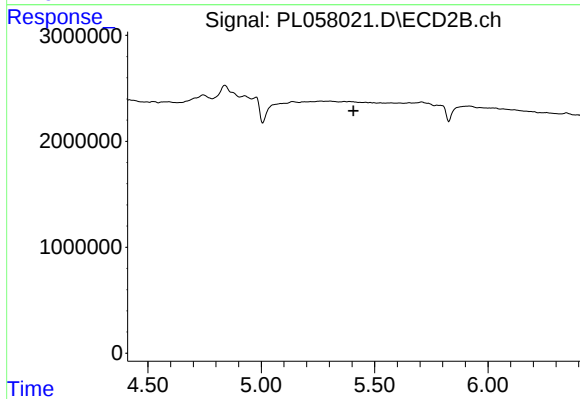

#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

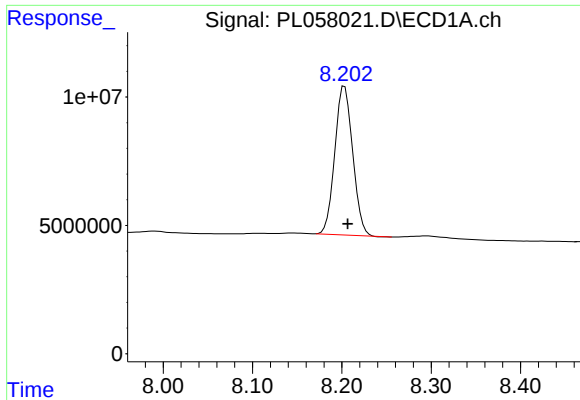


#28 Decachlorobiphenyl

R.T.: 8.203 min

Delta R.T.: -0.004 min

Response: 80451645

Conc: 7.80 ng/ml

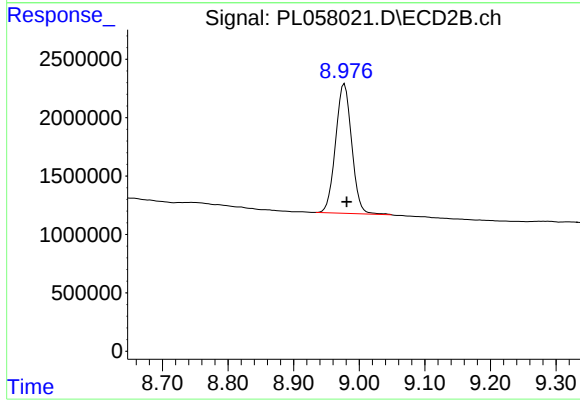

#28 Decachlorobiphenyl

R.T.: 8.977 min

Delta R.T.: -0.003 min

Response: 18907639

Conc: 8.46 ng/ml