

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
 Data File : PL058043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2020 23:53
 Operator : AJ\MA
 Sample : L2255-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:00:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	90894690	18891109	9.016	8.705
28)	SA Decachlor...	8.203	8.977	74011453	17510264	7.180	7.839
Target Compounds							
2)	A alpha-BHC	3.885	0.000	3057707	0	0.176	N.D. #
4)	MA Heptachlor	4.452f	5.134	665230	5092575	0.041	1.517 #
6)	B beta-BHC	4.452f	0.000	665230	0	0.105	N.D. #
9)	A Endosulfan I	5.493	0.000	1020052	0	0.083	N.D. #
15)	B Endosulfa...	6.291	0.000	1428454	0	0.129	N.D. #
22)	Mirex	7.342	0.000	442588	0	0.054	N.D. #
23)	Chlordane-1	4.312	0.000	420680	0	1.137	N.D. #
24)	Chlordane-2	4.807f	0.000	595205	0	1.474	N.D. #
27)	Chlordane-5	6.291	0.000	1428454	0	3.776	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
Data File : PL058043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2020 23:53
Operator : AJ\MA
Sample : L2255-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:00:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

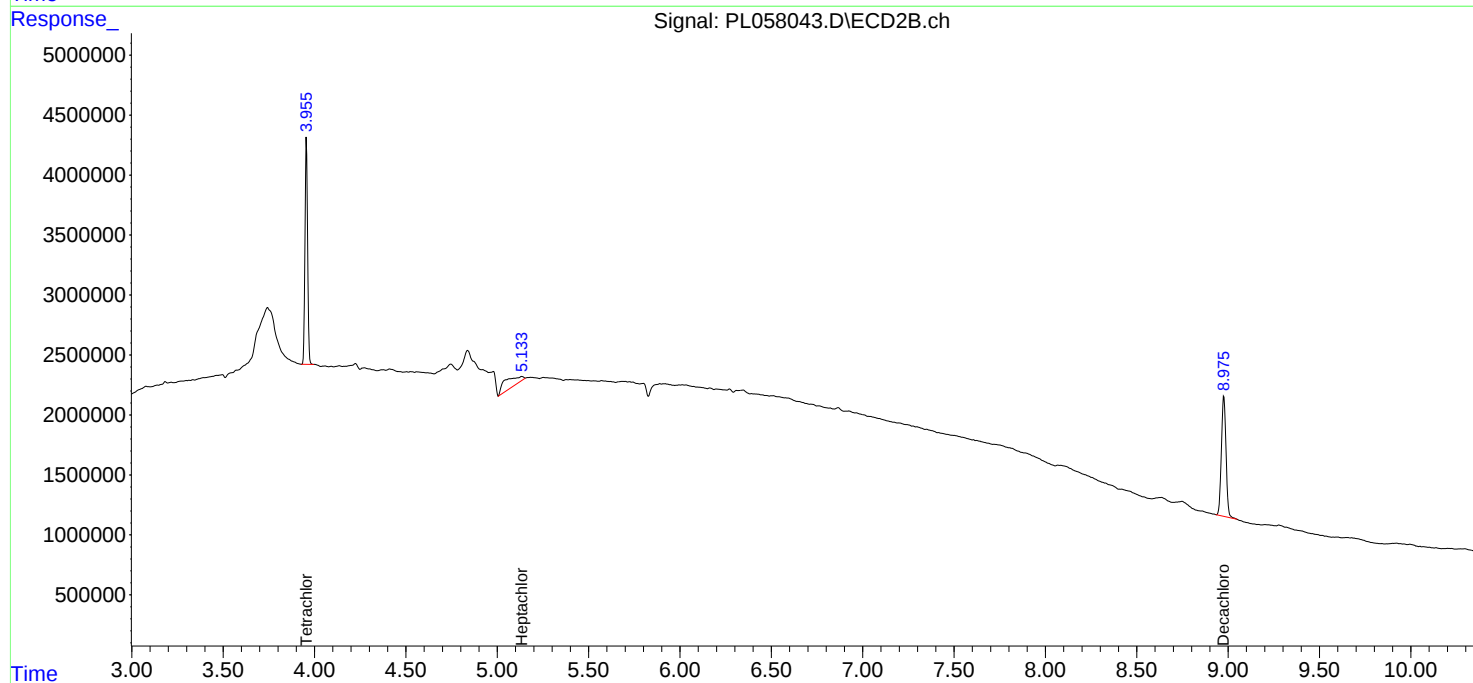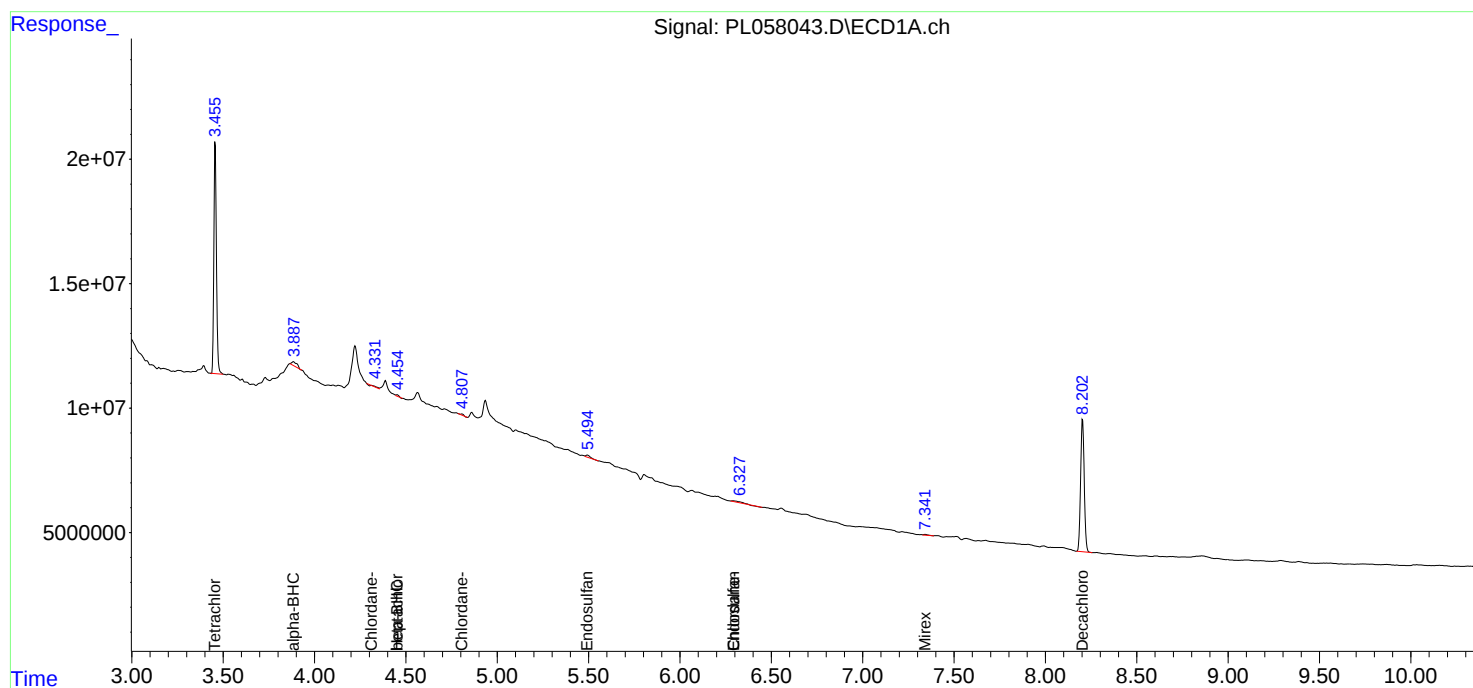


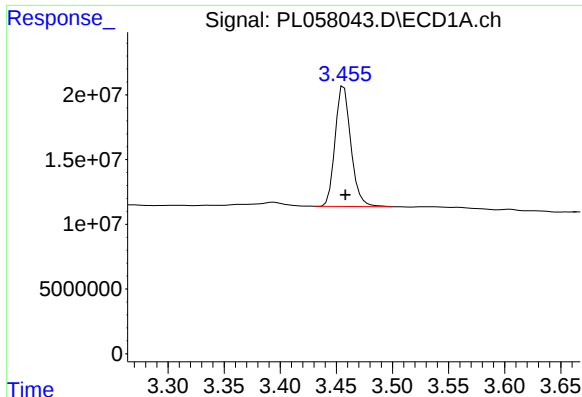

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 90894690
Conc: 9.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

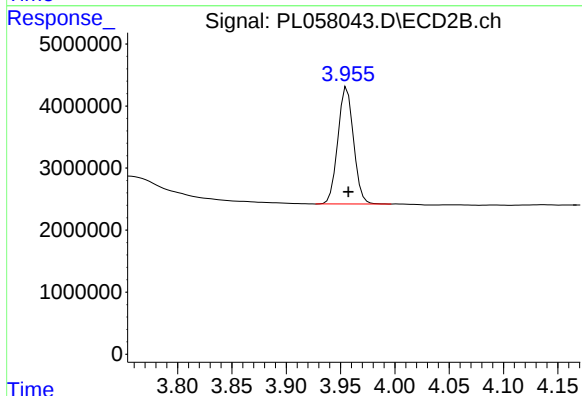


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 18891109
Conc: 8.70 ng/ml

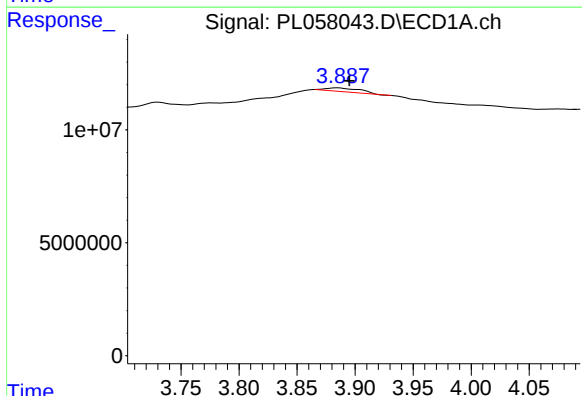


#2 alpha-BHC

R.T.: 3.885 min
Delta R.T.: -0.010 min
Response: 3057707
Conc: 0.18 ng/ml

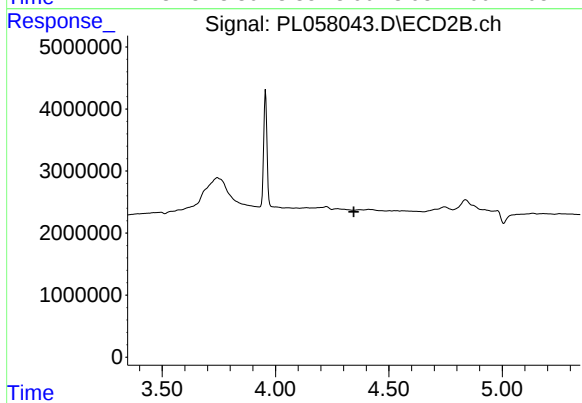

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

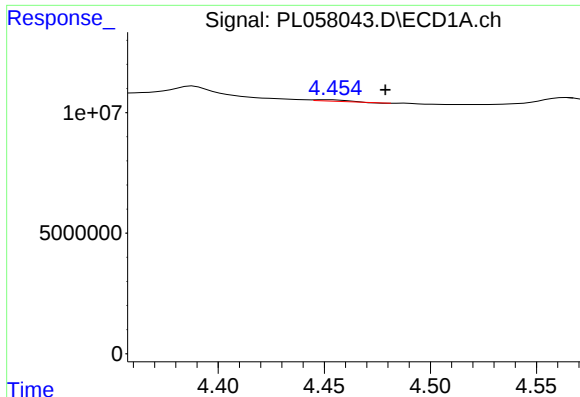

#4 Heptachlor


R.T.: 4.452 min
Delta R.T.: -0.027 min
Response: 665230
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

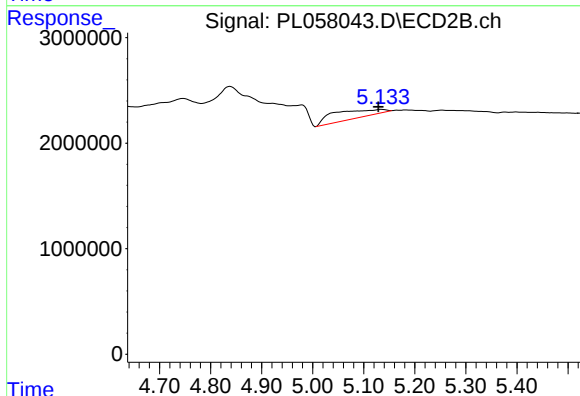


#4 Heptachlor

R.T.: 5.134 min
Delta R.T.: 0.005 min
Response: 5092575
Conc: 1.52 ng/ml

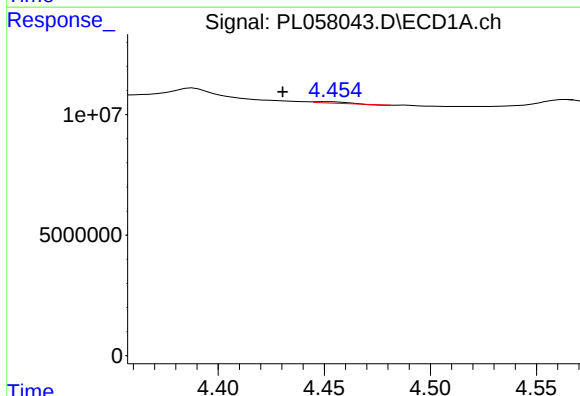


#6 beta-BHC

R.T.: 4.452 min
Delta R.T.: 0.022 min
Response: 665230
Conc: 0.11 ng/ml

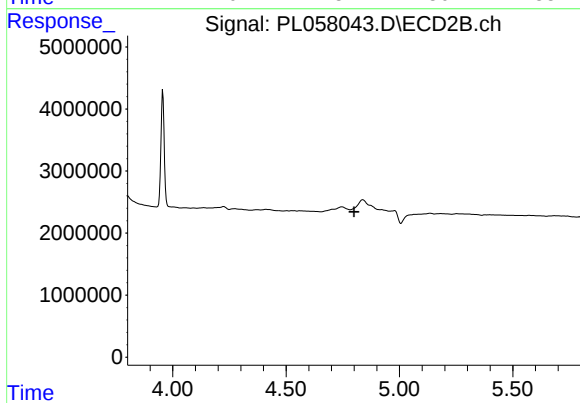

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

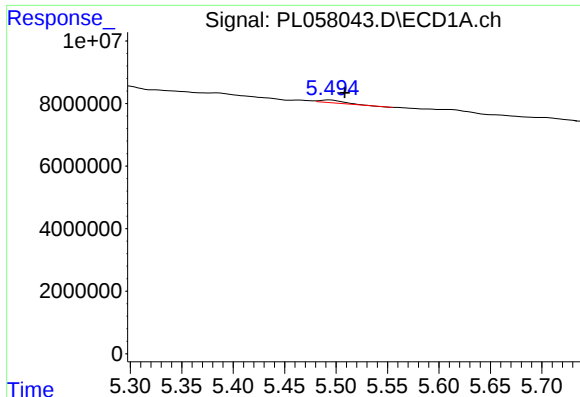

#9 Endosulfan I


R.T.: 5.493 min
Delta R.T.: -0.015 min
Response: 1020052
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

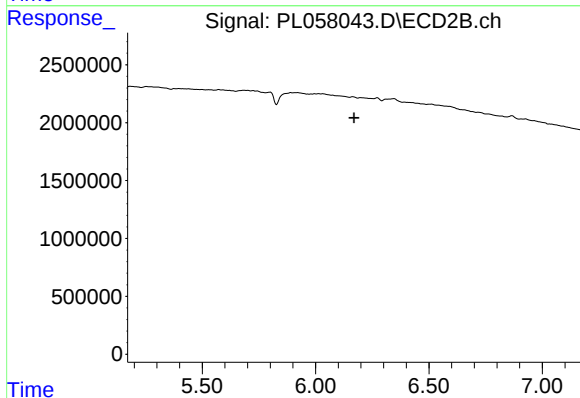


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

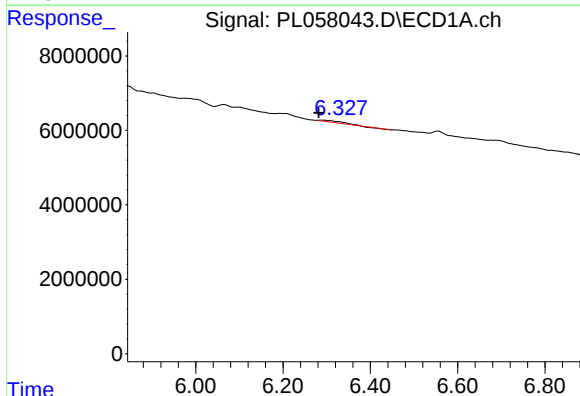


#15 Endosulfan II

R.T.: 6.291 min
Delta R.T.: 0.009 min
Response: 1428454
Conc: 0.13 ng/ml

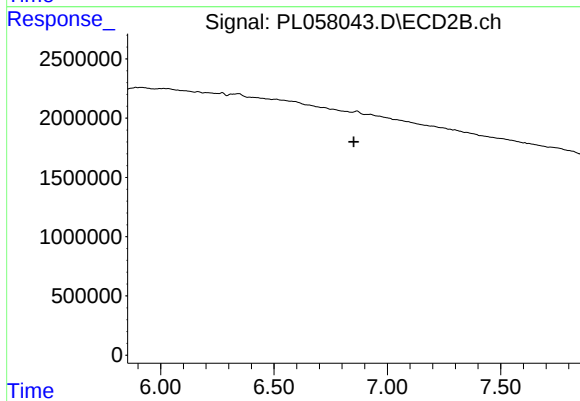

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

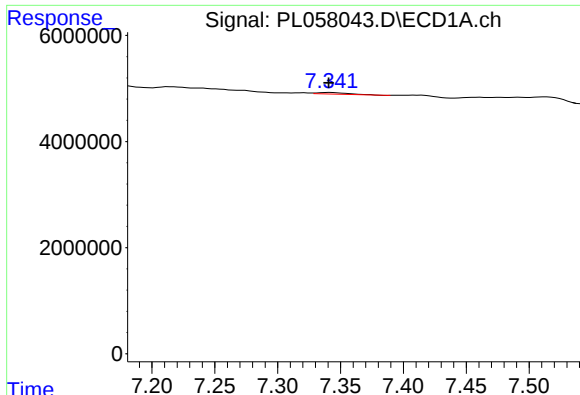

#22 Mirex


R.T.: 7.342 min
Delta R.T.: 0.001 min
Response: 442588
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

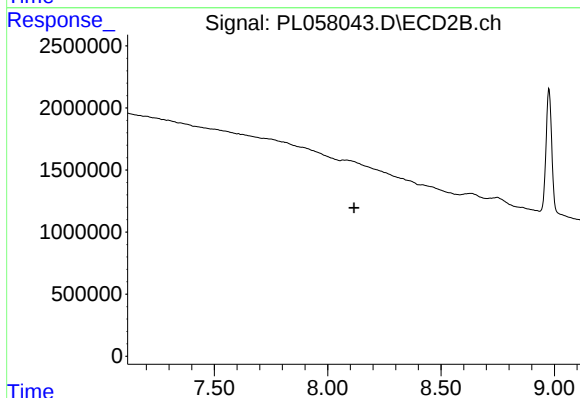


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.117 min
Response: 0
Conc: N.D.

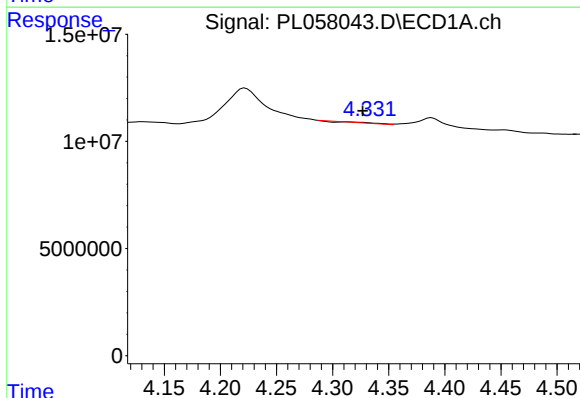


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: -0.015 min
Response: 420680
Conc: 1.14 ng/ml

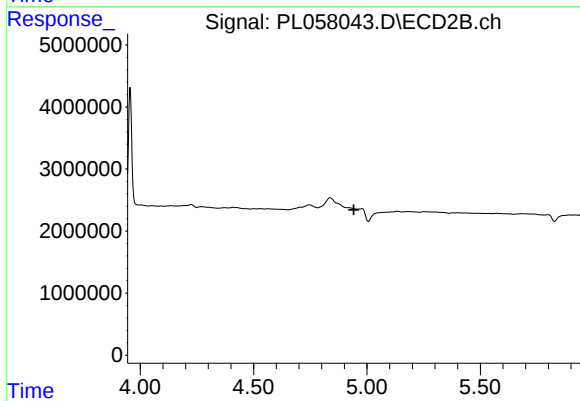

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

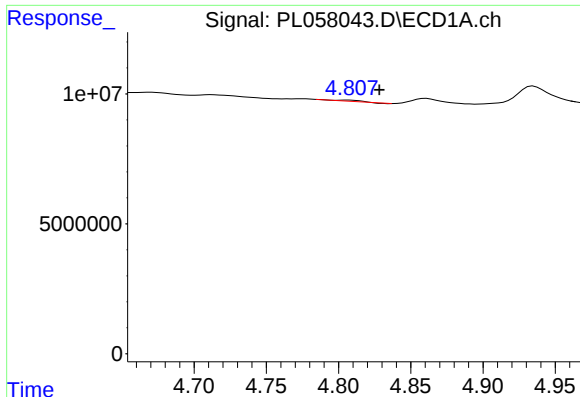

#24 Chlordane-2


R.T.: 4.807 min
Delta R.T.: -0.022 min
Response: 595205
Conc: 1.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

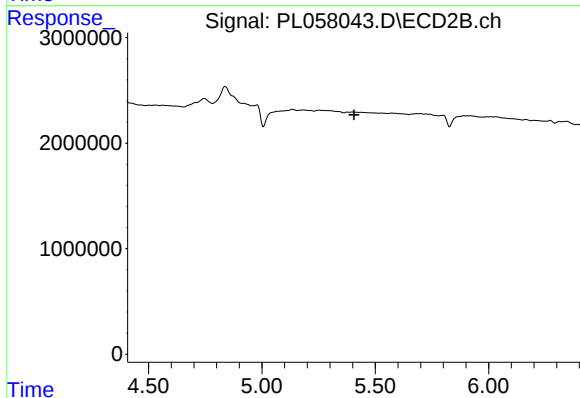


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

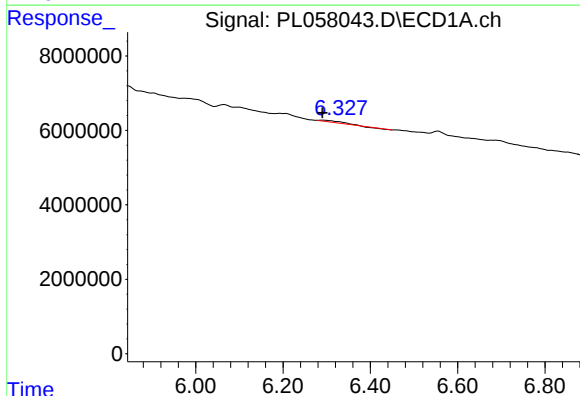


#27 Chlordane-5

R.T.: 6.291 min
Delta R.T.: 0.000 min
Response: 1428454
Conc: 3.78 ng/ml

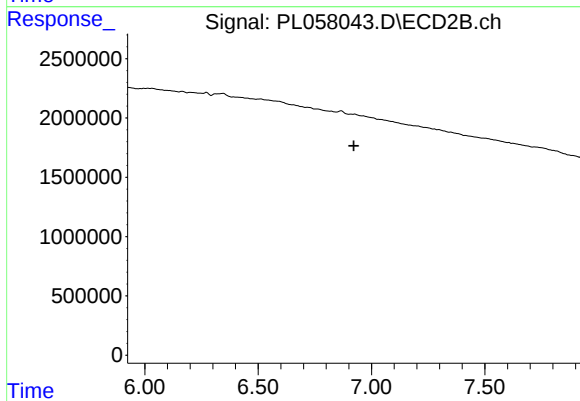

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

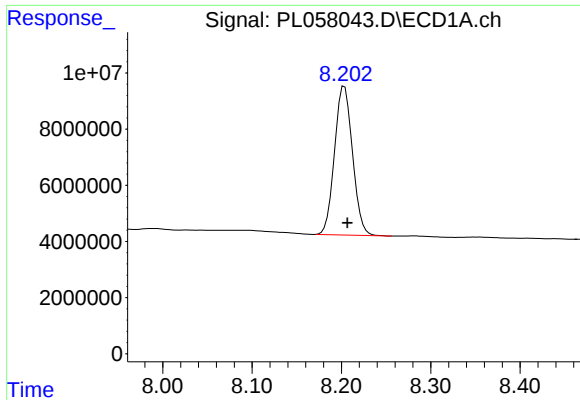

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.003 min
Response: 74011453
Conc: 7.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

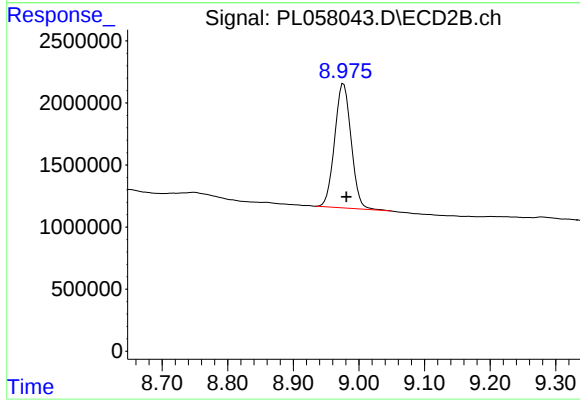

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 17510264
Conc: 7.84 ng/ml