

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
 Data File : PL058050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2020 01:33
 Operator : AJ\MA
 Sample : L2277-04
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 04:58:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	201.8E6	40824283	20.022	18.812
28)	SA Decachlor...	8.204	8.977	171.3E6	38144478	16.617	17.076
Target Compounds							
4)	MA Heptachlor	0.000	5.137	0	1014053	N.D.	0.302 #
5)	MB Aldrin	4.713	0.000	1781358	0	0.121	N.D. #
10)	B gamma-Chl...	0.000	6.042	0	730776	N.D.	0.226 #
15)	B Endosulfa...	0.000	6.868f	0	520012	N.D.	0.200 #
18)	B Endrin al...	0.000	6.949f	0	608446	N.D.	0.274 #
23)	Chlordane-1	4.314	0.000	1701648	0	4.601	N.D. #
24)	Chlordane-2	4.851f	0.000	15516711	0	38.435	N.D. #
25)	Chlordane-3	0.000	6.042	0	730776	N.D.	1.689 #
27)	Chlordane-5	0.000	6.924	0	282433	N.D.	3.313 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
Data File : PL058050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2020 01:33
Operator : AJ\MA
Sample : L2277-04
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 04:58:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

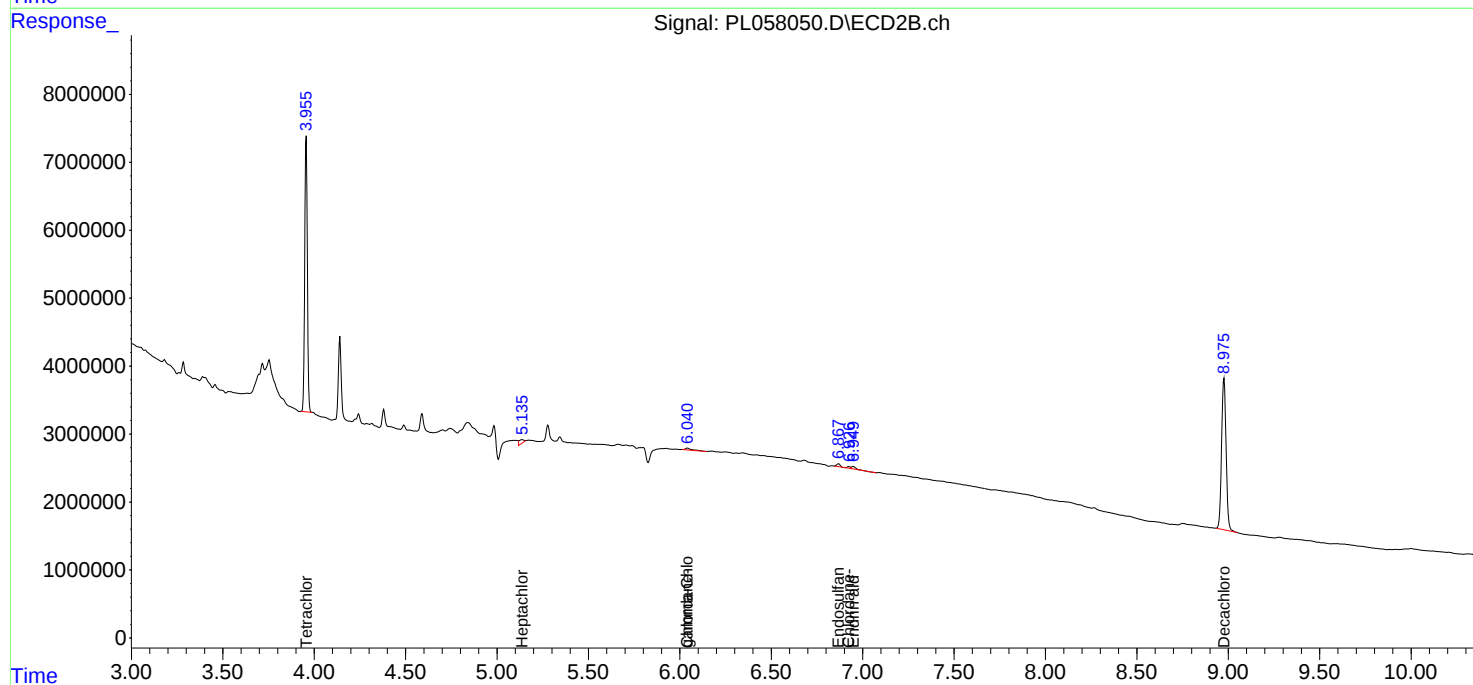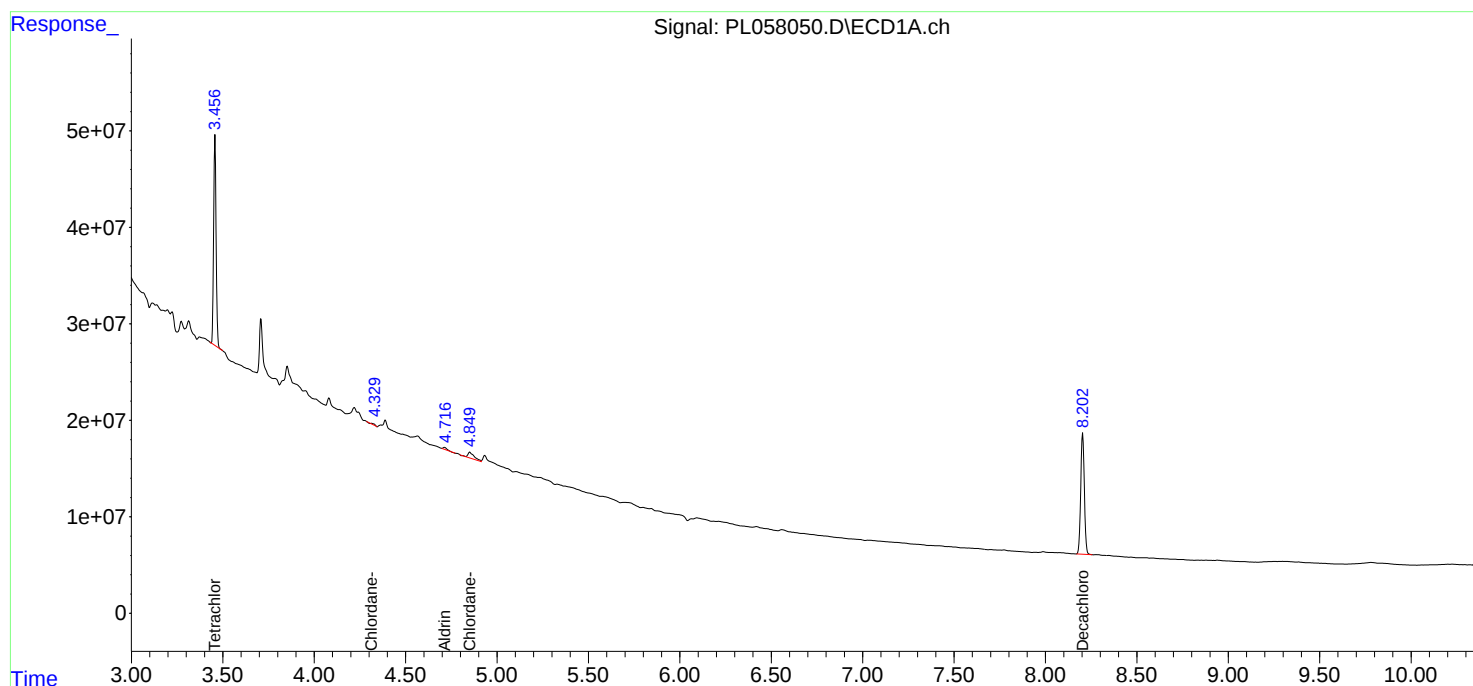


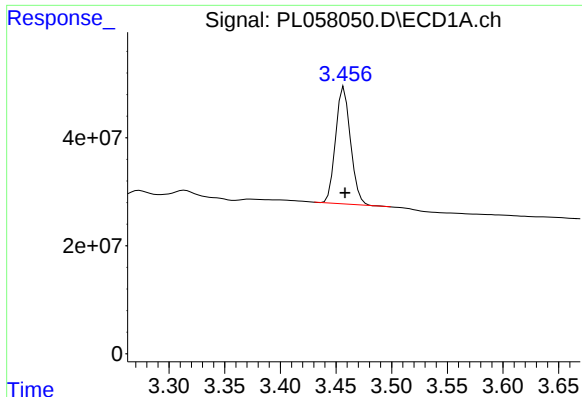

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 201837643
Conc: 20.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

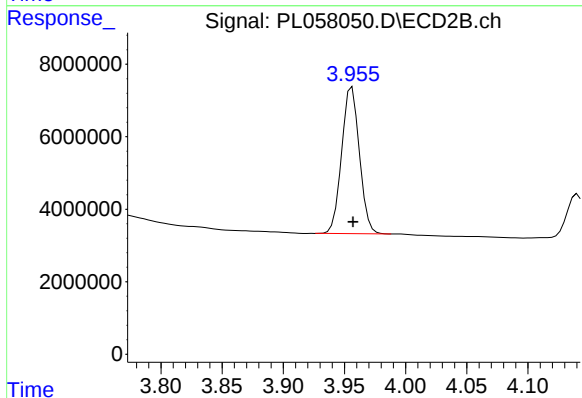


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 40824283
Conc: 18.81 ng/ml

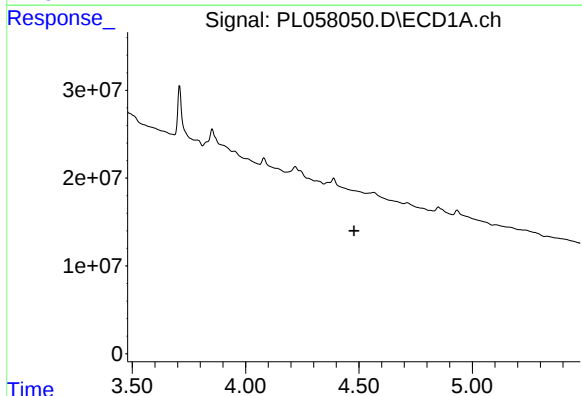


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

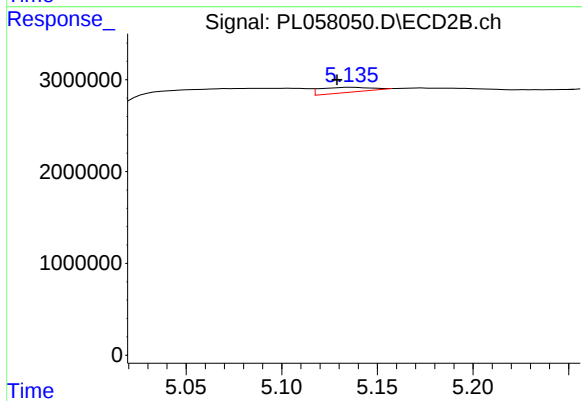

#4 Heptachlor


R.T.: 5.137 min
Delta R.T.: 0.008 min
Response: 1014053
Conc: 0.30 ng/ml

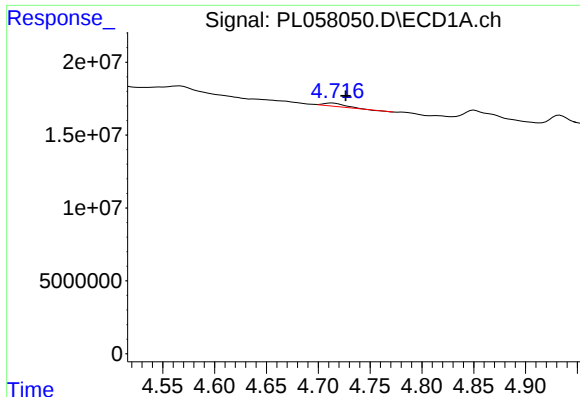

#5 Aldrin


R.T.: 4.713 min
Delta R.T.: -0.013 min
Response: 1781358
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

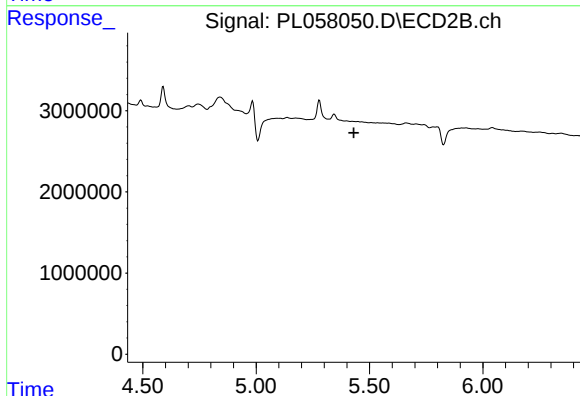


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.431 min
Response: 0
Conc: N.D.

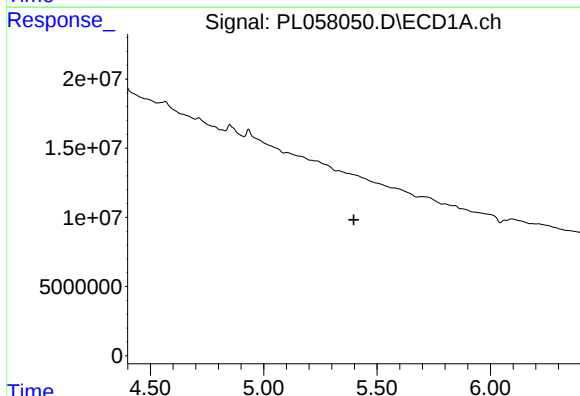


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

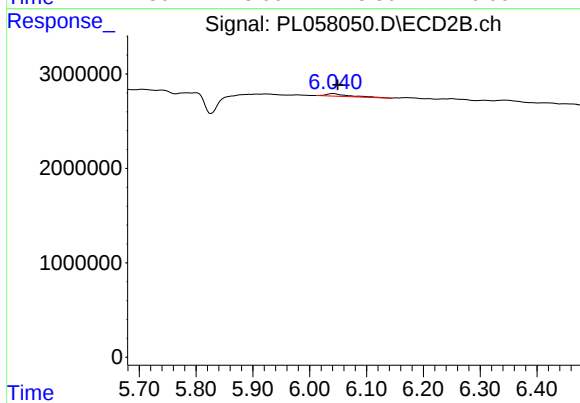

#10 gamma-Chlordane


R.T.: 6.042 min
Delta R.T.: -0.008 min
Response: 730776
Conc: 0.23 ng/ml

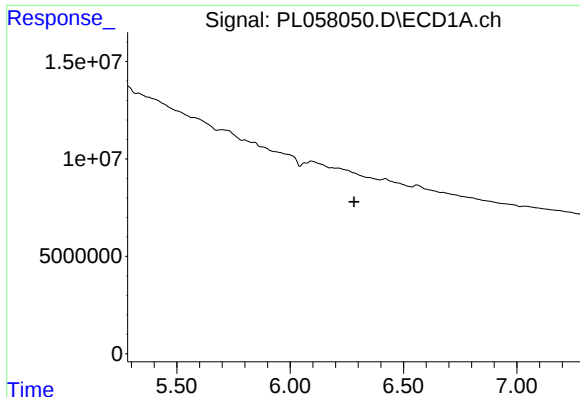

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

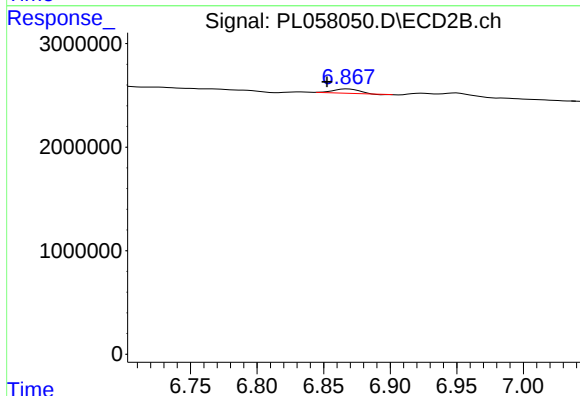


#15 Endosulfan II

R.T.: 6.868 min
Delta R.T.: 0.016 min
Response: 520012
Conc: 0.20 ng/ml

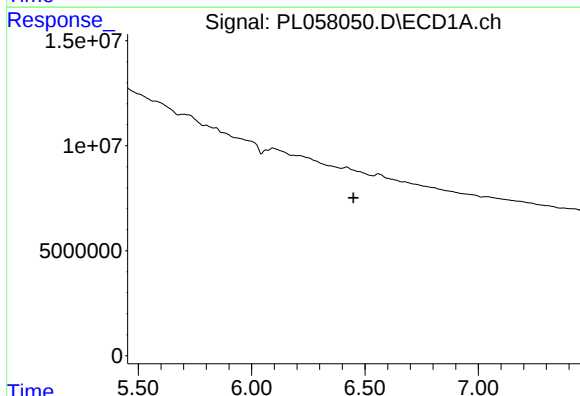


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.450 min
Response: 0
Conc: N.D.

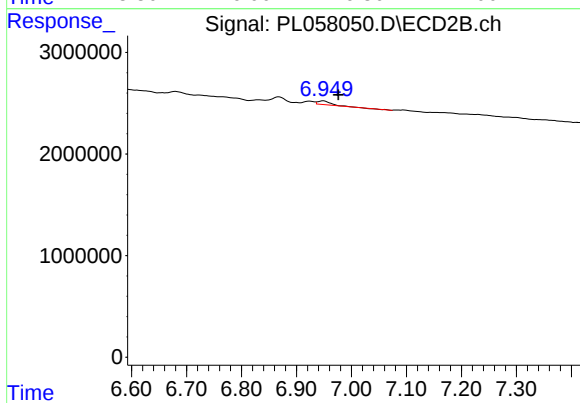

#18 Endrin aldehyde


R.T.: 6.949 min
Delta R.T.: -0.027 min
Response: 608446
Conc: 0.27 ng/ml

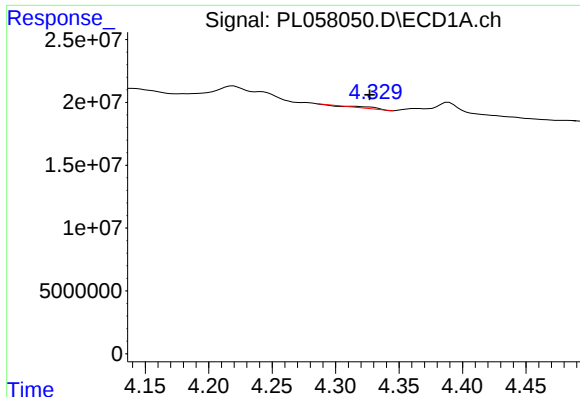

#23 Chlordane-1


R.T.: 4.314 min
Delta R.T.: -0.013 min
Response: 1701648
Conc: 4.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

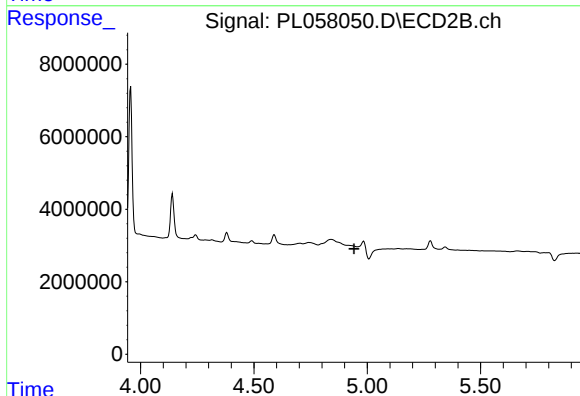


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

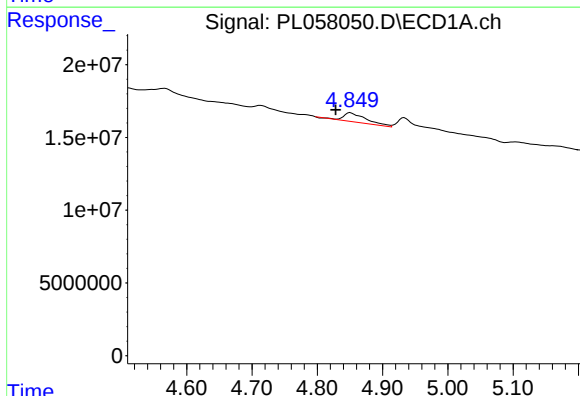


#24 Chlordane-2

R.T.: 4.851 min
Delta R.T.: 0.022 min
Response: 15516711
Conc: 38.43 ng/ml

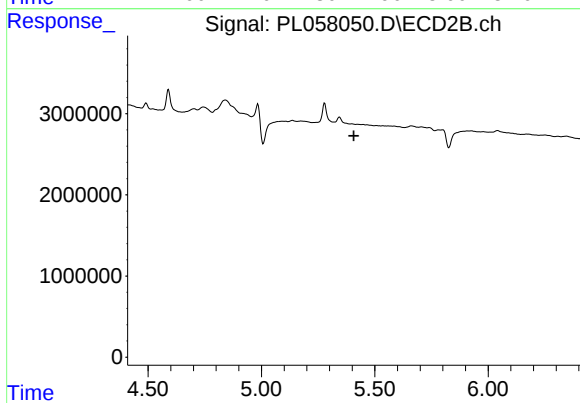

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

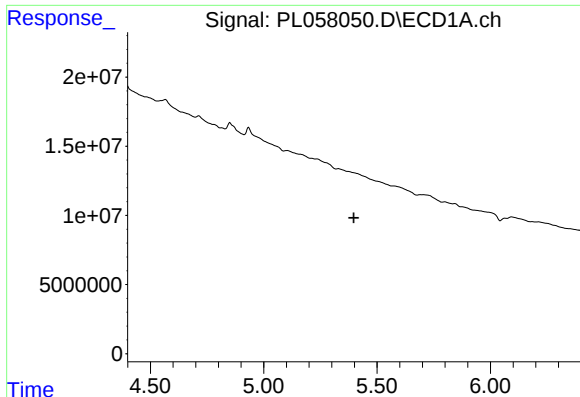

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

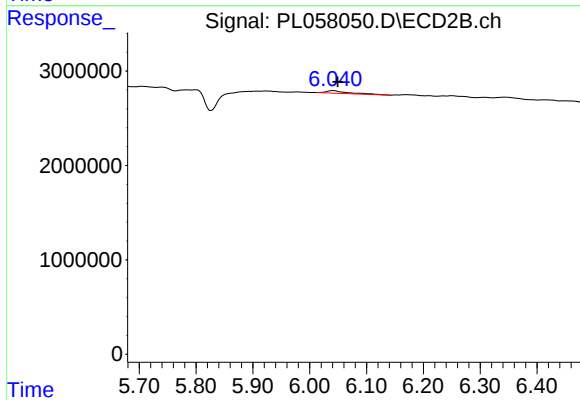


#25 Chlordane-3

R.T.: 6.042 min
Delta R.T.: -0.008 min
Response: 730776
Conc: 1.69 ng/ml

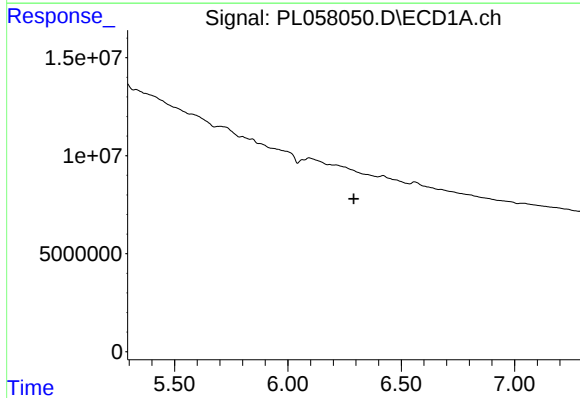


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.290 min
Response: 0
Conc: N.D.

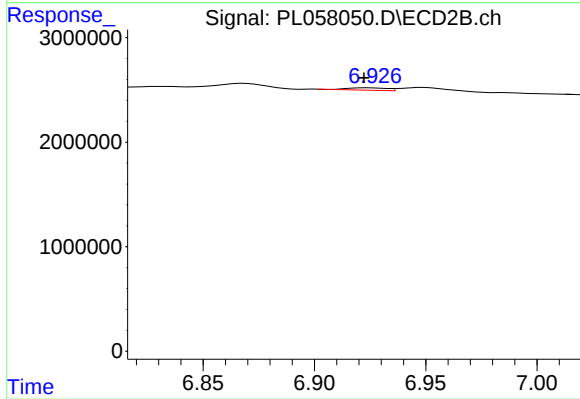

#27 Chlordane-5


R.T.: 6.924 min
Delta R.T.: 0.002 min
Response: 282433
Conc: 3.31 ng/ml

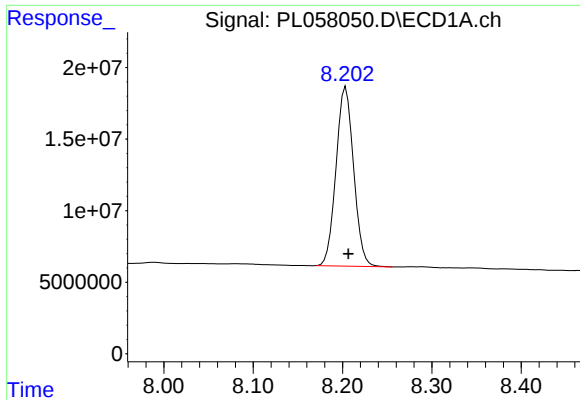

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 171298716
Conc: 16.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

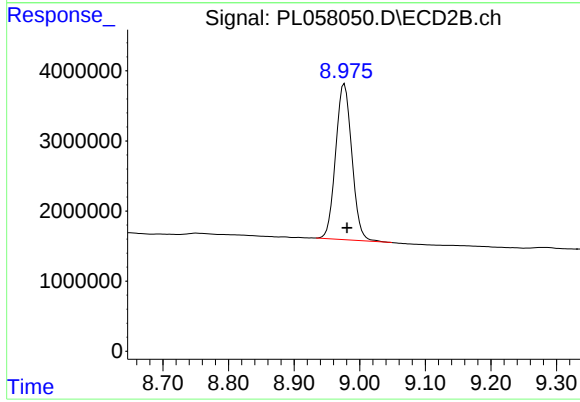

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 38144478
Conc: 17.08 ng/ml