

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
 Data File : PL058054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2020 02:29
 Operator : AJ\MA
 Sample : L2281-11
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 05:00:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.956	200.7E6	41231553	19.911	18.999
28)	SA Decachlor...	8.203	8.978	188.9E6	41341454	18.325	18.507
Target Compounds							
4)	MA Heptachlor	0.000	5.141	0	1269516	N.D.	0.378 #
5)	MB Aldrin	4.729	0.000	2749572	0	0.187	N.D. #
8)	B Heptachlo...	0.000	5.795f	0	6802181	N.D.	2.519 #
15)	B Endosulfa...	6.288	6.868f	1454260	383456	0.131	0.148
18)	B Endrin al...	0.000	6.950f	0	704313	N.D.	0.317 #
19)	B Endosulfa...	6.669	0.000	444190	0	0.044	N.D. #
24)	Chlordane-2	4.818	0.000	3320758	0	8.225	N.D. #
27)	Chlordane-5	6.288	6.950f	1454260	704313	3.844	8.261 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
Data File : PL058054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2020 02:29
Operator : AJ\MA
Sample : L2281-11
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 05:00:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

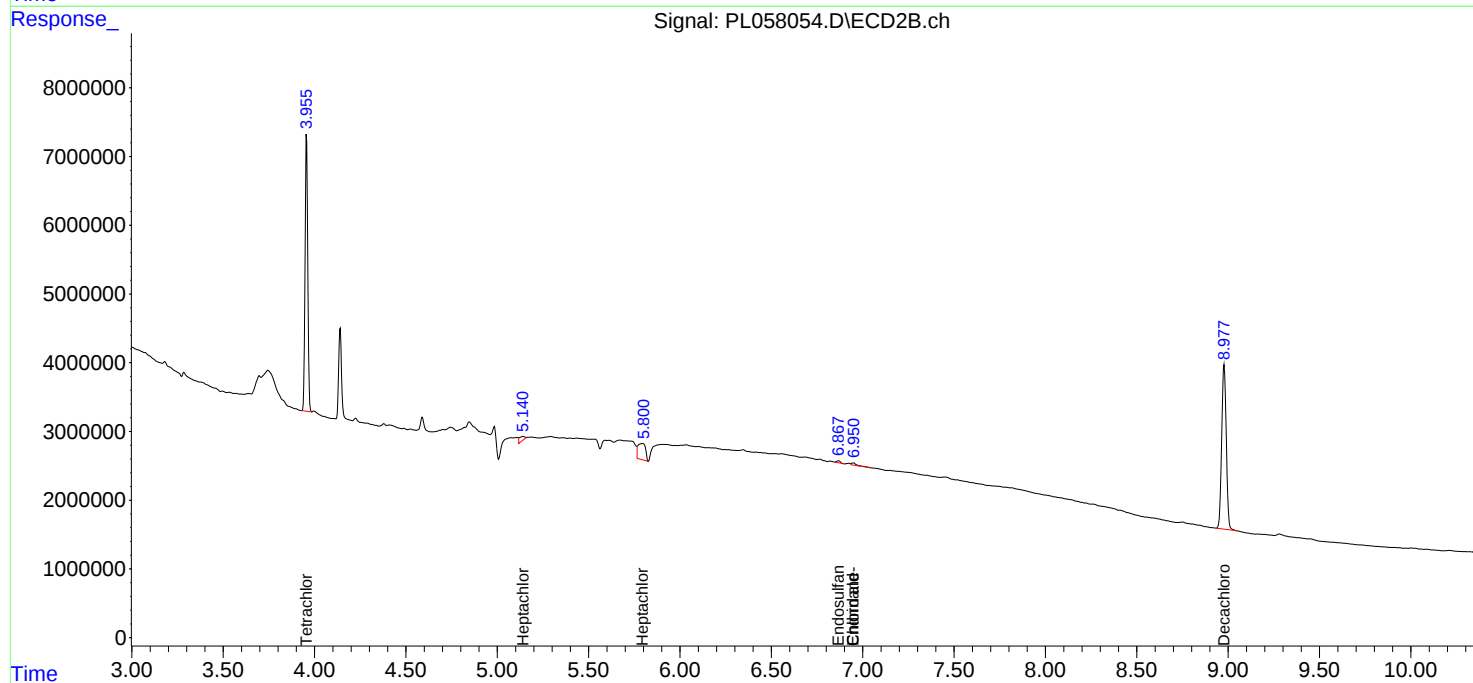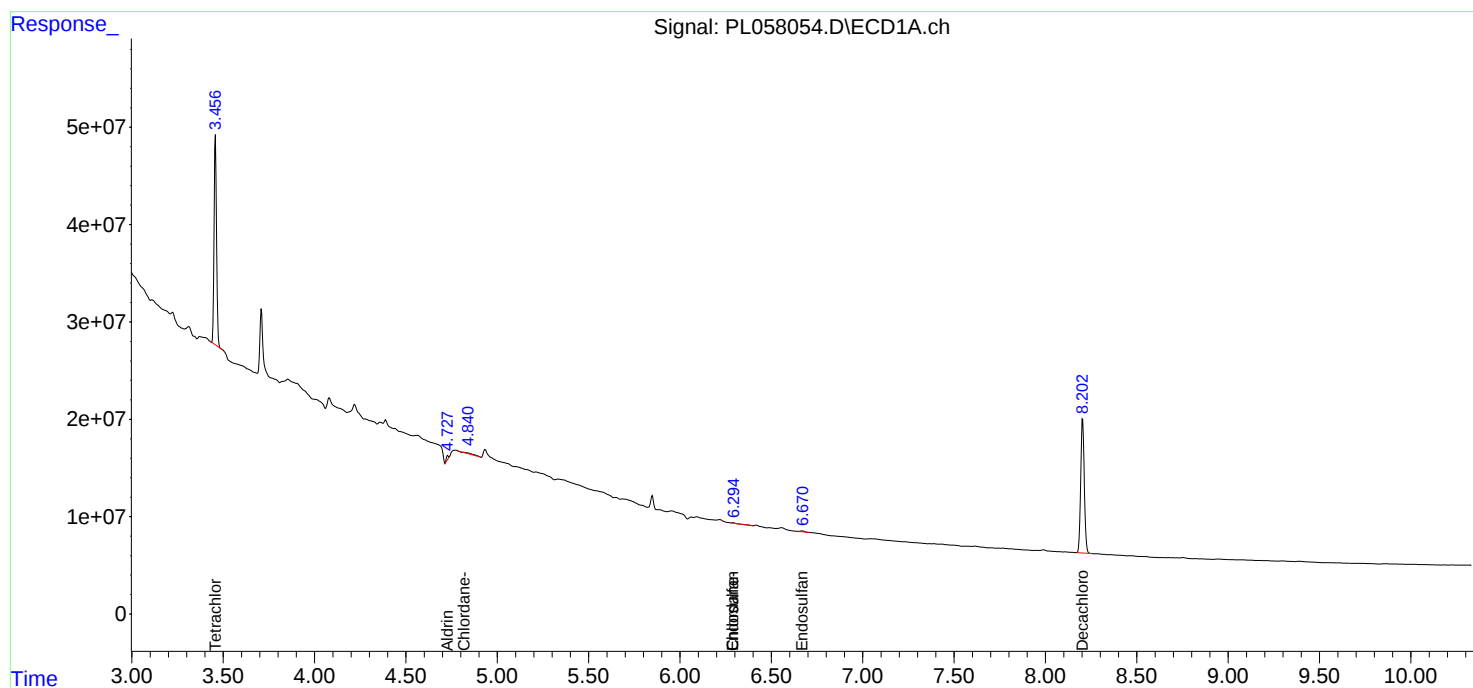


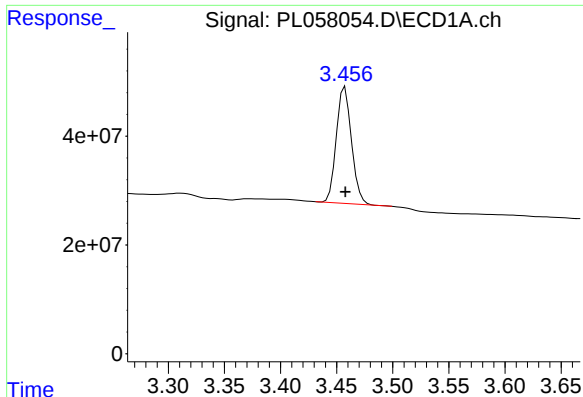

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 200718509
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

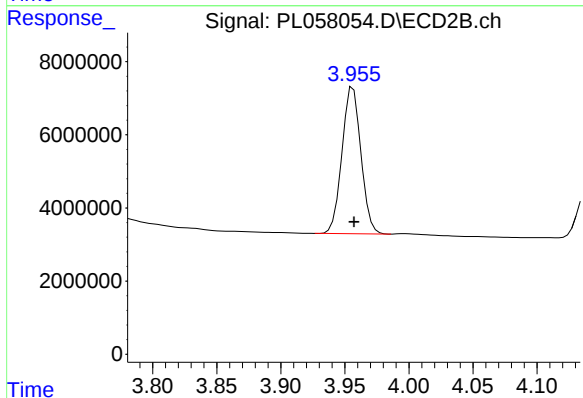


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 41231553
Conc: 19.00 ng/ml

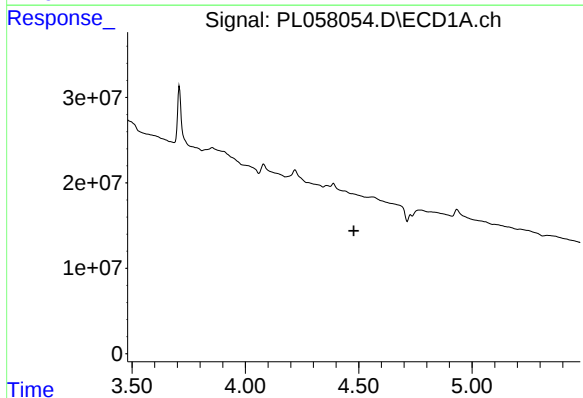


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

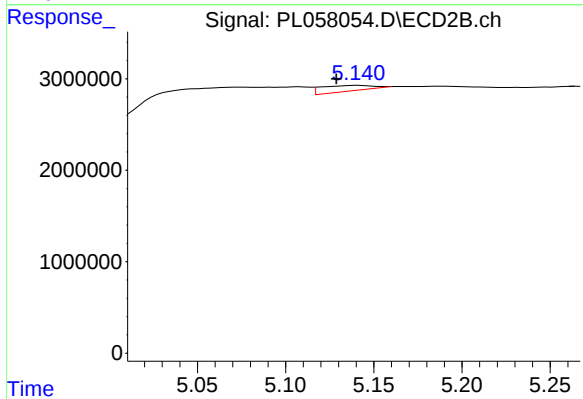

#4 Heptachlor


R.T.: 5.141 min
Delta R.T.: 0.012 min
Response: 1269516
Conc: 0.38 ng/ml

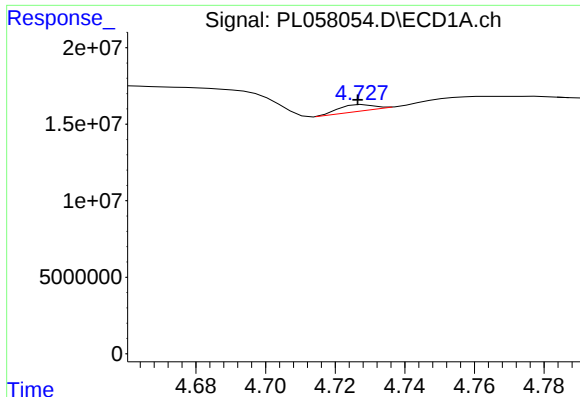

#5 Aldrin


R.T.: 4.729 min
Delta R.T.: 0.002 min
Response: 2749572
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

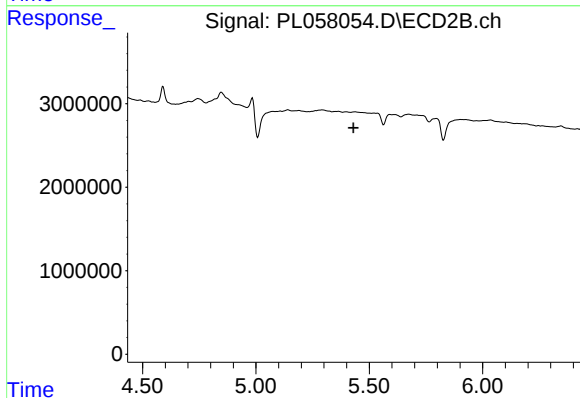


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.431 min
Response: 0
Conc: N.D.

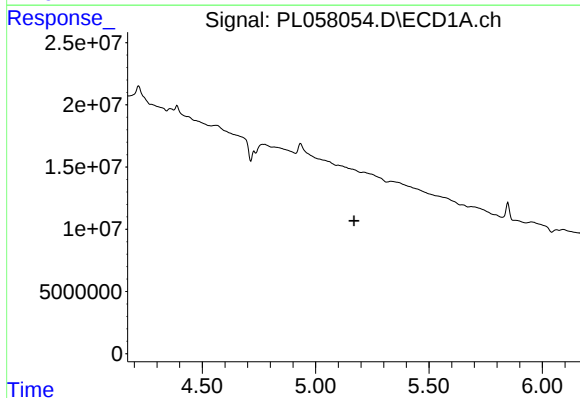


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

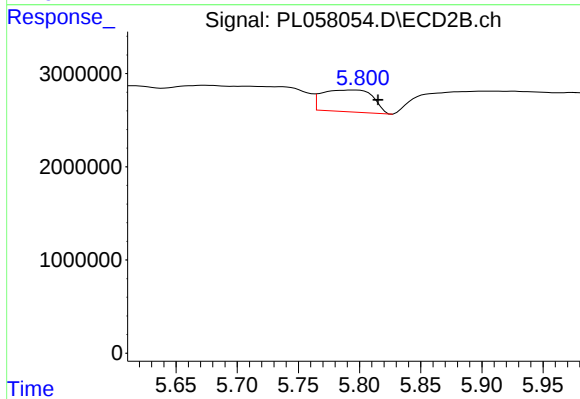

#8 Heptachlor epoxide


R.T.: 5.795 min
Delta R.T.: -0.020 min
Response: 6802181
Conc: 2.52 ng/ml

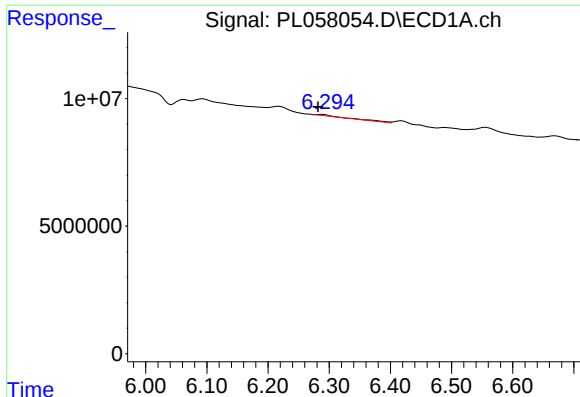

#15 Endosulfan II


R.T.: 6.288 min
Delta R.T.: 0.007 min
Response: 1454260
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

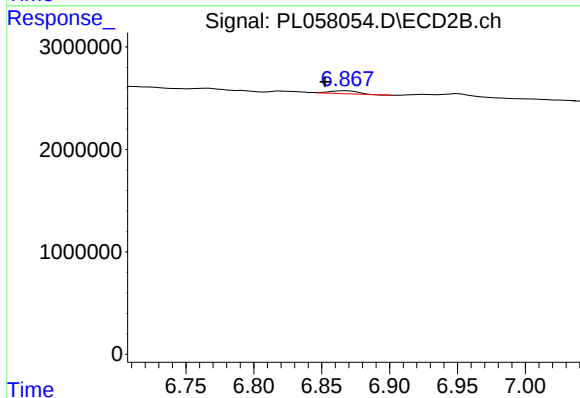


#15 Endosulfan II

R.T.: 6.868 min
Delta R.T.: 0.016 min
Response: 383456
Conc: 0.15 ng/ml

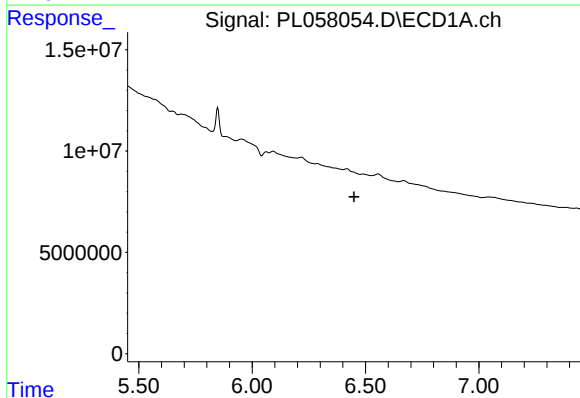


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.450 min
Response: 0
Conc: N.D.

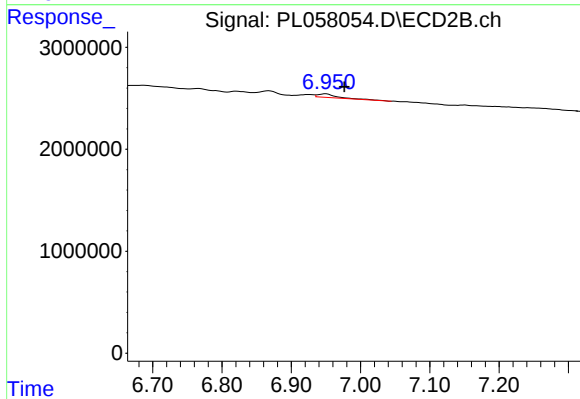

#18 Endrin aldehyde


R.T.: 6.950 min
Delta R.T.: -0.026 min
Response: 704313
Conc: 0.32 ng/ml

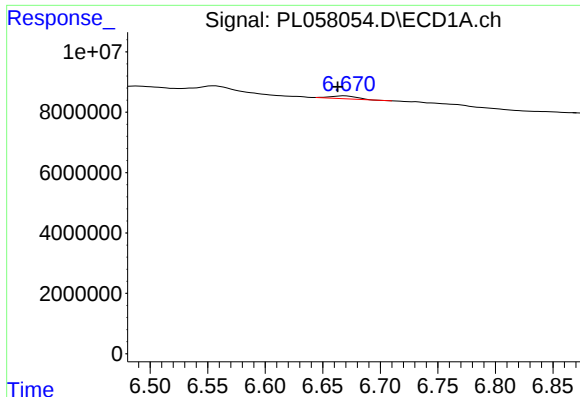

#19 Endosulfan Sulfate


R.T.: 6.669 min
Delta R.T.: 0.006 min
Response: 444190
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

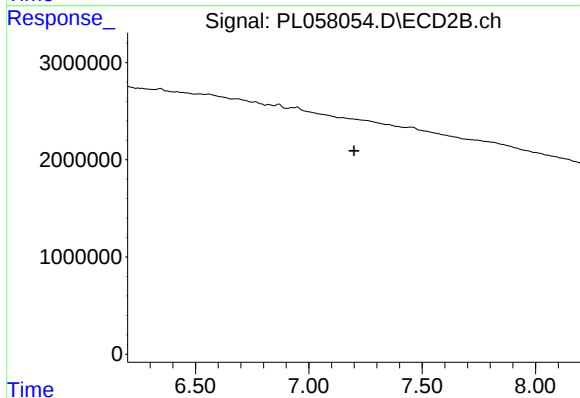


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

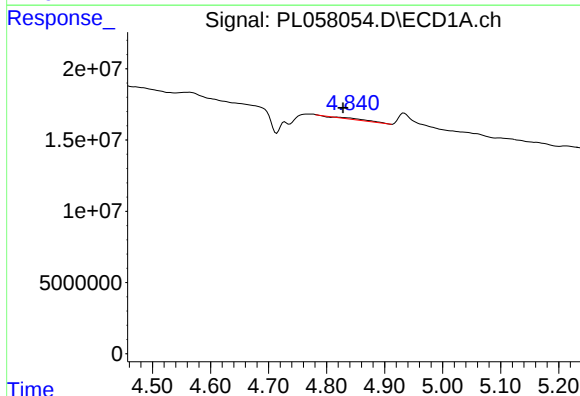


#24 Chlordane-2

R.T.: 4.818 min
Delta R.T.: -0.011 min
Response: 3320758
Conc: 8.23 ng/ml

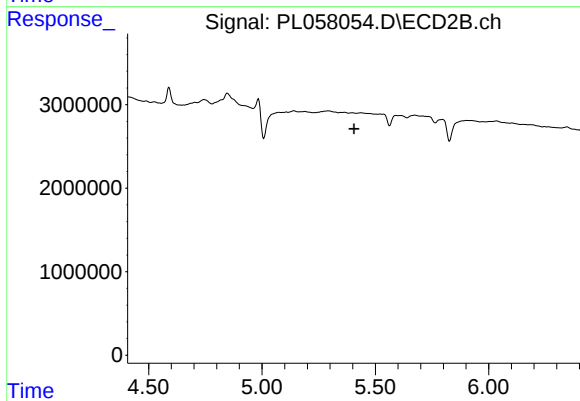

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

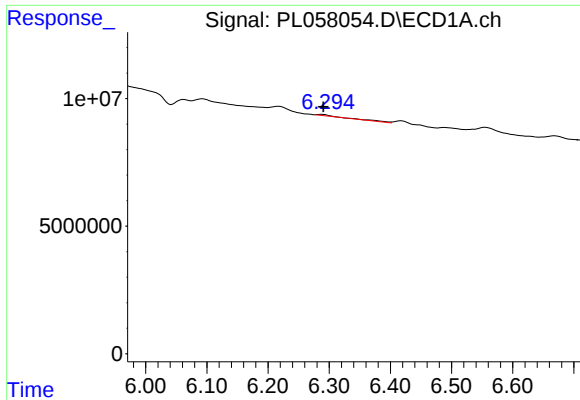

#27 Chlordane-5


R.T.: 6.288 min
Delta R.T.: -0.002 min
Response: 1454260
Conc: 3.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

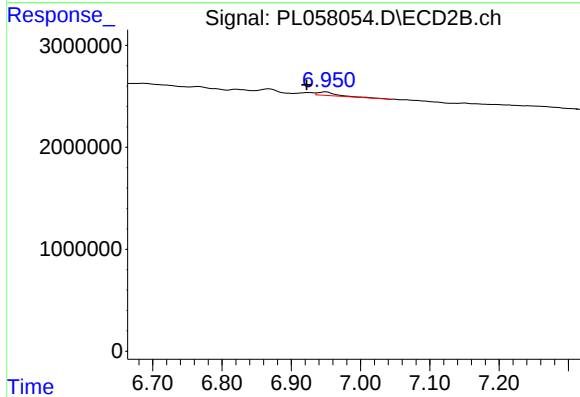


#27 Chlordane-5

R.T.: 6.950 min
Delta R.T.: 0.028 min
Response: 704313
Conc: 8.26 ng/ml

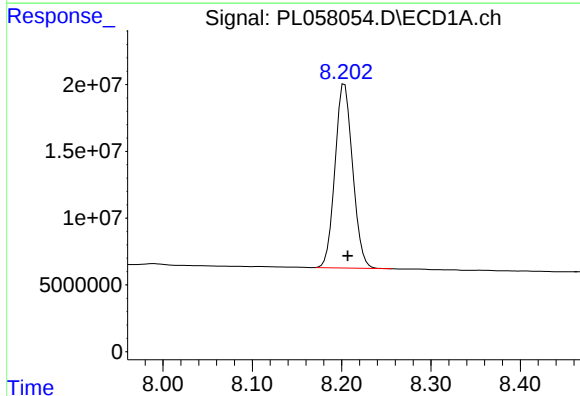

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.003 min
Response: 188902946
Conc: 18.33 ng/ml

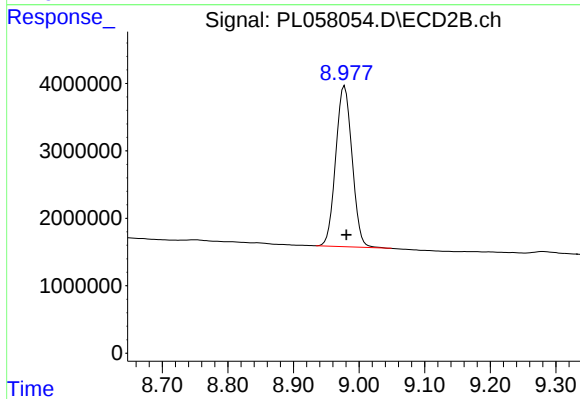

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.003 min
Response: 41341454
Conc: 18.51 ng/ml