

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
 Data File : PL058055.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2020 02:44
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 05:00:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	239.5E6	48055039	23.753	22.144
28)	SA Decachlor...	8.204	8.978	220.9E6	47390354	21.431	21.215
Target Compounds							
2)	A alpha-BHC	3.899	0.000	4099506	0	0.236	N.D. #
4)	MA Heptachlor	4.479	5.145f	999922	2308525	0.062	0.688 #
6)	B beta-BHC	4.415f	0.000	438119	0	0.069	N.D. #
8)	B Heptachlo...	5.172	5.811	3105961	21550044	0.231	7.981 #
12)	B 4,4'-DDE	5.640f	0.000	19955647	0	1.523	N.D. #
14)	MA Endrin	6.010	6.643	5472140	6639492	0.469	2.657 #
15)	B Endosulfa...	0.000	6.868f	0	311709	N.D.	0.120 #
23)	Chlordane-1	4.353f	0.000	3267333	0	8.834	N.D. #
24)	Chlordane-2	4.819	0.000	15106818	0	37.419	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041520\
Data File : PL058055.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2020 02:44
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 05:00:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

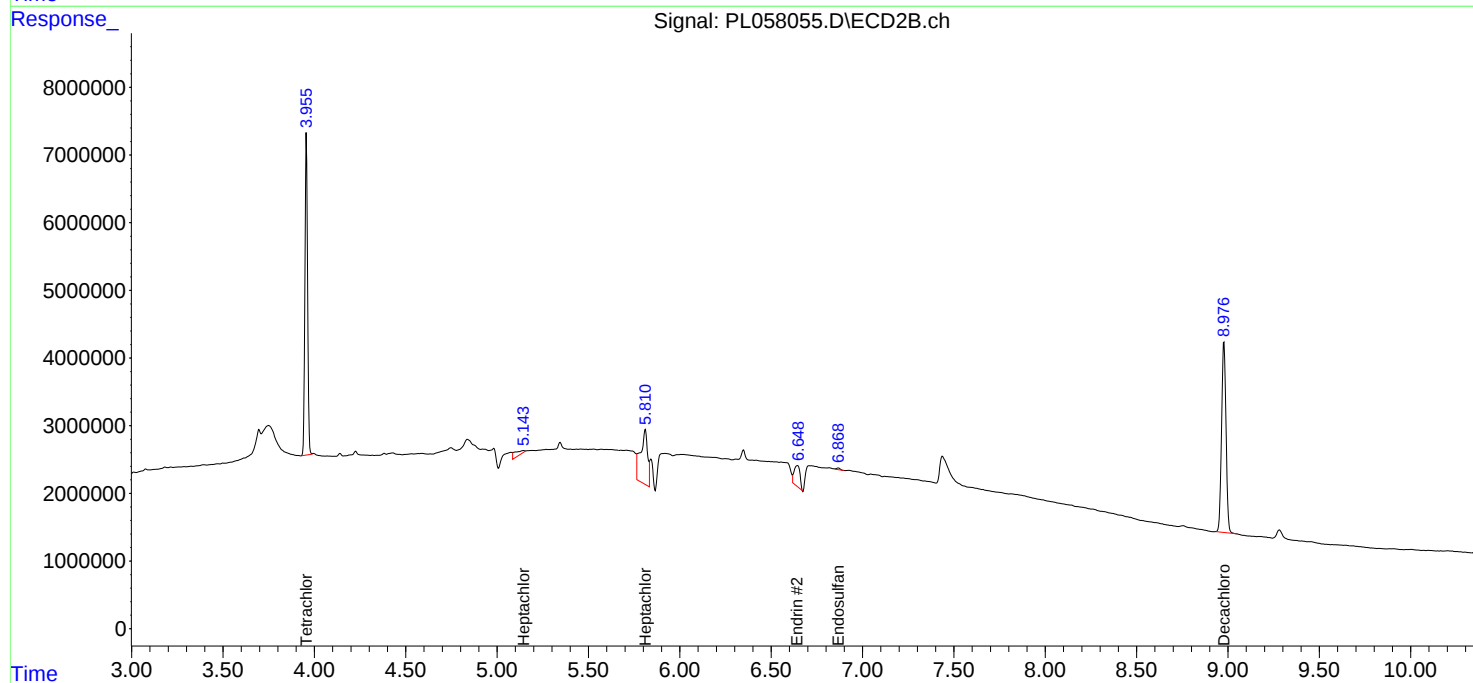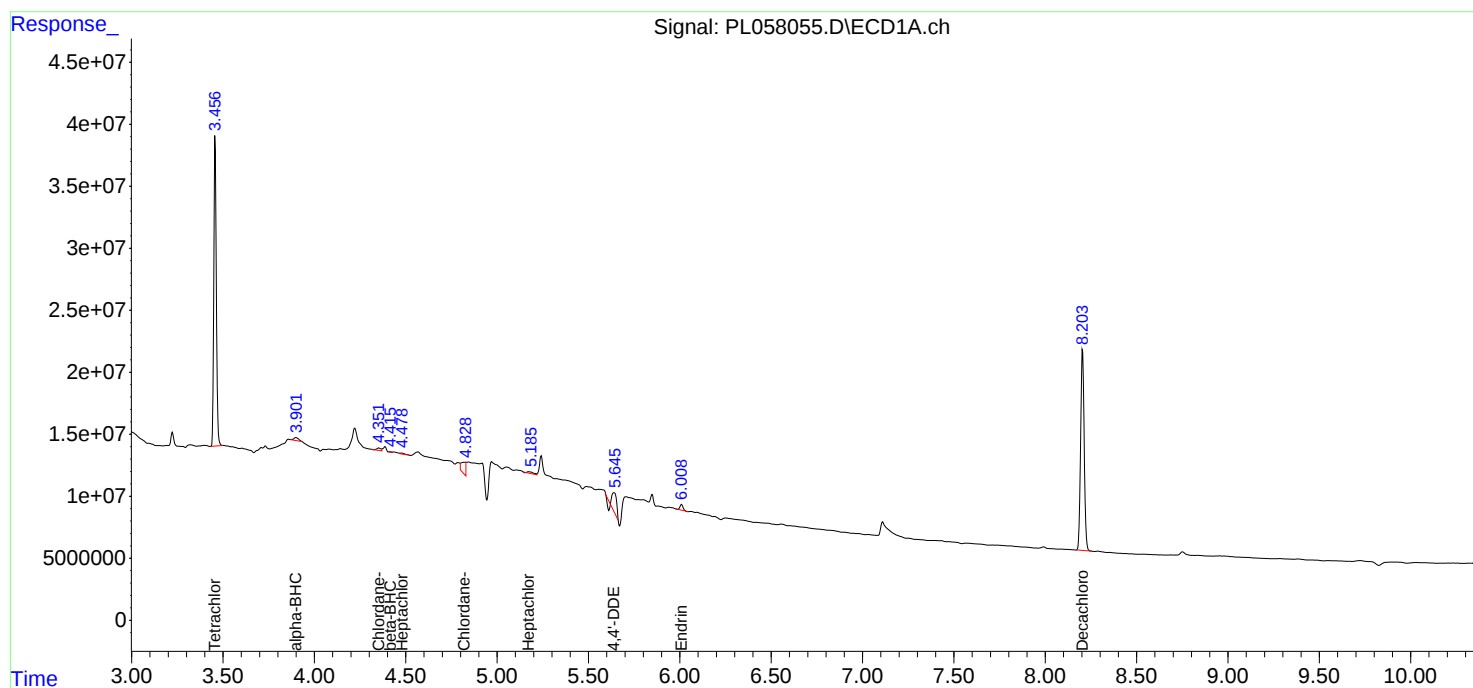


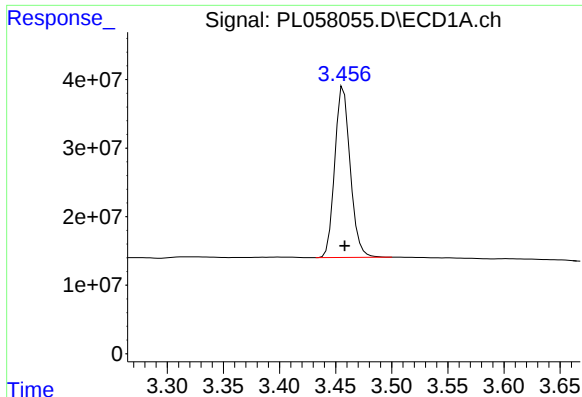

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 239453831
Conc: 23.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

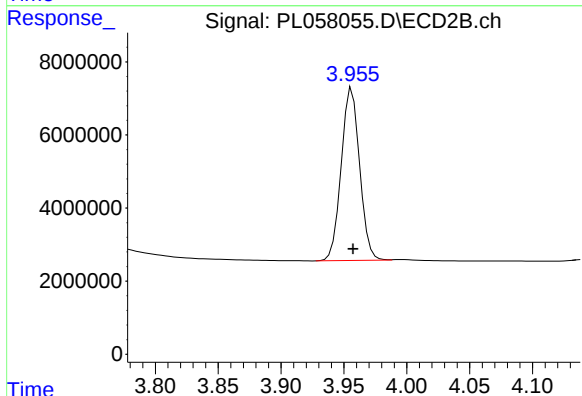


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 48055039
Conc: 22.14 ng/ml

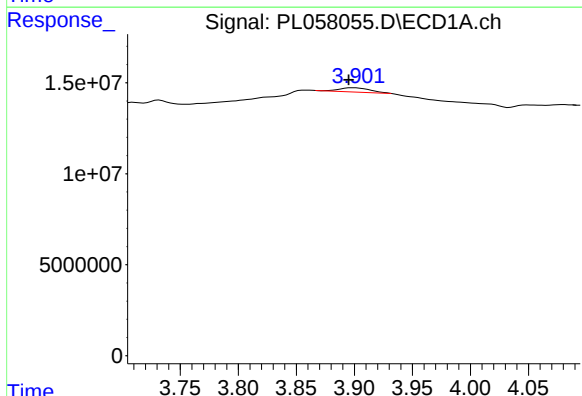


#2 alpha-BHC

R.T.: 3.899 min
Delta R.T.: 0.004 min
Response: 4099506
Conc: 0.24 ng/ml

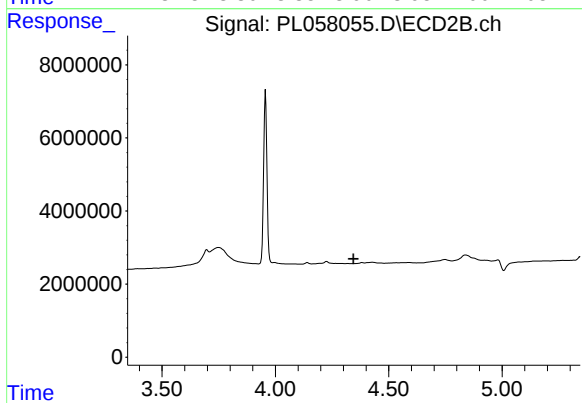

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

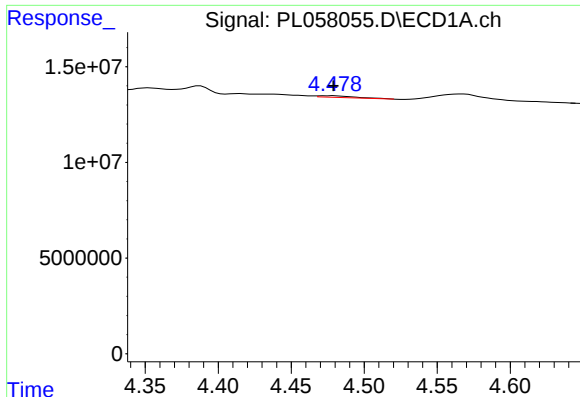

#4 Heptachlor


R.T.: 4.479 min
Delta R.T.: 0.000 min
Response: 999922
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

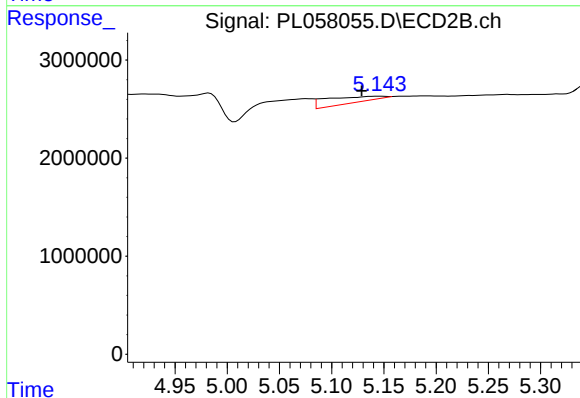


#4 Heptachlor

R.T.: 5.145 min
Delta R.T.: 0.016 min
Response: 2308525
Conc: 0.69 ng/ml

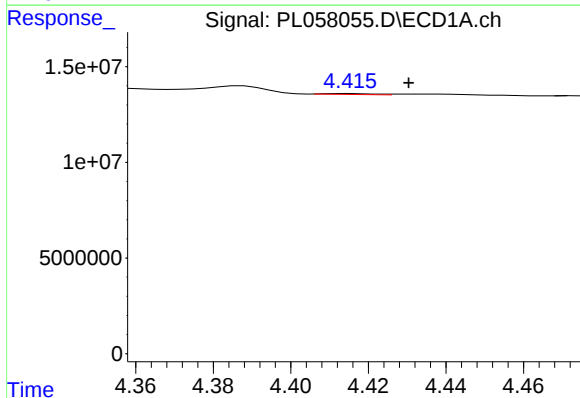


#6 beta-BHC

R.T.: 4.415 min
Delta R.T.: -0.016 min
Response: 438119
Conc: 0.07 ng/ml

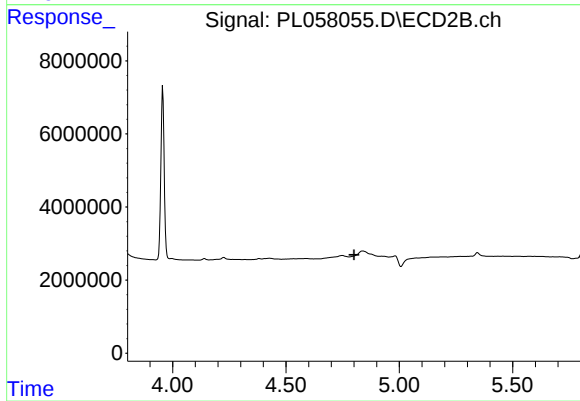

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

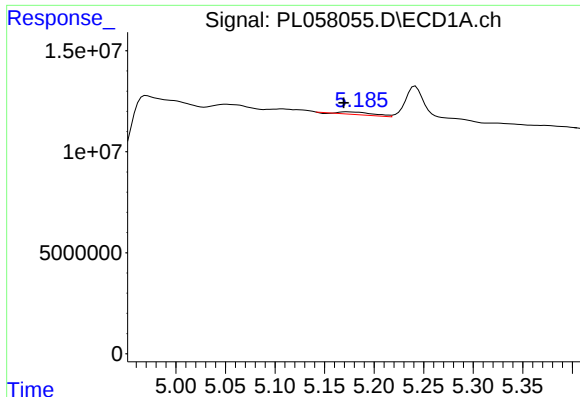

#8 Heptachlor epoxide


R.T.: 5.172 min
Delta R.T.: 0.003 min
Response: 3105961
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

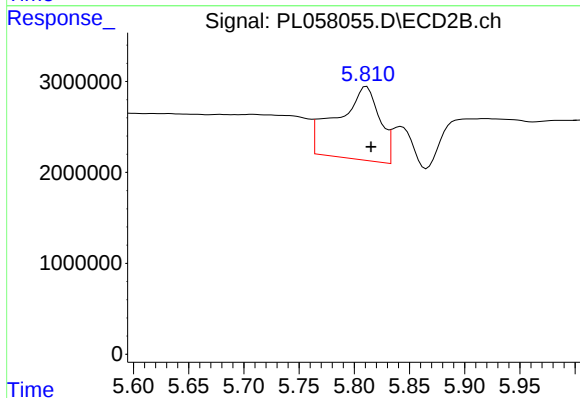


#8 Heptachlor epoxide

R.T.: 5.811 min
Delta R.T.: -0.004 min
Response: 21550044
Conc: 7.98 ng/ml

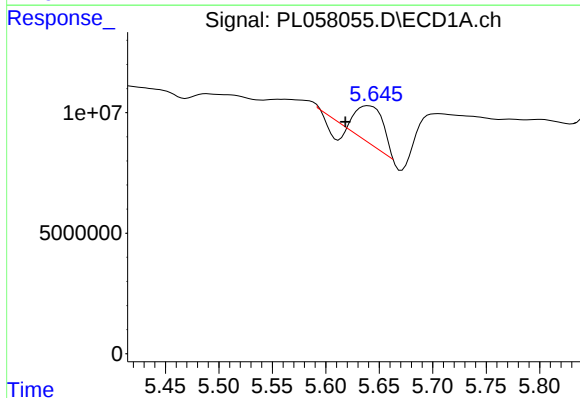


#12 4,4'-DDE

R.T.: 5.640 min
Delta R.T.: 0.022 min
Response: 19955647
Conc: 1.52 ng/ml

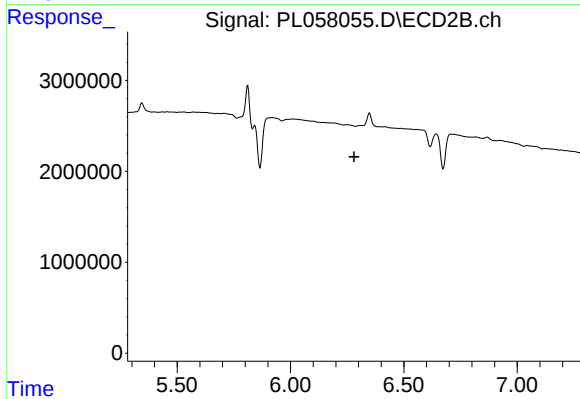

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.280 min
Response: 0
Conc: N.D.

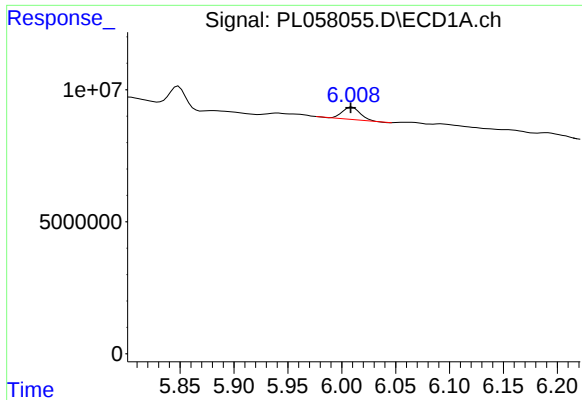

#14 Endrin


R.T.: 6.010 min
Delta R.T.: 0.001 min
Response: 5472140
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

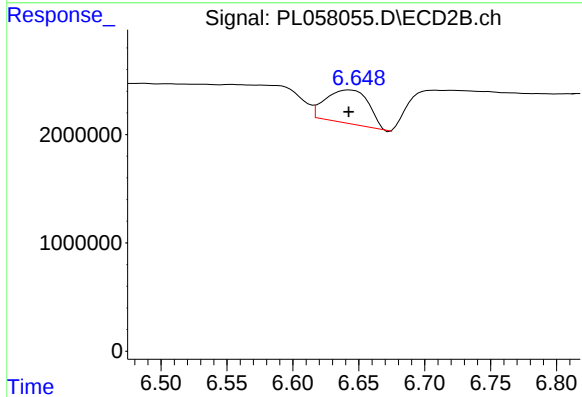


#14 Endrin

R.T.: 6.643 min
Delta R.T.: 0.001 min
Response: 6639492
Conc: 2.66 ng/ml

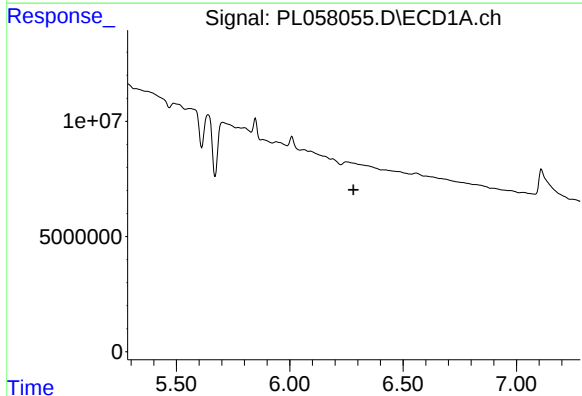


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

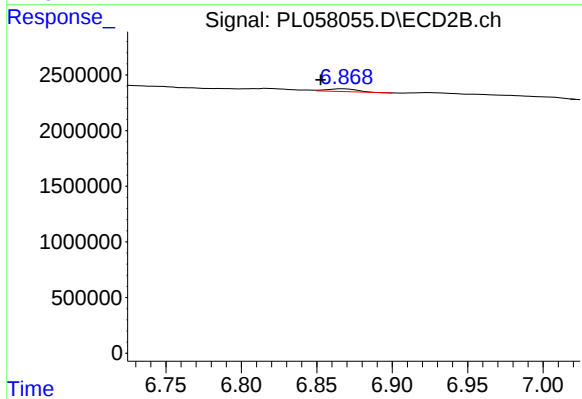

#15 Endosulfan II


R.T.: 6.868 min
Delta R.T.: 0.016 min
Response: 311709
Conc: 0.12 ng/ml

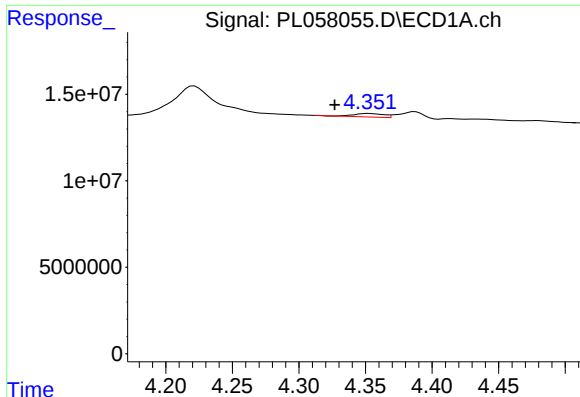

#23 Chlordane-1


R.T.: 4.353 min
Delta R.T.: 0.026 min
Response: 3267333
Conc: 8.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

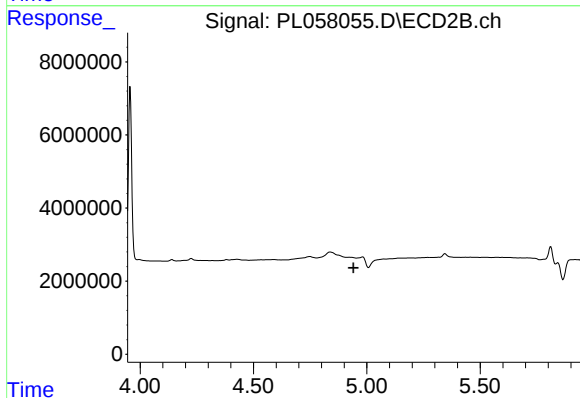


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

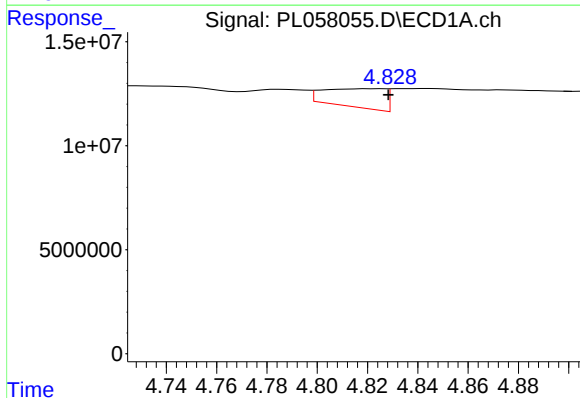


#24 Chlordane-2

R.T.: 4.819 min
Delta R.T.: -0.009 min
Response: 15106818
Conc: 37.42 ng/ml

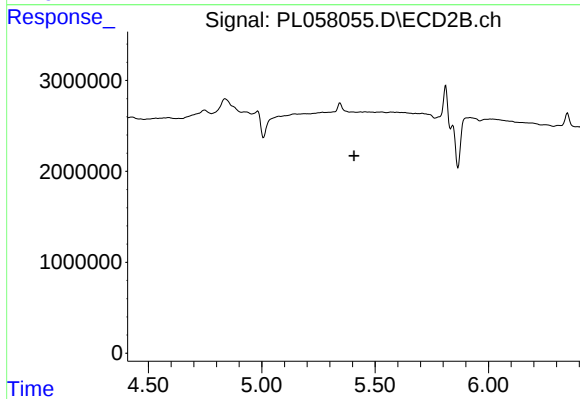

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

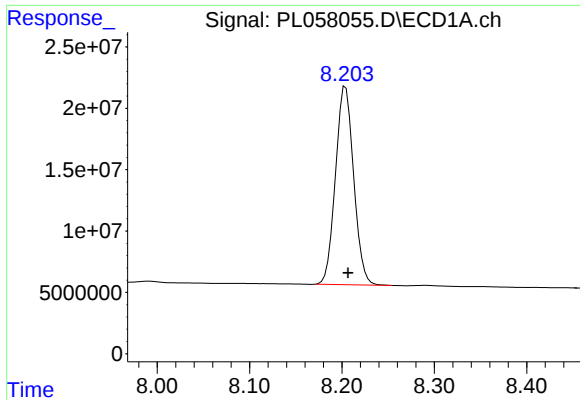

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 220916294
Conc: 21.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

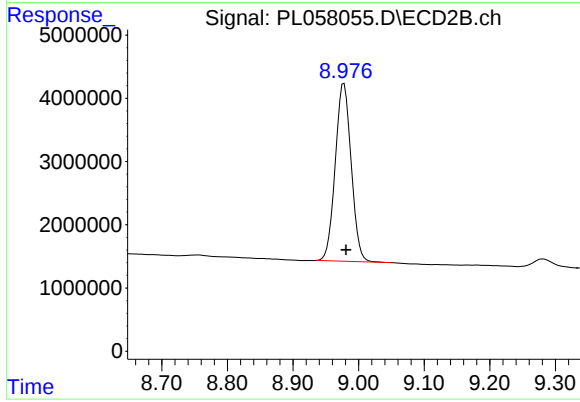

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.003 min
Response: 47390354
Conc: 21.22 ng/ml