

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
 Data File : PL0660153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2021 09:01
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 12:44:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	0.000	5.348f	0	3408902	N.D.	0.612 #
6) B	beta-BHC	4.421	5.033	1722553	11745704	0.977	0.309 #
12) B	4,4'-DDE	0.000	6.567f	0	142883	N.D.	0.035 #
14) MA	Endrin	5.976	0.000	1634661	0	0.469	N.D. #
15) B	Endosulfa...	0.000	7.128	0	701230	N.D.	0.201 #
21) B	Endrin ke...	0.000	7.974	0	934837	N.D.	0.254 #
22)	Mirex	0.000	8.443f	0	480174	N.D.	0.170 #
23)	Chlordane-1	4.317	0.000	6042039	0	52.852	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
Data File : PL0660153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2021 09:01
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 12:44:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

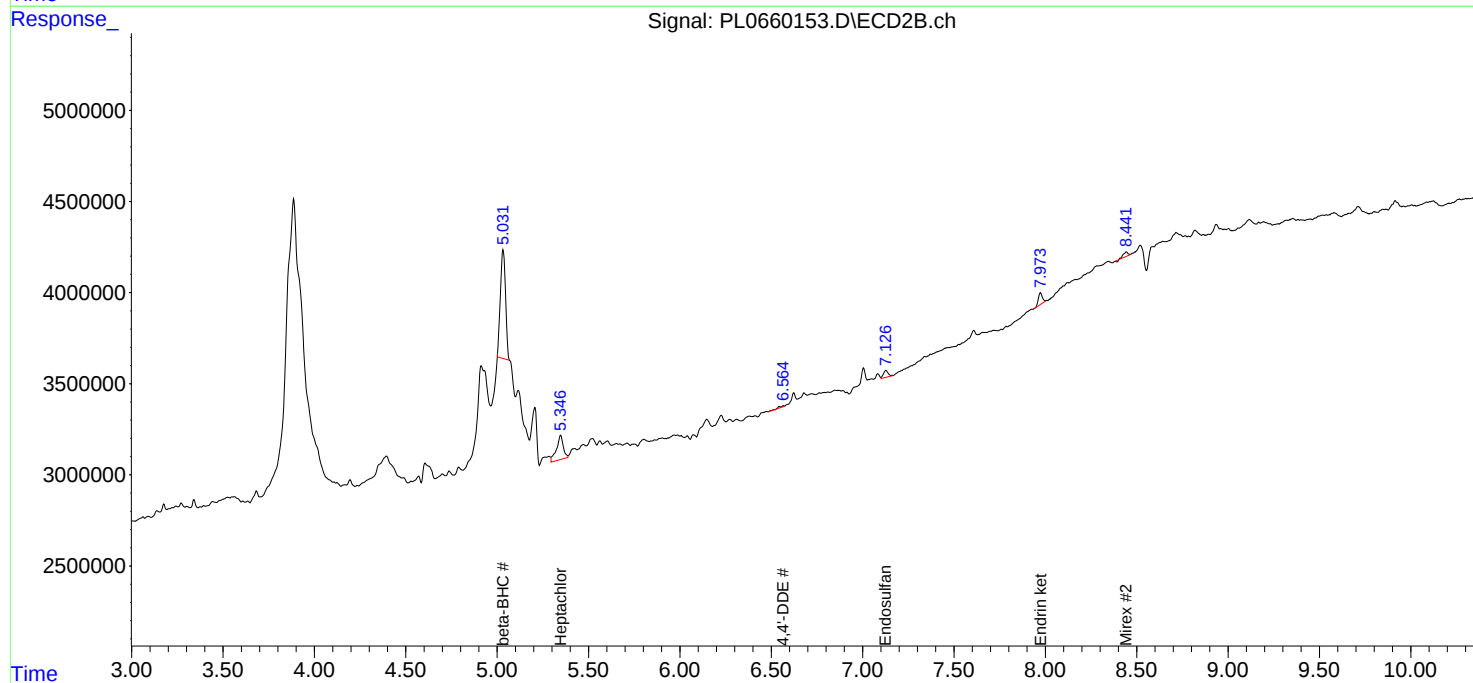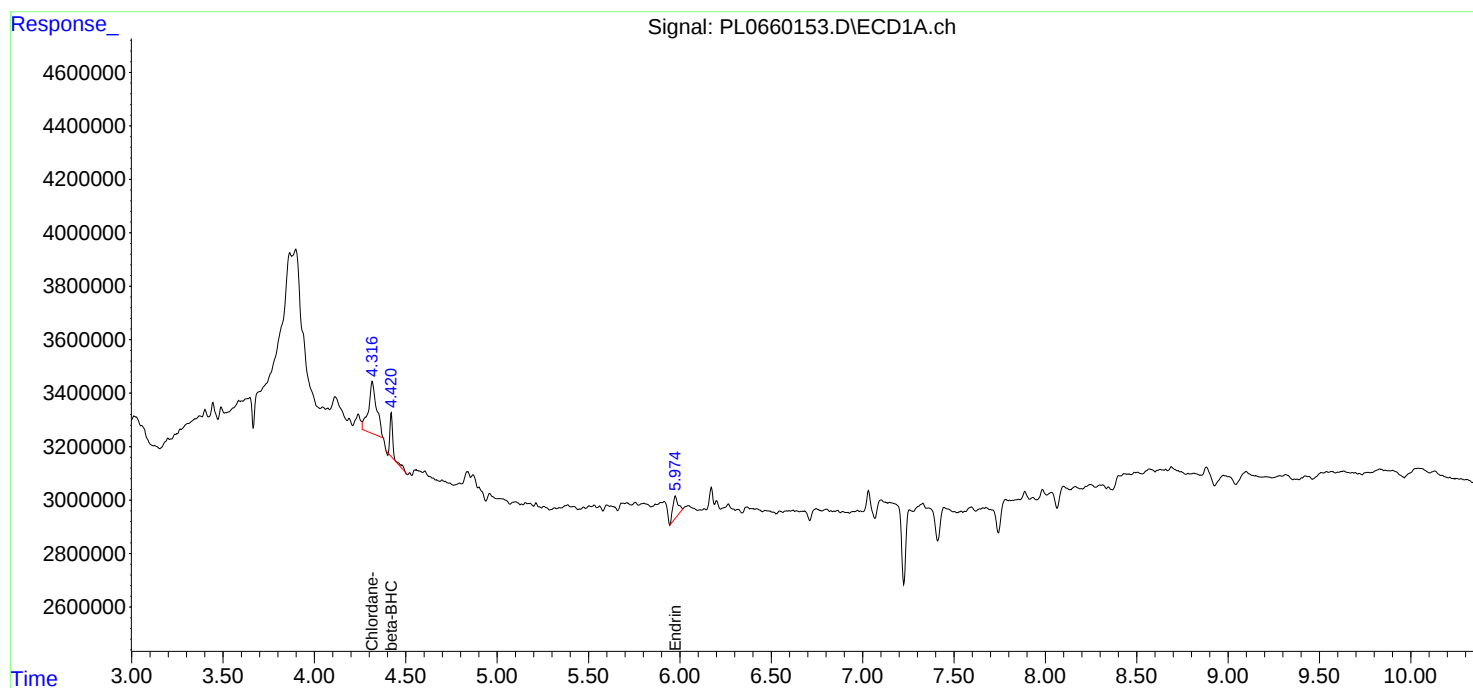


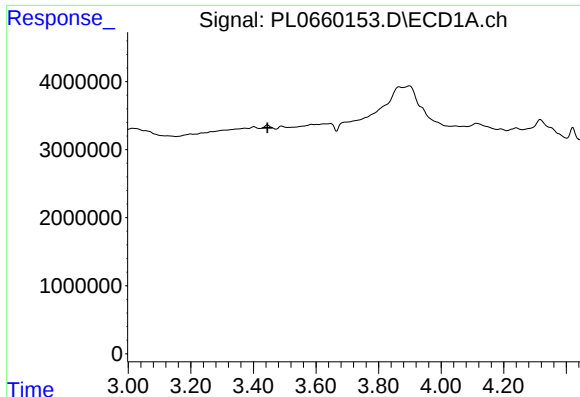

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.445 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

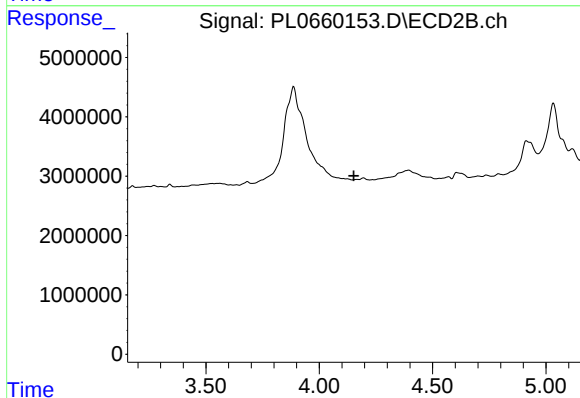


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

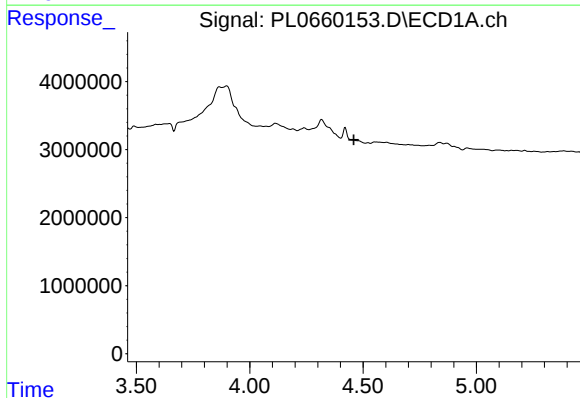


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.459 min
Response: 0
Conc: N.D.

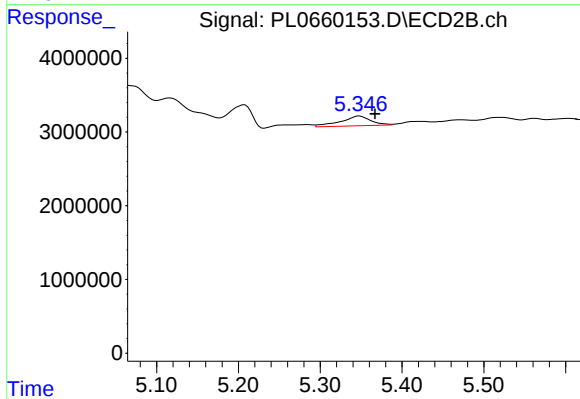

#4 Heptachlor


R.T.: 5.348 min
Delta R.T.: -0.019 min
Response: 3408902
Conc: 0.61 ng/ml

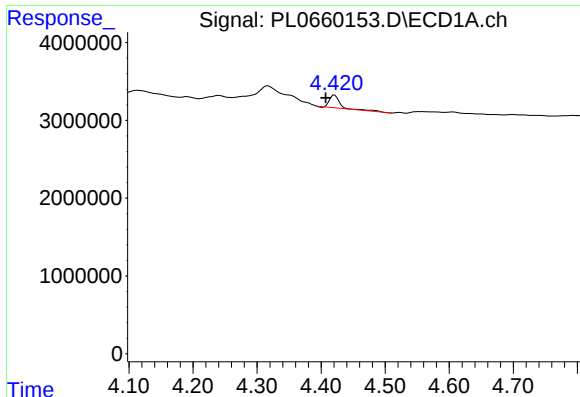

#6 beta-BHC


R.T.: 4.421 min
Delta R.T.: 0.014 min
Response: 1722553
Conc: 0.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

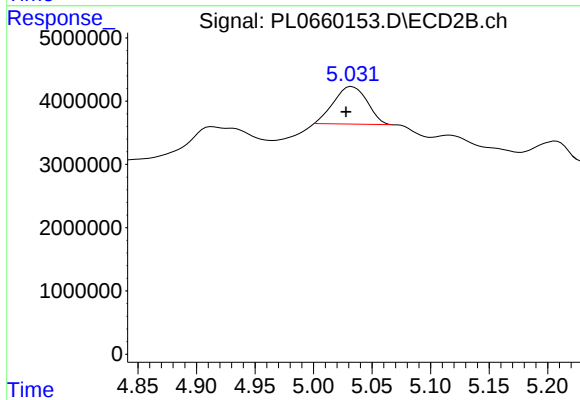


#6 beta-BHC

R.T.: 5.033 min
Delta R.T.: 0.005 min
Response: 11745704
Conc: 0.31 ng/ml

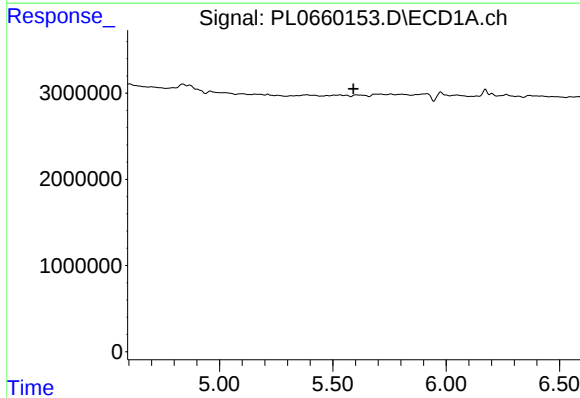


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.591 min
Response: 0
Conc: N.D.

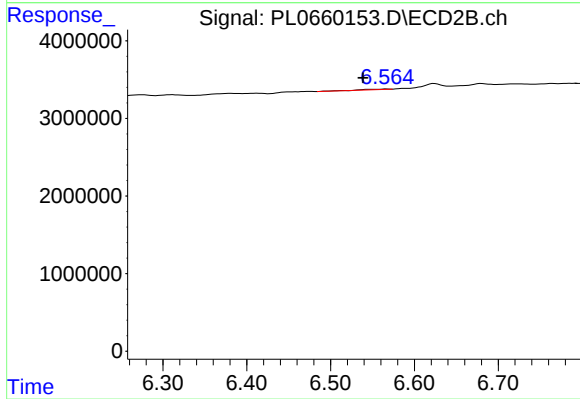

#12 4,4'-DDE


R.T.: 6.567 min
Delta R.T.: 0.028 min
Response: 142883
Conc: 0.03 ng/ml

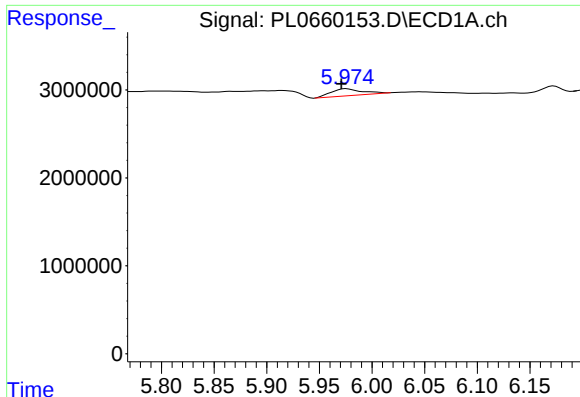

#14 Endrin


R.T.: 5.976 min
Delta R.T.: 0.005 min
Response: 1634661
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

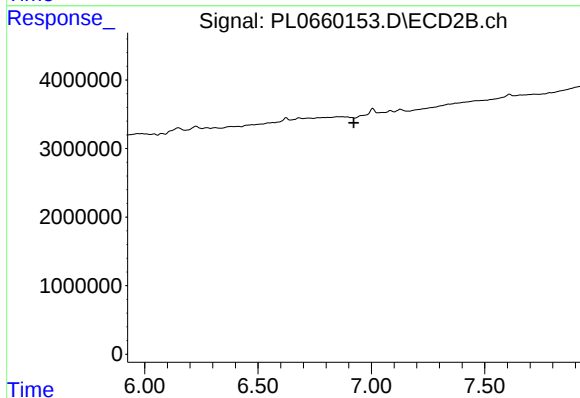


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

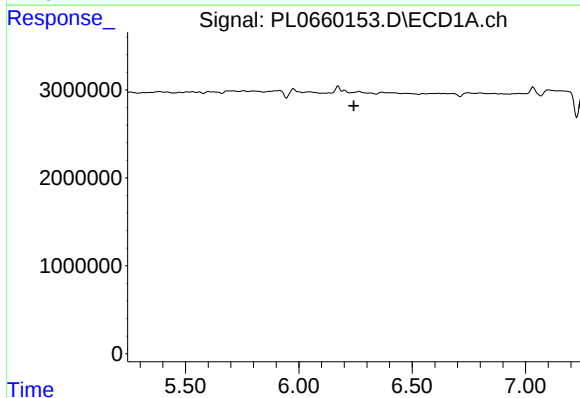


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

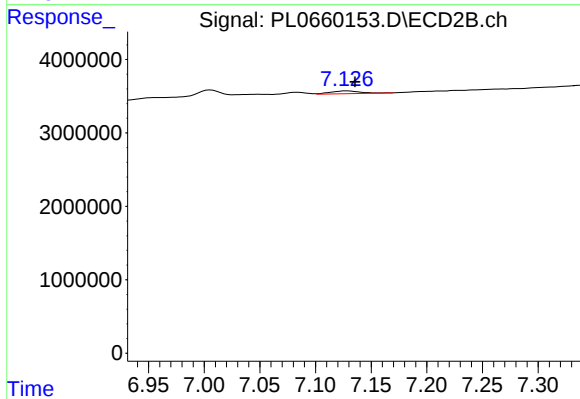

#15 Endosulfan II


R.T.: 7.128 min
Delta R.T.: -0.008 min
Response: 701230
Conc: 0.20 ng/ml

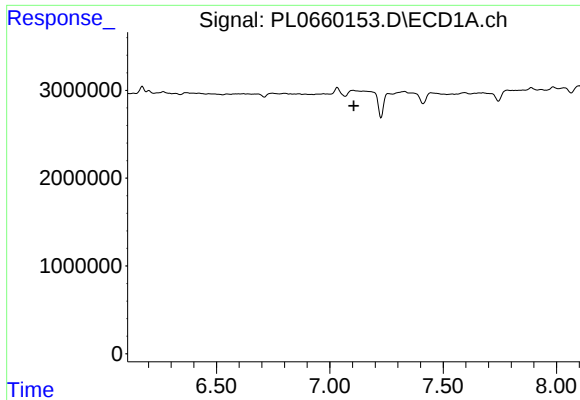

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.105 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

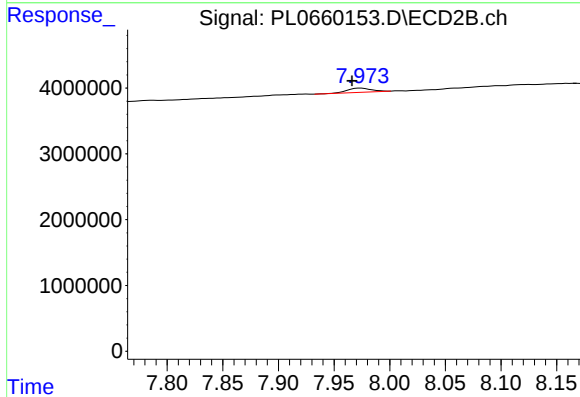


#21 Endrin ketone

R.T.: 7.974 min
Delta R.T.: 0.008 min
Response: 934837
Conc: 0.25 ng/ml

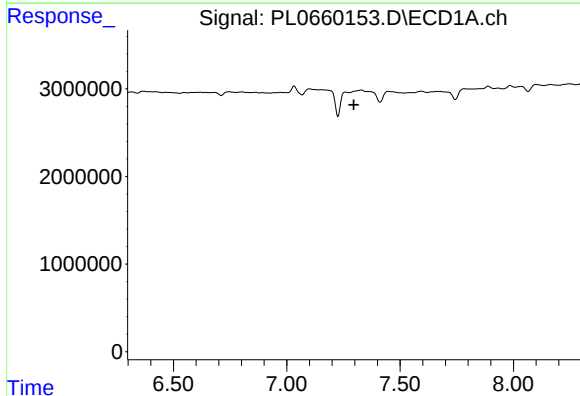


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.296 min
Response: 0
Conc: N.D.

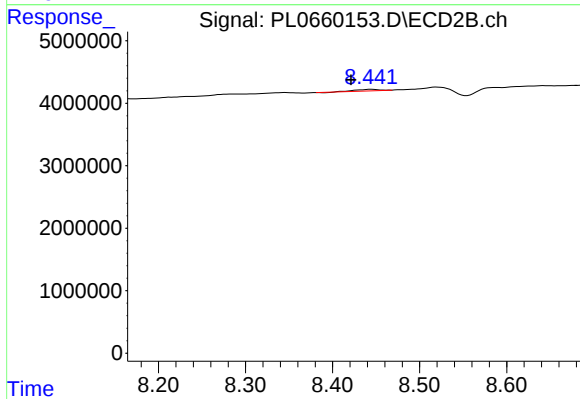

#22 Mirex


R.T.: 8.443 min
Delta R.T.: 0.022 min
Response: 480174
Conc: 0.17 ng/ml

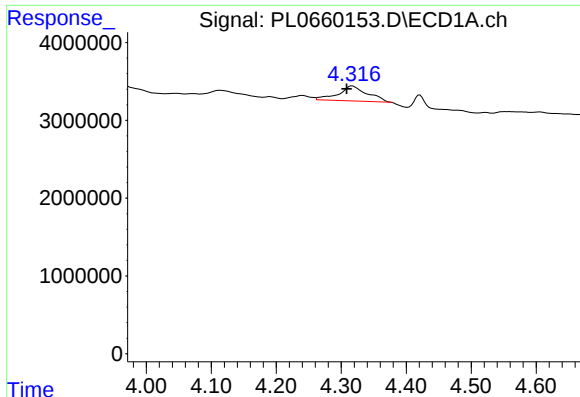

#23 Chlordane-1


R.T.: 4.317 min
Delta R.T.: 0.009 min
Response: 6042039
Conc: 52.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

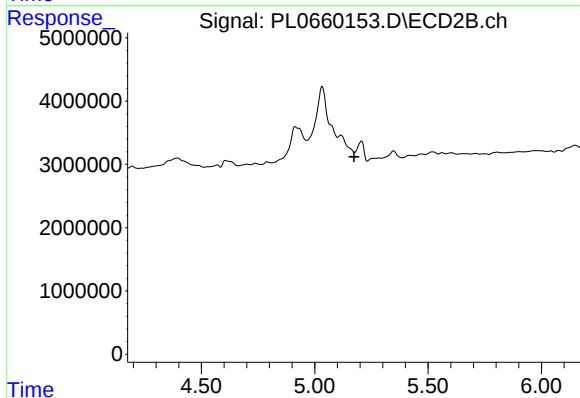


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.173 min
Response: 0
Conc: N.D.

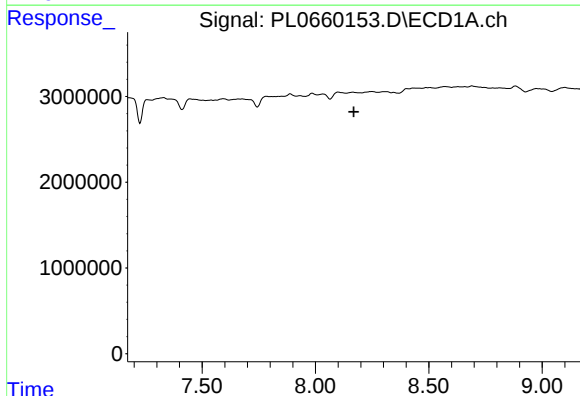

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.169 min
Response: 0
Conc: N.D.

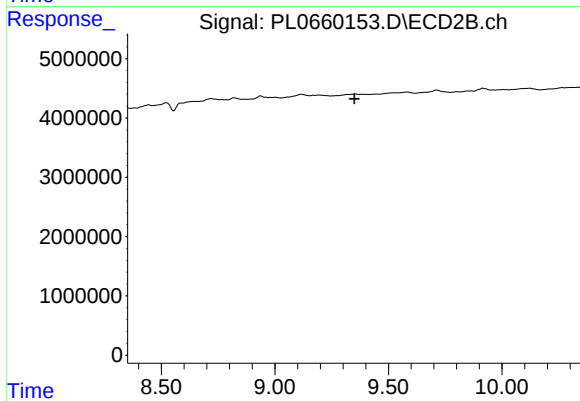

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.351 min
Response: 0
Conc: N.D.