

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
 Data File : PL066211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 00:39
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:43:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.155	49248830	80721270	19.349	20.067
28)	SA Decachlor...	8.171	9.356	44027700	61780121	18.458	18.917
Target Compounds							
2)	A alpha-BHC	3.871	0.000	1005423	0	0.244	N.D. #
4)	MA Heptachlor	0.000	5.352	0	1593604	N.D.	0.286 #
8)	B Heptachlo...	0.000	6.069	0	4450666	N.D.	0.964 #
14)	MA Endrin	5.976	0.000	1248700	0	0.358	N.D. #
15)	B Endosulfa...	0.000	7.127	0	1042102	N.D.	0.299 #
17)	MA 4,4'-DDT	0.000	7.345	0	3133648	N.D.	0.924 #
18)	B Endrin al...	0.000	7.267	0	757131	N.D.	0.271 #
23)	Chlordane-1	4.331f	0.000	3428104	0	29.987	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
Data File : PL066211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 00:39
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:43:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

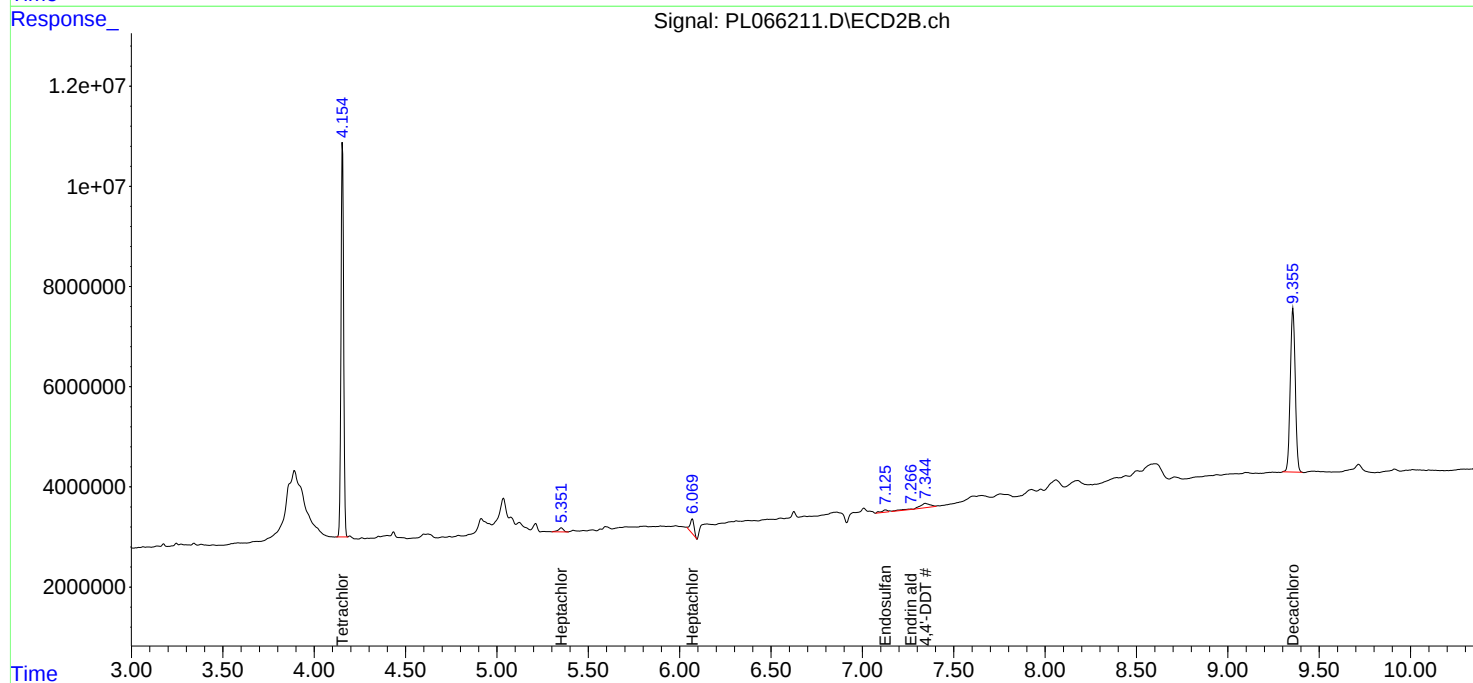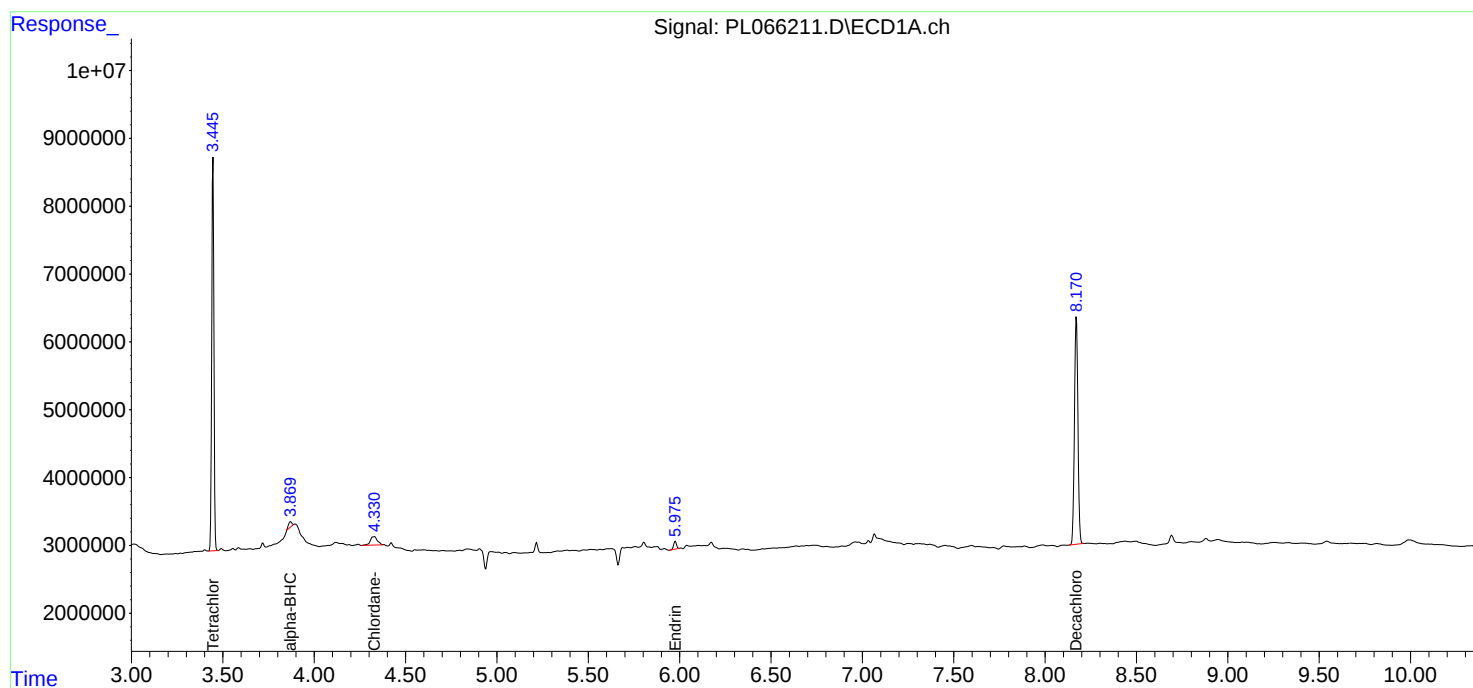


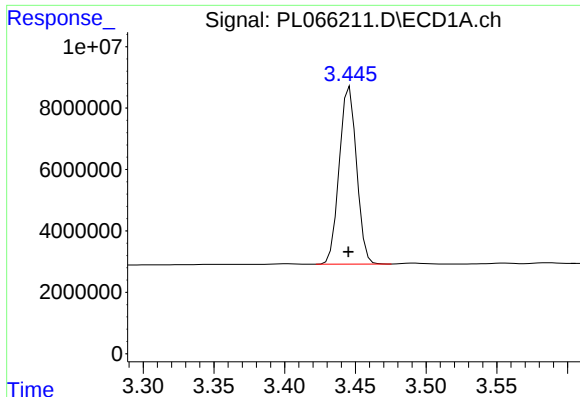

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: 0.001 min
Response: 49248830
Conc: 19.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

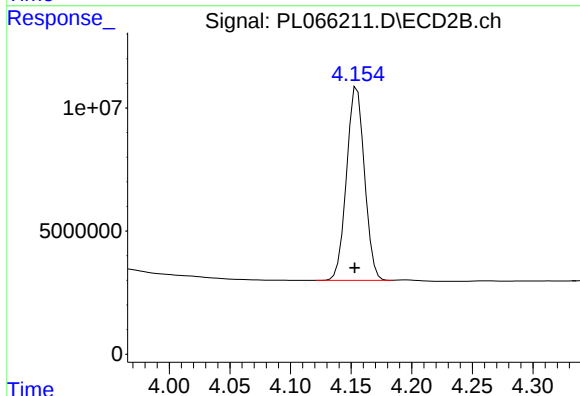


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 80721270
Conc: 20.07 ng/ml

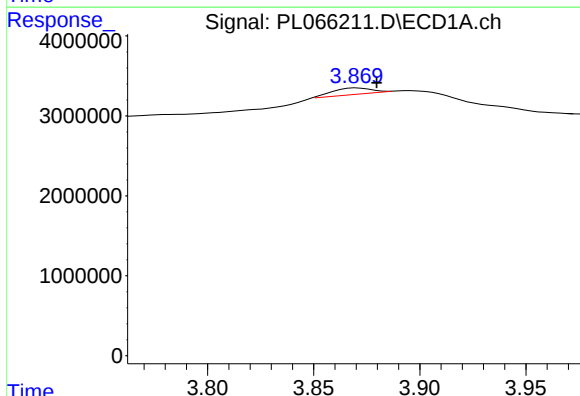


#2 alpha-BHC

R.T.: 3.871 min
Delta R.T.: -0.009 min
Response: 1005423
Conc: 0.24 ng/ml

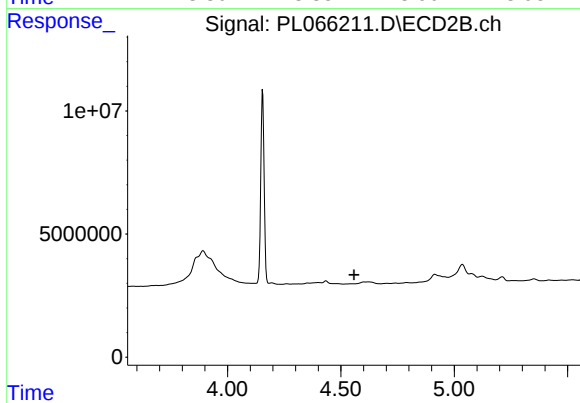

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.558 min
Response: 0
Conc: N.D.

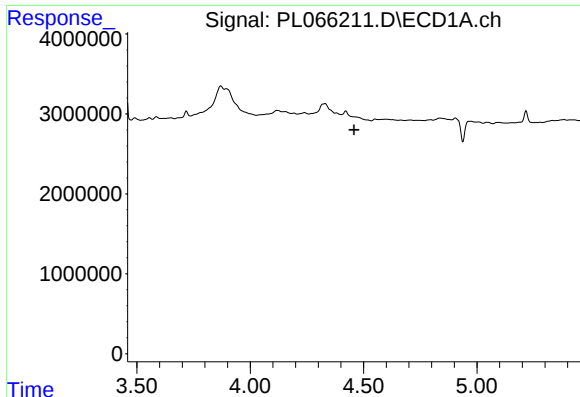

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

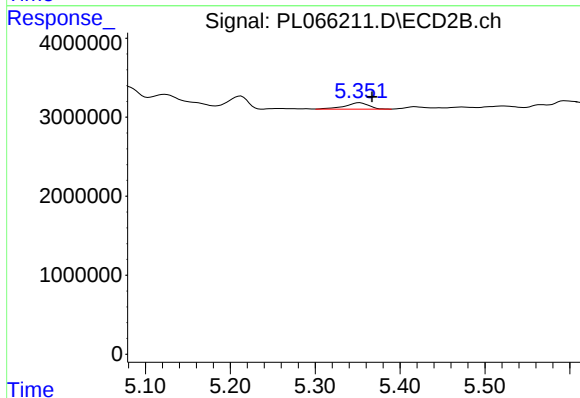


#4 Heptachlor

R.T.: 5.352 min
Delta R.T.: -0.015 min
Response: 1593604
Conc: 0.29 ng/ml

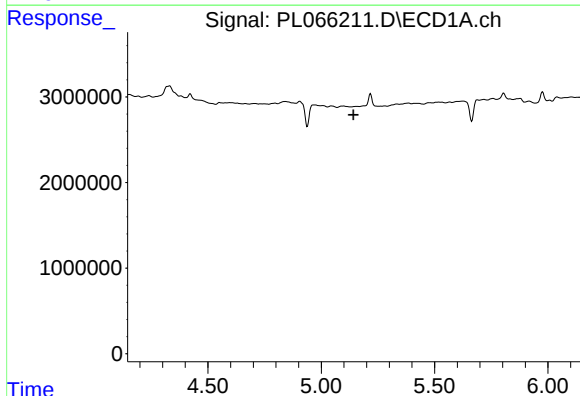


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.143 min
Response: 0
Conc: N.D.

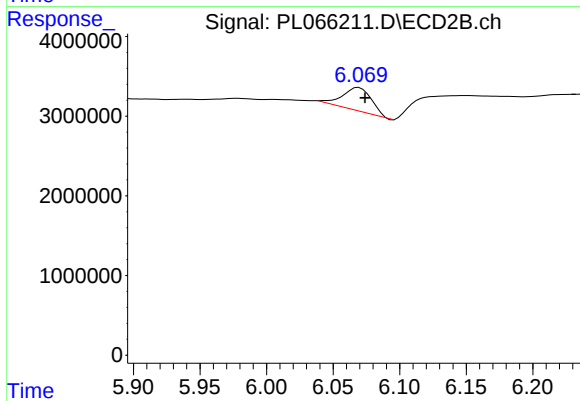

#8 Heptachlor epoxide


R.T.: 6.069 min
Delta R.T.: -0.005 min
Response: 4450666
Conc: 0.96 ng/ml

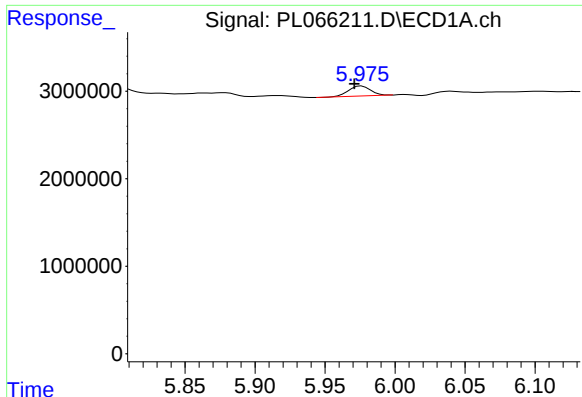

#14 Endrin


R.T.: 5.976 min
Delta R.T.: 0.005 min
Response: 1248700
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

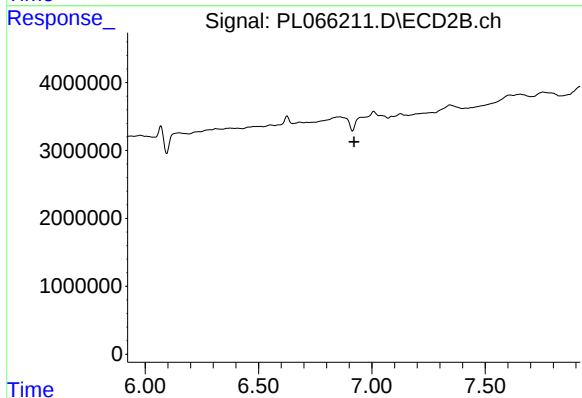


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

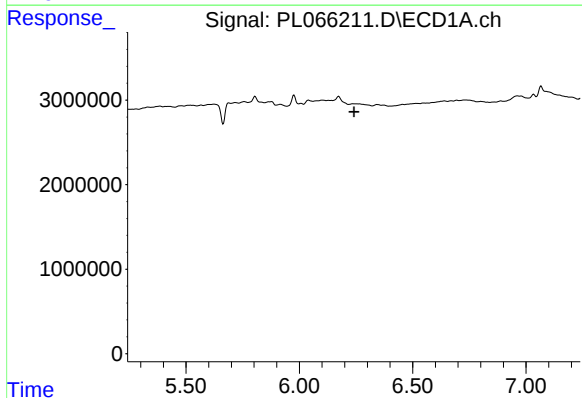


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

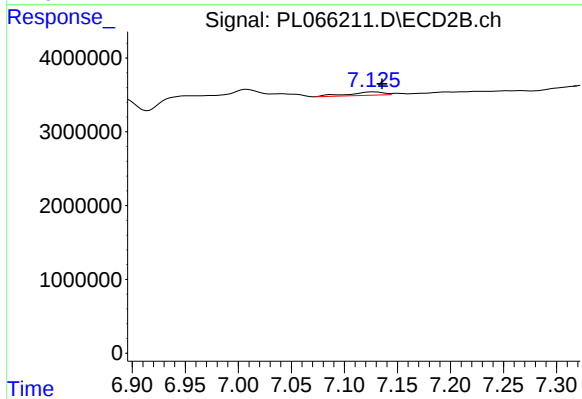

#15 Endosulfan II


R.T.: 7.127 min
Delta R.T.: -0.009 min
Response: 1042102
Conc: 0.30 ng/ml

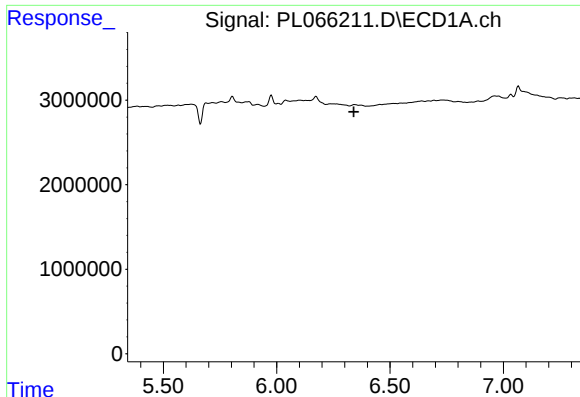

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

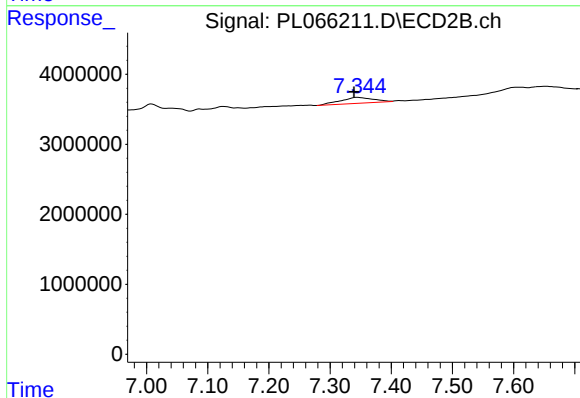


#17 4,4'-DDT

R.T.: 7.345 min
Delta R.T.: 0.006 min
Response: 3133648
Conc: 0.92 ng/ml

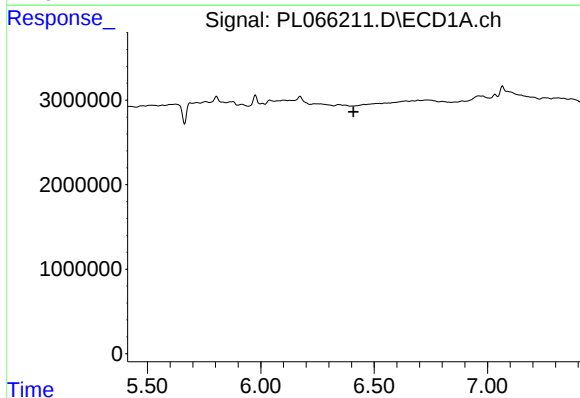


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

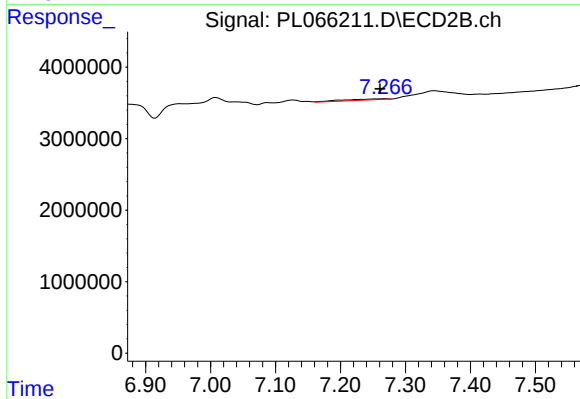

#18 Endrin aldehyde


R.T.: 7.267 min
Delta R.T.: 0.006 min
Response: 757131
Conc: 0.27 ng/ml

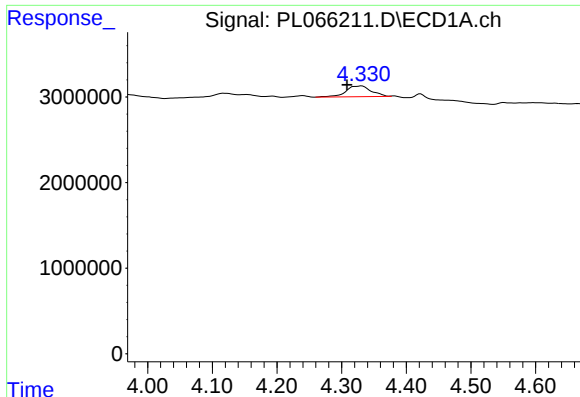

#23 Chlordane-1


R.T.: 4.331 min
Delta R.T.: 0.023 min
Response: 3428104
Conc: 29.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

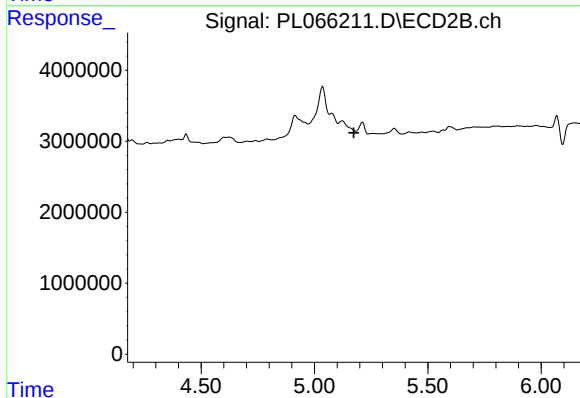


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.173 min
Response: 0
Conc: N.D.

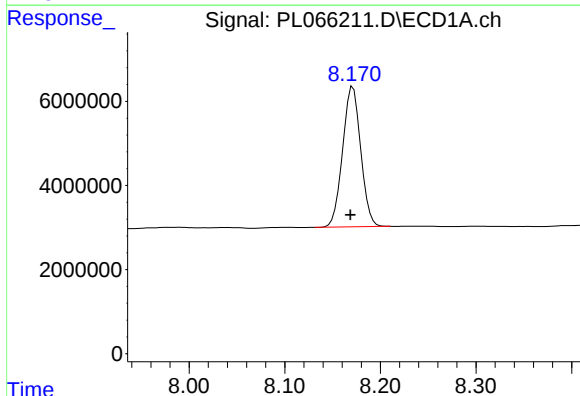

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.003 min
Response: 44027700
Conc: 18.46 ng/ml

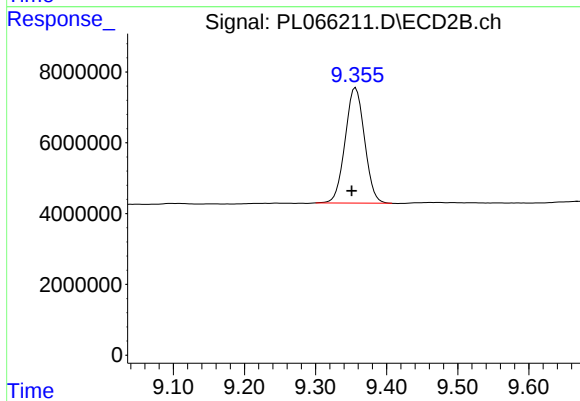

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.006 min
Response: 61780121
Conc: 18.92 ng/ml