

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
 Data File : PL066161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2021 10:58
 Operator : AR\AJ
 Sample : M2025-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-3

Manual Integrations
 APPROVED

Ankita
 4/16/2021 2:45:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 12:45:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.446	4.155	32637020	50194530	12.823	12.478
28) SA Decachlor...	8.171	9.355	26567984	38640952	11.138	11.832
Target Compounds						
11) B alpha-Chl...	5.425	6.386	2171328	3615795	0.586m	0.800 #
12) B 4,4'-DDE	5.592	6.542	8173419	7488005	2.191	1.809

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
Data File : PL066161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2021 10:58
Operator : AR\AJ
Sample : M2025-09
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-3


Manual Integrations
APPROVED

Ankita
4/16/2021 2:45:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 12:45:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

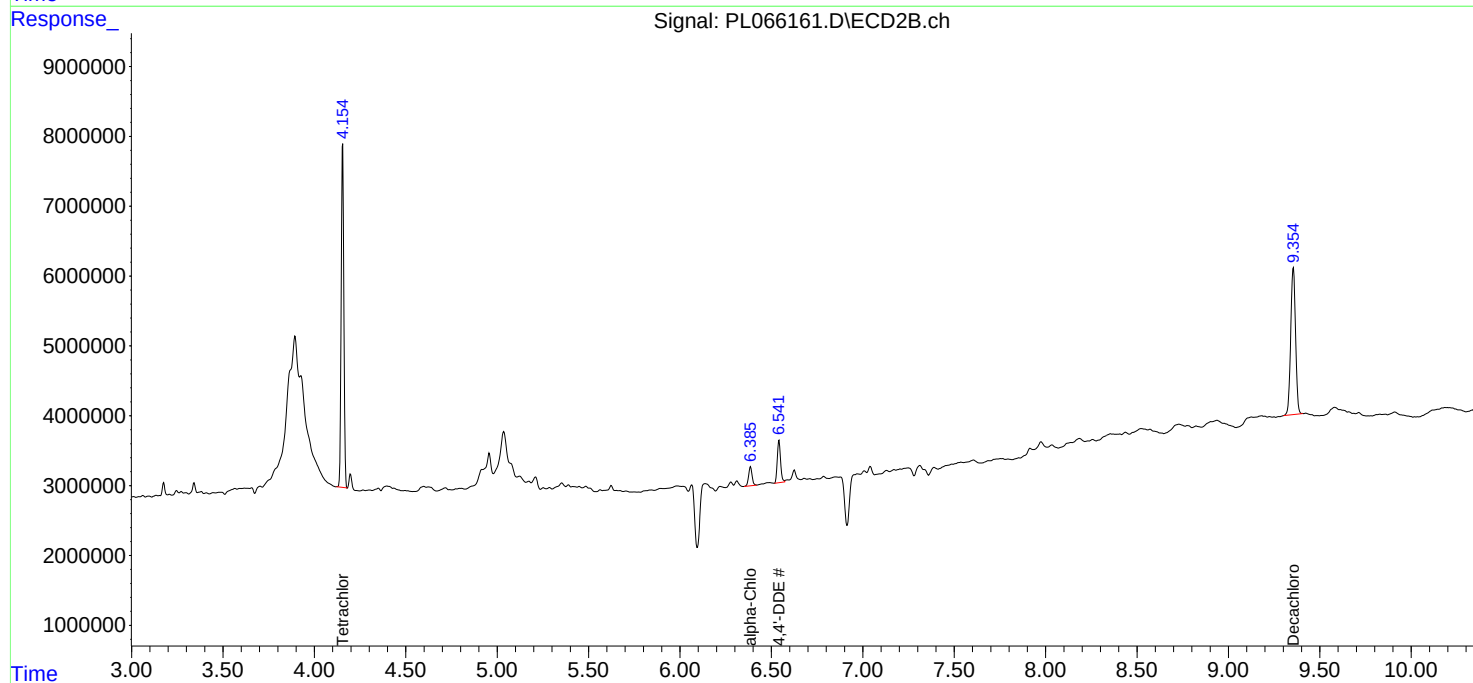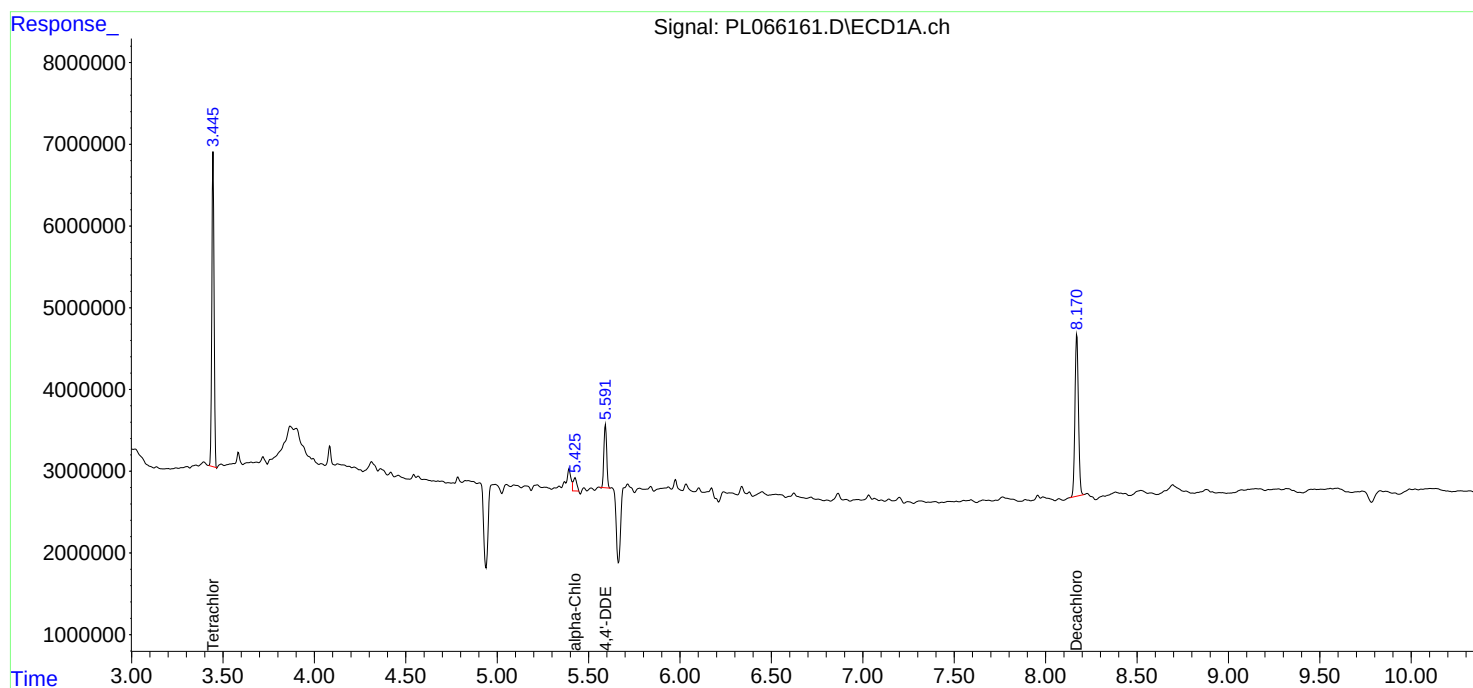

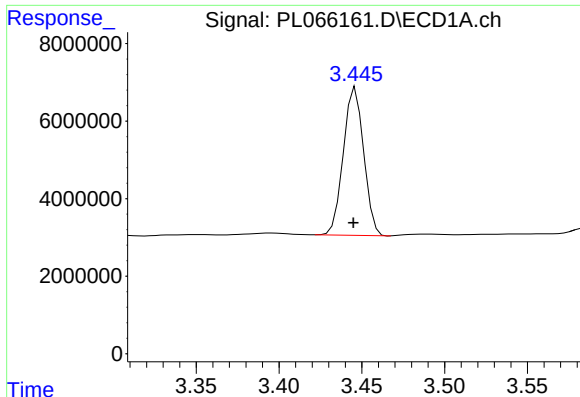


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.001 min
Response: 32637020
Conc: 12.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-3


Manual Integrations
APPROVED

Ankita
4/16/2021 2:45:42 PM

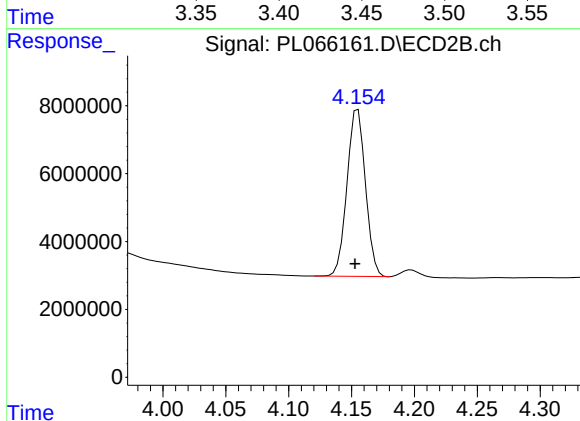


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 50194530
Conc: 12.48 ng/ml

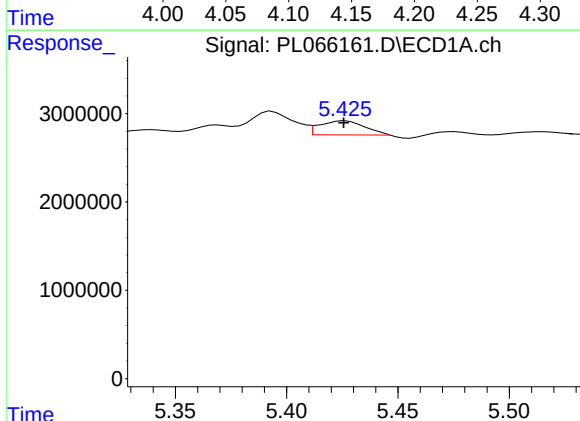


#11 alpha-Chlordane

R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 2171328
Conc: 0.59 ng/ml m

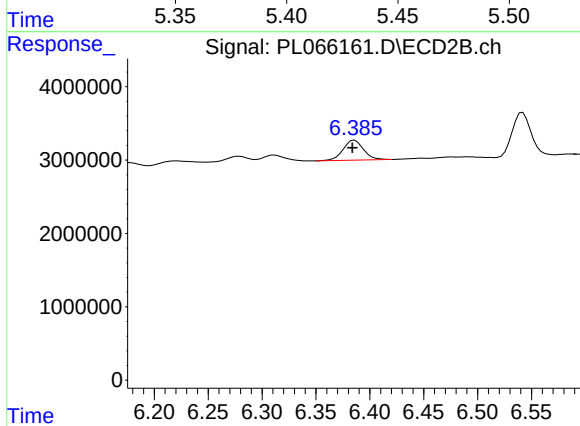

#11 alpha-Chlordane

R.T.: 6.386 min
Delta R.T.: 0.002 min
Response: 3615795
Conc: 0.80 ng/ml

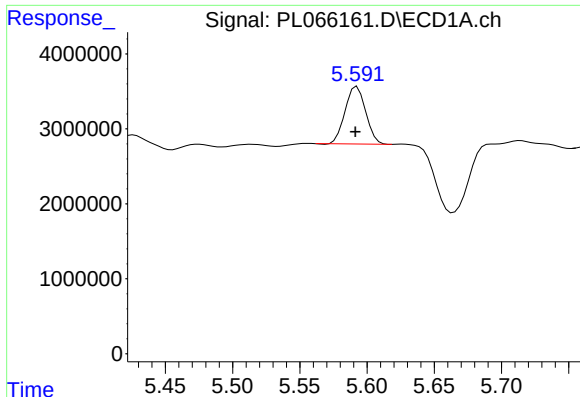


#12 4,4'-DDE

R.T.: 5.592 min
Delta R.T.: 0.001 min
Response: 8173419
Conc: 2.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-3


Manual Integrations
APPROVED

Ankita
4/16/2021 2:45:42 PM

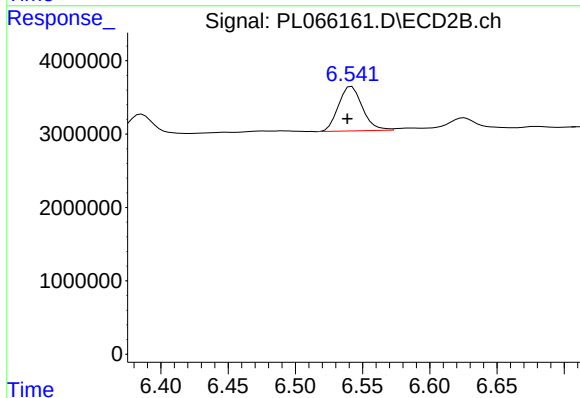


#12 4,4'-DDE

R.T.: 6.542 min
Delta R.T.: 0.003 min
Response: 7488005
Conc: 1.81 ng/ml

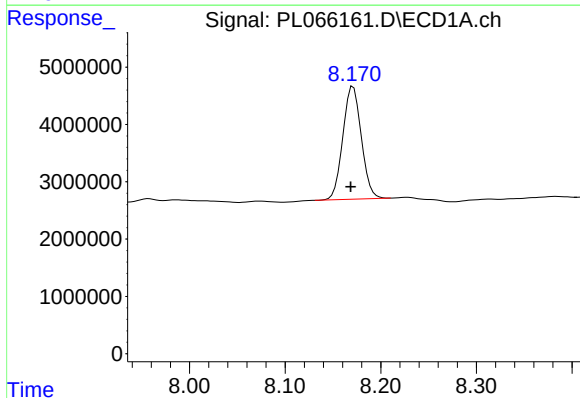

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.003 min
Response: 26567984
Conc: 11.14 ng/ml

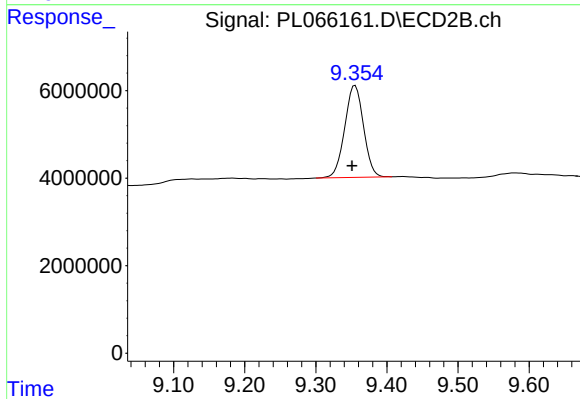

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.005 min
Response: 38640952
Conc: 11.83 ng/ml