

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
 Data File : PL066162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2021 11:12
 Operator : AR\AJ
 Sample : M2025-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 130-SB-1

Manual Integrations
 APPROVED

Ankita
 4/16/2021 2:45:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 12:45:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.155	52565807	81391322	20.652	20.234
28)	SA Decachlor...	8.172	9.355	42047920	62745325	17.628	19.212
Target Compounds							
11)	B alpha-Chl...	5.426	6.385	1698508	3667171	0.459m	0.811 #
12)	B 4,4'-DDE	5.592	6.540	3879693	4814561	1.040m	1.163

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
Data File : PL066162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2021 11:12
Operator : AR\AJ
Sample : M2025-11
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
130-SB-1


Manual Integrations
APPROVED

Ankita
4/16/2021 2:45:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 12:45:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

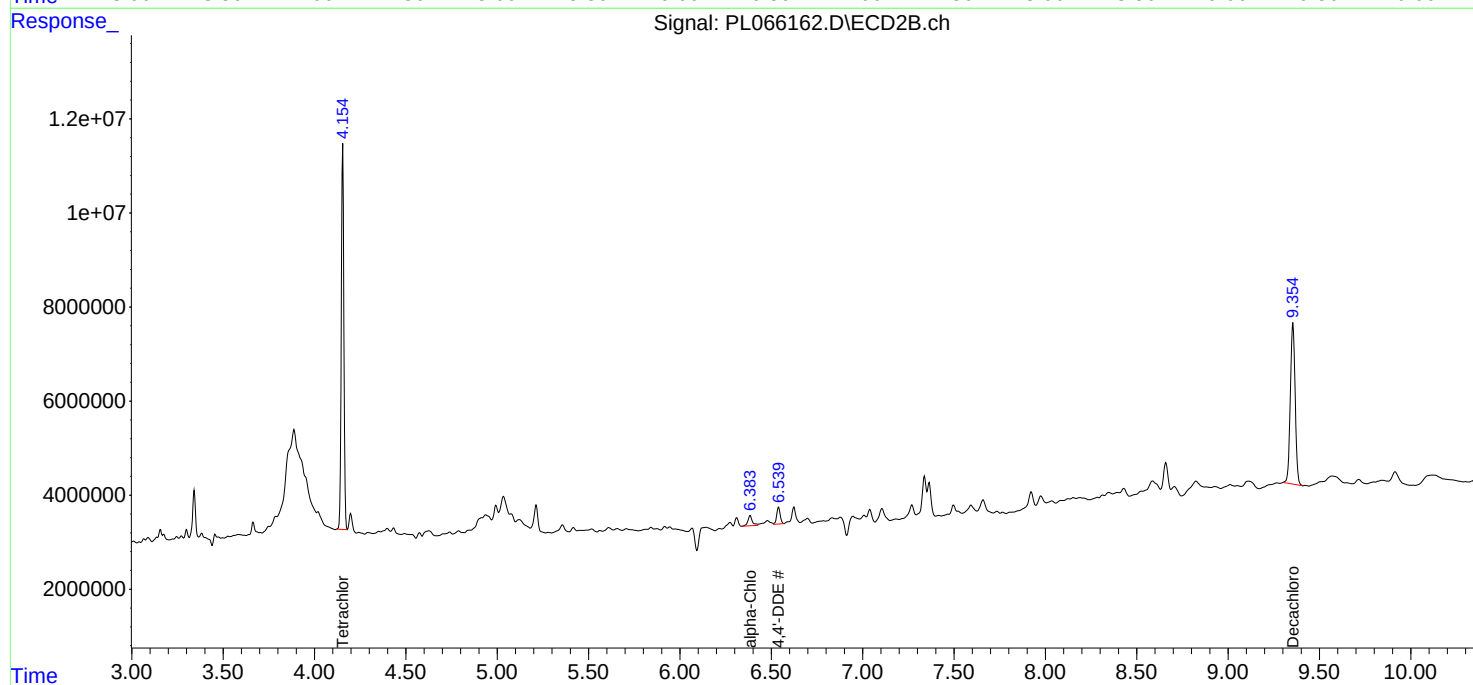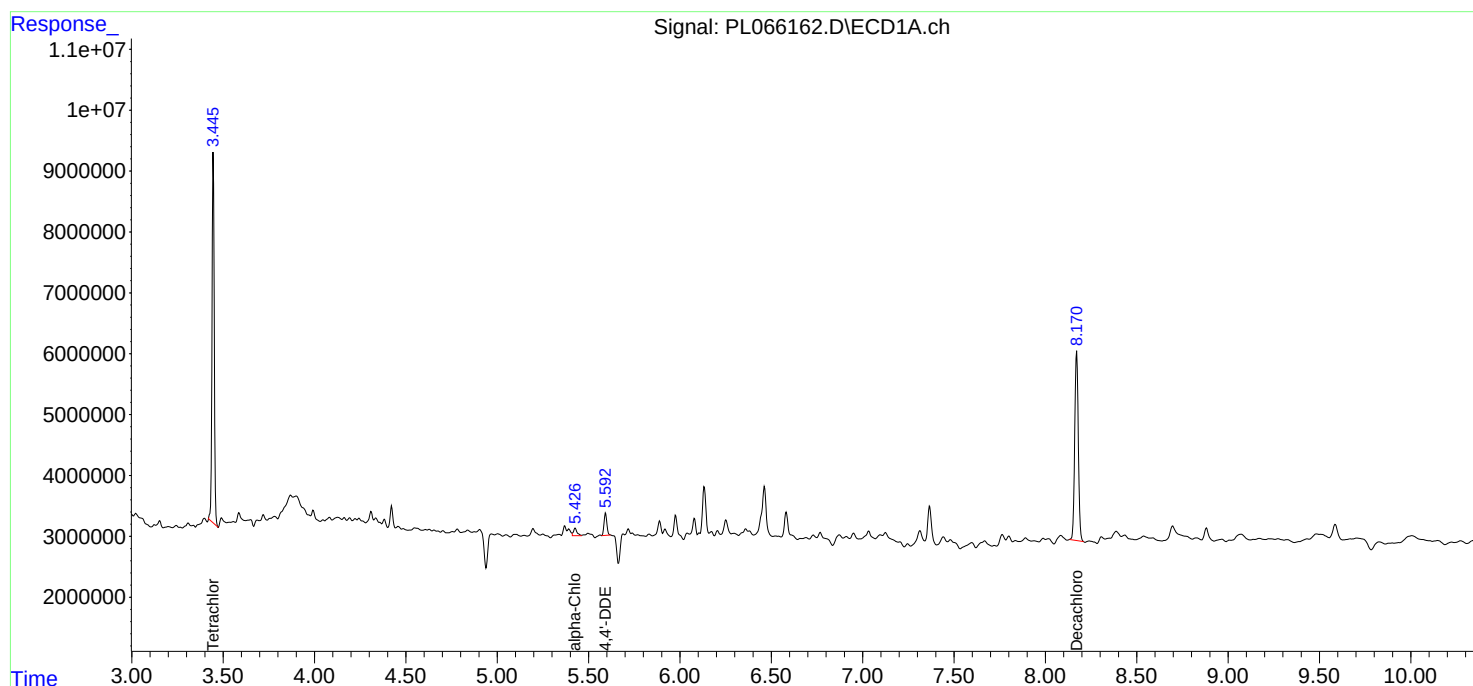

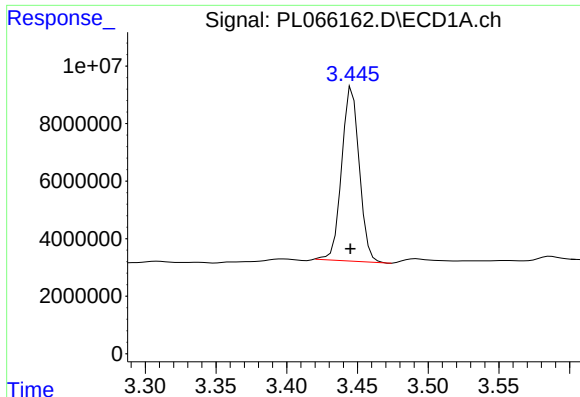


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.001 min
Response: 52565807
Conc: 20.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
130-SB-1


Manual Integrations
APPROVED

Ankita
4/16/2021 2:45:44 PM

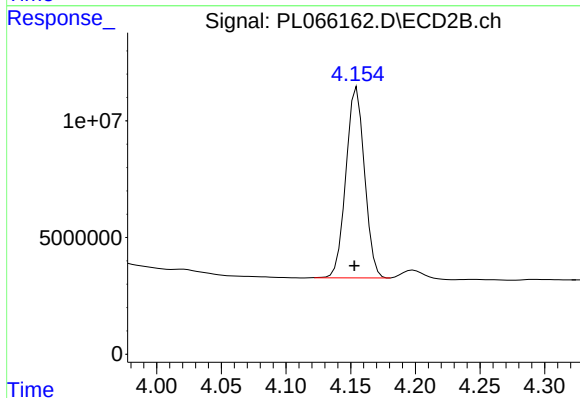


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 81391322
Conc: 20.23 ng/ml

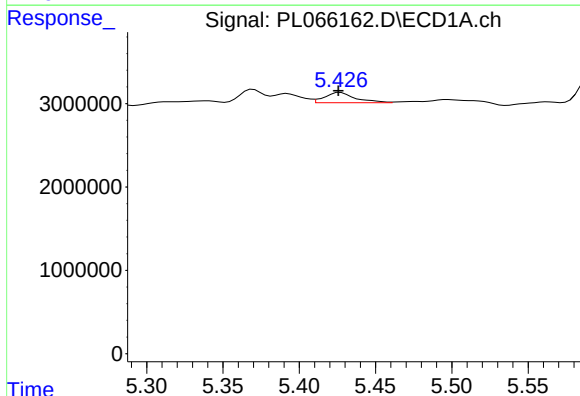


#11 alpha-Chlordane

R.T.: 5.426 min
Delta R.T.: 0.000 min
Response: 1698508
Conc: 0.46 ng/ml m

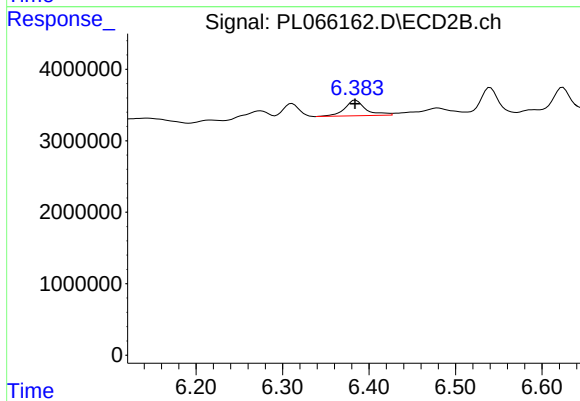

#11 alpha-Chlordane

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 3667171
Conc: 0.81 ng/ml

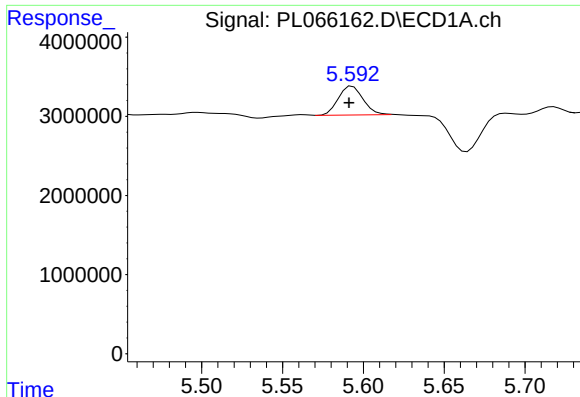


#12 4,4'-DDE

R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 3879693
Conc: 1.04 ng/ml m

Instrument :
ECD_L
ClientSampleId :
130-SB-1


Manual Integrations
APPROVED

Ankita
4/16/2021 2:45:44 PM

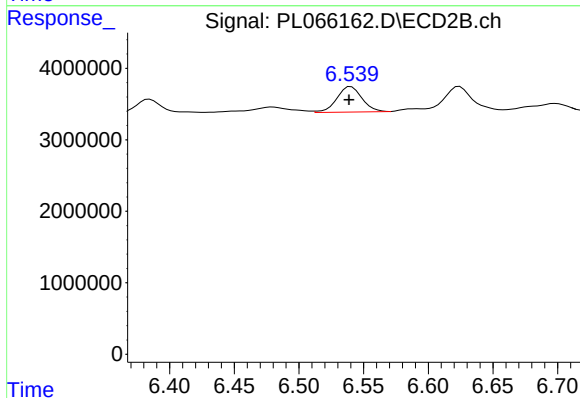


#12 4,4'-DDE

R.T.: 6.540 min
Delta R.T.: 0.001 min
Response: 4814561
Conc: 1.16 ng/ml

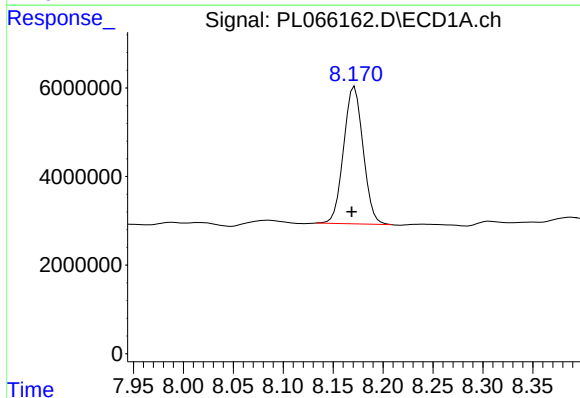

#28 Decachlorobiphenyl

R.T.: 8.172 min
Delta R.T.: 0.003 min
Response: 42047920
Conc: 17.63 ng/ml

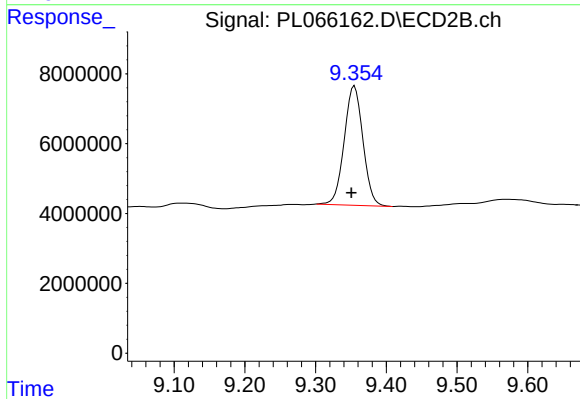

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.004 min
Response: 62745325
Conc: 19.21 ng/ml