

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
 Data File : PL066180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2021 17:00
 Operator : AR\AJ
 Sample : M2048-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-02-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/16/2021 2:45:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:33:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.155	32478821	51816232	12.760	12.881
28)	SA Decachlor...	8.174	9.357	41960572	57453466	17.592	17.592
Target Compounds							
12)	B 4,4'-DDE	5.595	6.540	18231433	18013767	4.888	4.352
17)	MA 4,4'-DDT	6.341	7.341	10349491	4469898	3.247m	1.318m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
Data File : PL066180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2021 17:00
Operator : AR\AJ
Sample : M2048-04
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:45:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:33:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

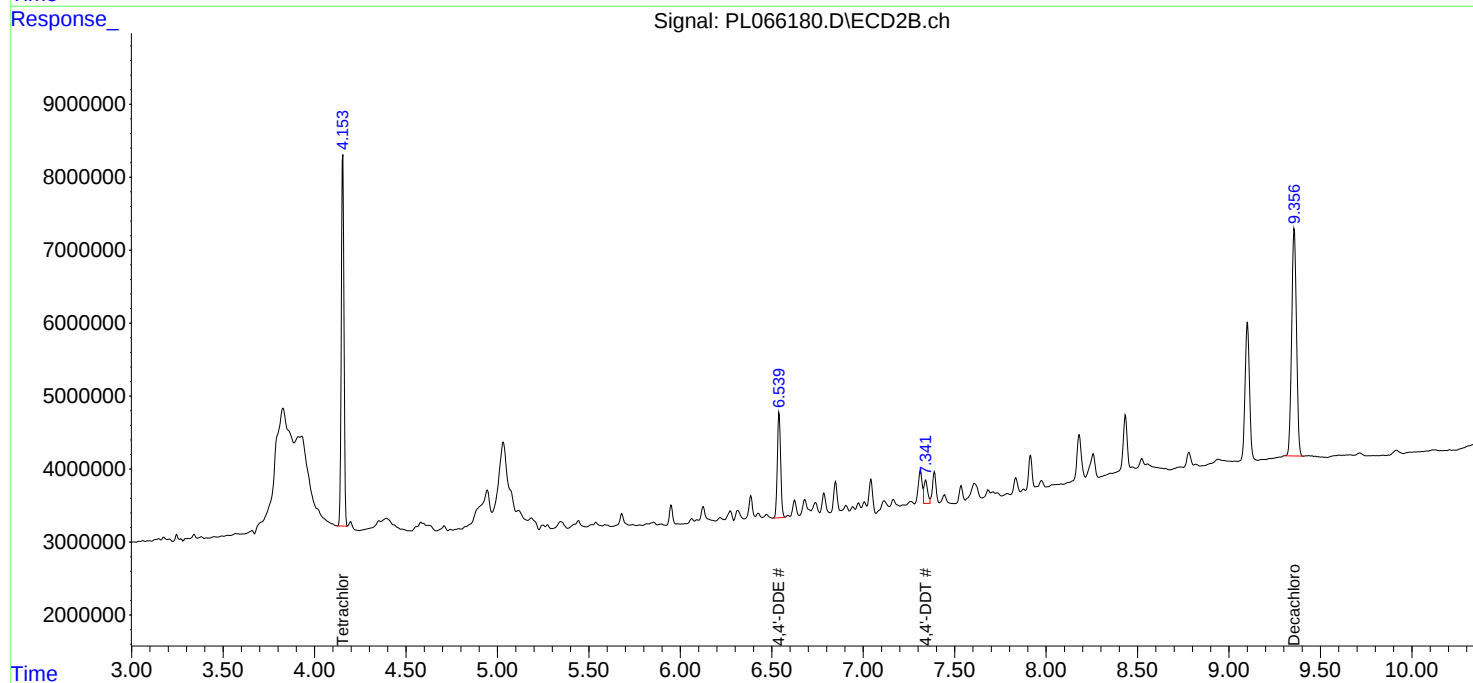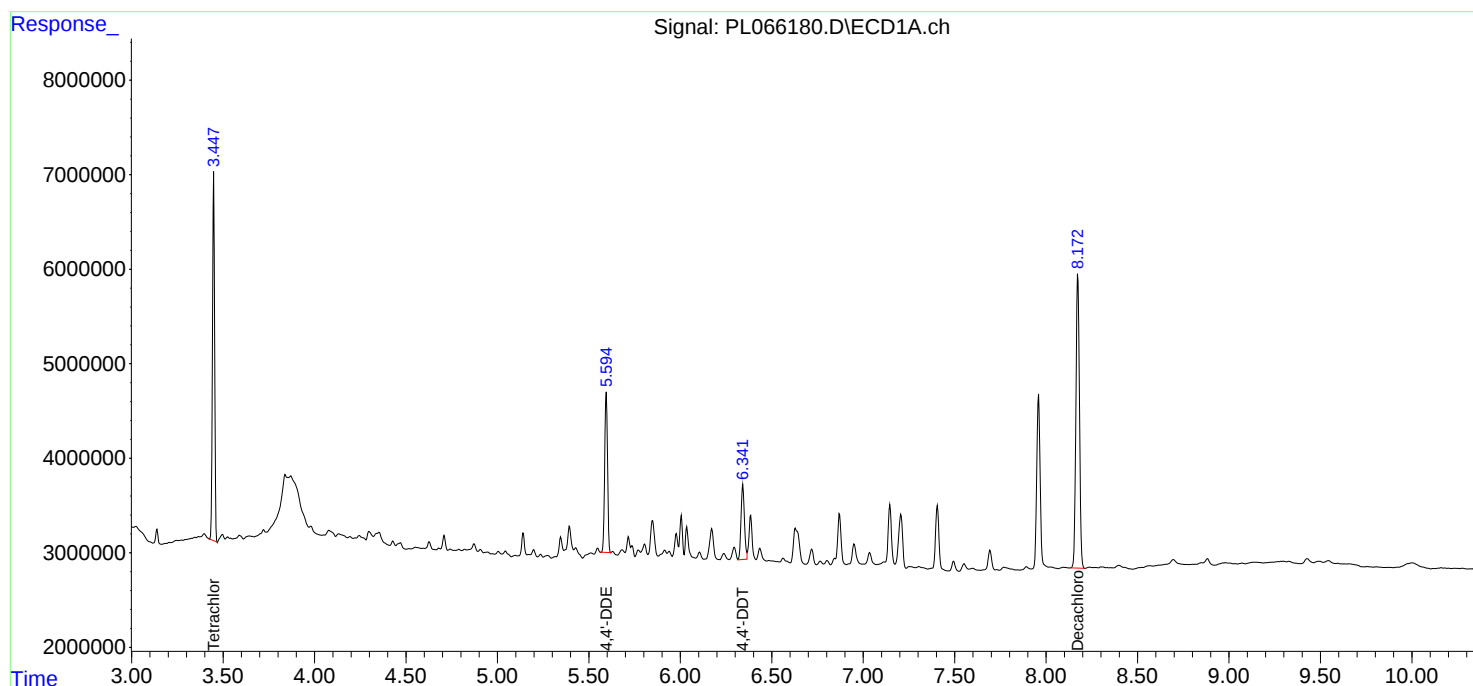

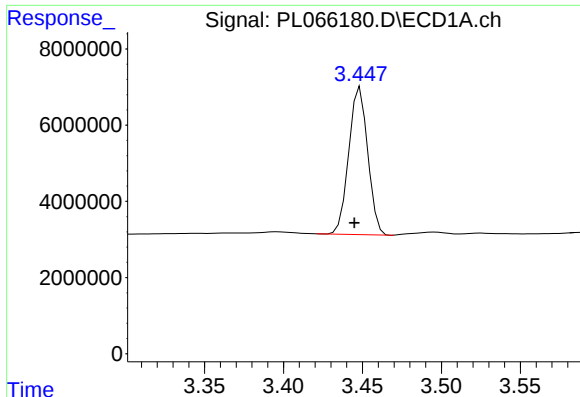


#1 Tetrachloro-m-xylene

R.T.: 3.449 min
Delta R.T.: 0.004 min
Response: 32478821
Conc: 12.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:45:58 PM

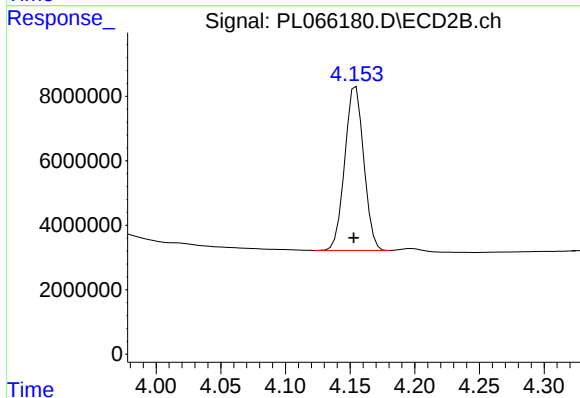


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 51816232
Conc: 12.88 ng/ml

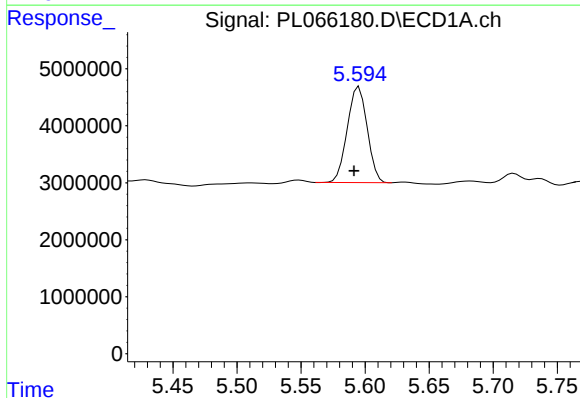


#12 4,4'-DDE

R.T.: 5.595 min
Delta R.T.: 0.004 min
Response: 18231433
Conc: 4.89 ng/ml

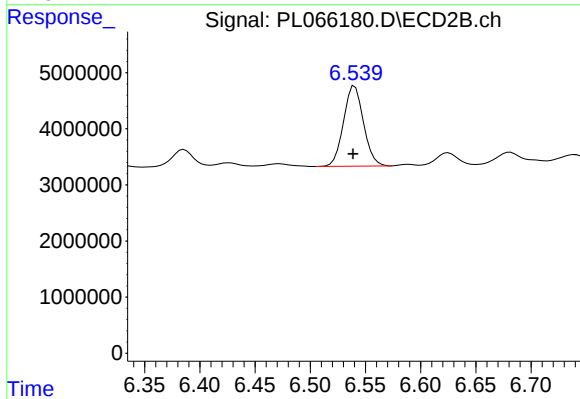

#12 4,4'-DDE

R.T.: 6.540 min
Delta R.T.: 0.002 min
Response: 18013767
Conc: 4.35 ng/ml

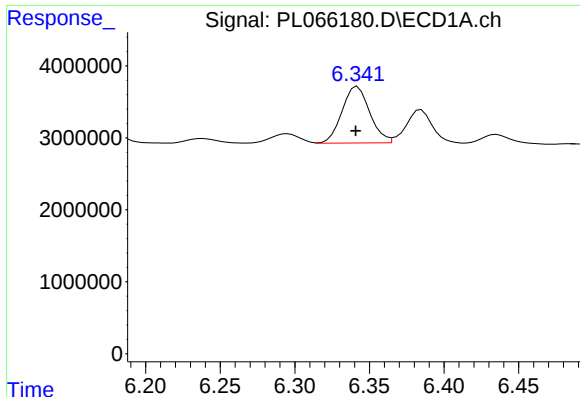


#17 4,4'-DDT

R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 10349491
Conc: 3.25 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:45:58 PM

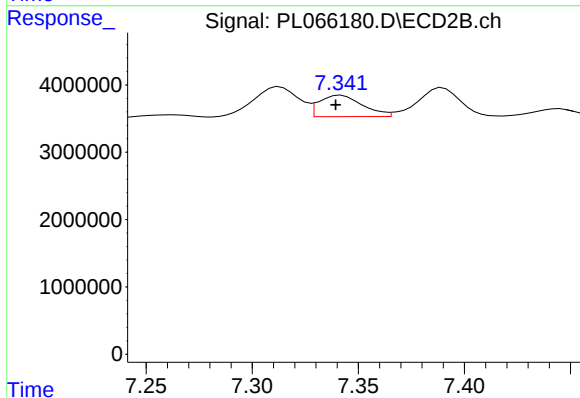


#17 4,4'-DDT

R.T.: 7.341 min
Delta R.T.: 0.001 min
Response: 4469898
Conc: 1.32 ng/ml m

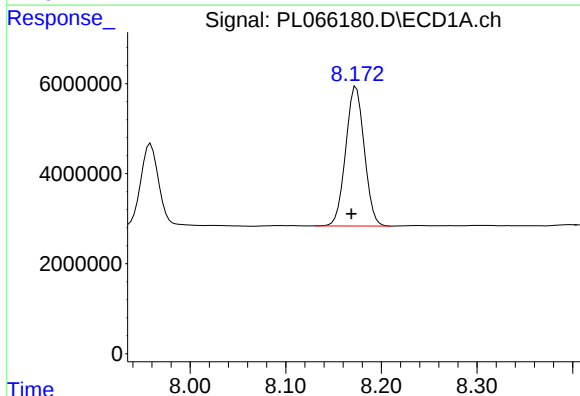

#28 Decachlorobiphenyl

R.T.: 8.174 min
Delta R.T.: 0.005 min
Response: 41960572
Conc: 17.59 ng/ml

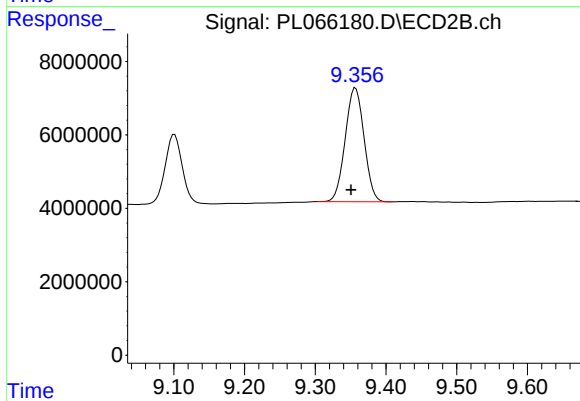

#28 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: 0.006 min
Response: 57453466
Conc: 17.59 ng/ml