

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
 Data File : PL066208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 00:11
 Operator : AR\AJ
 Sample : M2049-08
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-09-5.5-6.0

Manual Integrations
 APPROVED

Ankita
 4/16/2021 2:46:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:43:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.446	4.155	45866932	74797548	18.020	18.594
28) SA Decachlor...	8.172	9.356	40614043	54750368	17.027	16.764
Target Compounds						
12) B 4,4'-DDE	5.591	6.541	3306192	3502802	0.886m	0.846

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
Data File : PL066208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 00:11
Operator : AR\AJ
Sample : M2049-08
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-09-5.5-6.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:43:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

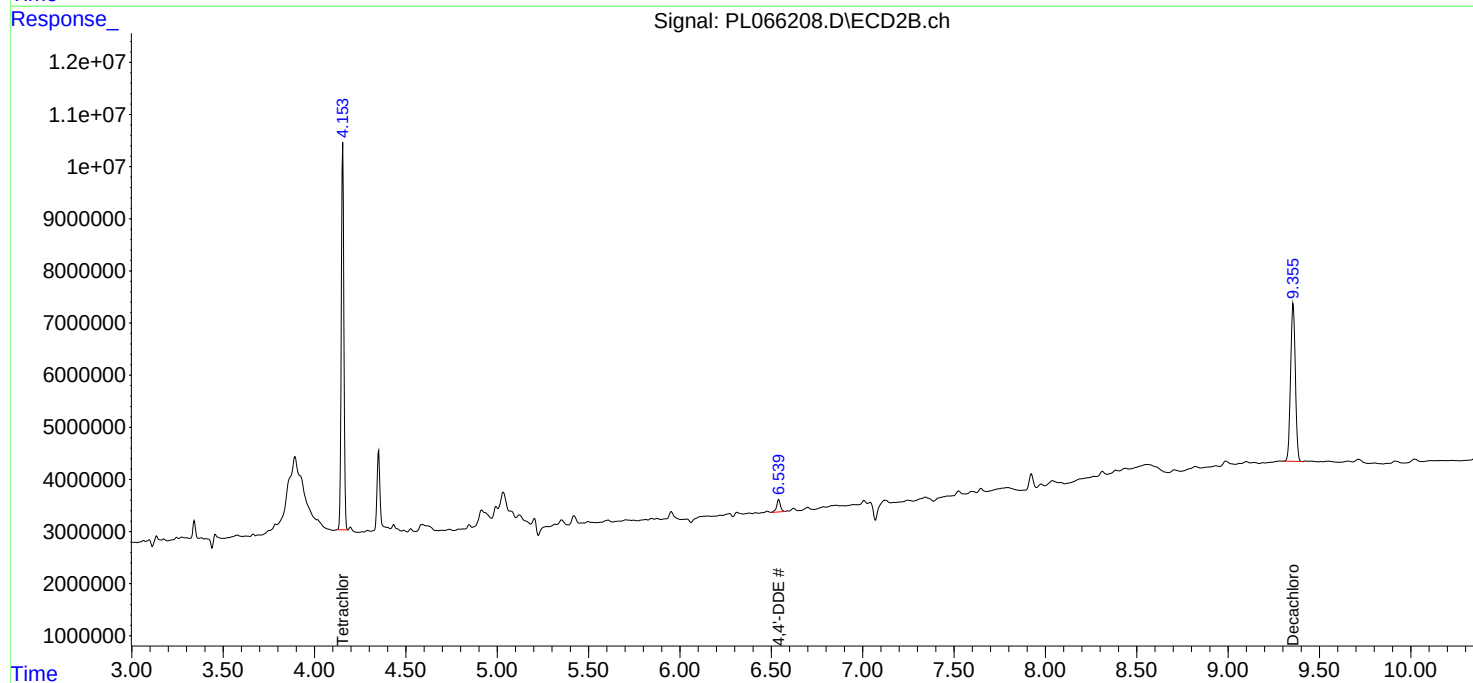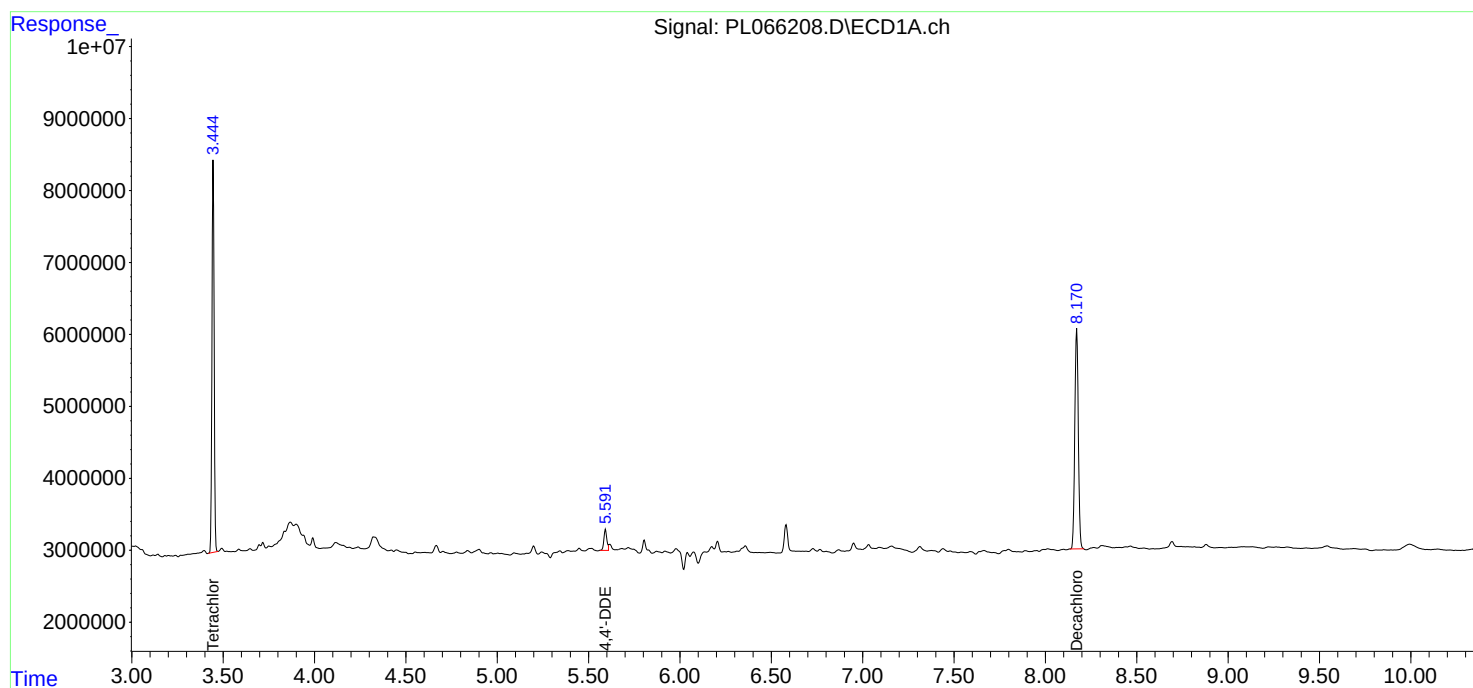

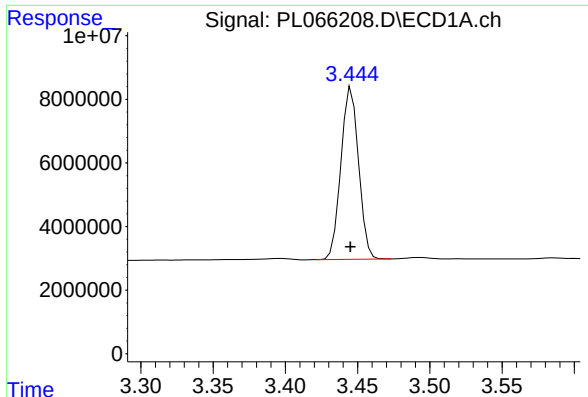


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.000 min
Response: 45866932
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-09-5.5-6.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:13 PM

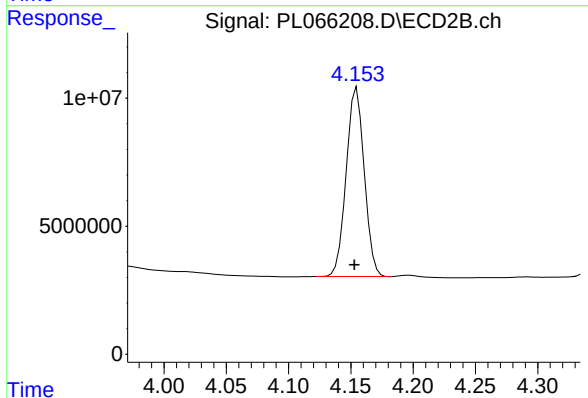


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 74797548
Conc: 18.59 ng/ml

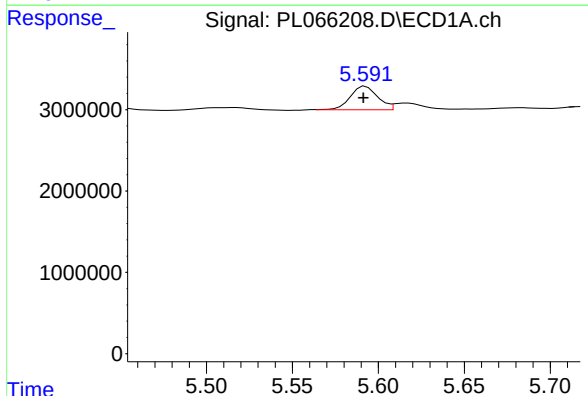


#12 4,4'-DDE

R.T.: 5.591 min
Delta R.T.: 0.000 min
Response: 3306192
Conc: 0.89 ng/ml m

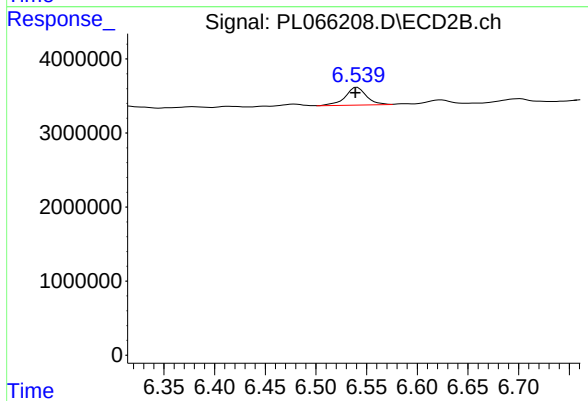

#12 4,4'-DDE

R.T.: 6.541 min
Delta R.T.: 0.002 min
Response: 3502802
Conc: 0.85 ng/ml

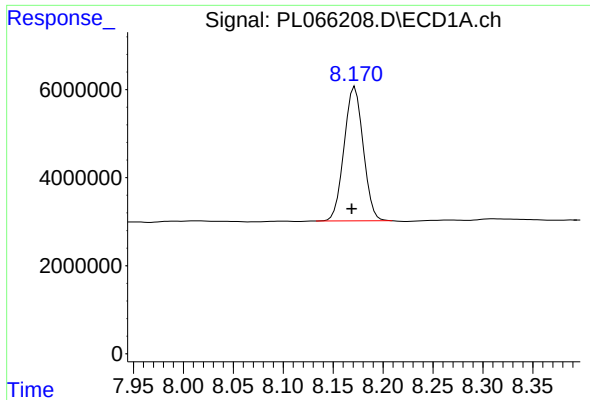


#28 Decachlorobiphenyl

R.T.: 8.172 min
Delta R.T.: 0.003 min
Response: 40614043
Conc: 17.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-09-5.5-6.0

Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:13 PM

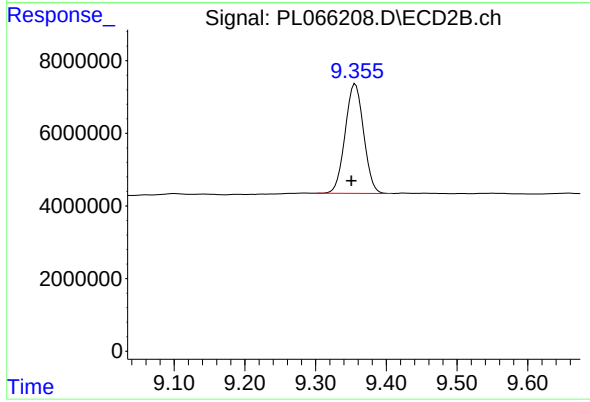

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.005 min
Response: 54750368
Conc: 16.76 ng/ml