

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
 Data File : PL066209.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 00:25
 Operator : AR\AJ
 Sample : M2049-10
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-10-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/16/2021 2:46:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:43:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.155	50861417	83998959	19.983	20.882
28)	SA Decachlor...	8.171	9.356	45102654	65163223	18.909	19.953
Target Compounds							
12)	B 4,4'-DDE	5.593	6.539	10177488	9542590	2.728	2.305m
17)	MA 4,4'-DDT	6.340	7.340	7927899	7169549	2.487m	2.113m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
Data File : PL066209.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 00:25
Operator : AR\AJ
Sample : M2049-10
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-10-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:43:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

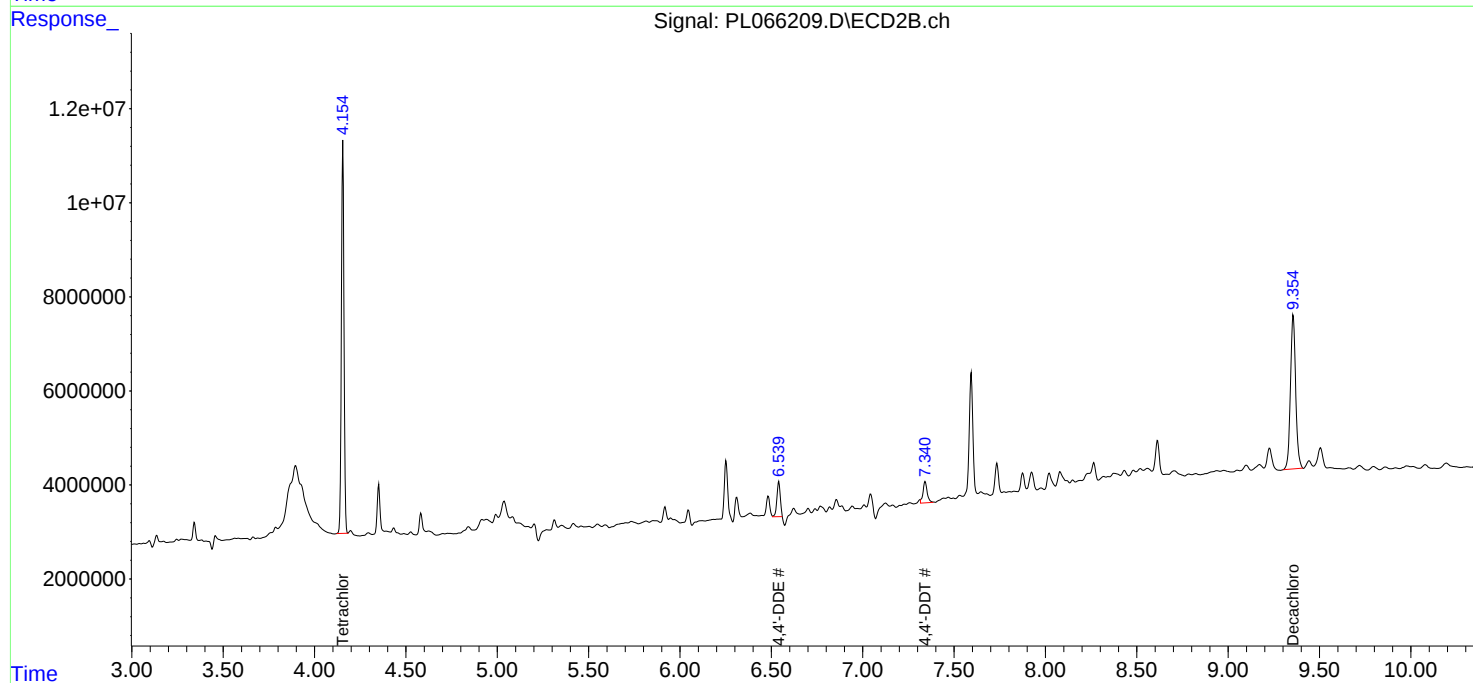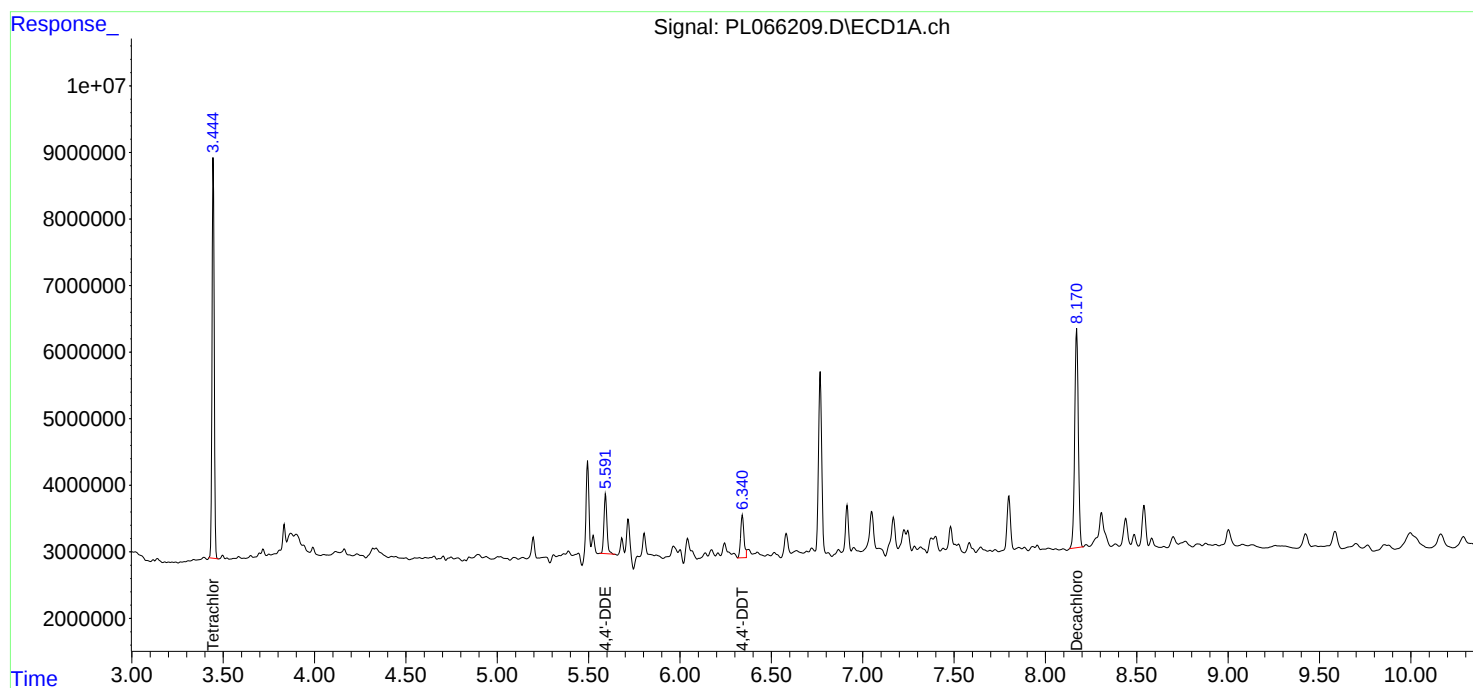

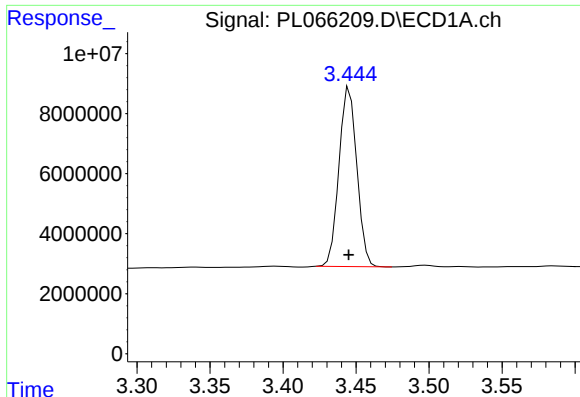


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.000 min
Response: 50861417
Conc: 19.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-10-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:15 PM

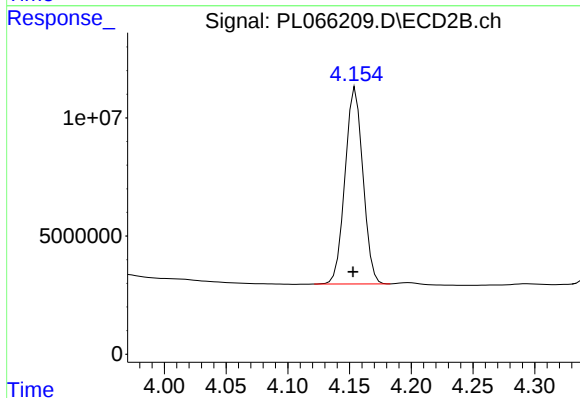


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 83998959
Conc: 20.88 ng/ml

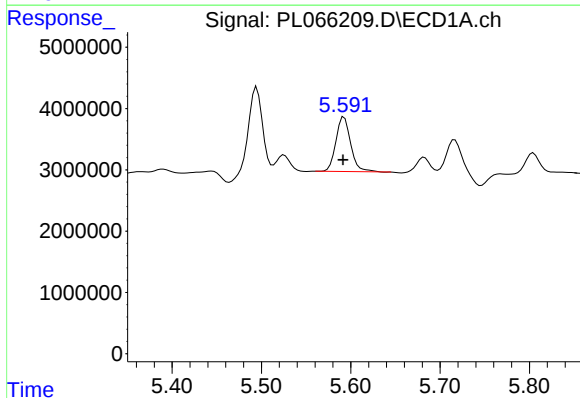


#12 4,4'-DDE

R.T.: 5.593 min
Delta R.T.: 0.001 min
Response: 10177488
Conc: 2.73 ng/ml

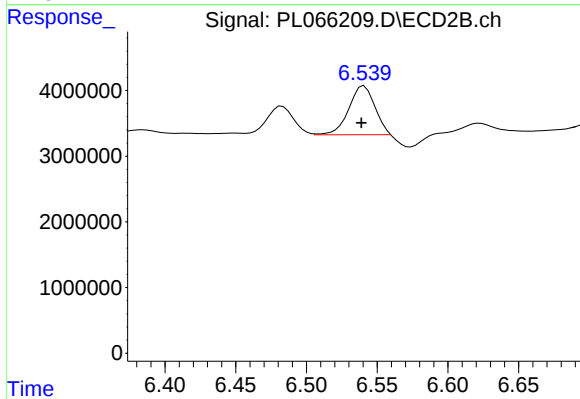

#12 4,4'-DDE

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 9542590
Conc: 2.31 ng/ml m

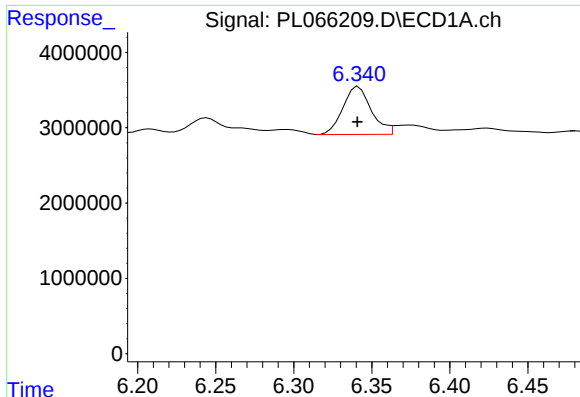


#17 4,4'-DDT

R.T.: 6.340 min
Delta R.T.: 0.000 min
Response: 7927899
Conc: 2.49 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-10-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:15 PM

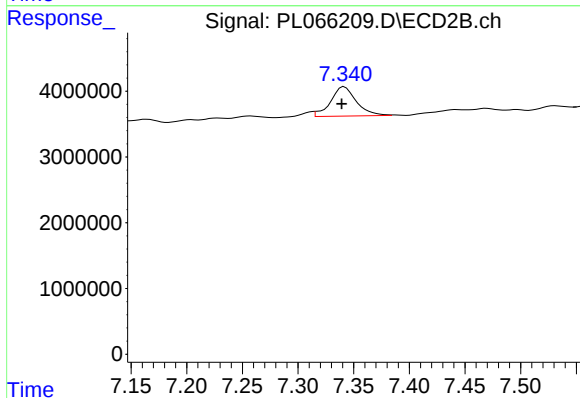


#17 4,4'-DDT

R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 7169549
Conc: 2.11 ng/ml m

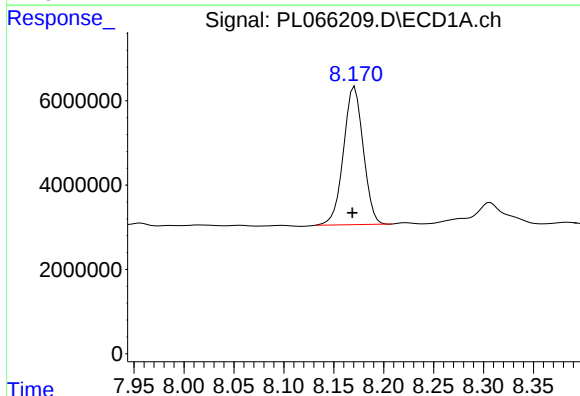

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.002 min
Response: 45102654
Conc: 18.91 ng/ml

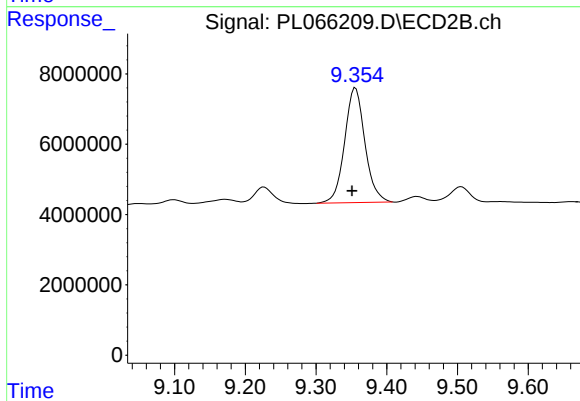

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.005 min
Response: 65163223
Conc: 19.95 ng/ml