

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
 Data File : PL066213.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 01:37
 Operator : AR\AJ
 Sample : M2049-13
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-11-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/16/2021 2:46:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 04:43:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.446	4.155	52151133	87375240	20.489	21.721
28) SA Decachlor...	8.172	9.356	49345809	68584173	20.688	21.000
Target Compounds						
12) B 4,4'-DDE	5.593	6.540	2560578	2956593	0.686	0.714m
13) MA Dieldrin	5.717	6.702	50401721	48441517	12.442m	11.594

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
Data File : PL066213.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 01:37
Operator : AR\AJ
Sample : M2049-13
Misc :
ALS Vial : 55 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-11-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 04:43:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

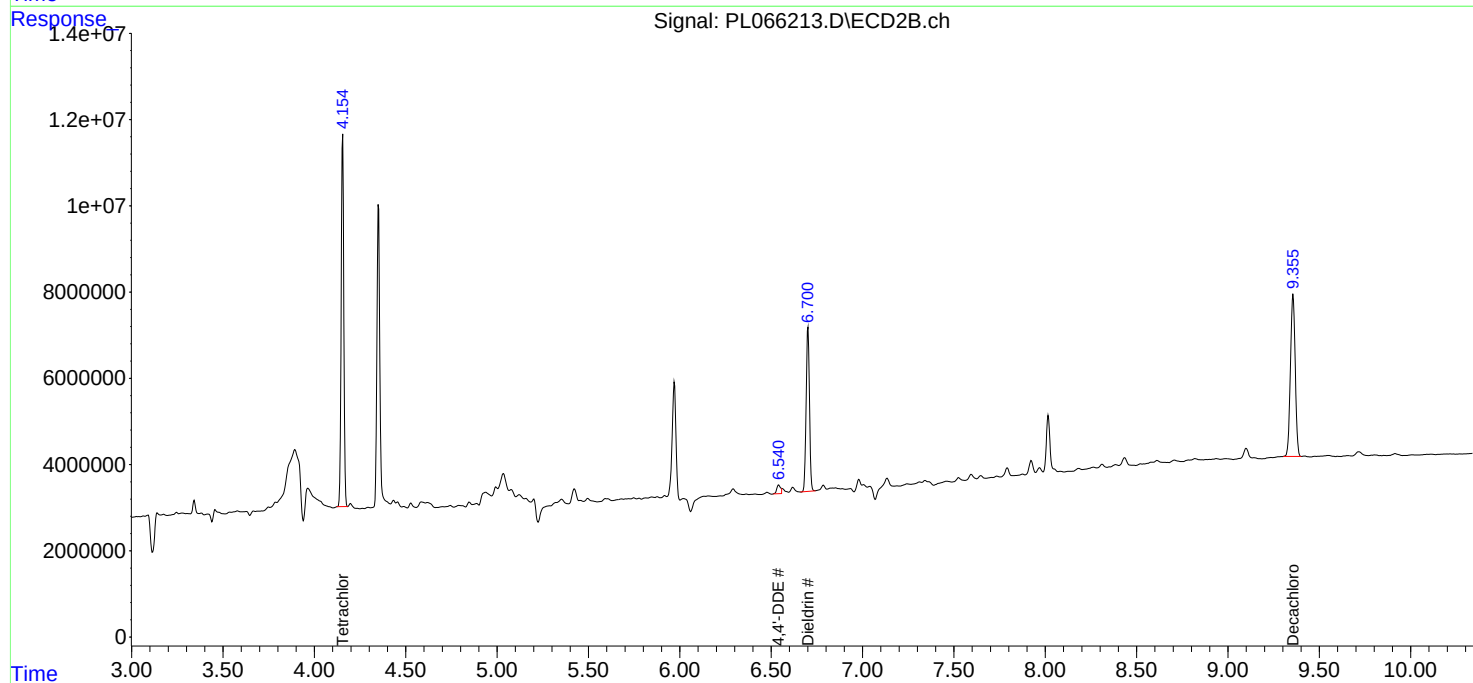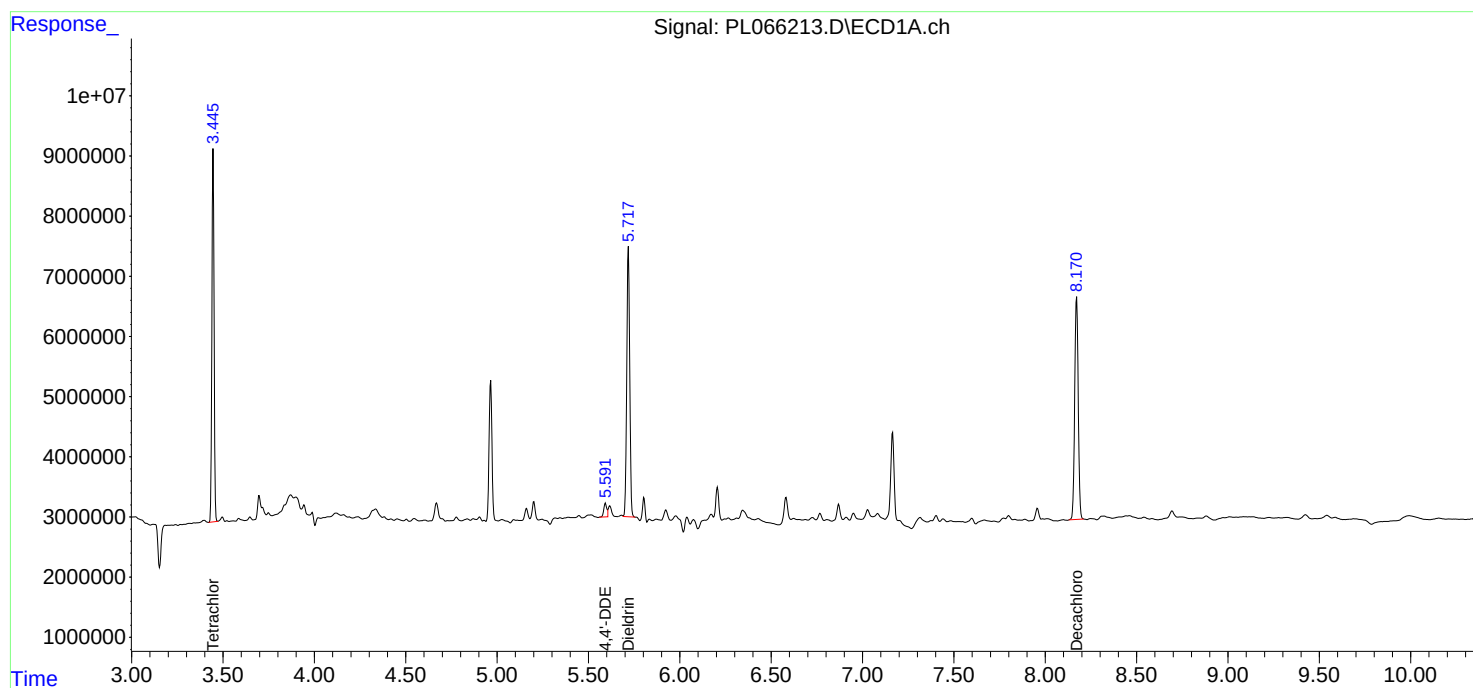

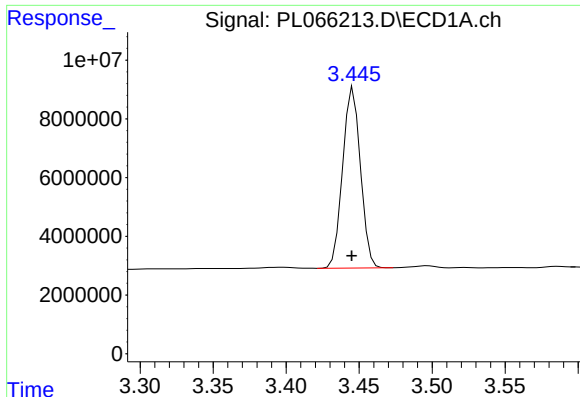


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.001 min
Response: 52151133
Conc: 20.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-11-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:18 PM

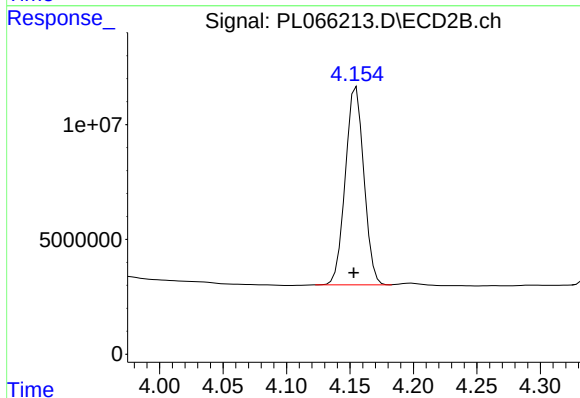


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 87375240
Conc: 21.72 ng/ml

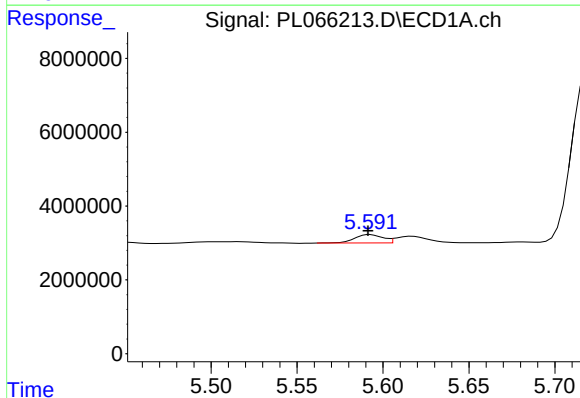


#12 4,4'-DDE

R.T.: 5.593 min
Delta R.T.: 0.001 min
Response: 2560578
Conc: 0.69 ng/ml

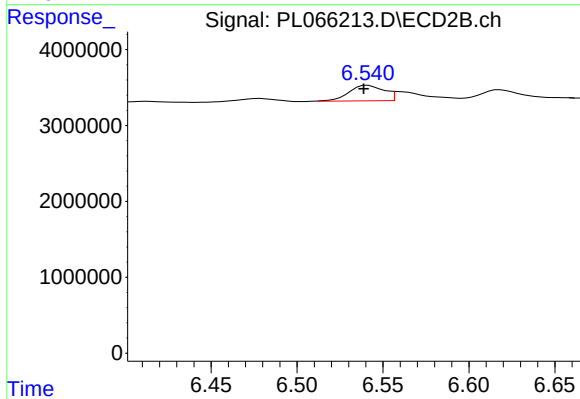

#12 4,4'-DDE

R.T.: 6.540 min
Delta R.T.: 0.000 min
Response: 2956593
Conc: 0.71 ng/ml m

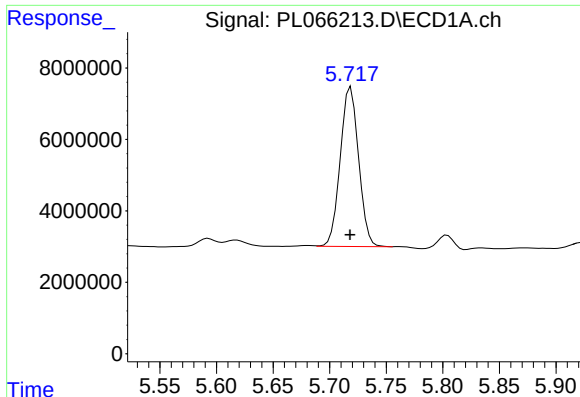


#13 Dieldrin

R.T.: 5.717 min
Delta R.T.: 0.000 min
Response: 50401721
Conc: 12.44 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-11-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:18 PM

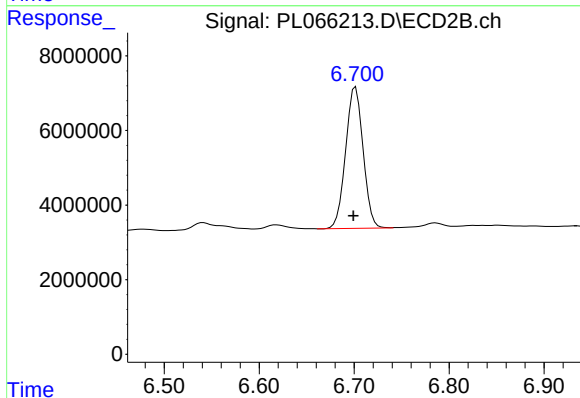


#13 Dieldrin

R.T.: 6.702 min
Delta R.T.: 0.002 min
Response: 48441517
Conc: 11.59 ng/ml

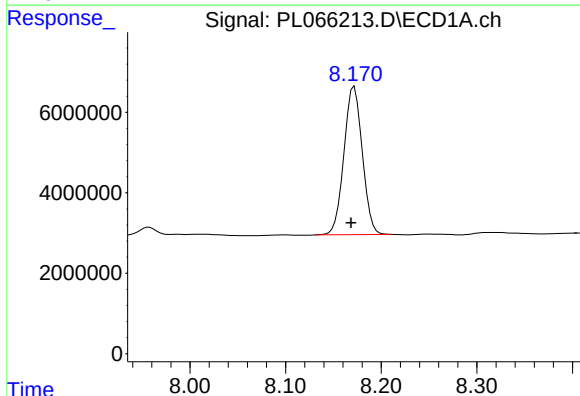

#28 Decachlorobiphenyl

R.T.: 8.172 min
Delta R.T.: 0.003 min
Response: 49345809
Conc: 20.69 ng/ml

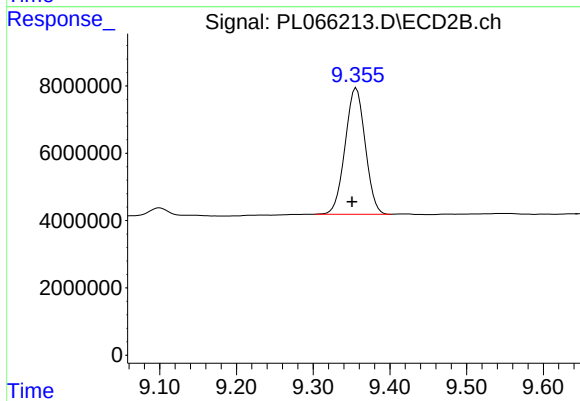

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.005 min
Response: 68584173
Conc: 21.00 ng/ml