

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
 Data File : PL066215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 02:06
 Operator : AR\AJ
 Sample : M2049-16
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-12-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/16/2021 2:46:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 04:44:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.446	4.155	48991064	80587297	19.248	20.034
28) SA Decachlor...	8.172	9.357	41393595	57317971	17.354	17.550
Target Compounds						
12) B 4,4'-DDE	5.593	6.541	8136823	8363340	2.181	2.021
17) MA 4,4'-DDT	6.342	7.341	4250212	4040278	1.333	1.191m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
Data File : PL066215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 02:06
Operator : AR\AJ
Sample : M2049-16
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-12-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 04:44:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

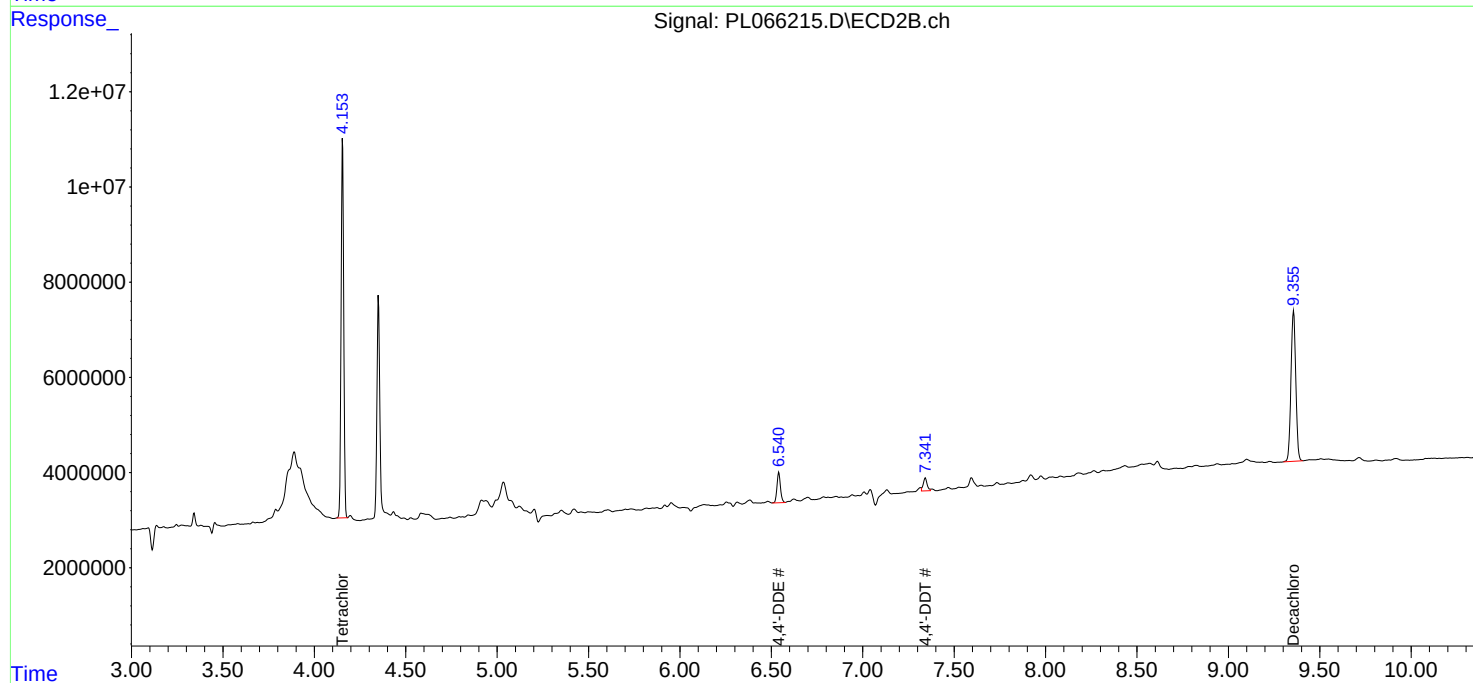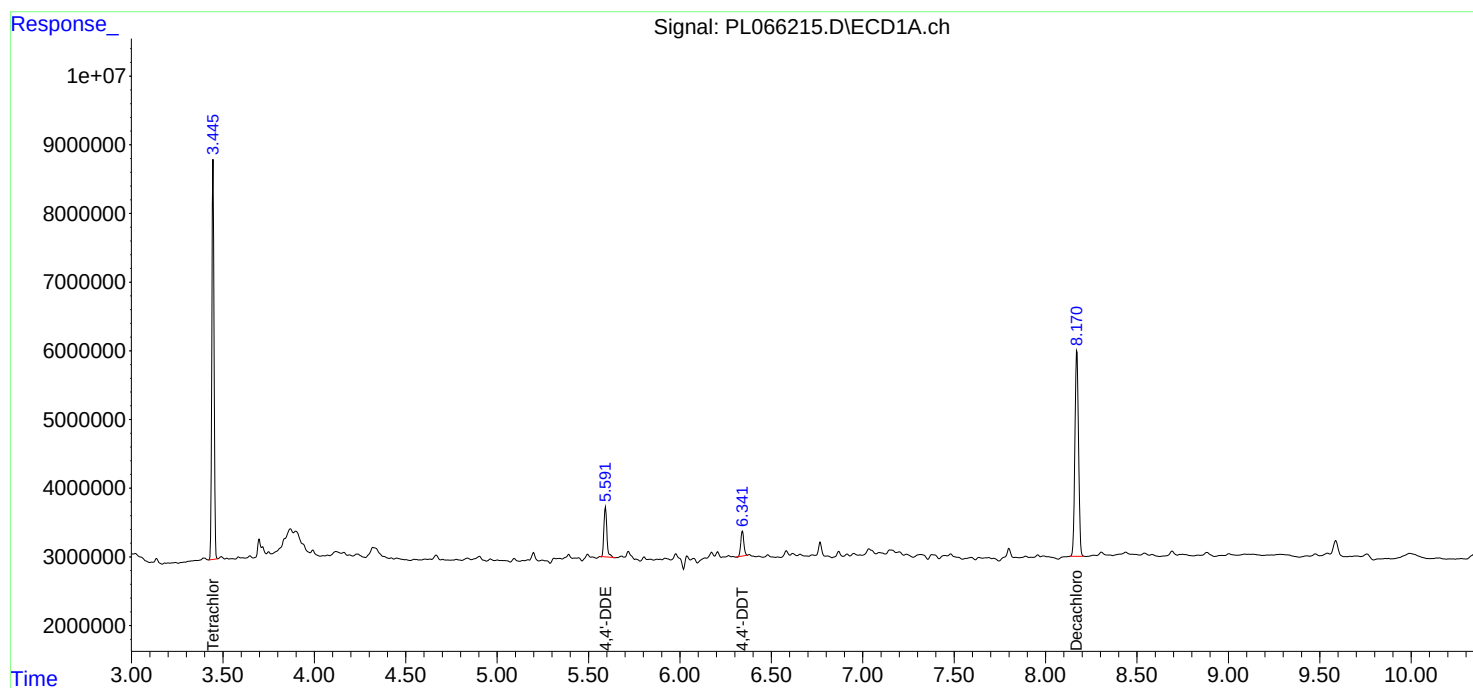

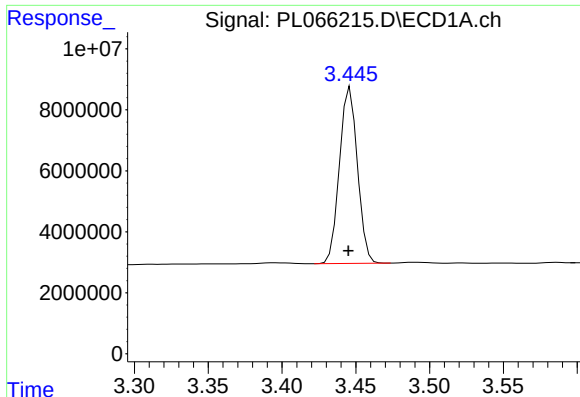


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.001 min
Response: 48991064
Conc: 19.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-12-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:20 PM

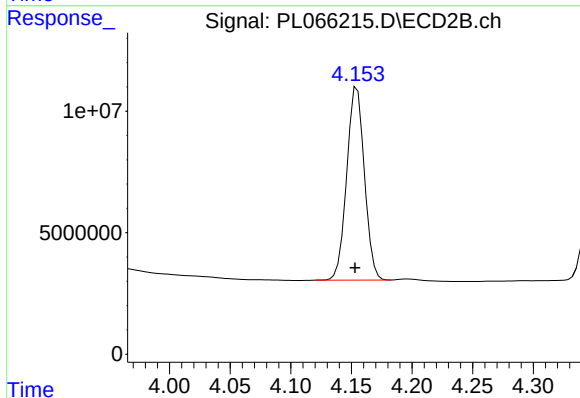


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 80587297
Conc: 20.03 ng/ml

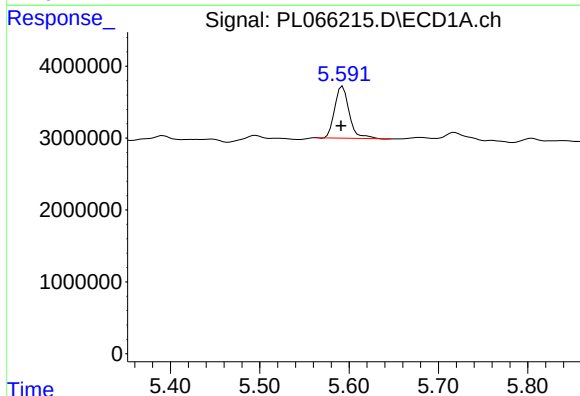


#12 4,4'-DDE

R.T.: 5.593 min
Delta R.T.: 0.001 min
Response: 8136823
Conc: 2.18 ng/ml

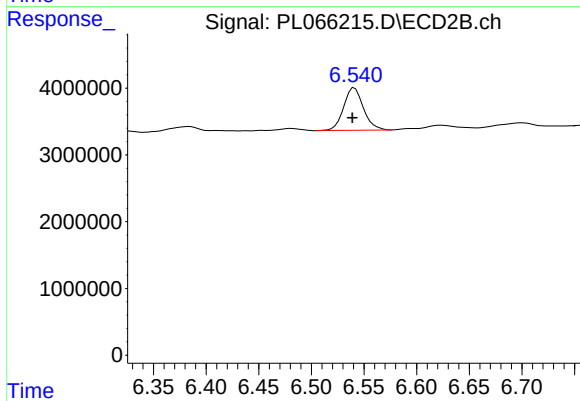

#12 4,4'-DDE

R.T.: 6.541 min
Delta R.T.: 0.002 min
Response: 8363340
Conc: 2.02 ng/ml

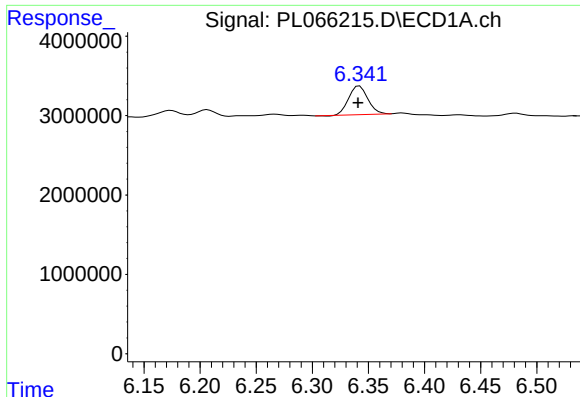


#17 4,4'-DDT

R.T.: 6.342 min
Delta R.T.: 0.001 min
Response: 4250212
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-12-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:20 PM

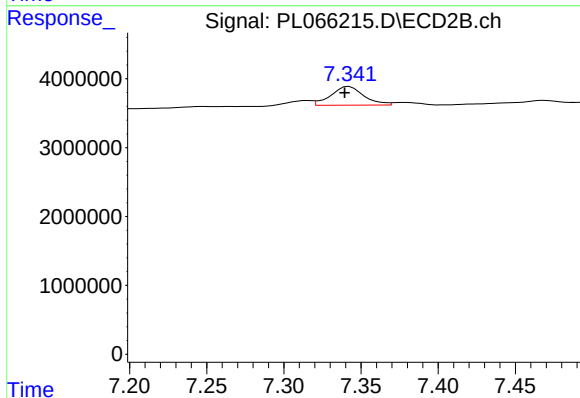


#17 4,4'-DDT

R.T.: 7.341 min
Delta R.T.: 0.002 min
Response: 4040278
Conc: 1.19 ng/ml m

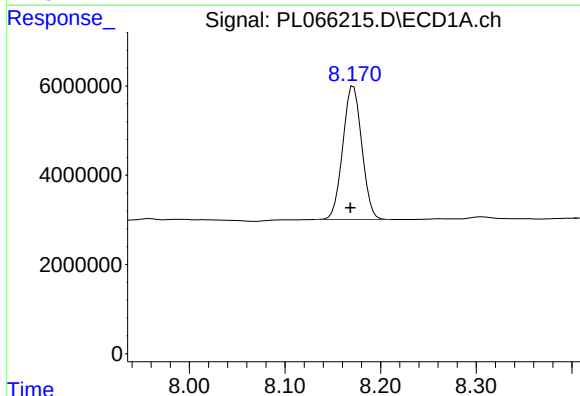

#28 Decachlorobiphenyl

R.T.: 8.172 min
Delta R.T.: 0.003 min
Response: 41393595
Conc: 17.35 ng/ml

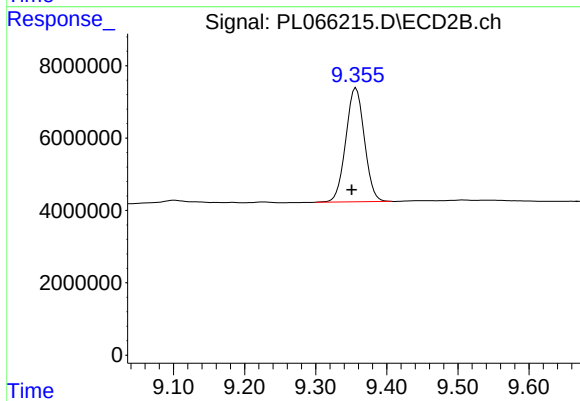

#28 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: 0.006 min
Response: 57317971
Conc: 17.55 ng/ml