

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
 Data File : PL066216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 02:20
 Operator : AR\AJ
 Sample : M2049-18
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-12-13.5-14.0

Manual Integrations
 APPROVED

Ankita
 4/16/2021 2:46:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 04:44:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.155	48477609	80576893	19.046	20.031
28)	SA Decachlor...	8.171	9.356	41179670	57281220	17.264	17.539
Target Compounds							
12)	B 4,4'-DDE	5.590	6.541	7829588	8385187	2.099m	2.026
17)	MA 4,4'-DDT	6.341	7.341	4217455	4238369	1.323	1.249m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041521\
Data File : PL066216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 02:20
Operator : AR\AJ
Sample : M2049-18
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-12-13.5-14.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 04:44:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

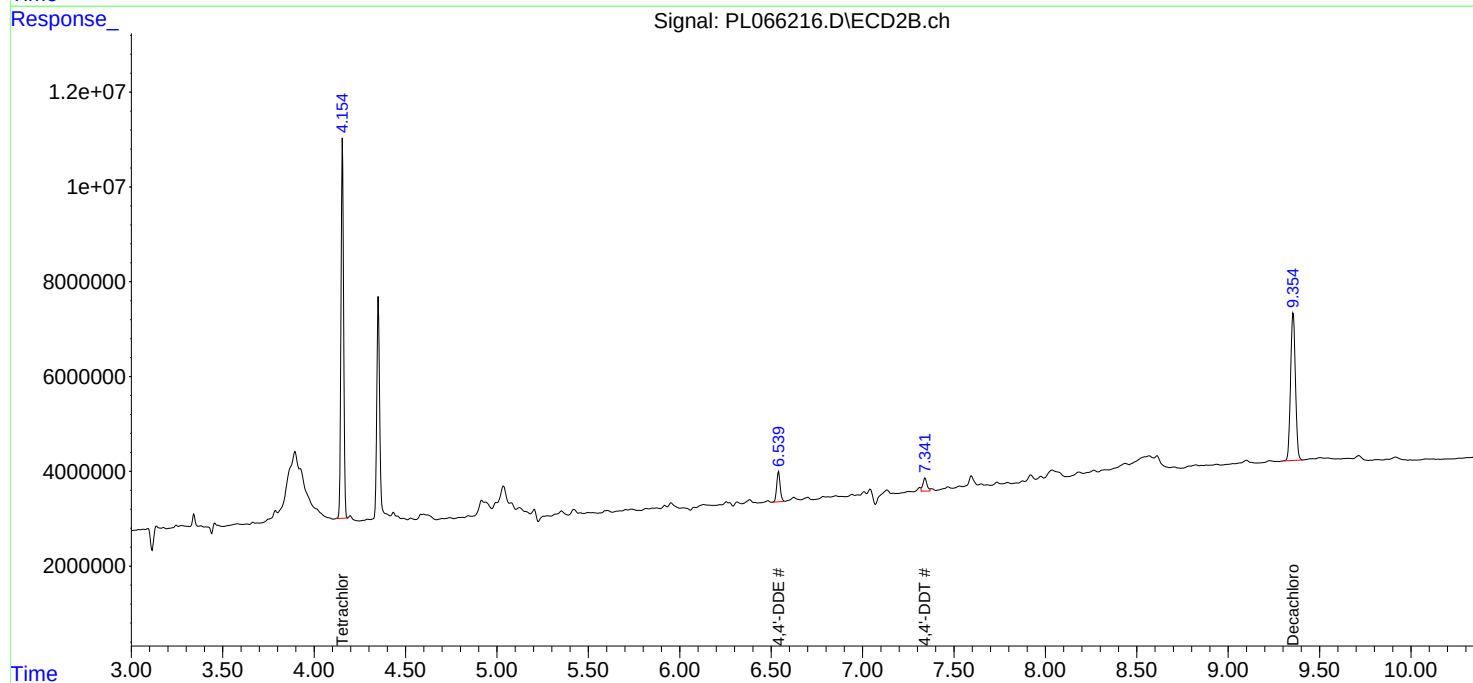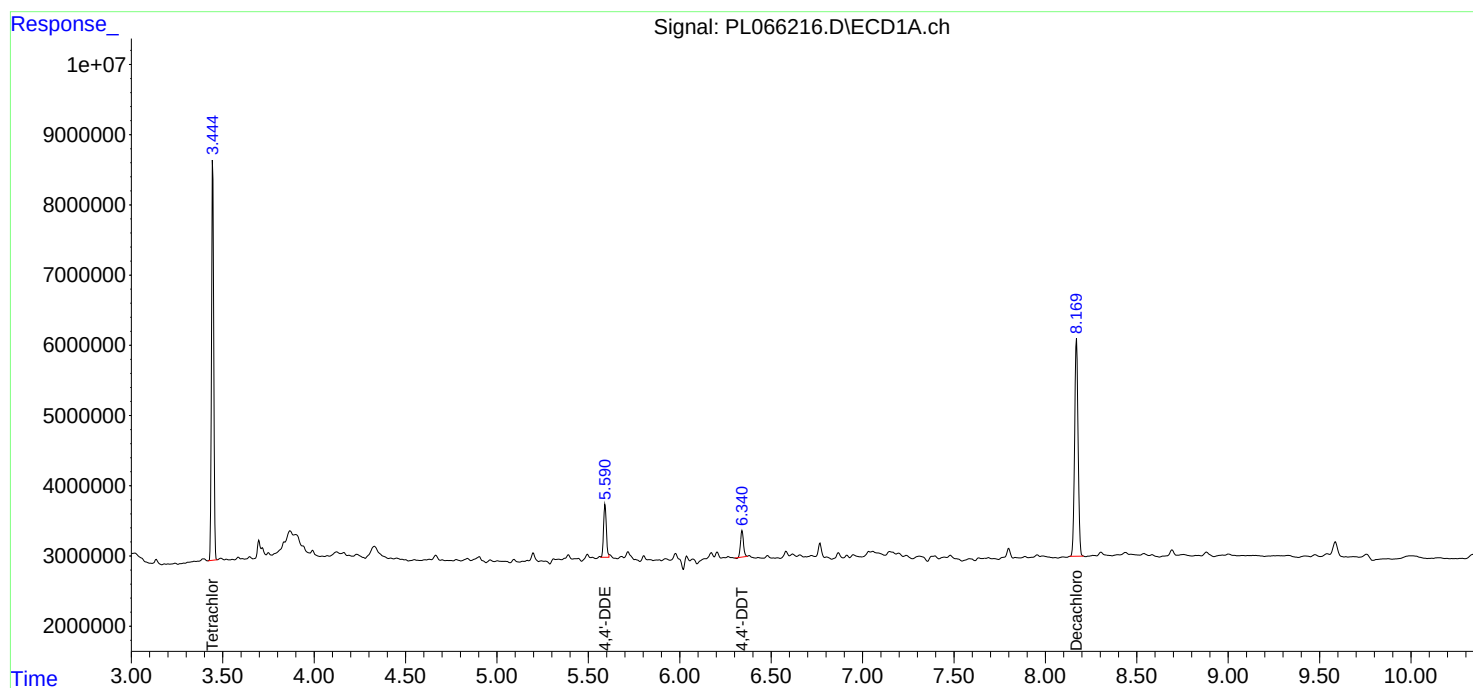

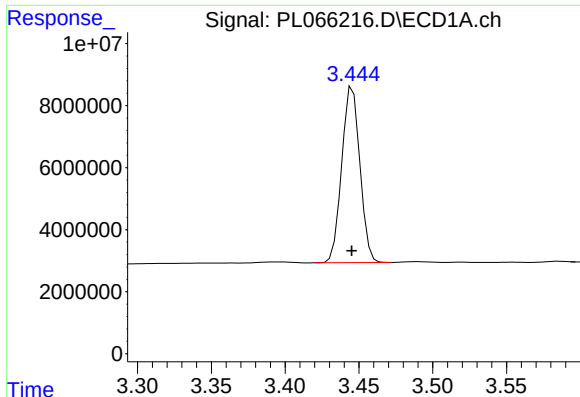


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.000 min
Response: 48477609
Conc: 19.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-12-13.5-14.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:22 PM

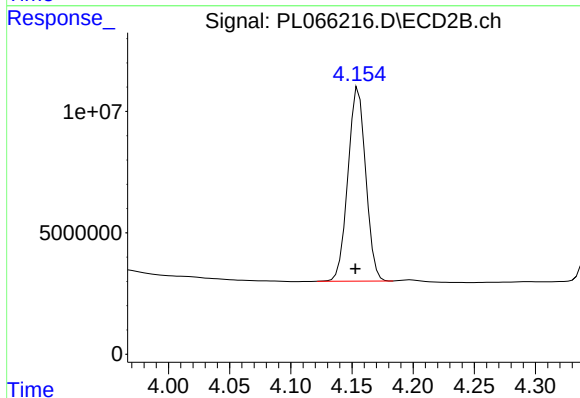


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 80576893
Conc: 20.03 ng/ml

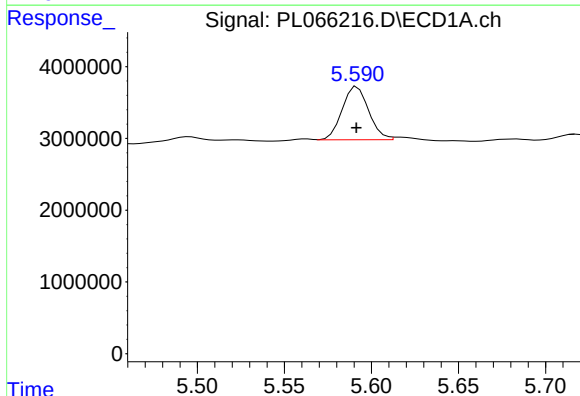


#12 4,4'-DDE

R.T.: 5.590 min
Delta R.T.: 0.000 min
Response: 7829588
Conc: 2.10 ng/ml m

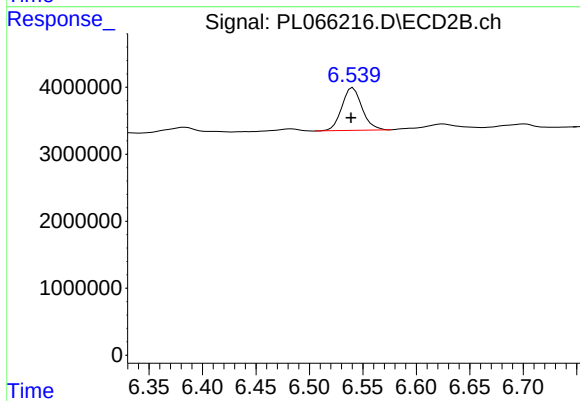

#12 4,4'-DDE

R.T.: 6.541 min
Delta R.T.: 0.002 min
Response: 8385187
Conc: 2.03 ng/ml

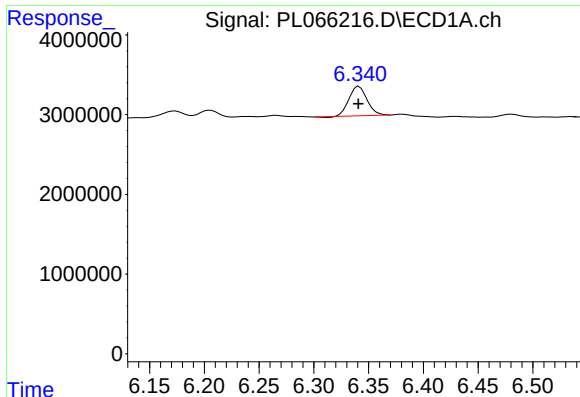


#17 4,4'-DDT

R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 4217455
Conc: 1.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-12-13.5-14.0


Manual Integrations
APPROVED

Ankita
4/16/2021 2:46:22 PM

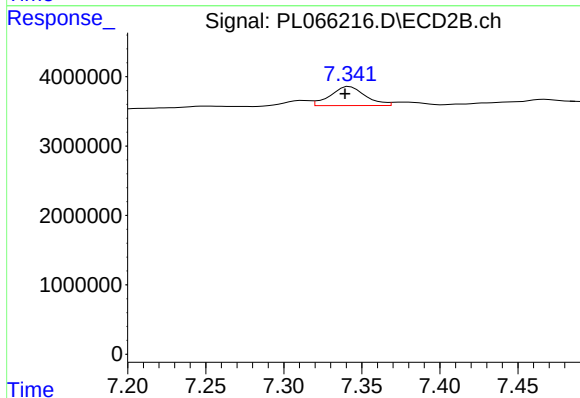


#17 4,4'-DDT

R.T.: 7.341 min
Delta R.T.: 0.001 min
Response: 4238369
Conc: 1.25 ng/ml m

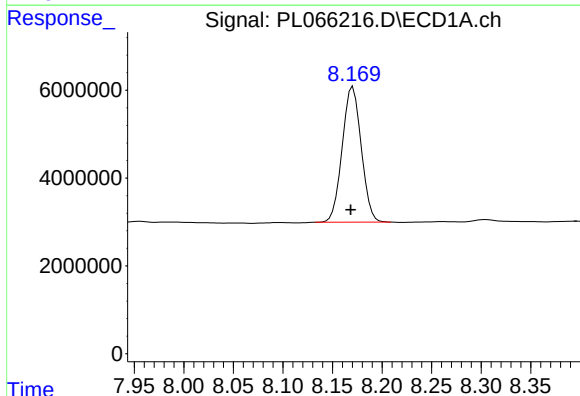

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.002 min
Response: 41179670
Conc: 17.26 ng/ml

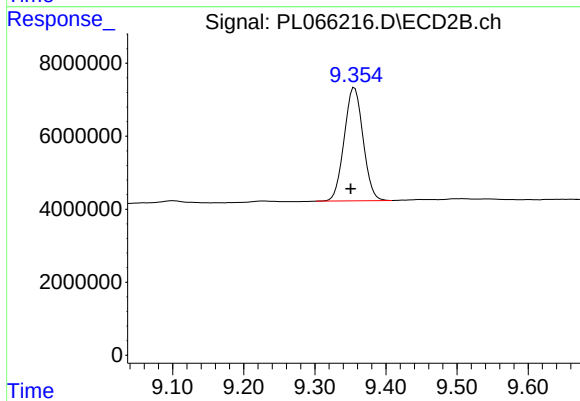

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.005 min
Response: 57281220
Conc: 17.54 ng/ml