

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041522\
 Data File : PL074117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 18:22
 Operator : AR\AJ
 Sample : N2392-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-212

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/18/2022
 Supervised By : mohammad ahmed 04/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 03:42:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.647	5.486	4235223	22353802	13.108m	12.537
28) SA Decachlor...	10.418	11.334	7991422	27450099	15.367	15.541

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041522\
Data File : PL074117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 18:22
Operator : AR\AJ
Sample : N2392-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VNJ-212


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/18/2022
Supervised By : mohammad ahmed 04/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 03:42:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

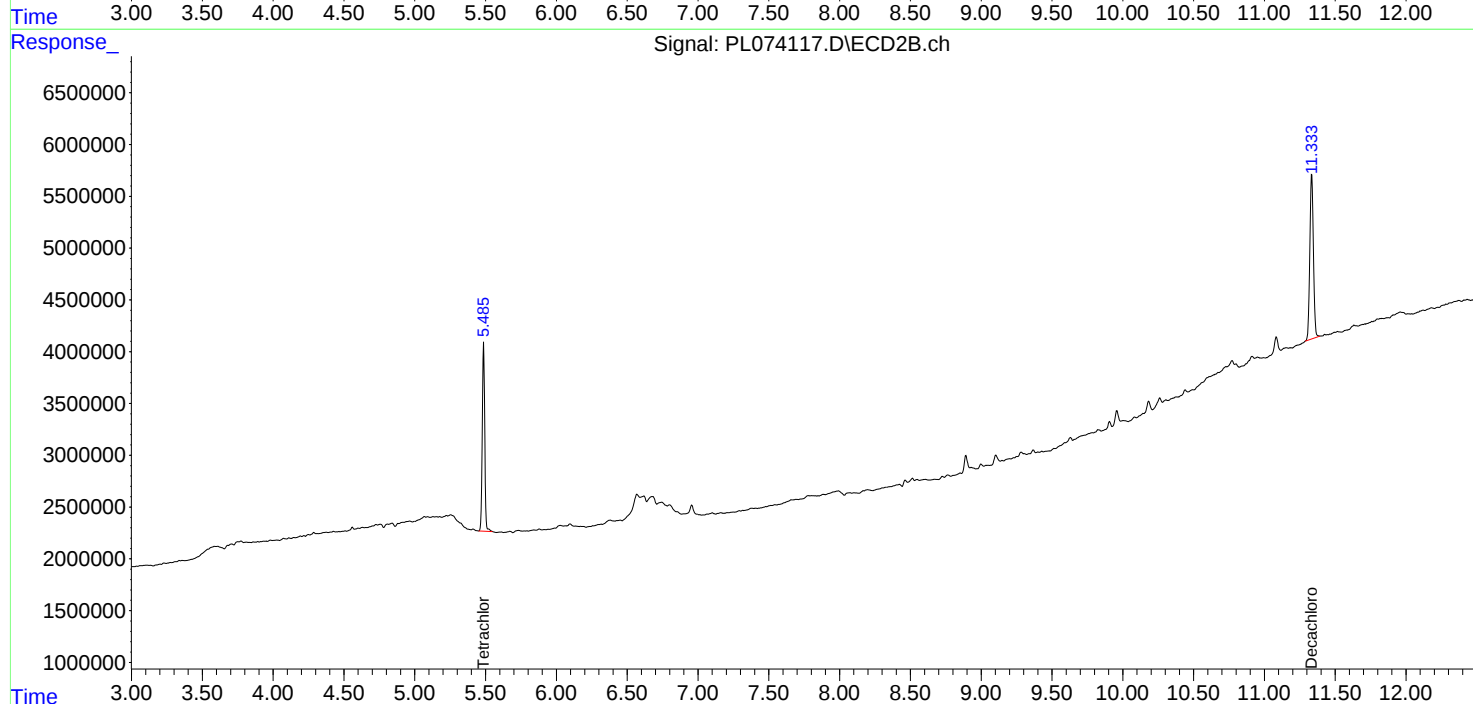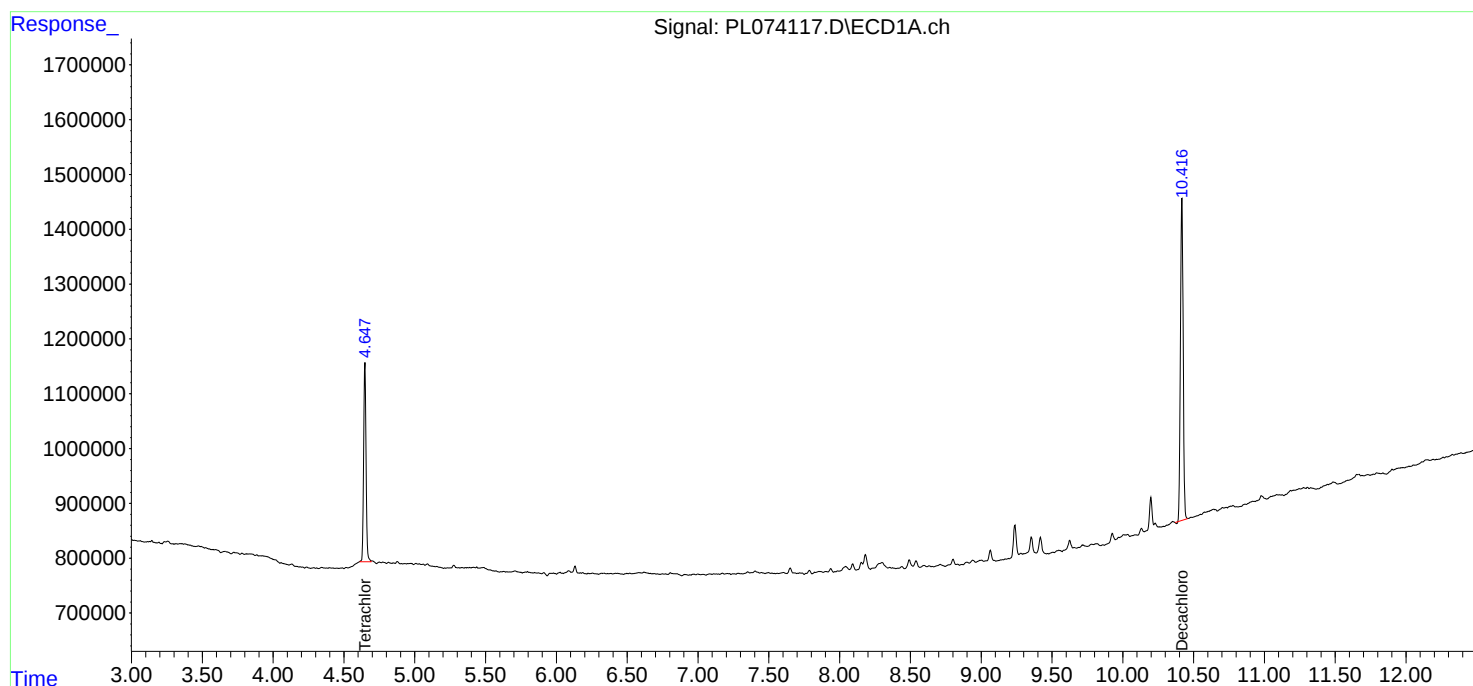

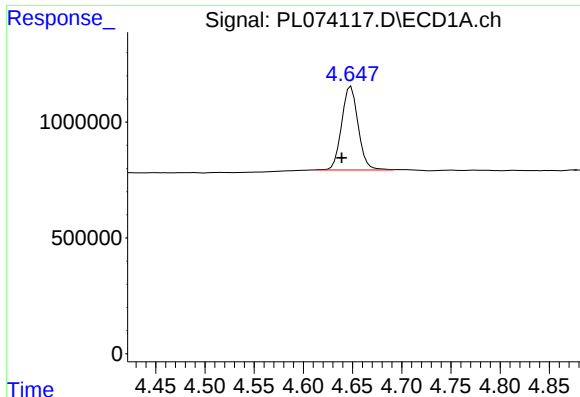


#1 Tetrachloro-m-xylene

R.T.: 4.647 min
Delta R.T.: 0.008 min
Response: 4235223
Conc: 13.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-212


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/18/2022
Supervised By :mohammad ahmed 04/18/2022

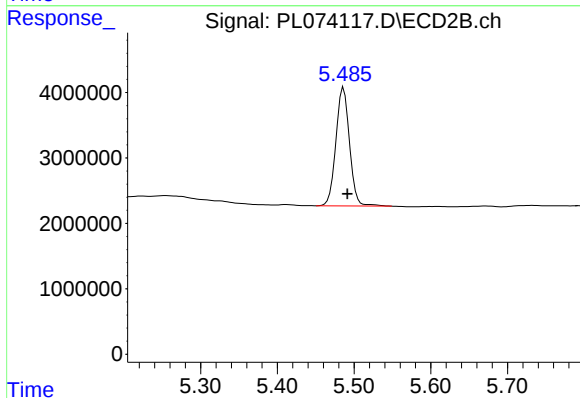


#1 Tetrachloro-m-xylene

R.T.: 5.486 min
Delta R.T.: -0.005 min
Response: 22353802
Conc: 12.54 ng/ml

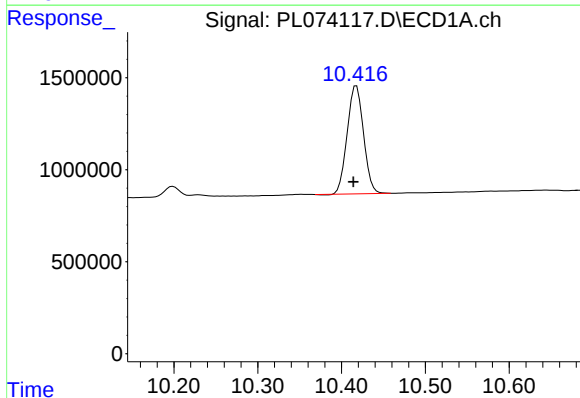

#28 Decachlorobiphenyl

R.T.: 10.418 min
Delta R.T.: 0.004 min
Response: 7991422
Conc: 15.37 ng/ml

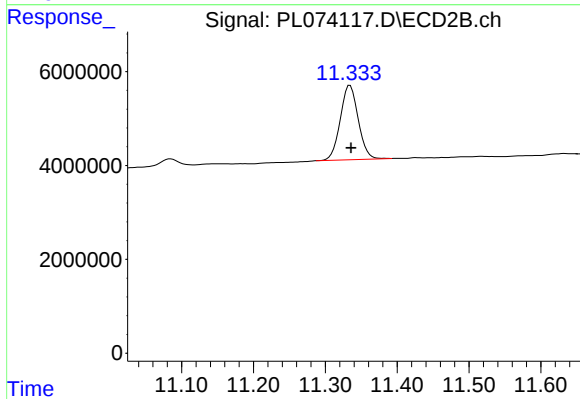

#28 Decachlorobiphenyl

R.T.: 11.334 min
Delta R.T.: -0.002 min
Response: 27450099
Conc: 15.54 ng/ml