

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041523\
 Data File : PL082067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2023 17:33
 Operator : AR\AJ
 Sample : 02283-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20230323-COMP-1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/14/2023
 Supervised By :Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 22:45:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.326	2.652	37899551	36109092	16.295	18.089
28) SA Decachlor...	8.746	7.765	24993899	29615344	13.966	14.933m
Target Compounds						
12) B 4,4'-DDE	5.957	5.090	1613372	1091925	0.716	0.554

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041523\
Data File : PL082067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2023 17:33
Operator : AR\AJ
Sample : 02283-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20230323-COMP-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/14/2023
Supervised By :Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 22:45:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

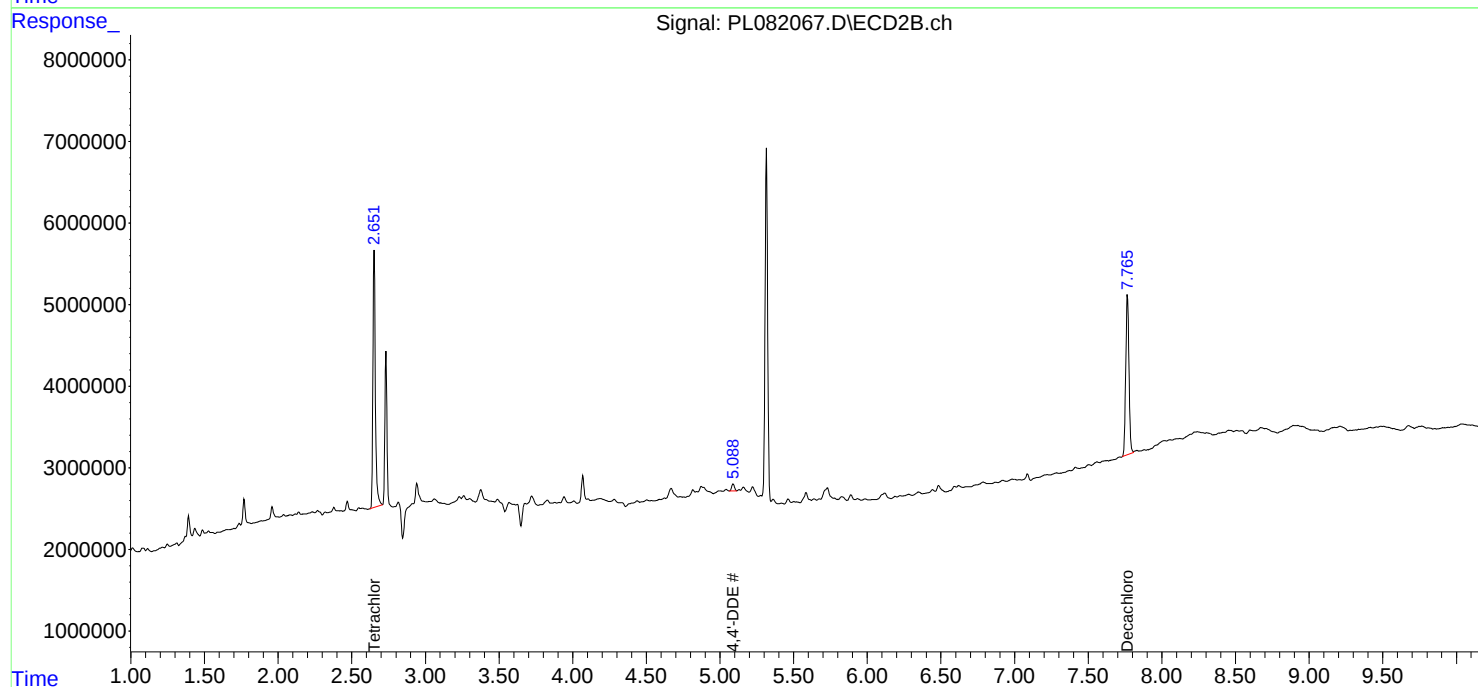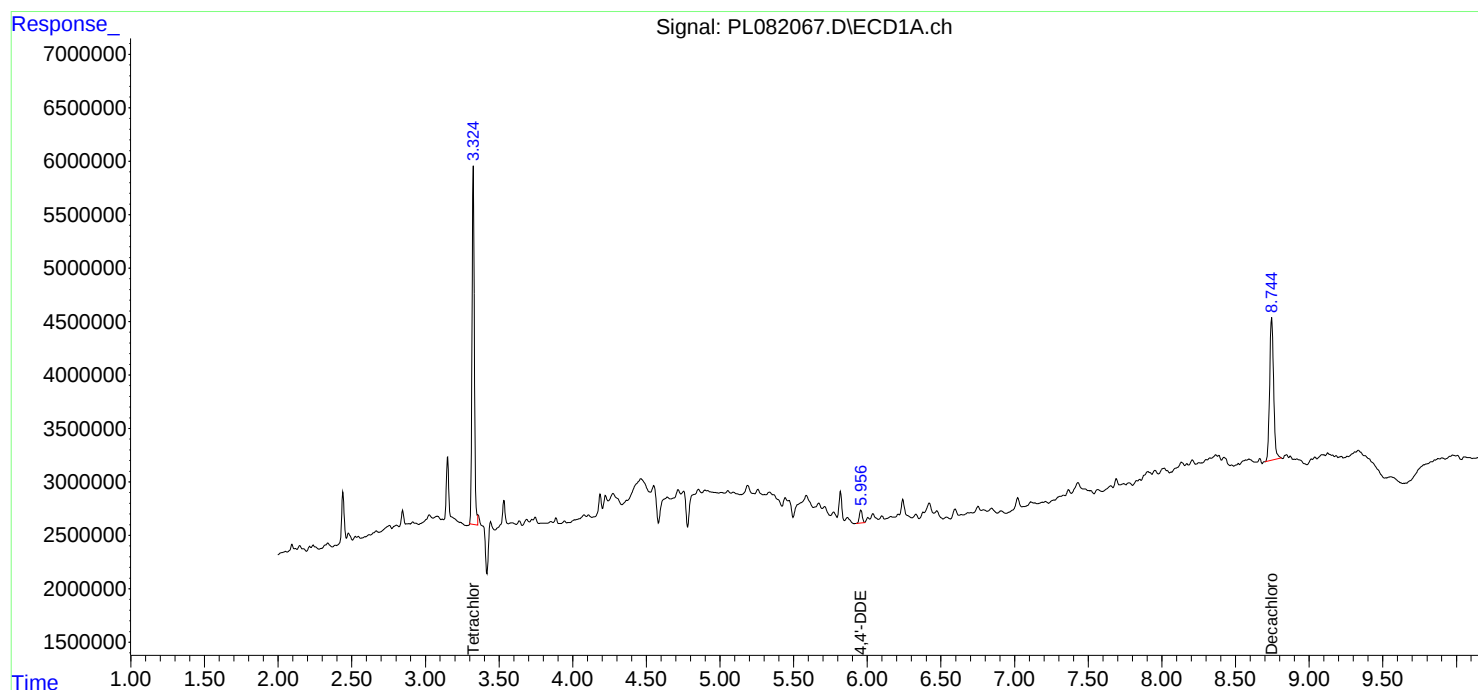

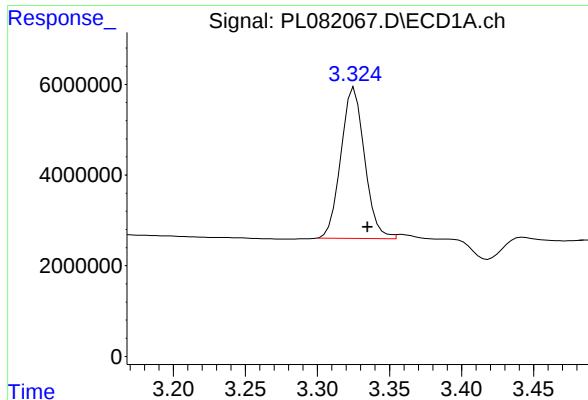


#1 Tetrachloro-m-xylene

R.T.: 3.326 min
Delta R.T.: -0.009 min
Response: 37899551
Conc: 16.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
20230323-COMP-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/14/2023
Supervised By :Ankita Jodhani 04/14/2023

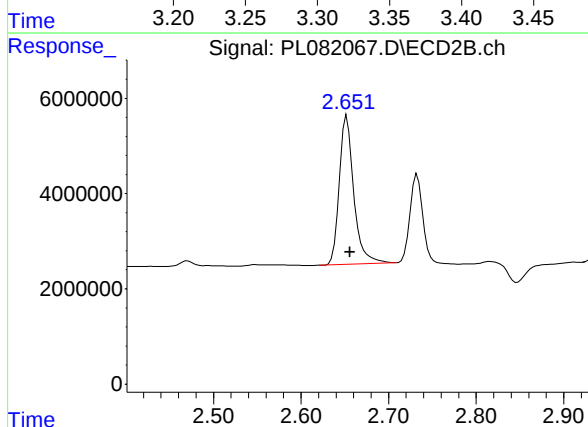


#1 Tetrachloro-m-xylene

R.T.: 2.652 min
Delta R.T.: -0.004 min
Response: 36109092
Conc: 18.09 ng/ml

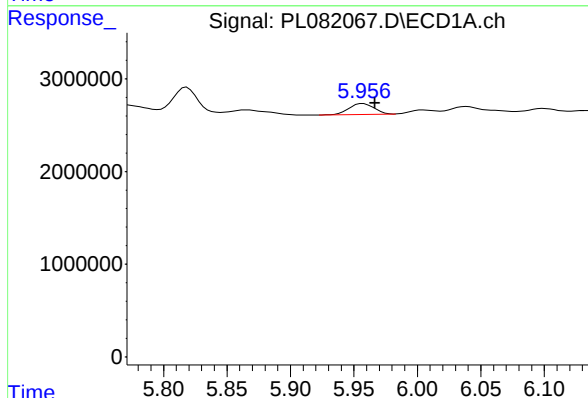


#12 4,4'-DDE

R.T.: 5.957 min
Delta R.T.: -0.010 min
Response: 1613372
Conc: 0.72 ng/ml

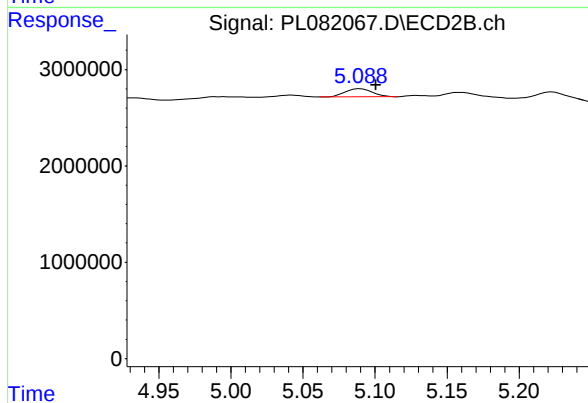

#12 4,4'-DDE

R.T.: 5.090 min
Delta R.T.: -0.011 min
Response: 1091925
Conc: 0.55 ng/ml

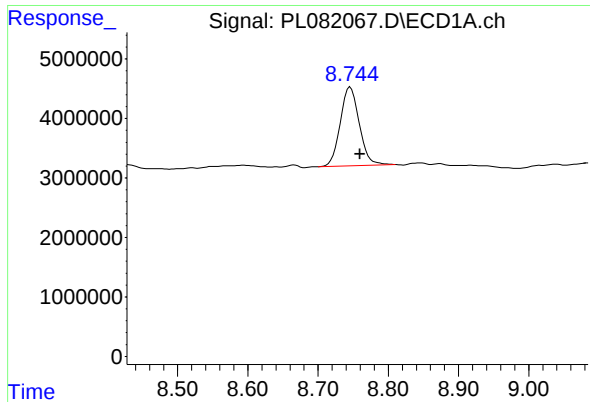


#28 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: -0.014 min
Response: 24993899
Conc: 13.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
20230323-COMP-1

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/14/2023
Supervised By :Ankita Jodhani 04/14/2023

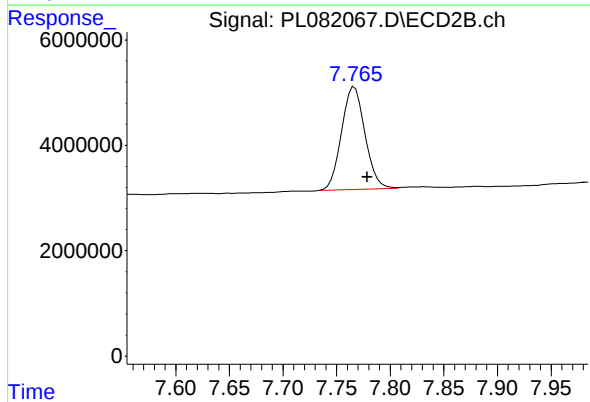

#28 Decachlorobiphenyl

R.T.: 7.765 min
Delta R.T.: -0.013 min
Response: 29615344
Conc: 14.93 ng/ml m