

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041523\
 Data File : PL082076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2023 19:39
 Operator : AR\AJ
 Sample : 02305-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-232

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/14/2023
 Supervised By : Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 22:56:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.324	2.652	28867663	18231036	12.411	9.133 #
28) SA Decachlor...	8.746	7.765	29029428	34680562	16.221	17.487m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041523\
Data File : PL082076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2023 19:39
Operator : AR\AJ
Sample : 02305-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VNJ-232


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/14/2023
Supervised By : Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 22:56:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

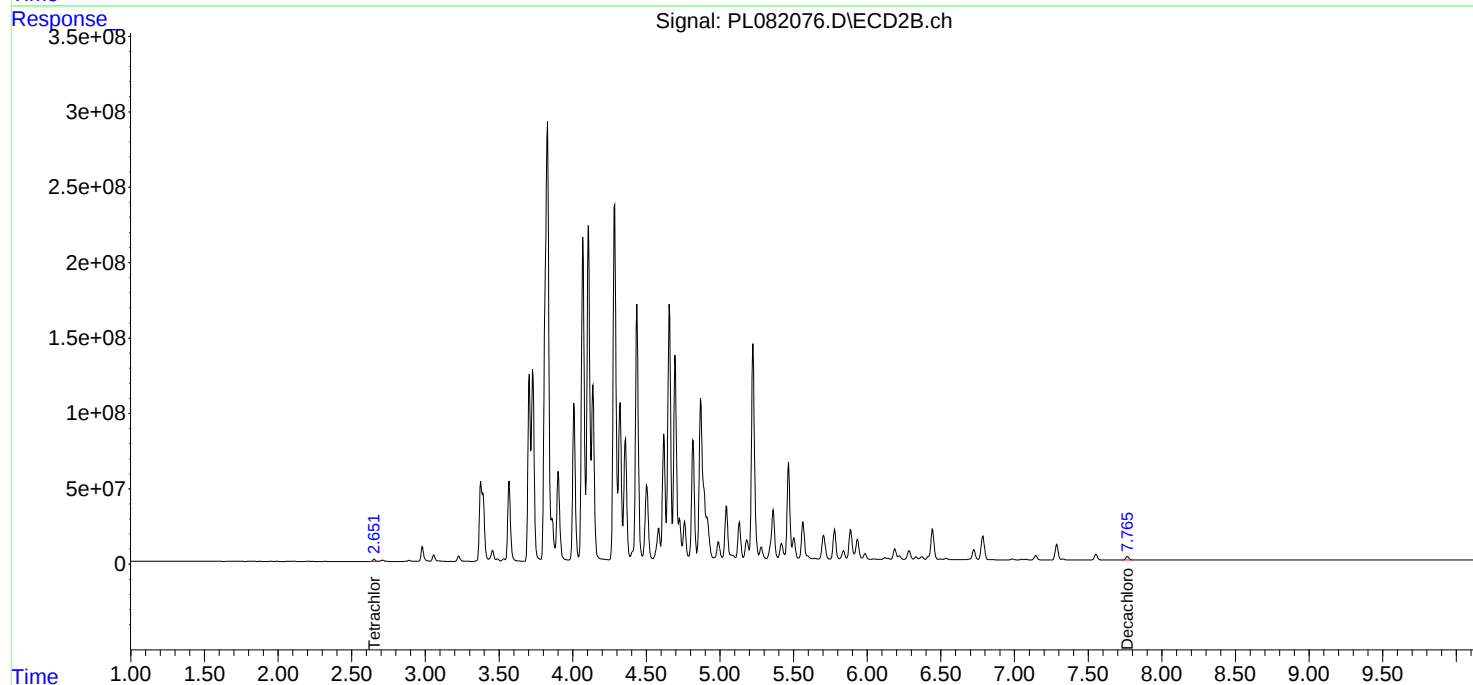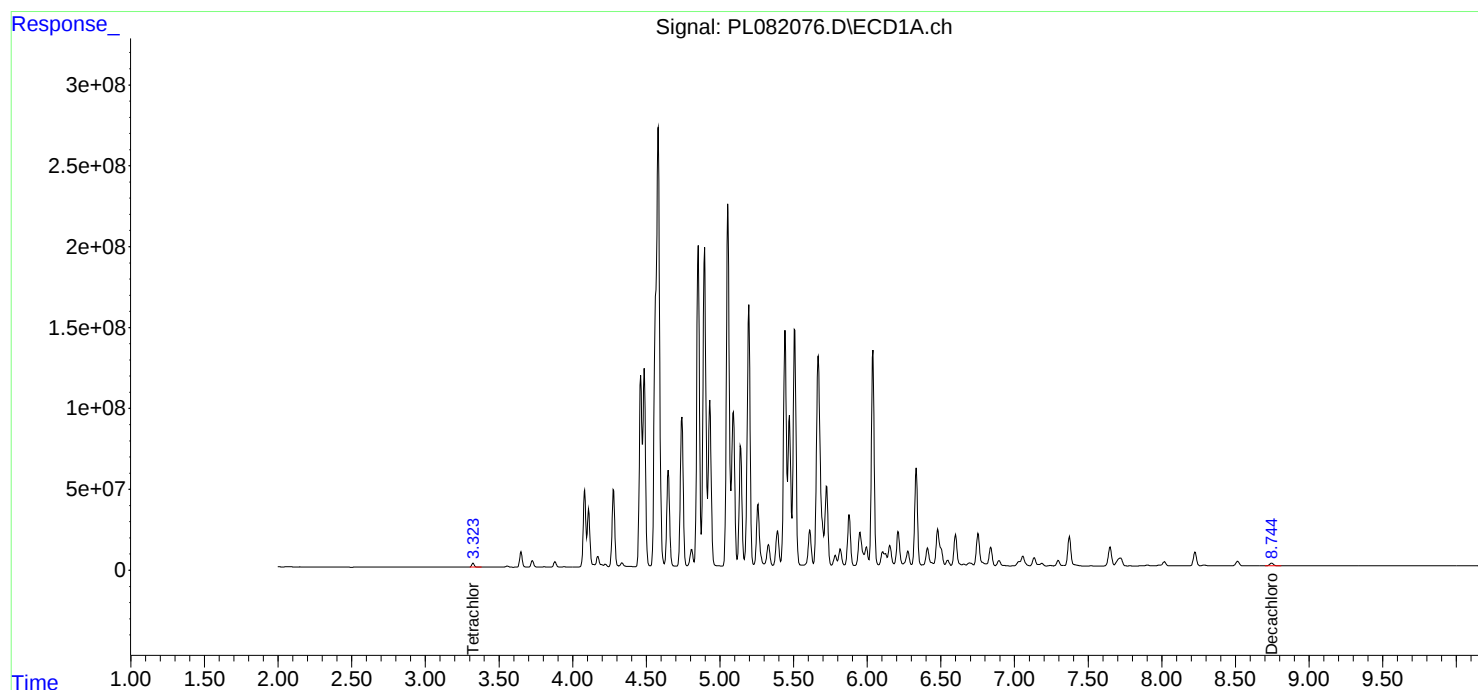

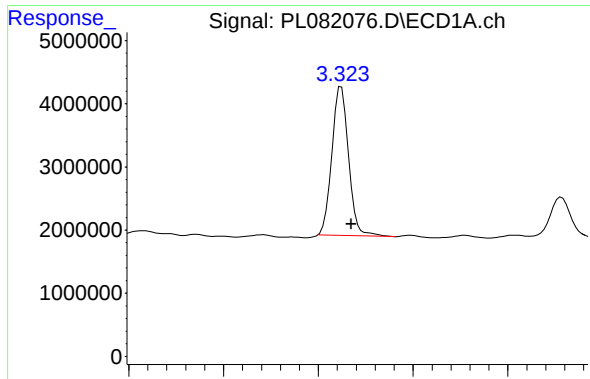


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: -0.011 min
Response: 28867663
Conc: 12.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-232


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/14/2023
Supervised By :Ankita Jodhani 04/14/2023

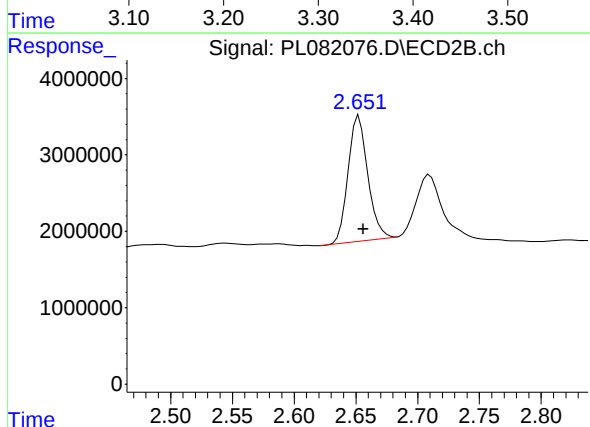


#1 Tetrachloro-m-xylene

R.T.: 2.652 min
Delta R.T.: -0.004 min
Response: 18231036
Conc: 9.13 ng/ml

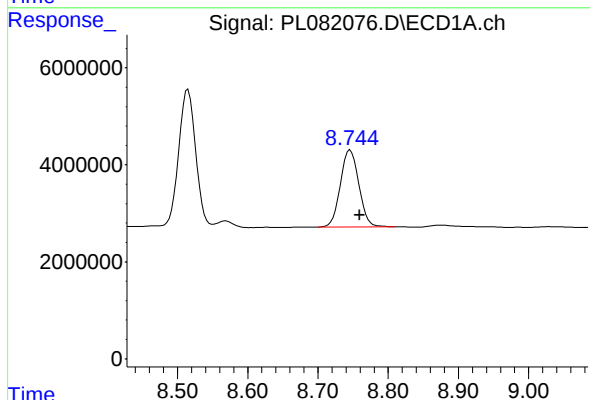

#28 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: -0.014 min
Response: 29029428
Conc: 16.22 ng/ml

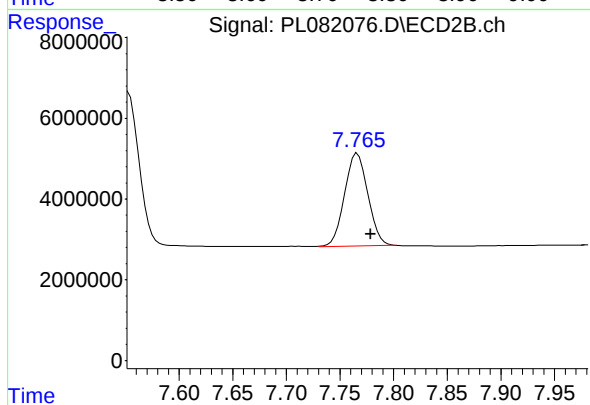

#28 Decachlorobiphenyl

R.T.: 7.765 min
Delta R.T.: -0.014 min
Response: 34680562
Conc: 17.49 ng/ml m