

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041524\
 Data File : PL089029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2024 16:09
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 16:44:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041524.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 15 16:40:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.796	150.1E6	123.9E6	73.819	74.122
28)	SA Decachlor...	9.065	7.950	93828243	103.3E6	73.953	74.123
Target Compounds							
23)	Chlordane-1	4.713	3.800	64209303	37365806	738.869	739.622
24)	Chlordane-2	5.241	4.379	63864627	45225568	736.998	739.665
25)	Chlordane-3	5.952	5.010	223.0E6	129.7E6	738.478	744.083
26)	Chlordane-4	6.034	5.074	272.5E6	120.4E6	738.621	745.059
27)	Chlordane-5	6.882	5.740	52764466	35876356	737.001	738.445



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041524\
Data File : PL089029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2024 16:09
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 16:44:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041524.M
Quant Title : GC Extractables
QLast Update : Mon Apr 15 16:40:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

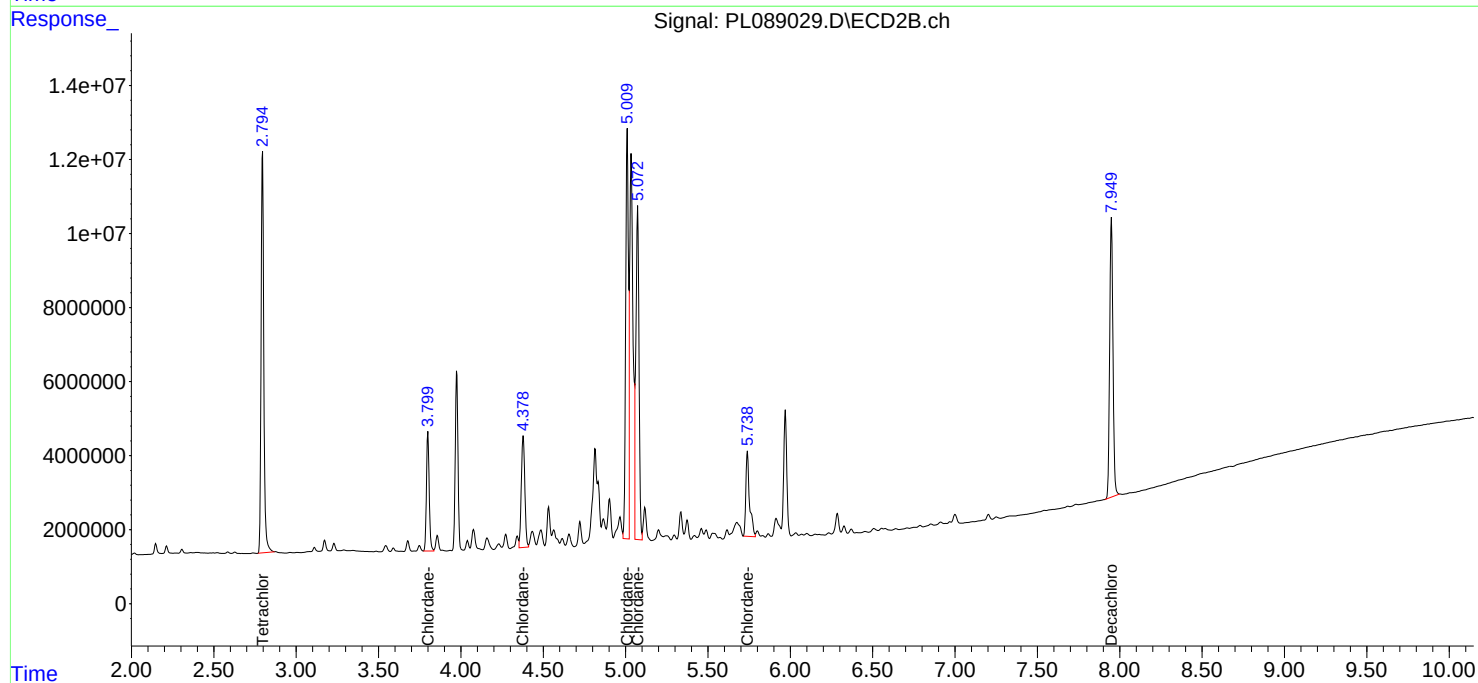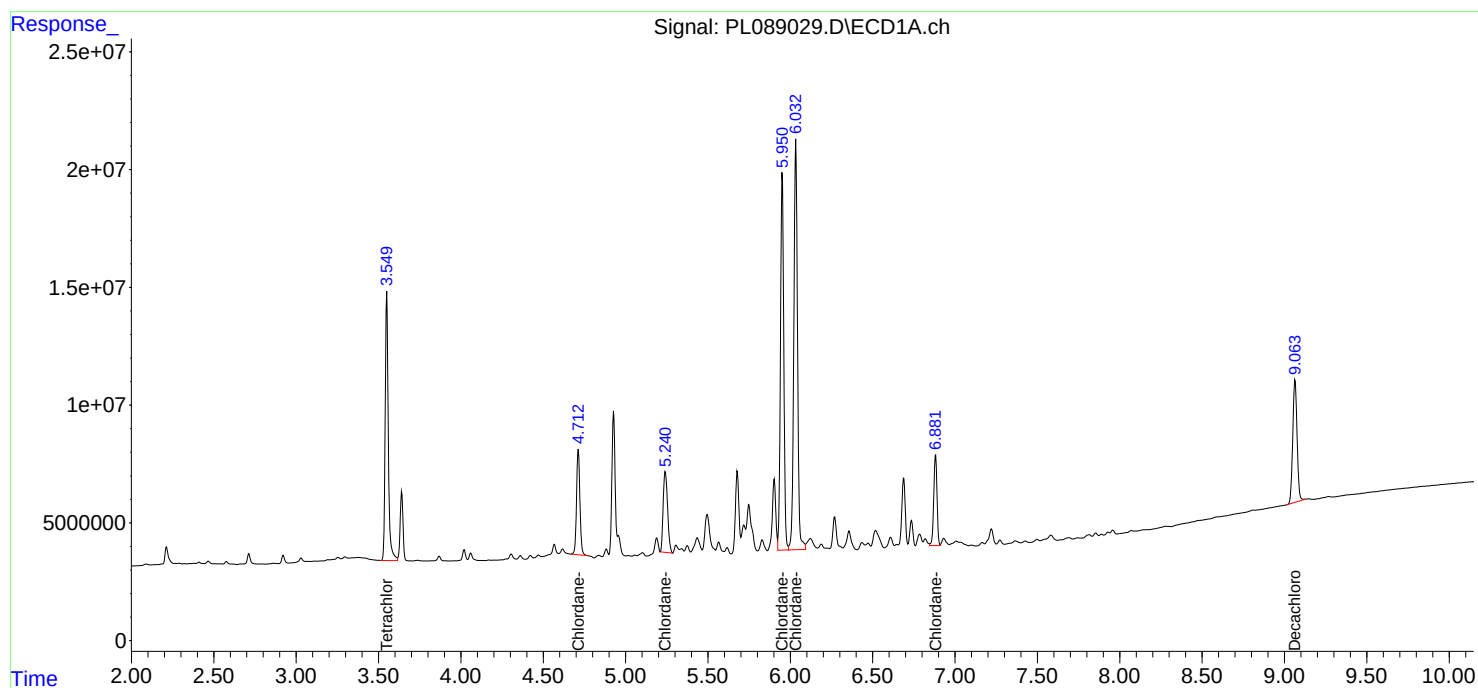


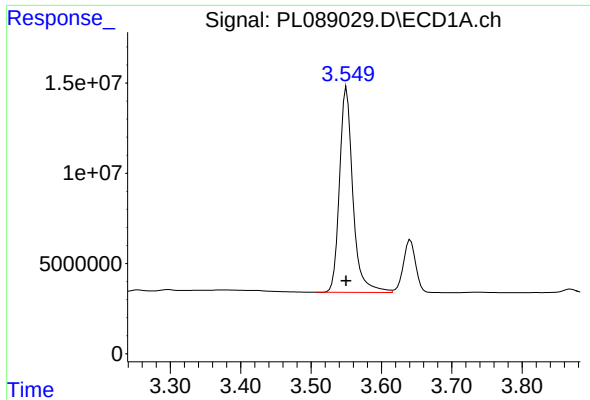

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 150135597
Conc: 73.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

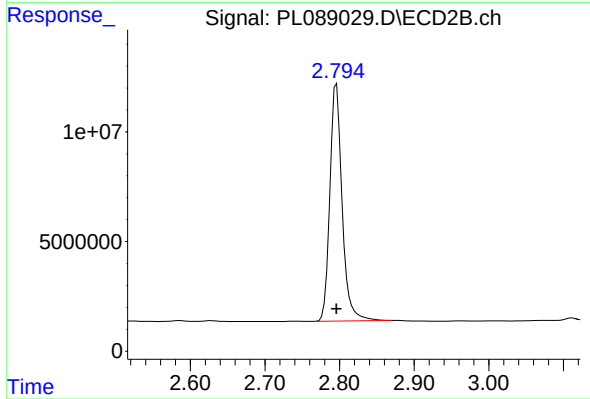


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 123885678
Conc: 74.12 ng/ml

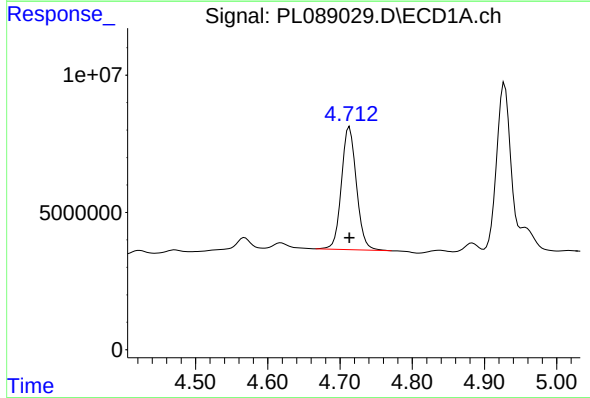


#23 Chlordane-1

R.T.: 4.713 min
Delta R.T.: 0.000 min
Response: 64209303
Conc: 738.87 ng/ml

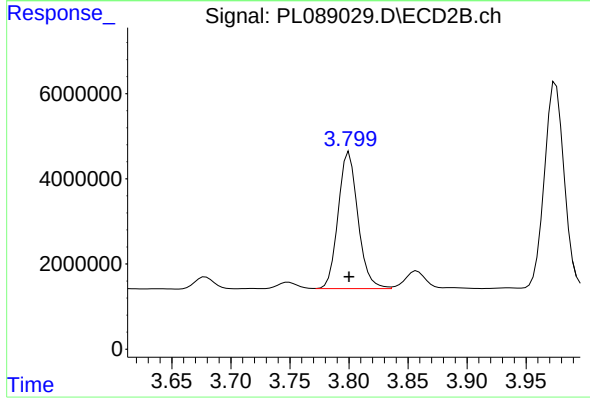

#23 Chlordane-1


R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 37365806
Conc: 739.62 ng/ml

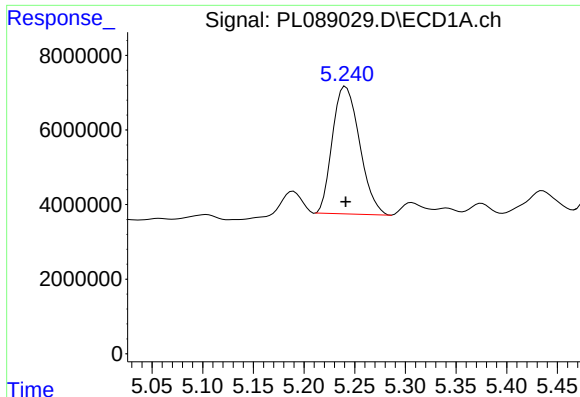

#24 Chlordane-2


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 63864627
Conc: 737.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

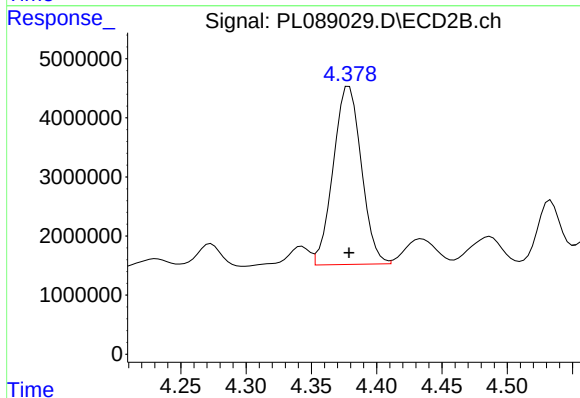


#24 Chlordane-2

R.T.: 4.379 min
Delta R.T.: 0.000 min
Response: 45225568
Conc: 739.67 ng/ml

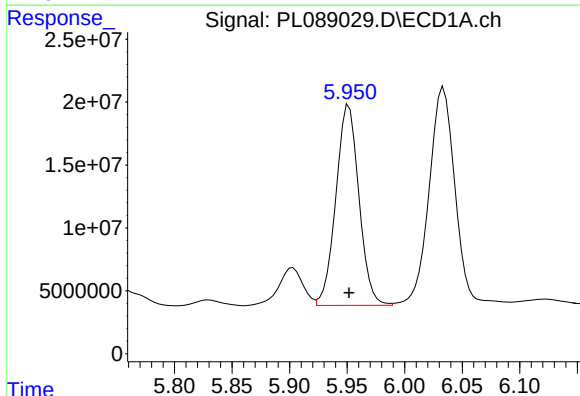


#25 Chlordane-3

R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 222976478
Conc: 738.48 ng/ml

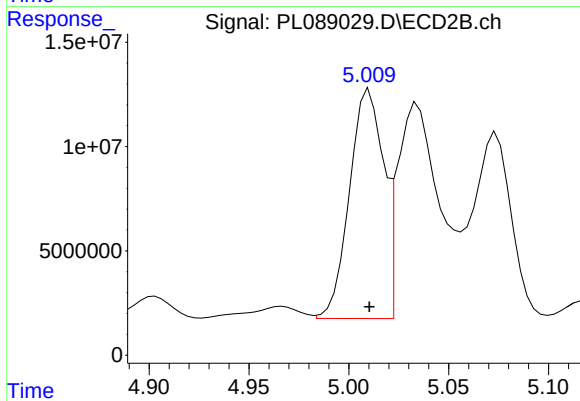

#25 Chlordane-3


R.T.: 5.010 min
Delta R.T.: 0.000 min
Response: 129715175
Conc: 744.08 ng/ml

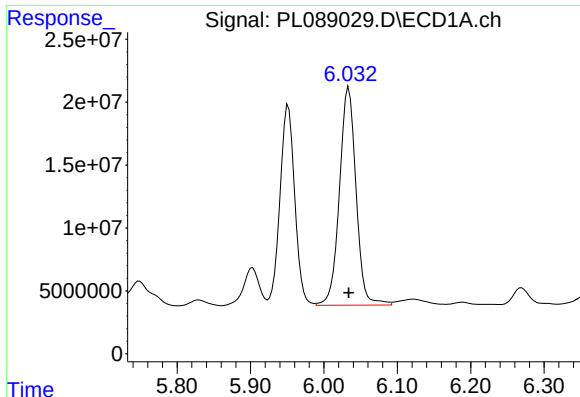

#26 Chlordane-4


R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 272528747
Conc: 738.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

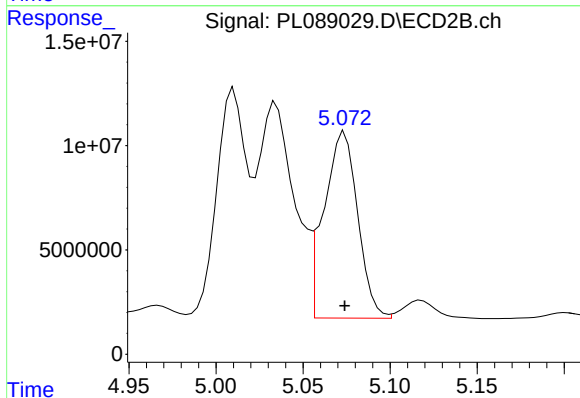


#26 Chlordane-4

R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 120442556
Conc: 745.06 ng/ml

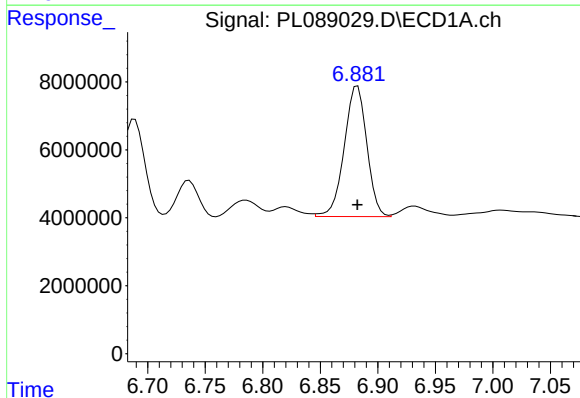


#27 Chlordane-5

R.T.: 6.882 min
Delta R.T.: 0.000 min
Response: 52764466
Conc: 737.00 ng/ml

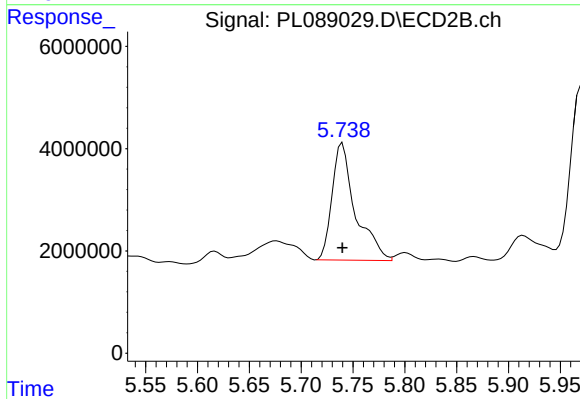

#27 Chlordane-5


R.T.: 5.740 min
Delta R.T.: 0.000 min
Response: 35876356
Conc: 738.44 ng/ml

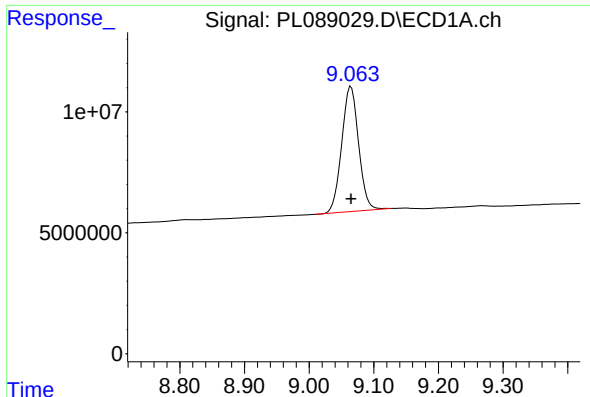

#28 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: 0.000 min
Response: 93828243
Conc: 73.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

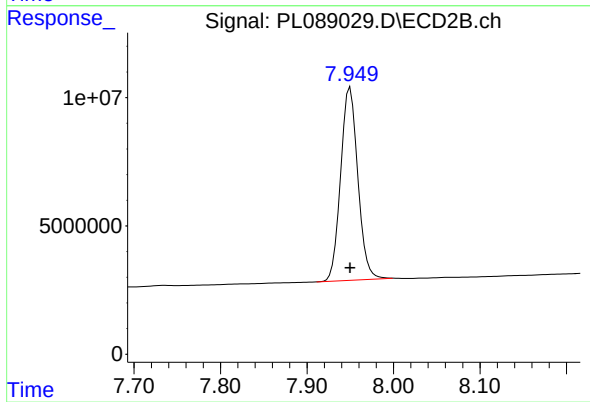

#28 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 103273837
Conc: 74.12 ng/ml