

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041524\
 Data File : PL089031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2024 16:36
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 16:48:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041524.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 15 16:47:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.796	55040254	41475123	26.515	24.861
28)	SA Decachlor...	9.063	7.949	32910377	36325172	25.698	25.795
Target Compounds							
23)	Chlordane-1	4.712	3.800	23564575	12922983	265.543	254.324
24)	Chlordane-2	5.241	4.378	24569863	16618956	274.336	266.004
25)	Chlordane-3	5.951	5.010	81365238	42173520	264.327	243.890
26)	Chlordane-4	6.033	5.073	99805205	39601867	265.064	246.214
27)	Chlordane-5	6.881	5.740	20323879	12632007	274.577	257.430



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041524\
Data File : PL089031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2024 16:36
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 16:48:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041524.M
Quant Title : GC Extractables
QLast Update : Mon Apr 15 16:47:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

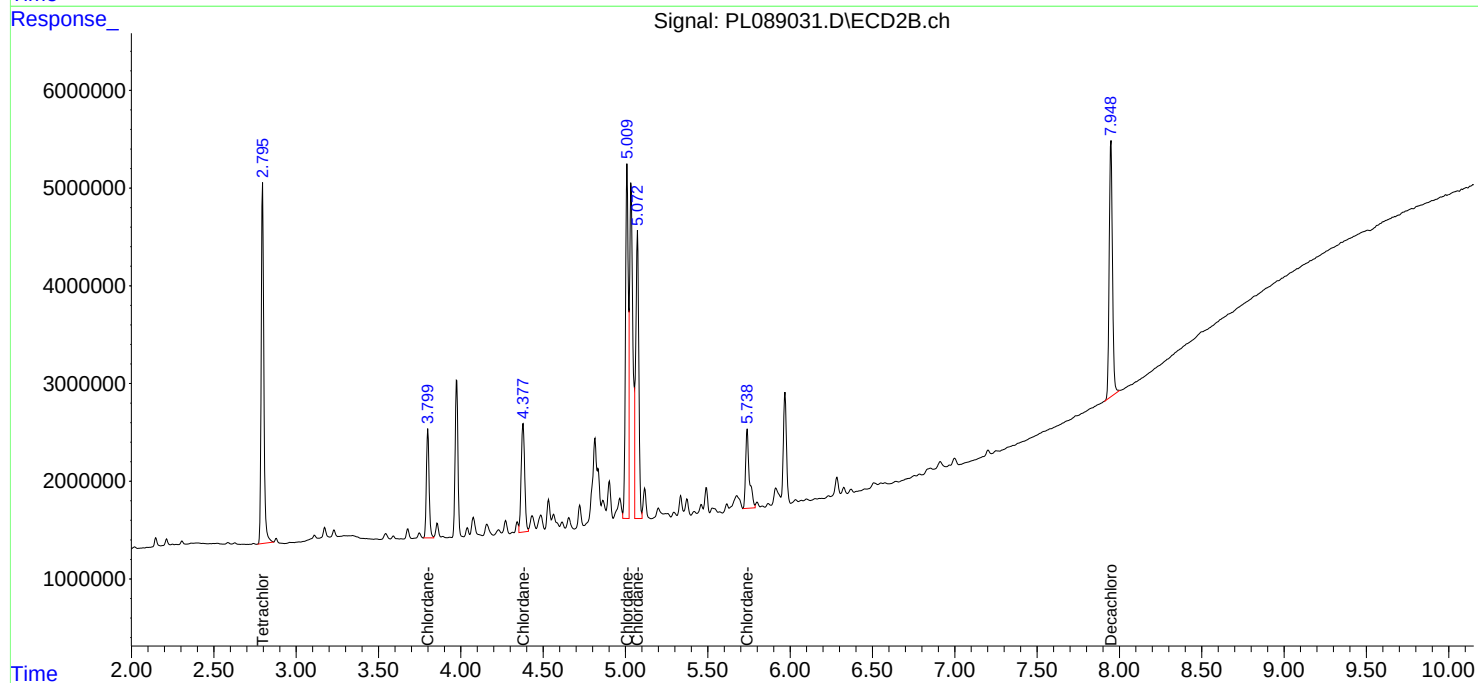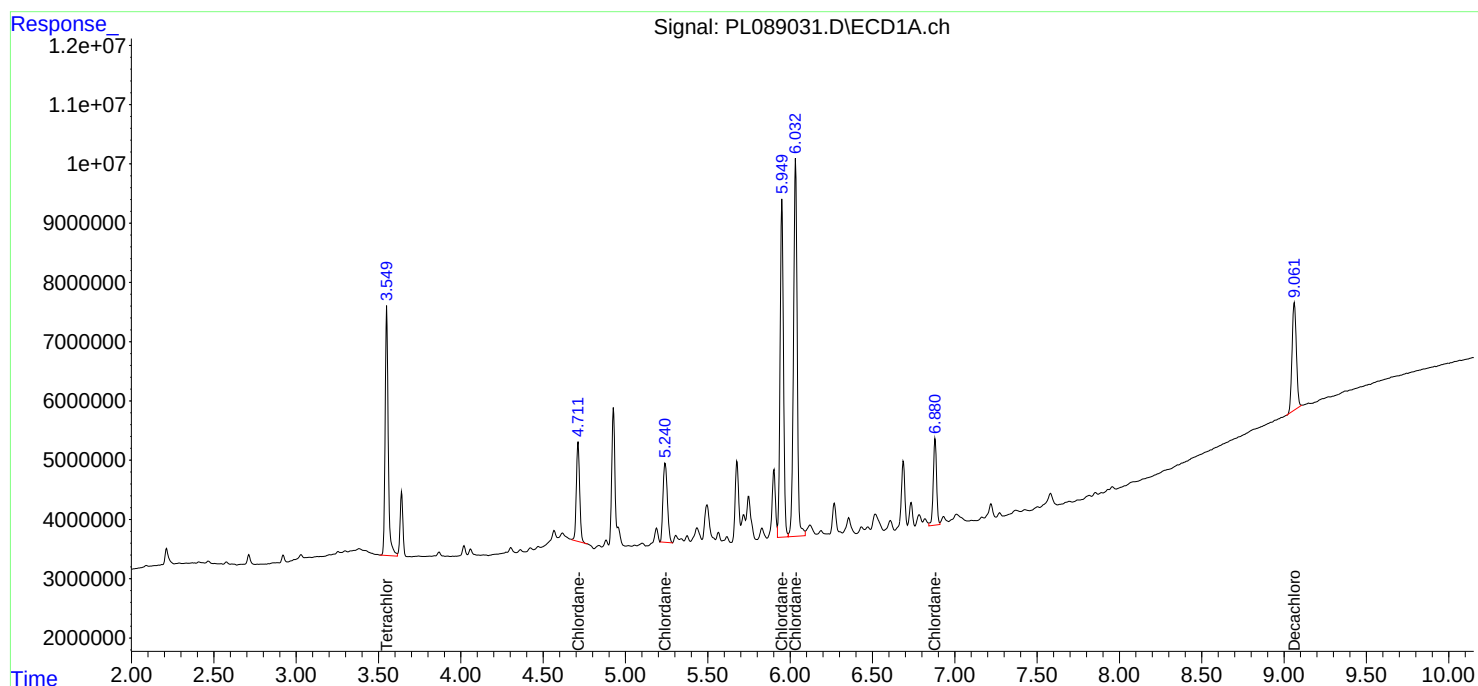


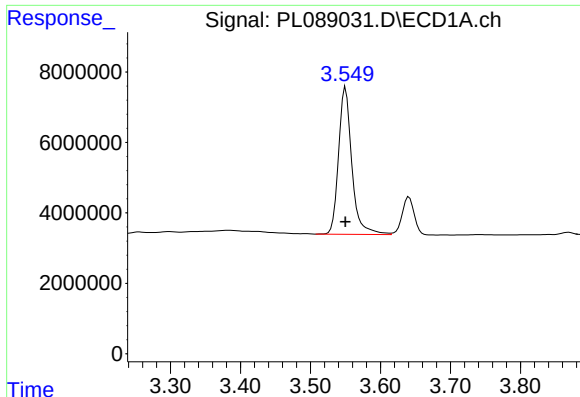

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 55040254
Conc: 26.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

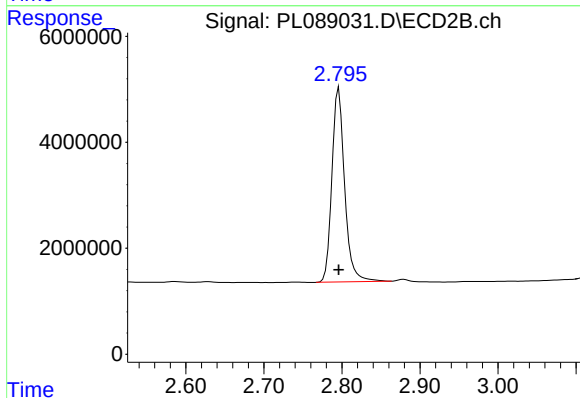


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 41475123
Conc: 24.86 ng/ml

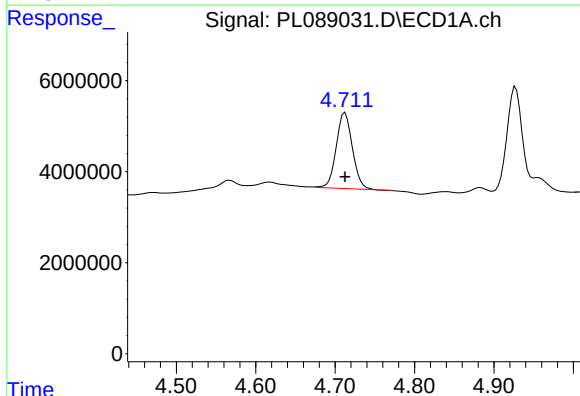


#23 Chlordane-1

R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 23564575
Conc: 265.54 ng/ml

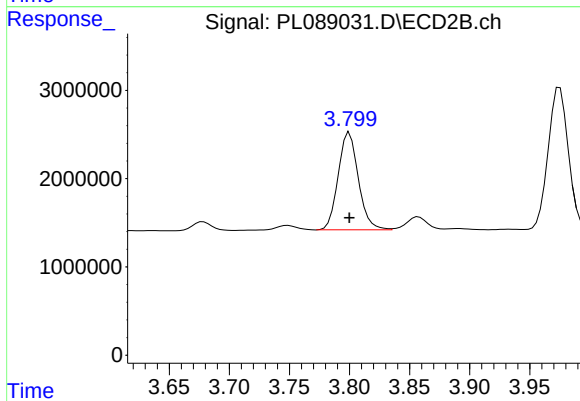

#23 Chlordane-1


R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 12922983
Conc: 254.32 ng/ml

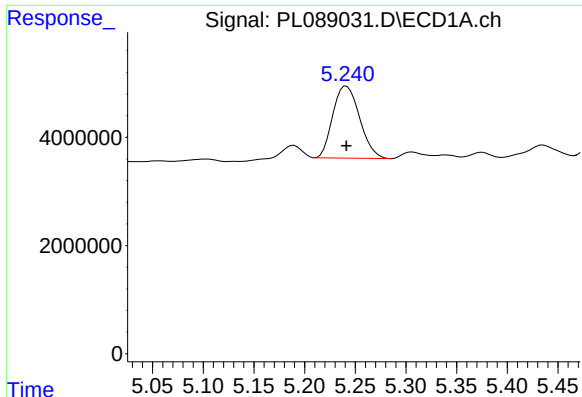

#24 Chlordane-2


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 24569863
Conc: 274.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

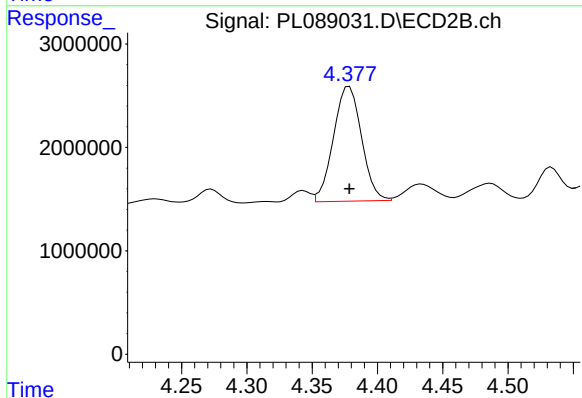


#24 Chlordane-2

R.T.: 4.378 min
Delta R.T.: 0.000 min
Response: 16618956
Conc: 266.00 ng/ml

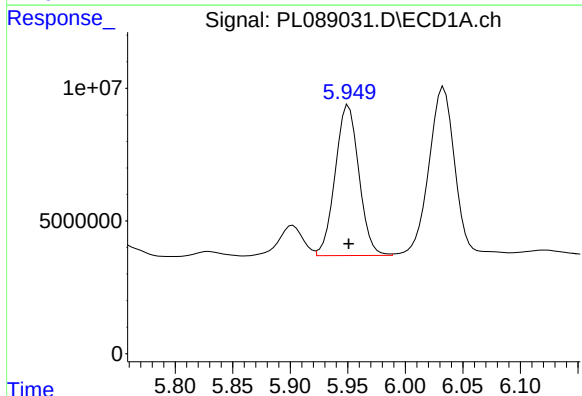


#25 Chlordane-3

R.T.: 5.951 min
Delta R.T.: 0.000 min
Response: 81365238
Conc: 264.33 ng/ml

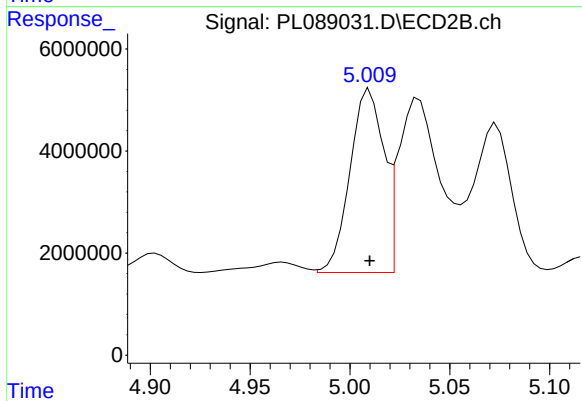

#25 Chlordane-3


R.T.: 5.010 min
Delta R.T.: 0.000 min
Response: 42173520
Conc: 243.89 ng/ml

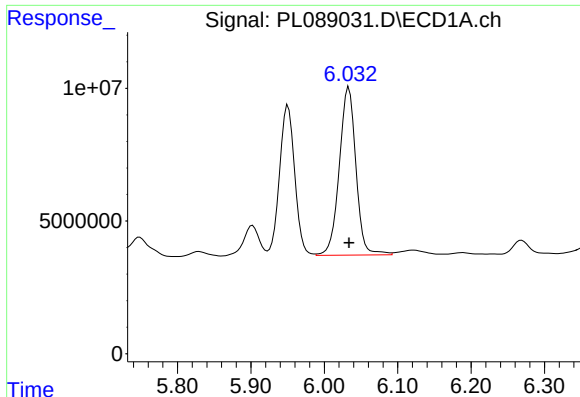

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 99805205
Conc: 265.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

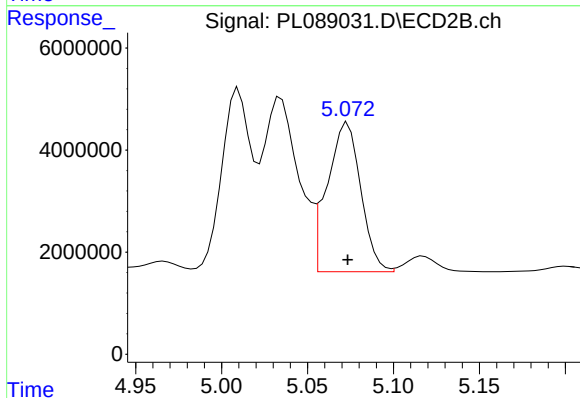


#26 Chlordane-4

R.T.: 5.073 min
Delta R.T.: 0.000 min
Response: 39601867
Conc: 246.21 ng/ml

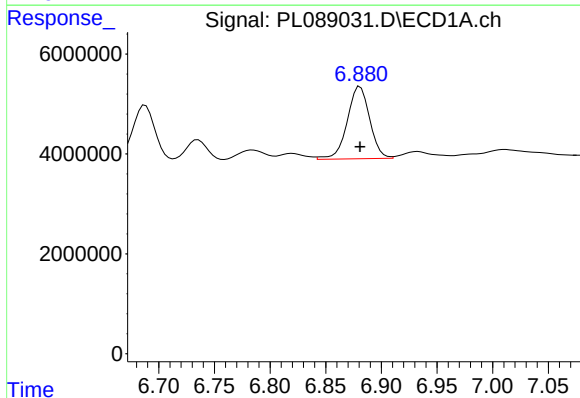


#27 Chlordane-5

R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 20323879
Conc: 274.58 ng/ml

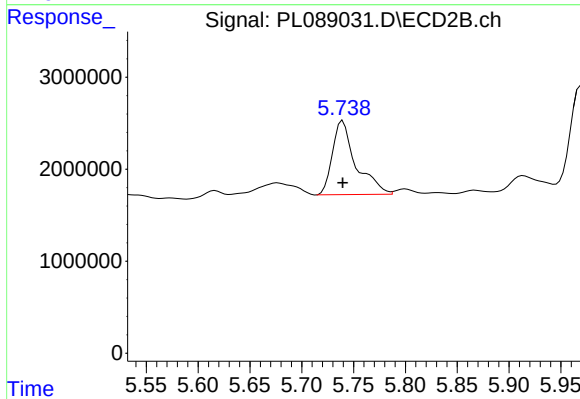

#27 Chlordane-5


R.T.: 5.740 min
Delta R.T.: 0.000 min
Response: 12632007
Conc: 257.43 ng/ml

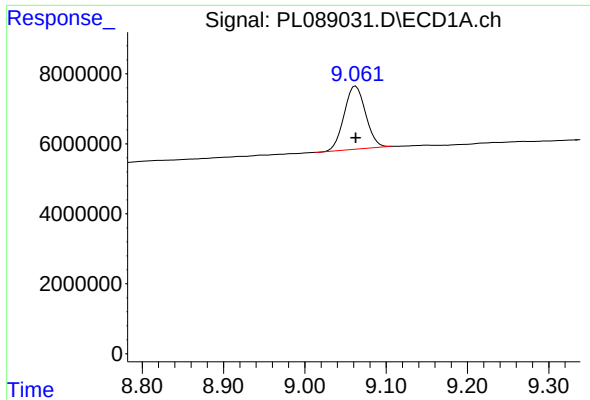

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: 0.000 min
Response: 32910377
Conc: 25.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

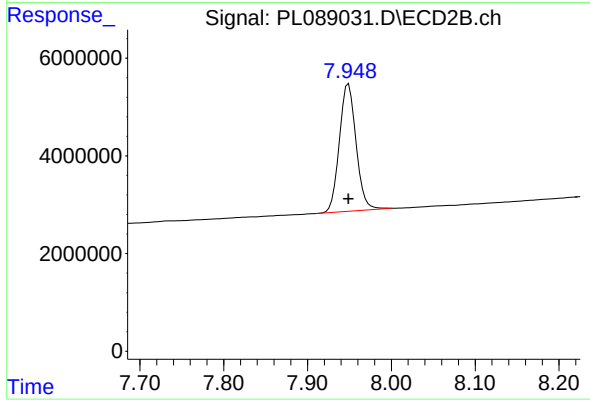

#28 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 36325172
Conc: 25.80 ng/ml