

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041525\
 Data File : PL095223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2025 10:24
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 12:00:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 14 19:12:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.680	0.000	25214301	0	7.853	N.D. #
10) B	gamma-Chl...	5.953f	0.000	10345459	0	3.097	N.D. #
14) MA	Endrin	0.000	5.646f	0	27534763	N.D.	6.591 #
23)	Chlordane-1	4.686	0.000	34041448	0	261.841	N.D. #
25)	Chlordane-3	5.953	0.000	10345459	0	21.104	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041525\
Data File : PL095223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2025 10:24
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 12:00:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
Quant Title : GC Extractables
QLast Update : Mon Apr 14 19:12:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

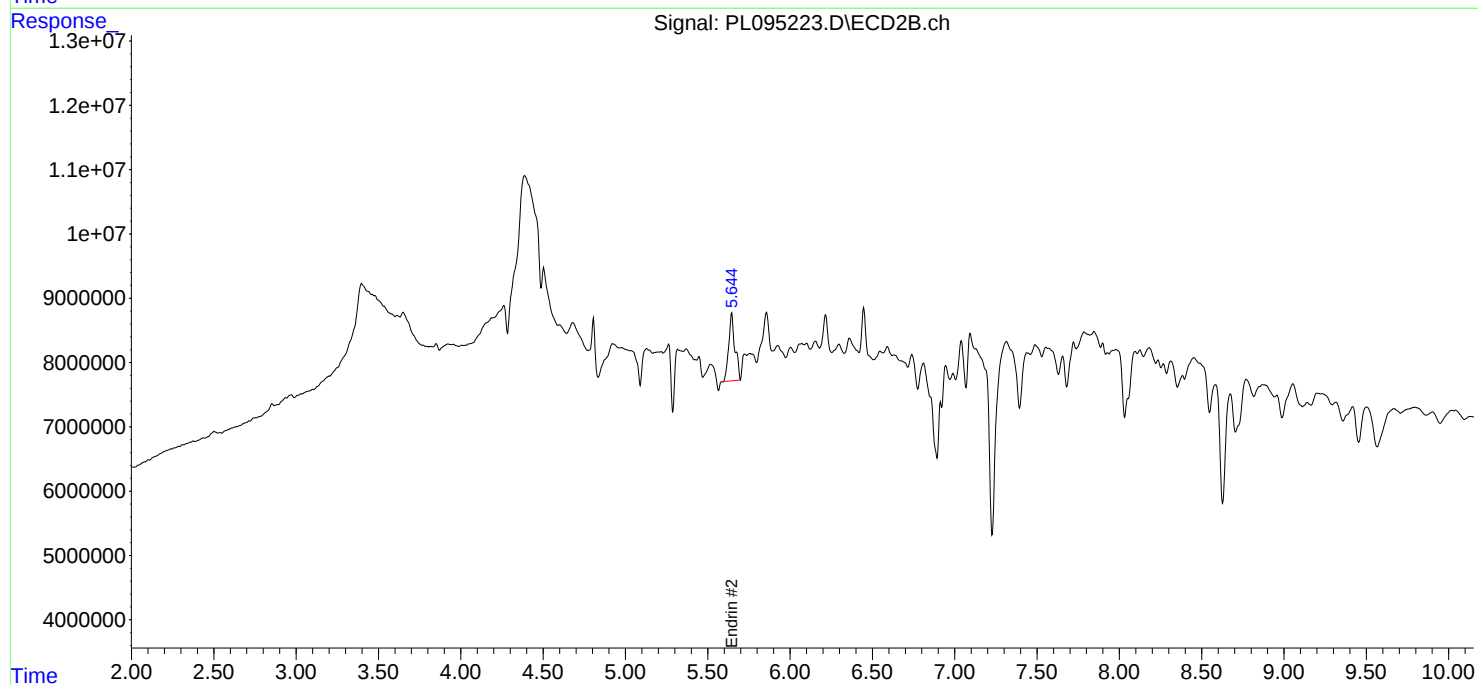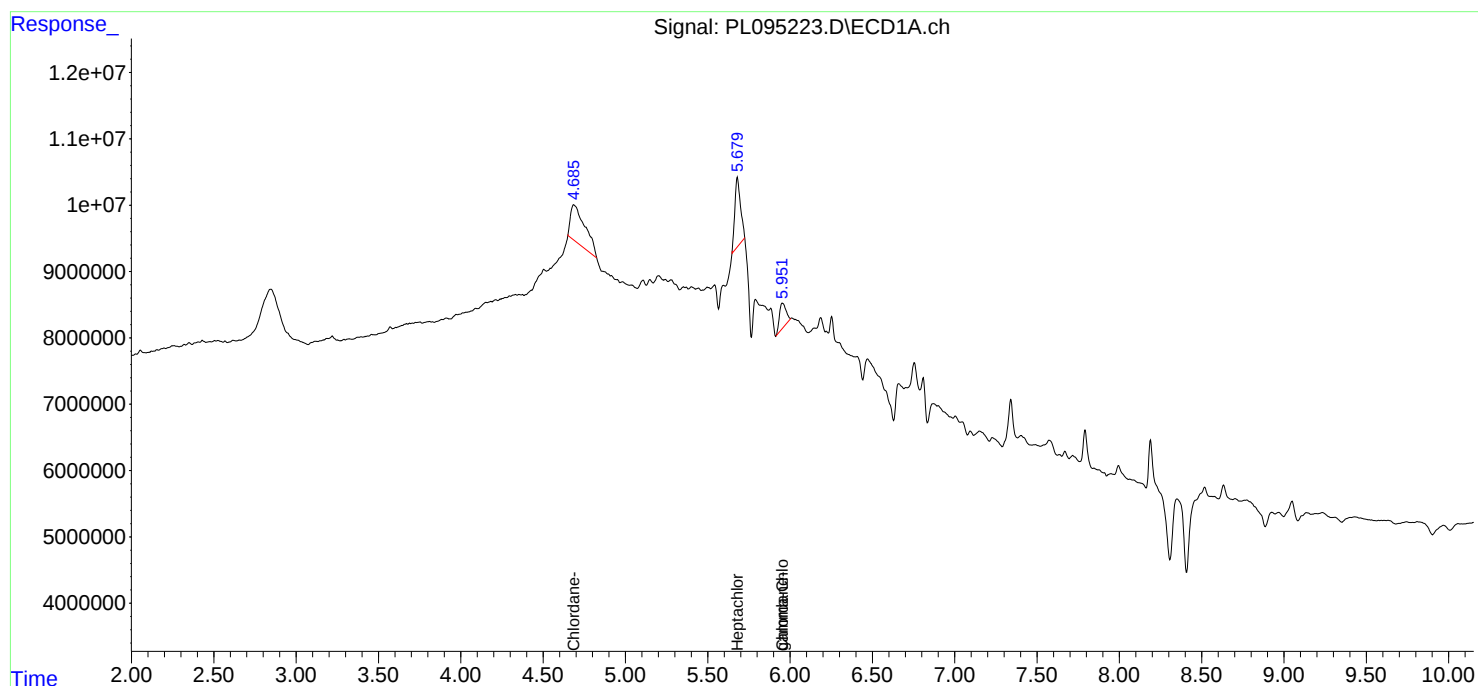


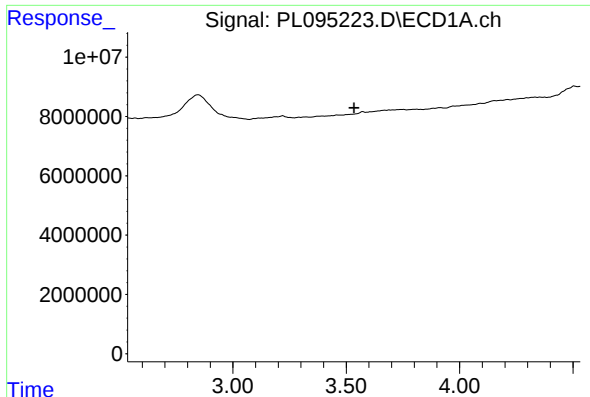

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.535 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

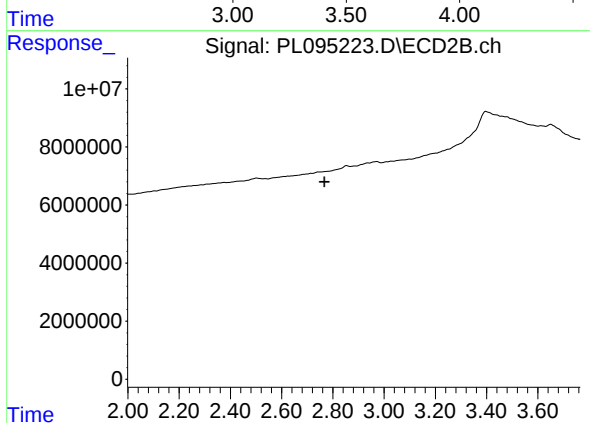


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.767 min
Response: 0
Conc: N.D.

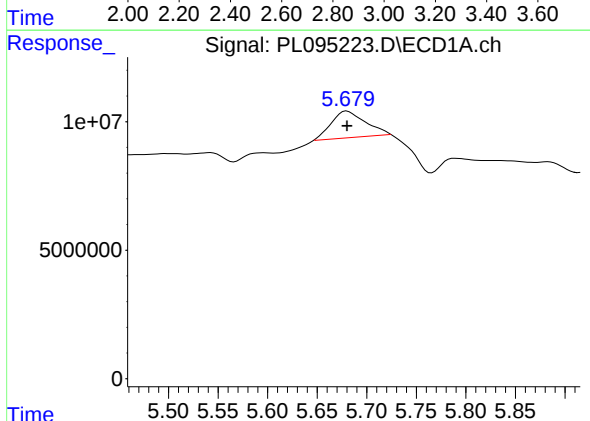


#8 Heptachlor epoxide

R.T.: 5.680 min
Delta R.T.: 0.000 min
Response: 25214301
Conc: 7.85 ng/ml

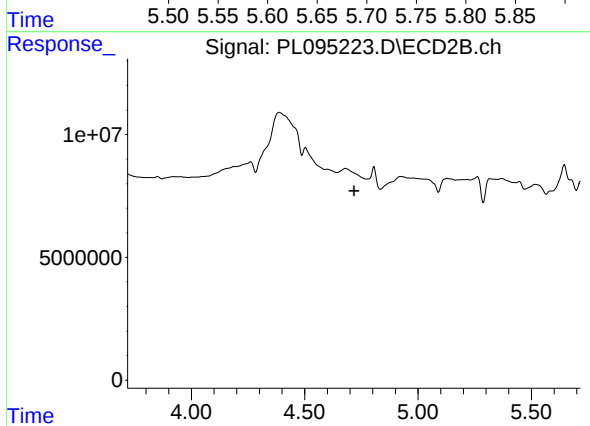

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.718 min
Response: 0
Conc: N.D.

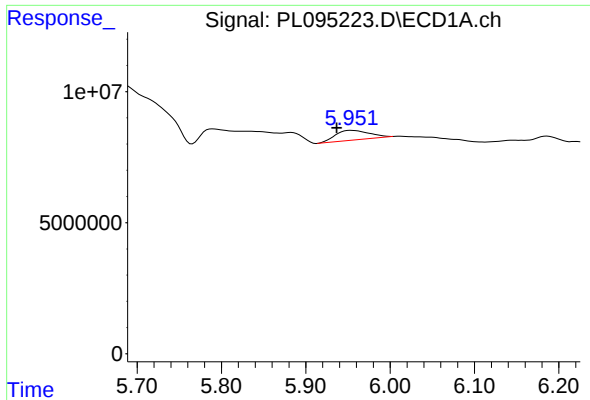

#10 gamma-Chlordane


R.T.: 5.953 min
Delta R.T.: 0.016 min
Response: 10345459
Conc: 3.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

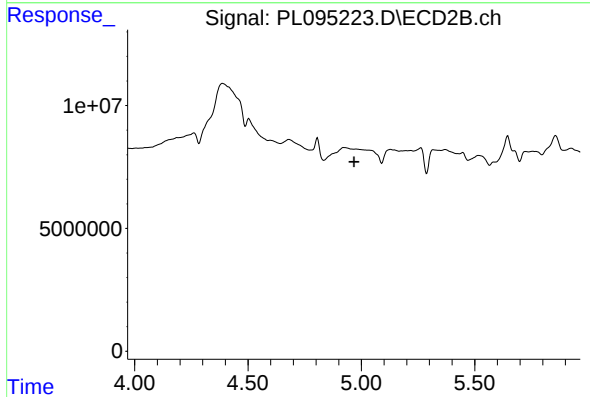


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.968 min
Response: 0
Conc: N.D.

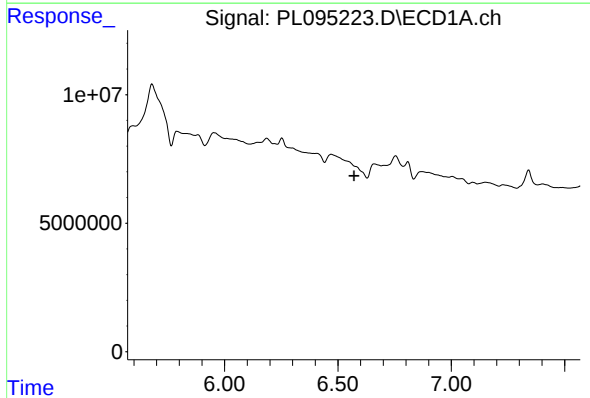


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.571 min
Response: 0
Conc: N.D.

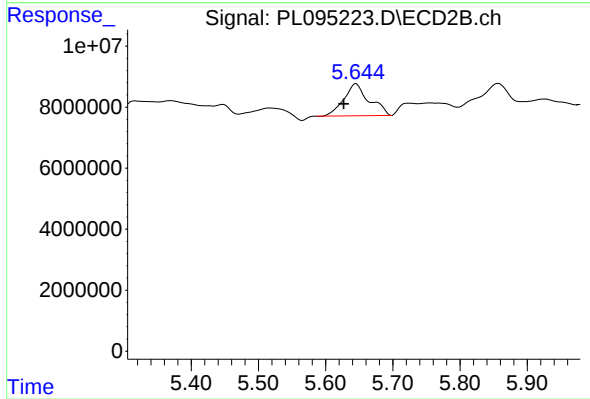

#14 Endrin


R.T.: 5.646 min
Delta R.T.: 0.019 min
Response: 27534763
Conc: 6.59 ng/ml

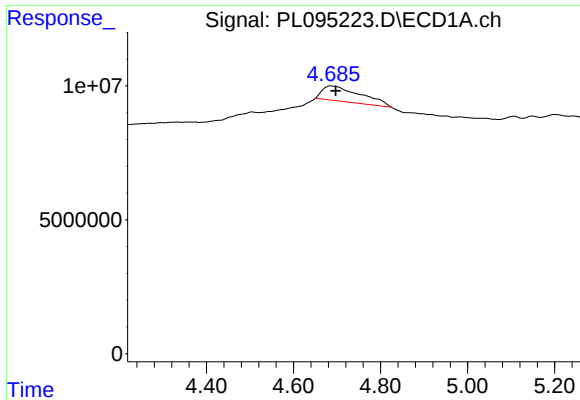

#23 Chlordane-1


R.T.: 4.686 min
Delta R.T.: -0.011 min
Response: 34041448
Conc: 261.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

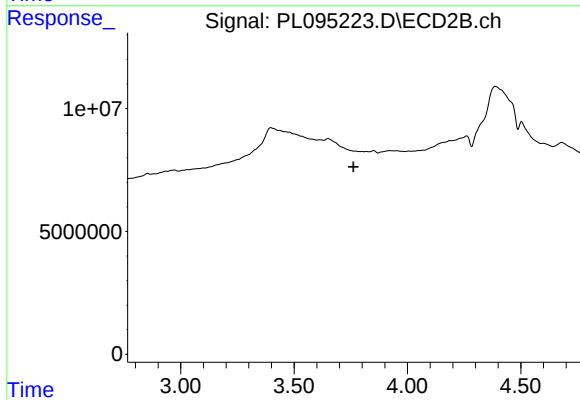


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 3.763 min
Response: 0
Conc: N.D.

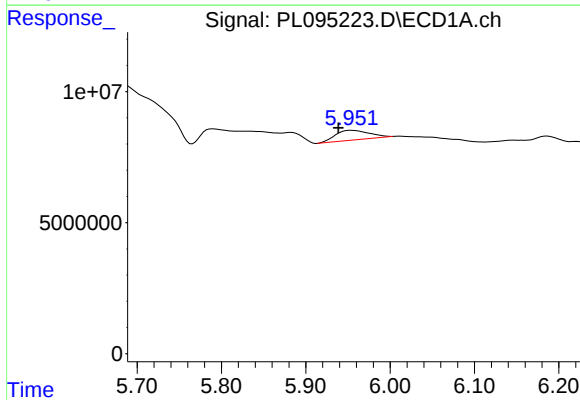


#25 Chlordane-3

R.T.: 5.953 min
Delta R.T.: 0.014 min
Response: 10345459
Conc: 21.10 ng/ml

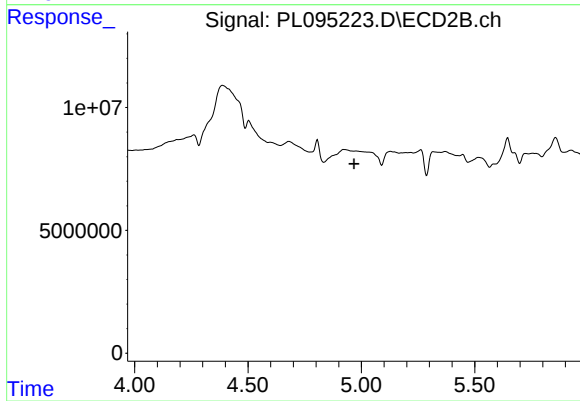

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.968 min
Response: 0
Conc: N.D.

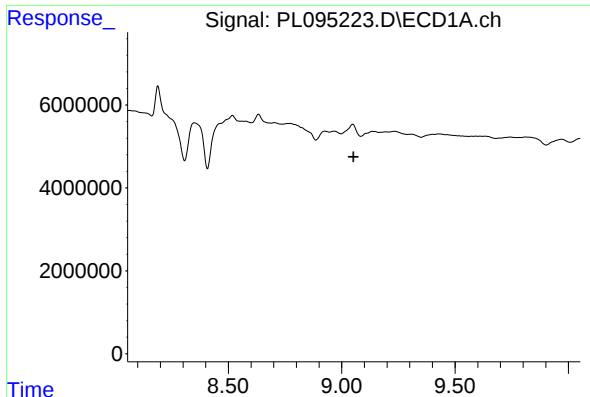

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

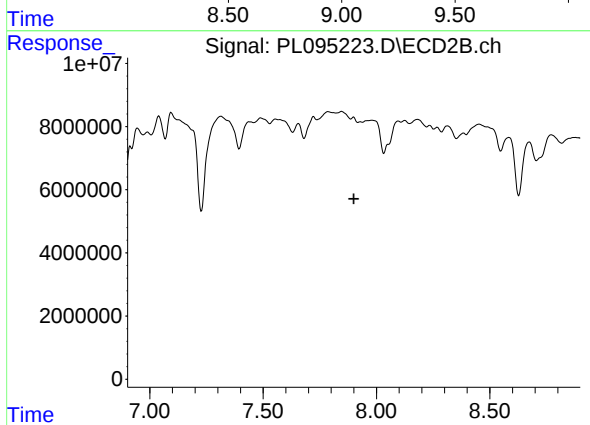

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.900 min
Response: 0
Conc: N.D.