

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041525\
 Data File : PL095238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2025 15:40
 Operator : AR\AJ
 Sample : Q1787-09 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:24:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 14 19:12:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.768	27575371	14627140	10.052	3.931 #
28)	SA Decachlor...	9.059	7.904	11011990	14112607	4.574	3.208 #
Target Compounds							
7)	B delta-BHC	4.767	0.000	5509290	0	1.406	N.D. #
10)	B gamma-Chl...	5.933	0.000	7152250	0	2.141	N.D. #
12)	B 4,4'-DDE	0.000	5.223	0	14015641	N.D.	2.911 #
25)	Chlordane-3	5.933	0.000	7152250	0	14.590	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041525\
Data File : PL095238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2025 15:40
Operator : AR\AJ
Sample : Q1787-09 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:24:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
Quant Title : GC Extractables
QLast Update : Mon Apr 14 19:12:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

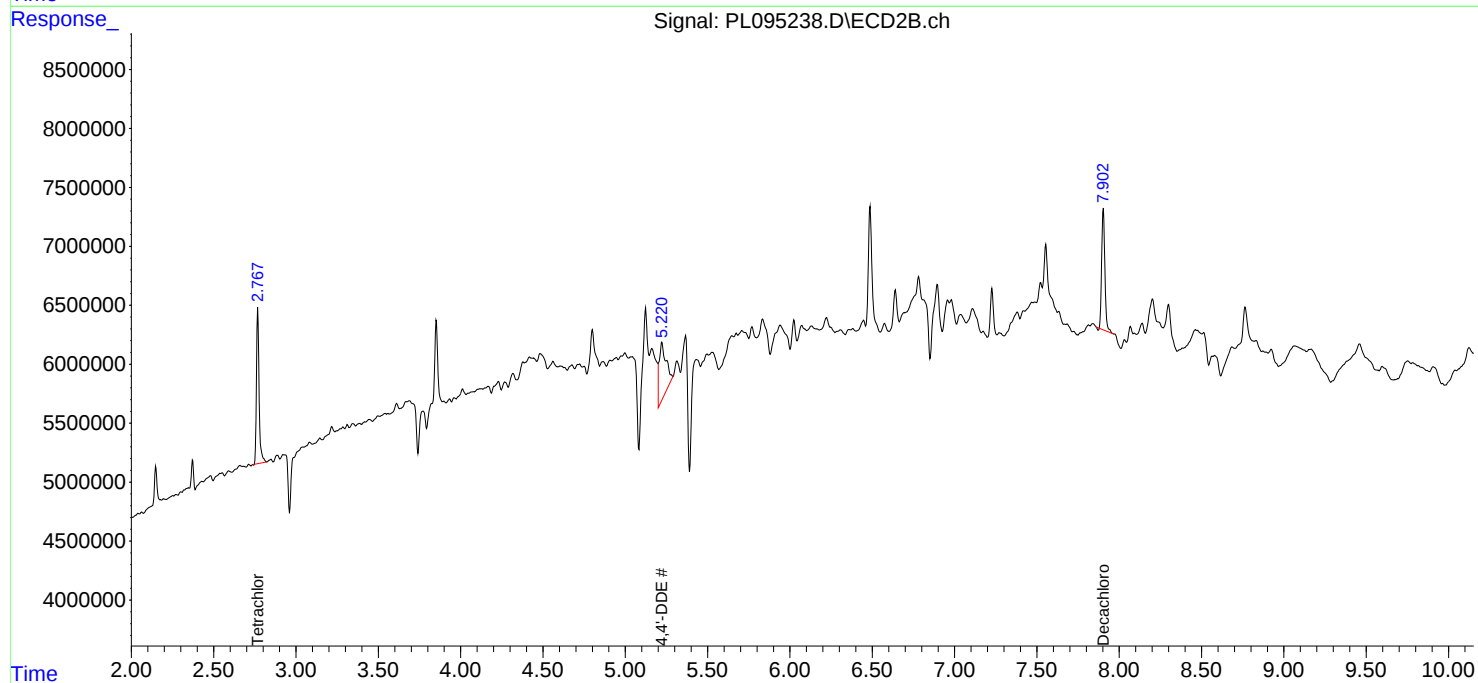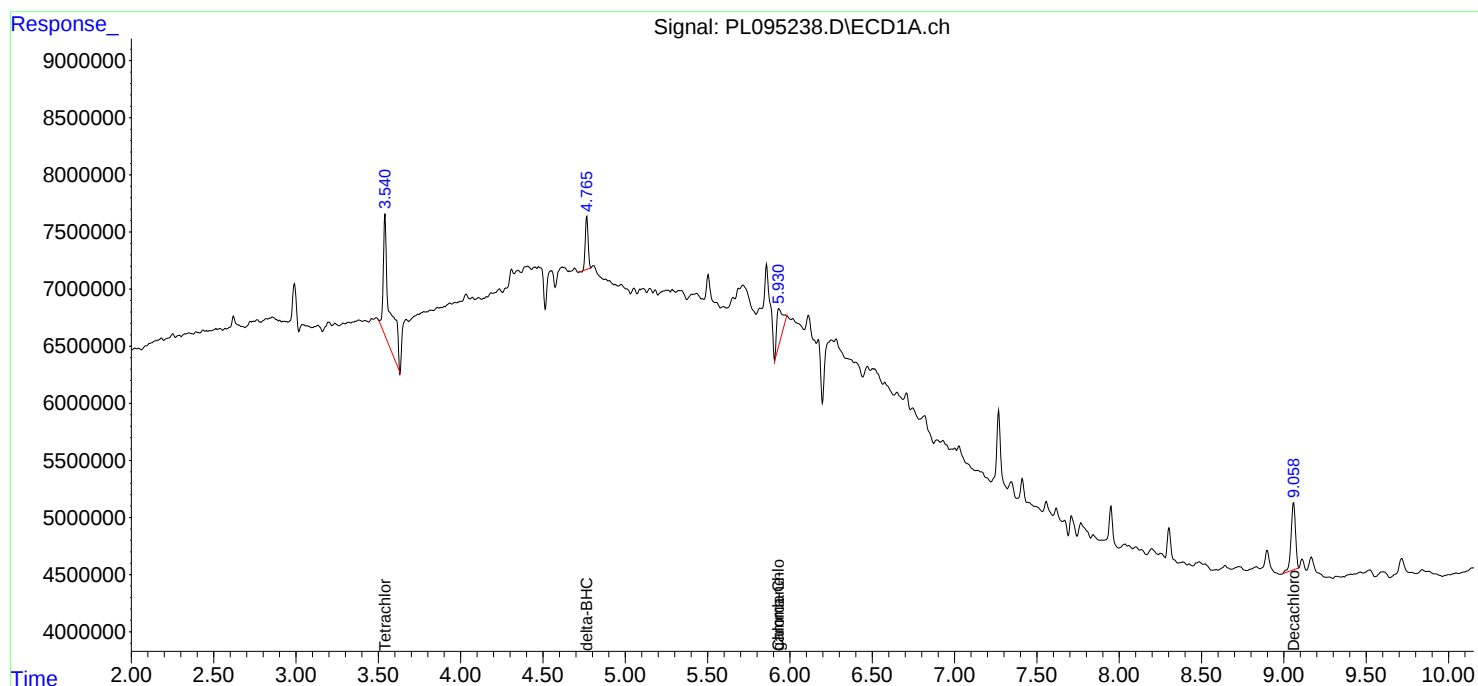


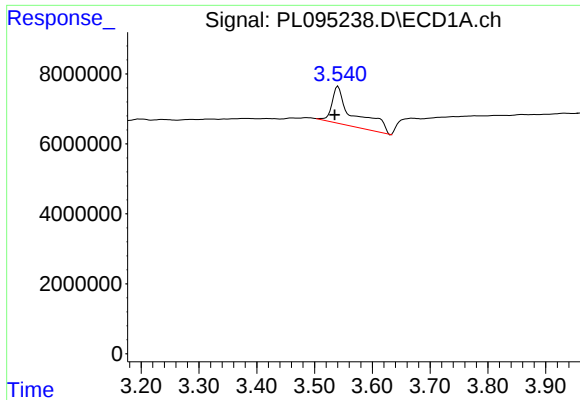

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.006 min
Response: 27575371
Conc: 10.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

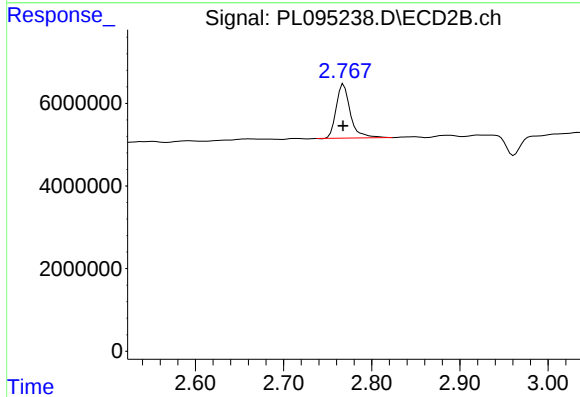


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 14627140
Conc: 3.93 ng/ml

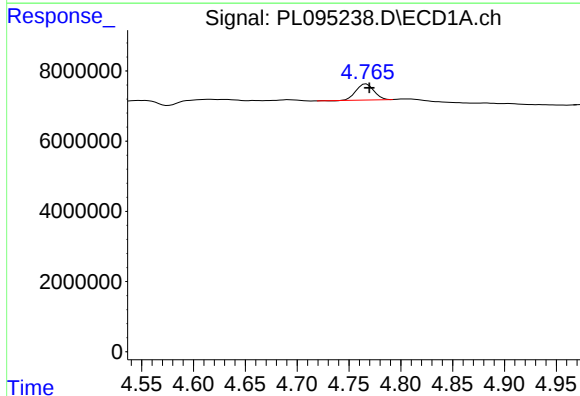


#7 delta-BHC

R.T.: 4.767 min
Delta R.T.: -0.003 min
Response: 5509290
Conc: 1.41 ng/ml

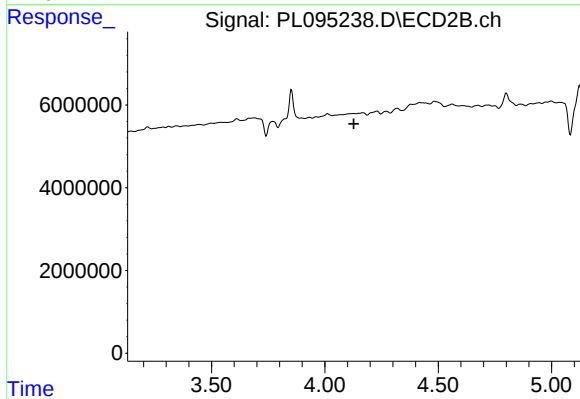

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.128 min
Response: 0
Conc: N.D.

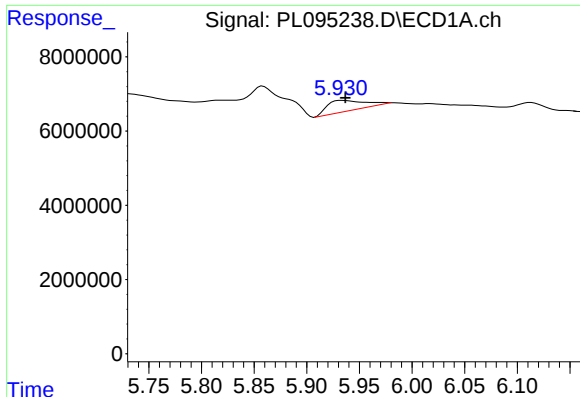

#10 gamma-Chlordane


R.T.: 5.933 min
Delta R.T.: -0.004 min
Response: 7152250
Conc: 2.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

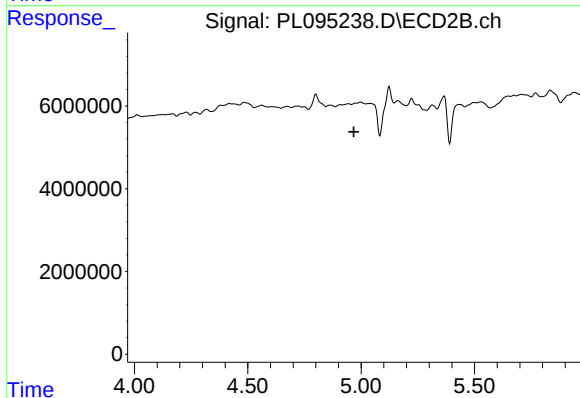


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.968 min
Response: 0
Conc: N.D.

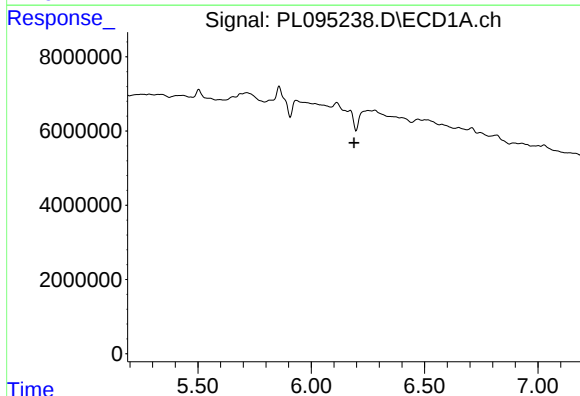


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.190 min
Response: 0
Conc: N.D.

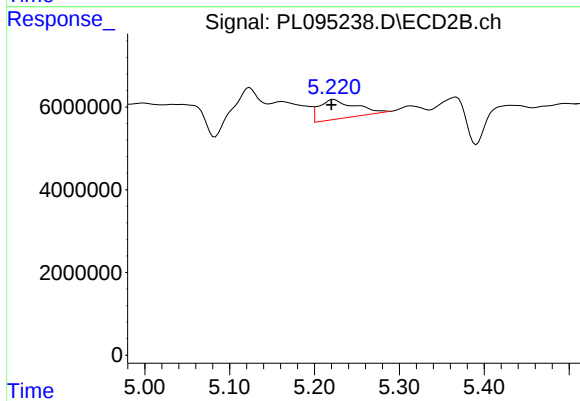

#12 4,4'-DDE


R.T.: 5.223 min
Delta R.T.: 0.003 min
Response: 14015641
Conc: 2.91 ng/ml

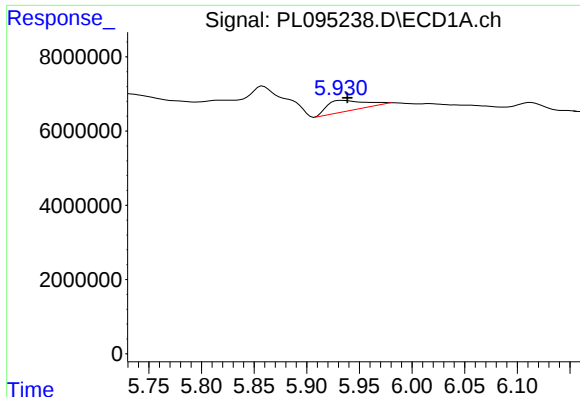

#25 Chlordane-3


R.T.: 5.933 min
Delta R.T.: -0.006 min
Response: 7152250
Conc: 14.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

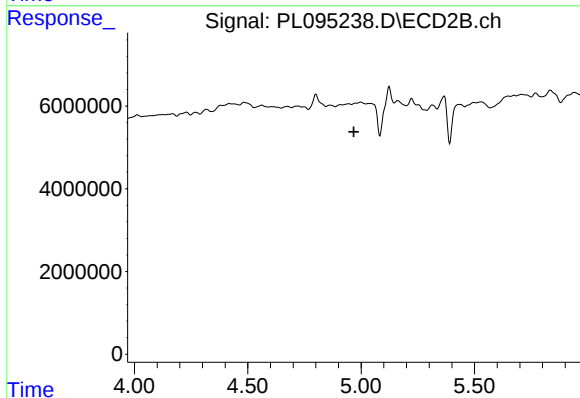


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.968 min
Response: 0
Conc: N.D.

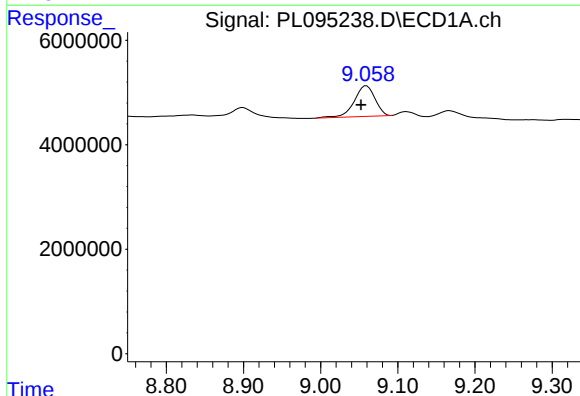

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: 0.007 min
Response: 11011990
Conc: 4.57 ng/ml

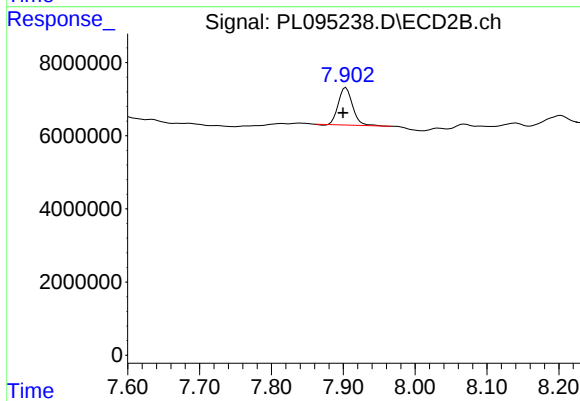

#28 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: 0.004 min
Response: 14112607
Conc: 3.21 ng/ml