

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041525\
 Data File : PL095244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2025 17:02
 Operator : AR\AJ
 Sample : Q1806-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-041425

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:25:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 14 19:12:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.768	28381750	44851643	10.346	12.053
28)	SA Decachlor...	9.055	7.901	23987283	35752840	9.963	8.127
Target Compounds							
4)	MA Heptachlor	0.000	3.931	0	16961027	N.D.	3.262 #
5)	MB Aldrin	0.000	4.219	0	10689336	N.D.	2.193 #
10)	B gamma-Chl...	5.937	4.991f	21094129	34640371	6.315	7.192
11)	B alpha-Chl...	6.019	5.032	14312038	42116880	4.312	8.886 #
12)	B 4,4'-DDE	0.000	5.220	0	33224657	N.D.	6.901 #
24)	Chlordane-2	0.000	4.374f	0	14573625	N.D.	84.044 #
25)	Chlordane-3	5.937	4.991f	21094129	34640371	43.030	68.687 #
26)	Chlordane-4	6.019	5.032	14312038	42116880	24.714	84.417 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041525\
Data File : PL095244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2025 17:02
Operator : AR\AJ
Sample : Q1806-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-03-041425

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:25:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
Quant Title : GC Extractables
QLast Update : Mon Apr 14 19:12:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

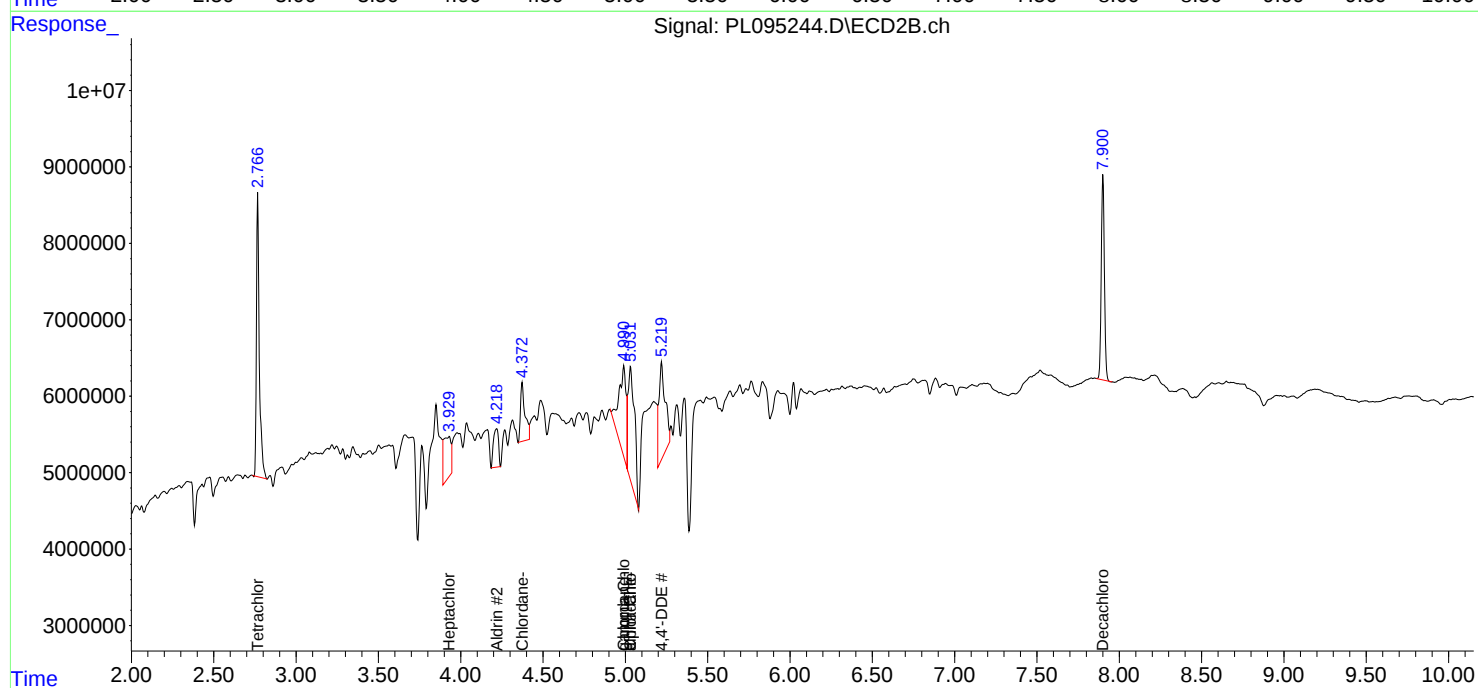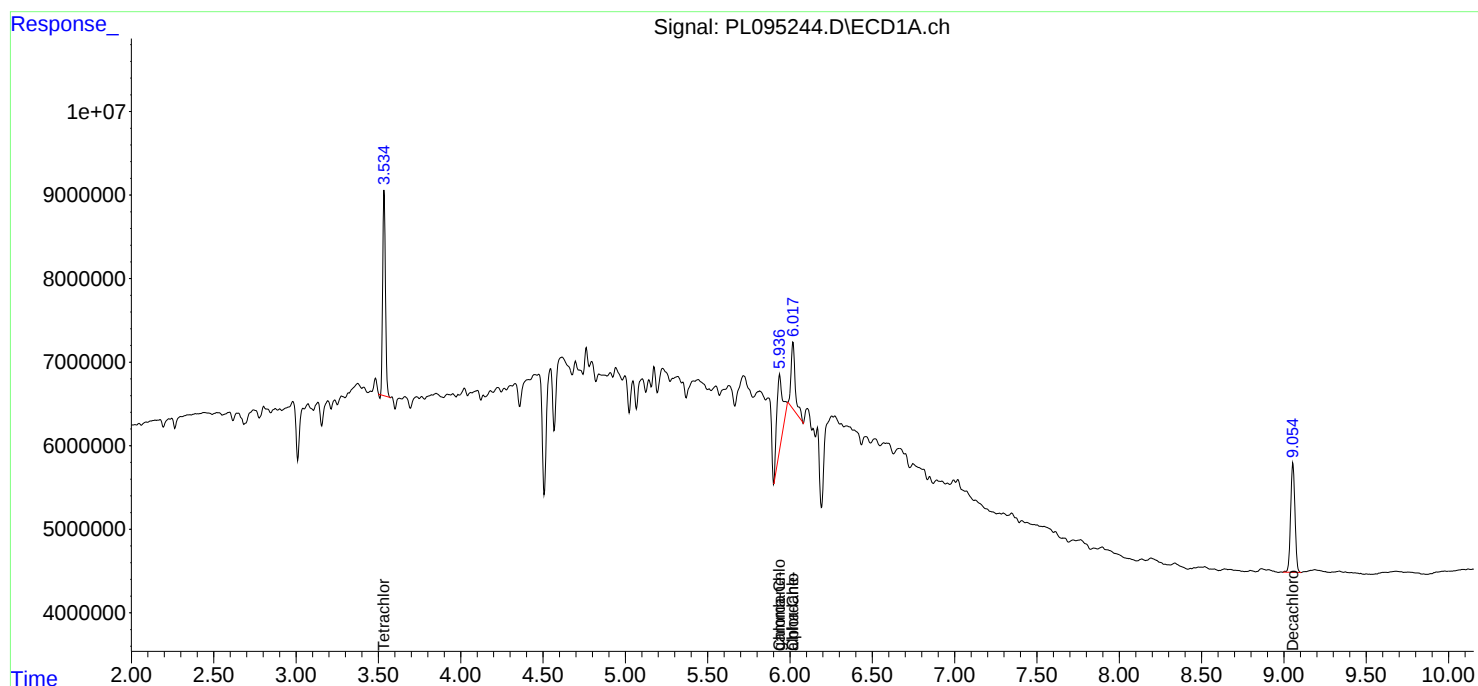


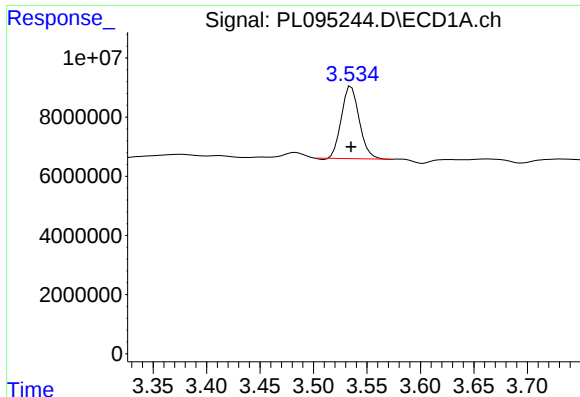

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 28381750
Conc: 10.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-041425

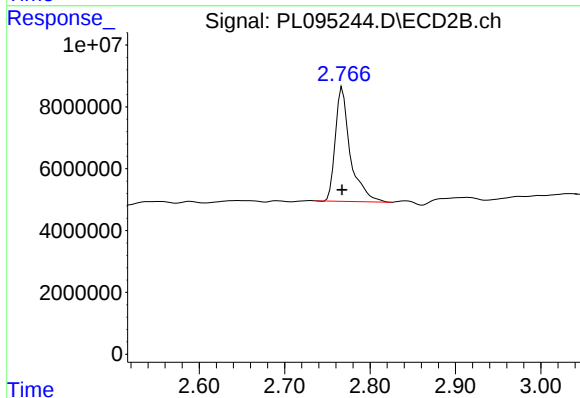


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 44851643
Conc: 12.05 ng/ml

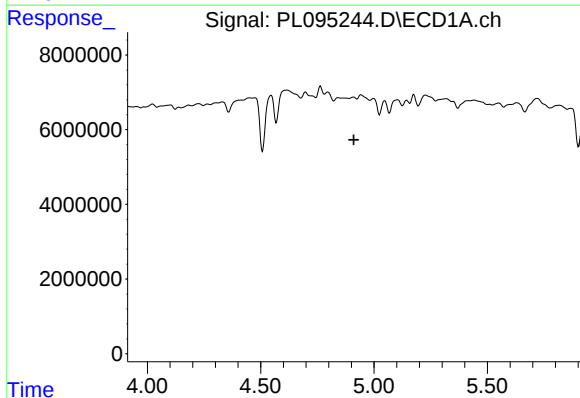


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.911 min
Response: 0
Conc: N.D.

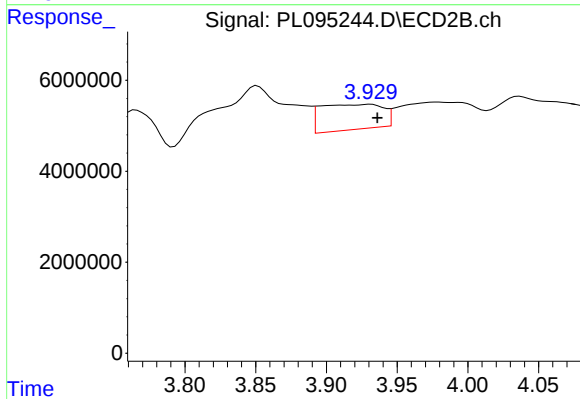

#4 Heptachlor


R.T.: 3.931 min
Delta R.T.: -0.005 min
Response: 16961027
Conc: 3.26 ng/ml

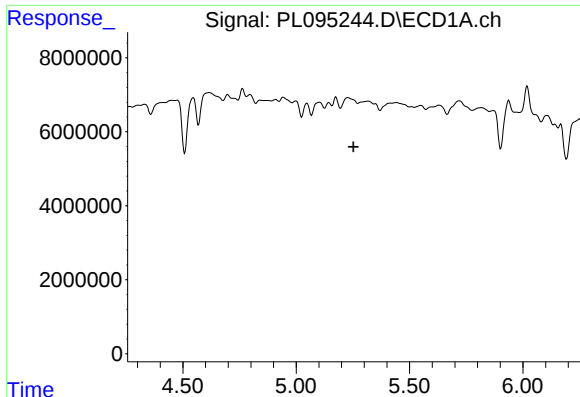

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-03-041425

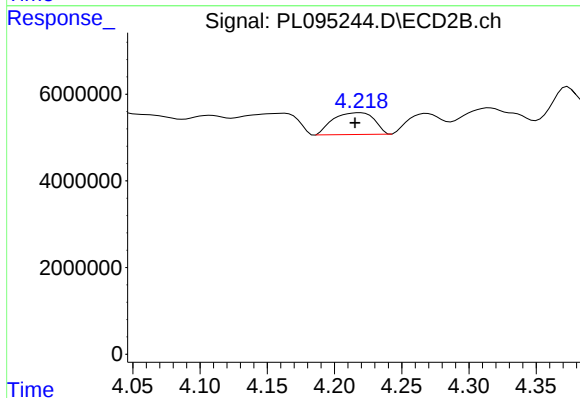


#5 Aldrin

R.T.: 4.219 min
Delta R.T.: 0.004 min
Response: 10689336
Conc: 2.19 ng/ml

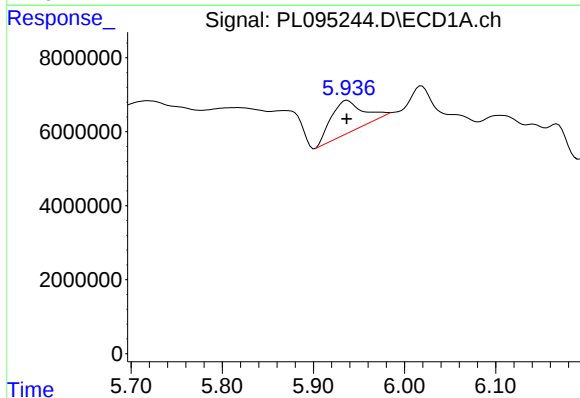


#10 gamma-Chlordane

R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 21094129
Conc: 6.31 ng/ml

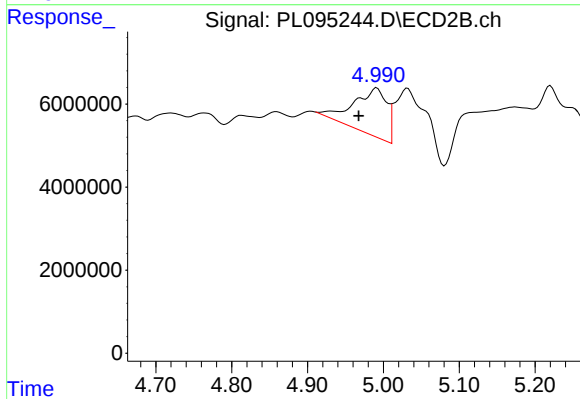

#10 gamma-Chlordane


R.T.: 4.991 min
Delta R.T.: 0.024 min
Response: 34640371
Conc: 7.19 ng/ml

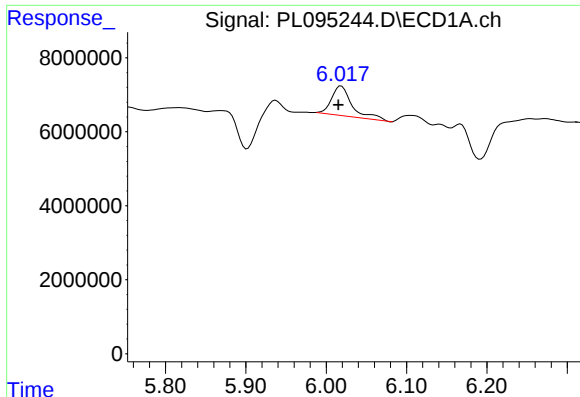

#11 alpha-Chlordane


R.T.: 6.019 min
Delta R.T.: 0.004 min
Response: 14312038
Conc: 4.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-041425

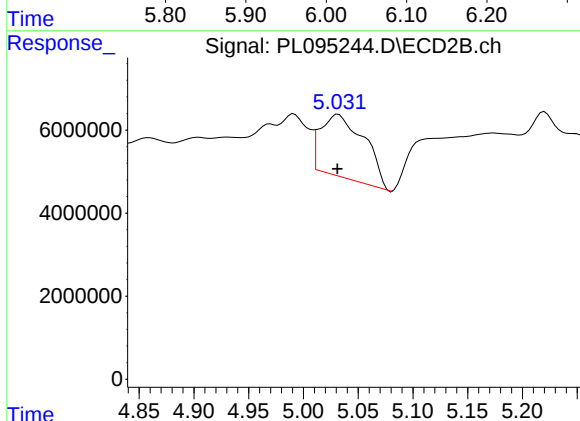


#11 alpha-Chlordane

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 42116880
Conc: 8.89 ng/ml

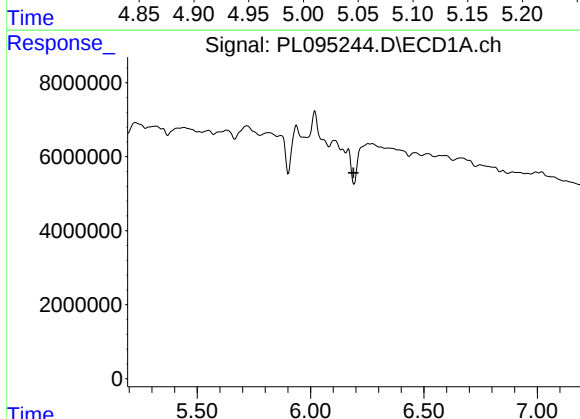


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.190 min
Response: 0
Conc: N.D.

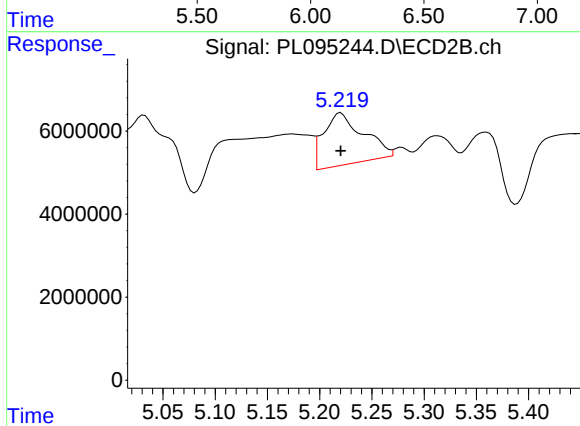

#12 4,4'-DDE


R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 33224657
Conc: 6.90 ng/ml

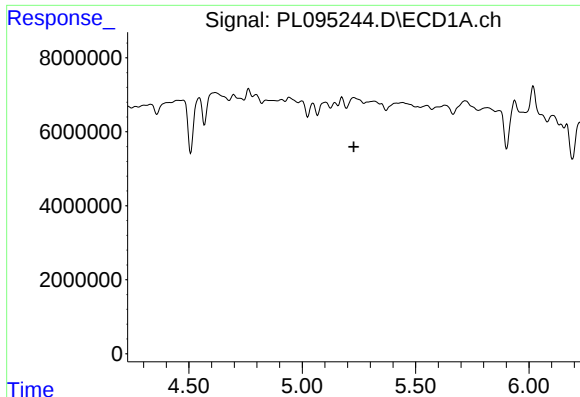

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.228 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-03-041425

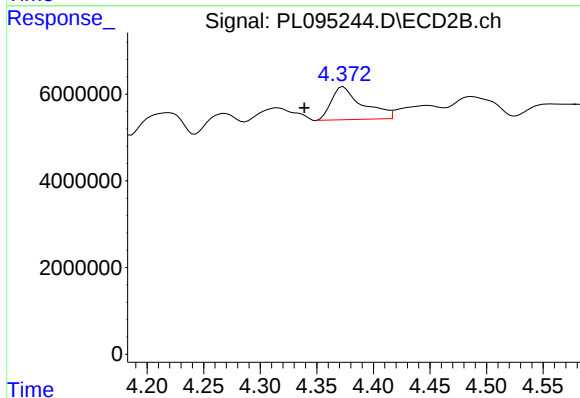


#24 Chlordane-2

R.T.: 4.374 min
Delta R.T.: 0.035 min
Response: 14573625
Conc: 84.04 ng/ml

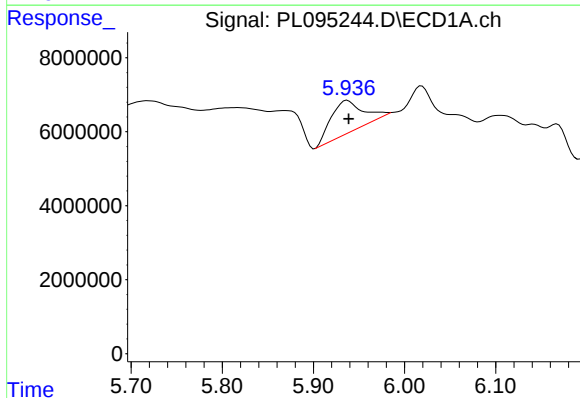


#25 Chlordane-3

R.T.: 5.937 min
Delta R.T.: -0.001 min
Response: 21094129
Conc: 43.03 ng/ml

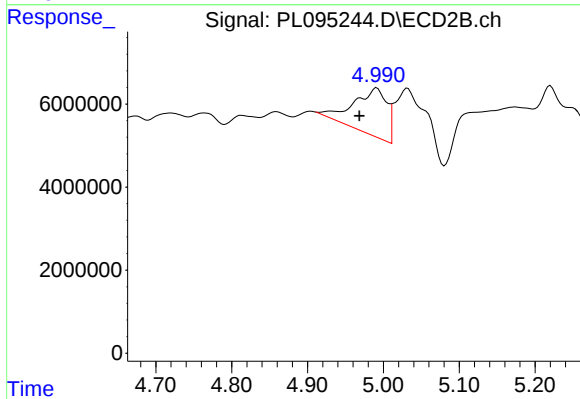

#25 Chlordane-3


R.T.: 4.991 min
Delta R.T.: 0.023 min
Response: 34640371
Conc: 68.69 ng/ml

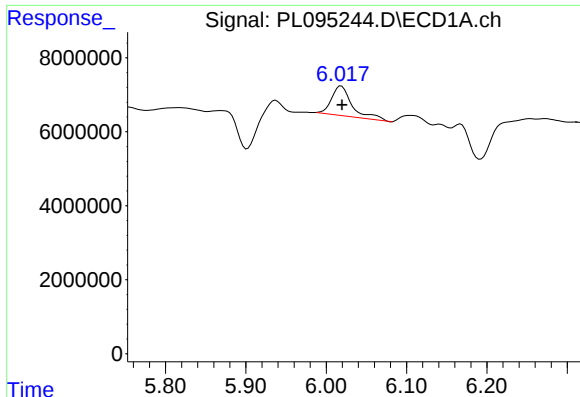

#26 Chlordane-4


R.T.: 6.019 min
Delta R.T.: -0.001 min
Response: 14312038
Conc: 24.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-041425

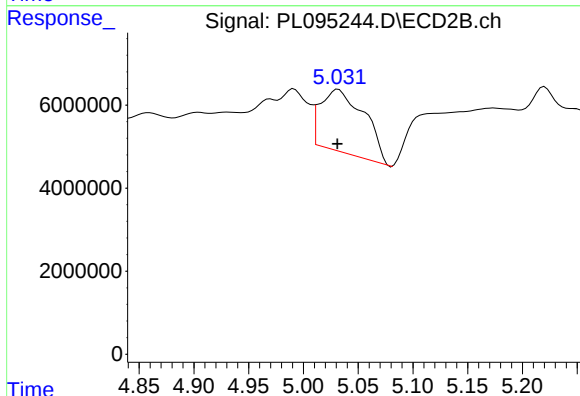


#26 Chlordane-4

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 42116880
Conc: 84.42 ng/ml

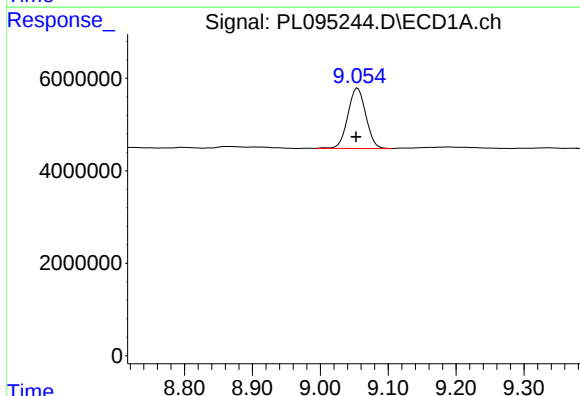

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.002 min
Response: 23987283
Conc: 9.96 ng/ml

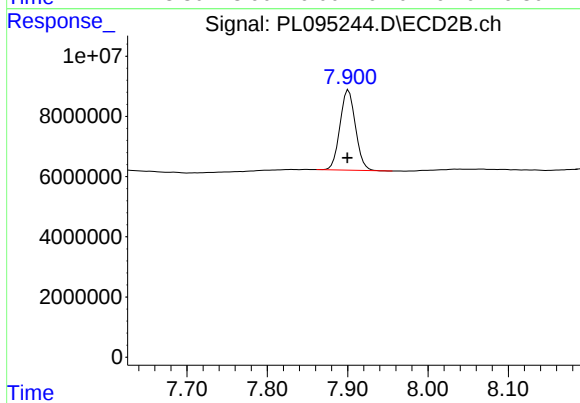

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: 0.002 min
Response: 35752840
Conc: 8.13 ng/ml