

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041525\
 Data File : PL095249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2025 18:10
 Operator : AR\AJ
 Sample : Q1808-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LAW-25-0060

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:26:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 14 19:12:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.768	45532748	56214092	16.598	15.106
28)	SA Decachlor...	9.054	7.901	26154024	42349093	10.863	9.627
Target Compounds							
6)	B beta-BHC	0.000	3.905	0	6525203	N.D.	2.816 #
7)	B delta-BHC	4.762	0.000	21971515	0	5.607	N.D. #
10)	B gamma-Chl...	5.921f	0.000	6658818	0	1.993	N.D. #
12)	B 4,4'-DDE	0.000	5.221	0	4752672	N.D.	0.987 #
15)	B Endosulfa...	0.000	5.909	0	17177974	N.D.	3.913 #
17)	MA 4,4'-DDT	7.019	6.028	6717975	8361115	2.639	2.007
18)	B Endrin al...	0.000	6.105	0	4268458	N.D.	1.267 #
19)	B Endosulfa...	0.000	6.343f	0	1572949	N.D.	0.377 #
20)	A Methoxychlor	0.000	6.613	0	5218273	N.D.	2.324 #
21)	B Endrin ke...	7.635	0.000	12913381	0	4.473	N.D. #
25)	Chlordane-3	5.921f	0.000	6658818	0	13.583	N.D. #
27)	Chlordane-5	0.000	5.909	0	17177974	N.D.	91.942 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041525\
Data File : PL095249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2025 18:10
Operator : AR\AJ
Sample : Q1808-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LAW-25-0060

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:26:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
Quant Title : GC Extractables
QLast Update : Mon Apr 14 19:12:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

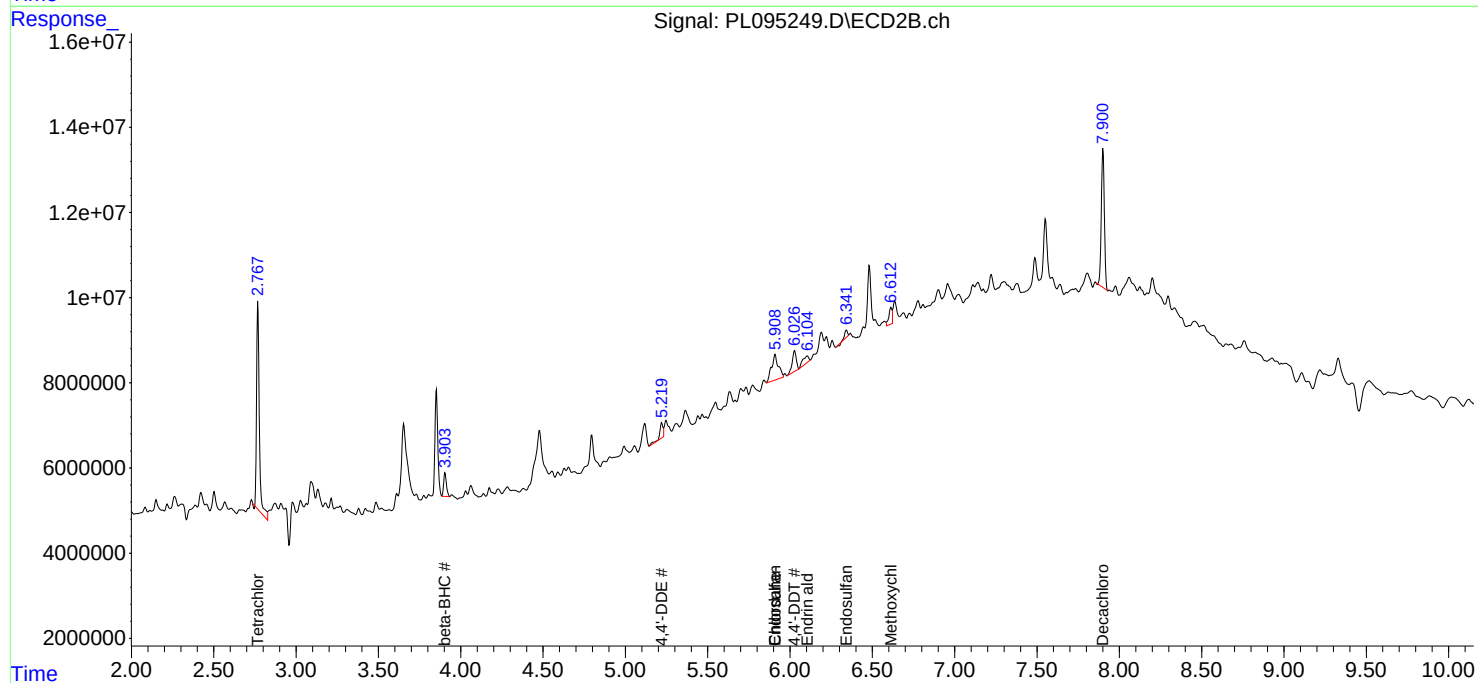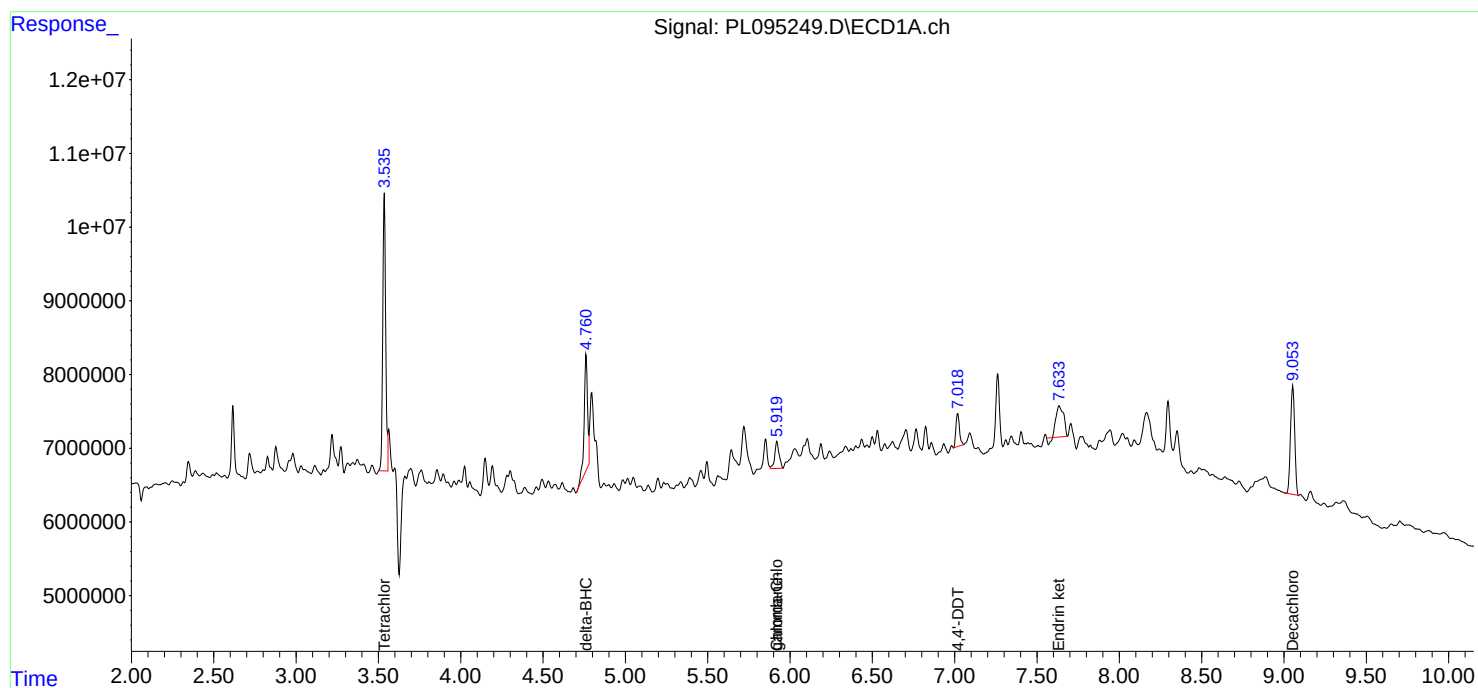


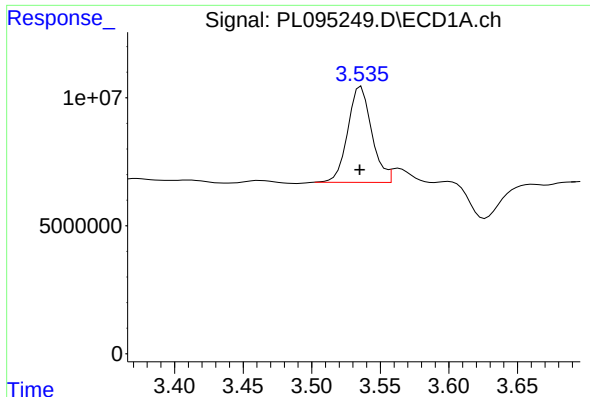

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: 0.001 min
Response: 45532748
Conc: 16.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
LAW-25-0060

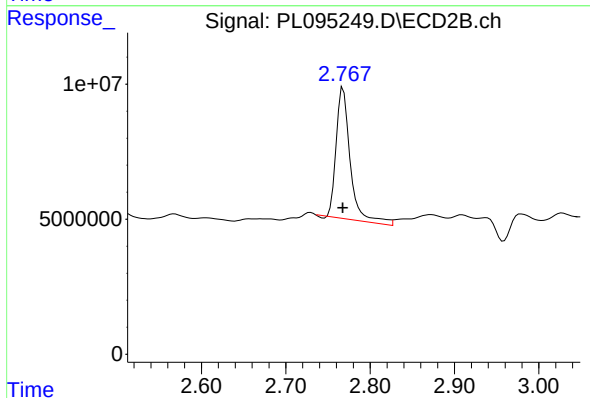


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 56214092
Conc: 15.11 ng/ml

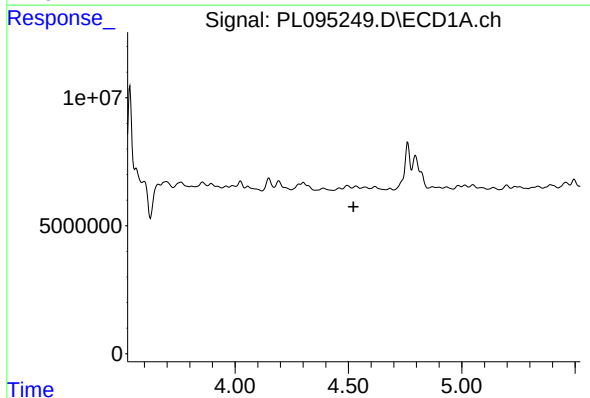


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.523 min
Response: 0
Conc: N.D.

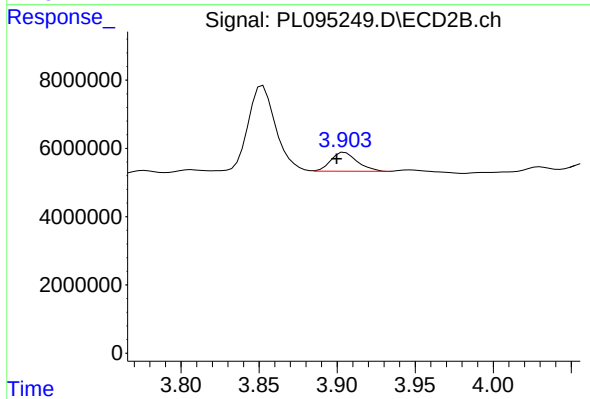

#6 beta-BHC


R.T.: 3.905 min
Delta R.T.: 0.005 min
Response: 6525203
Conc: 2.82 ng/ml

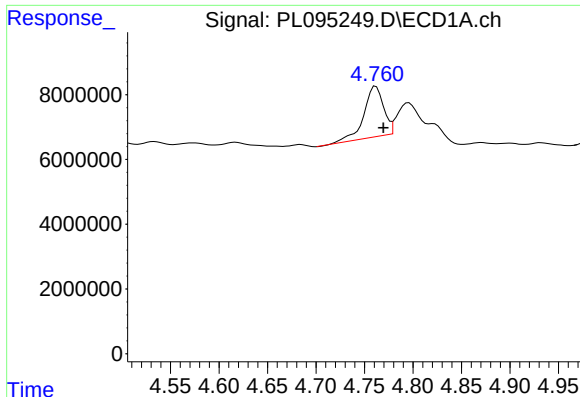

#7 delta-BHC


R.T.: 4.762 min
Delta R.T.: -0.008 min
Response: 21971515
Conc: 5.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
LAW-25-0060

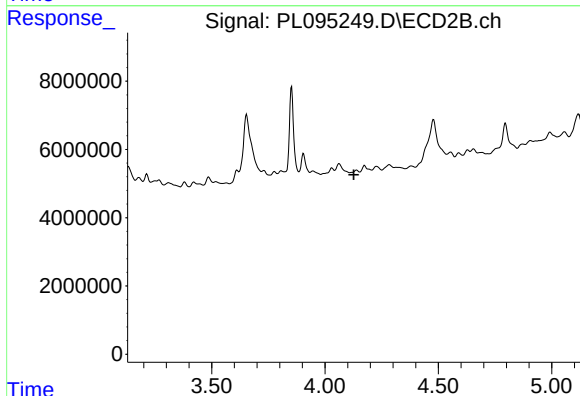


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.128 min
Response: 0
Conc: N.D.

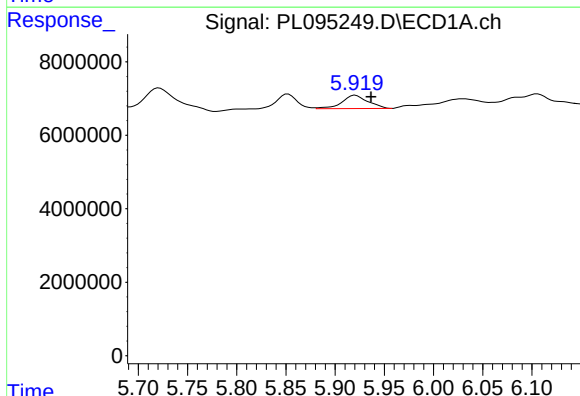


#10 gamma-Chlordane

R.T.: 5.921 min
Delta R.T.: -0.016 min
Response: 6658818
Conc: 1.99 ng/ml

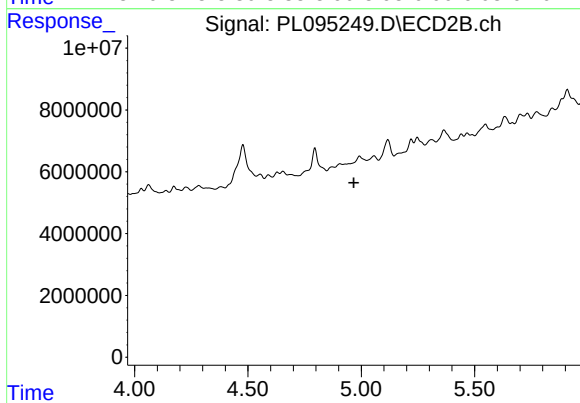

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.968 min
Response: 0
Conc: N.D.

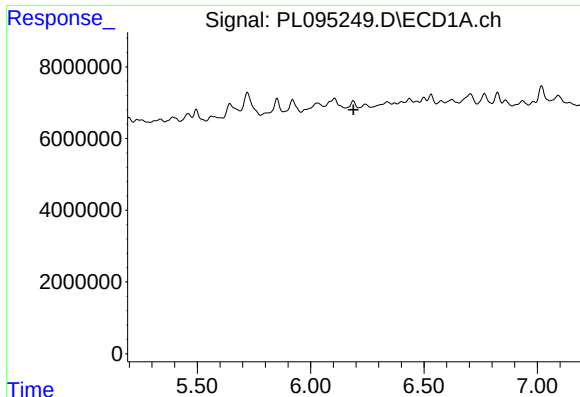

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
LAW-25-0060

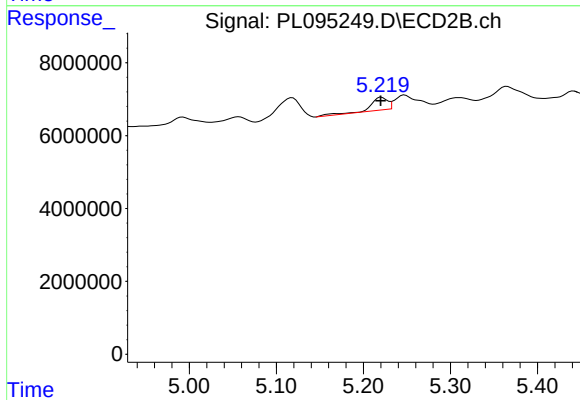


#12 4,4'-DDE

R.T.: 5.221 min
Delta R.T.: 0.000 min
Response: 4752672
Conc: 0.99 ng/ml

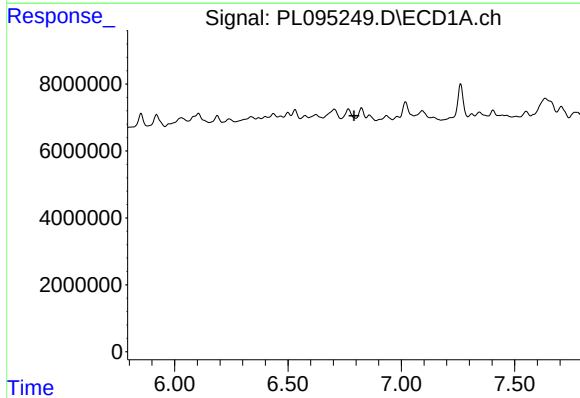


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.792 min
Response: 0
Conc: N.D.

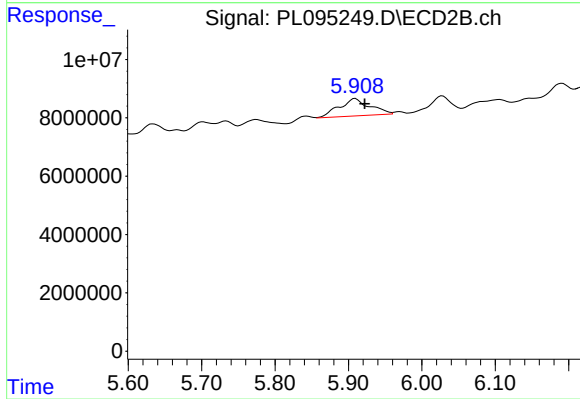

#15 Endosulfan II


R.T.: 5.909 min
Delta R.T.: -0.013 min
Response: 17177974
Conc: 3.91 ng/ml

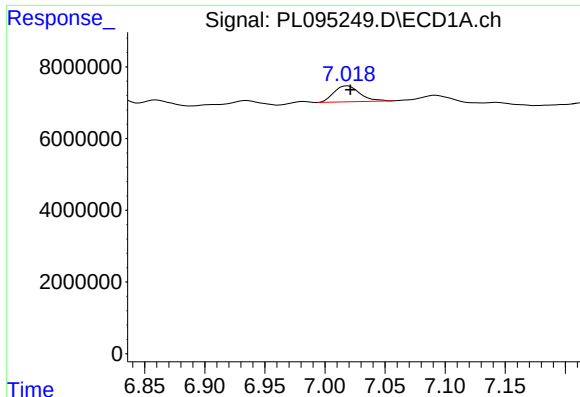

#17 4,4'-DDT


R.T.: 7.019 min
Delta R.T.: -0.002 min
Response: 6717975
Conc: 2.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
LAW-25-0060

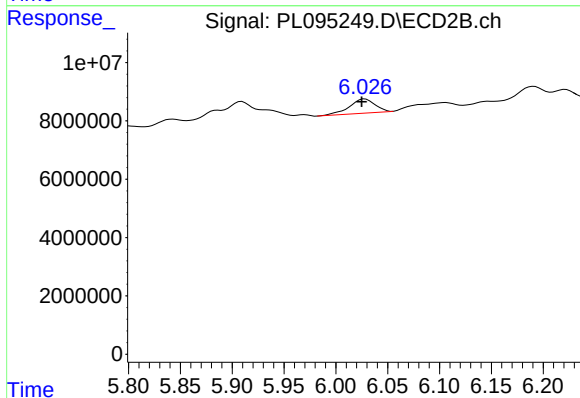


#17 4,4'-DDT

R.T.: 6.028 min
Delta R.T.: 0.003 min
Response: 8361115
Conc: 2.01 ng/ml

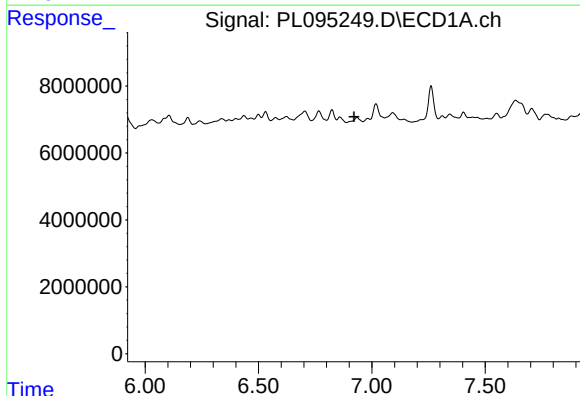


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

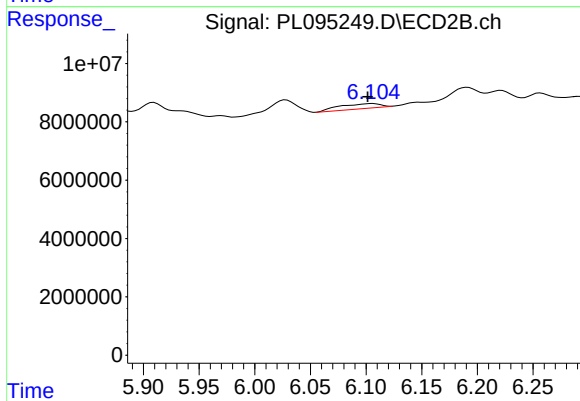

#18 Endrin aldehyde


R.T.: 6.105 min
Delta R.T.: 0.004 min
Response: 4268458
Conc: 1.27 ng/ml

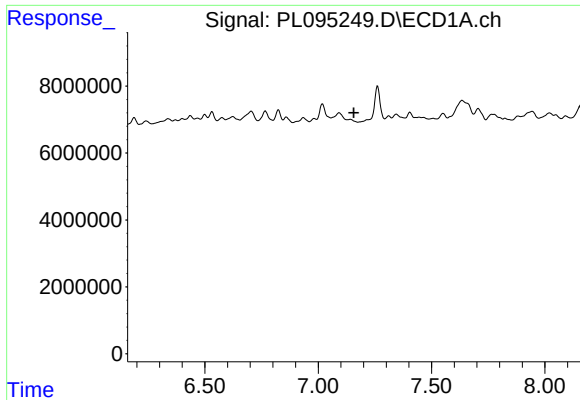

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.157 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
LAW-25-0060

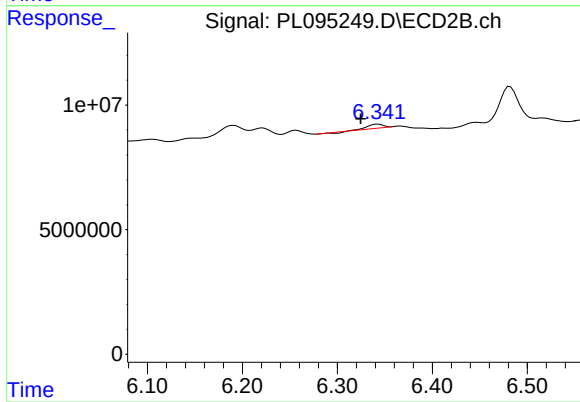


#19 Endosulfan Sulfate

R.T.: 6.343 min
Delta R.T.: 0.018 min
Response: 1572949
Conc: 0.38 ng/ml

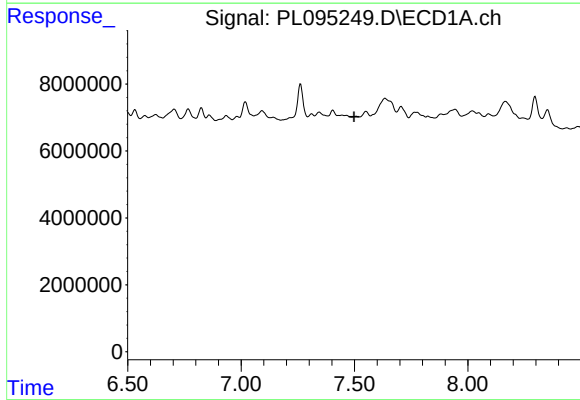


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.498 min
Response: 0
Conc: N.D.

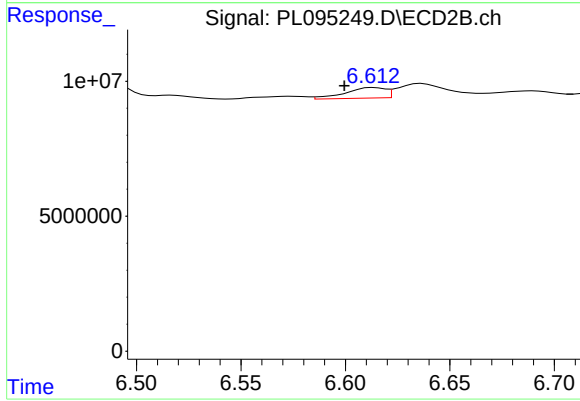

#20 Methoxychlor


R.T.: 6.613 min
Delta R.T.: 0.014 min
Response: 5218273
Conc: 2.32 ng/ml

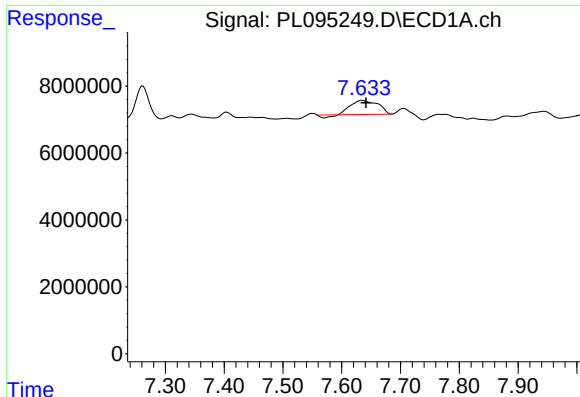

#21 Endrin ketone


R.T.: 7.635 min
Delta R.T.: -0.007 min
Response: 12913381
Conc: 4.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
LAW-25-0060

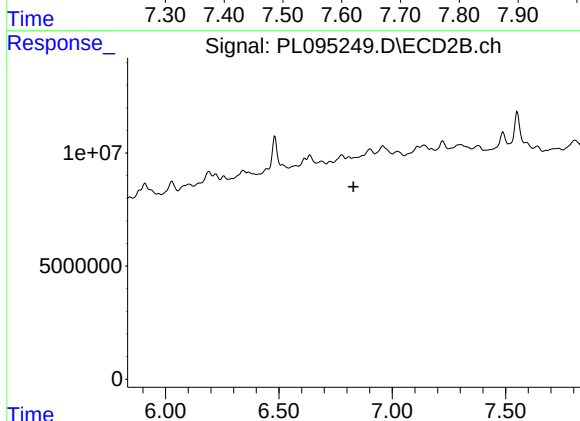


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.829 min
Response: 0
Conc: N.D.

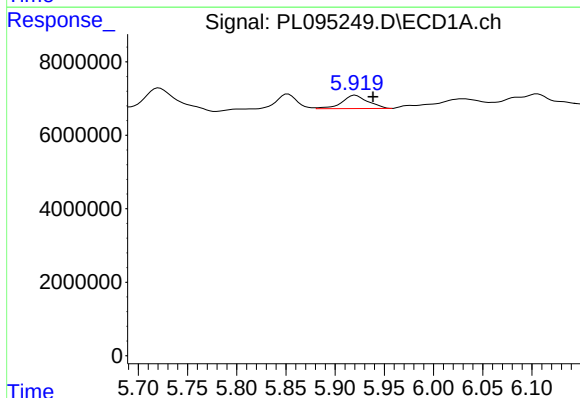


#25 Chlordane-3

R.T.: 5.921 min
Delta R.T.: -0.018 min
Response: 6658818
Conc: 13.58 ng/ml

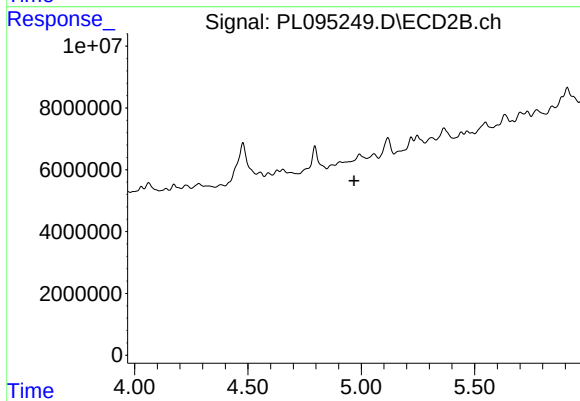

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.968 min
Response: 0
Conc: N.D.

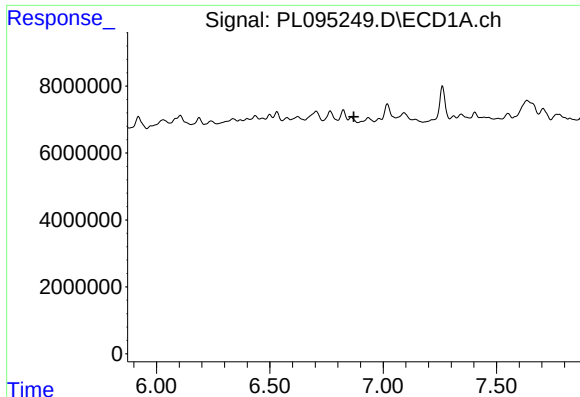

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.870 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
LAW-25-0060

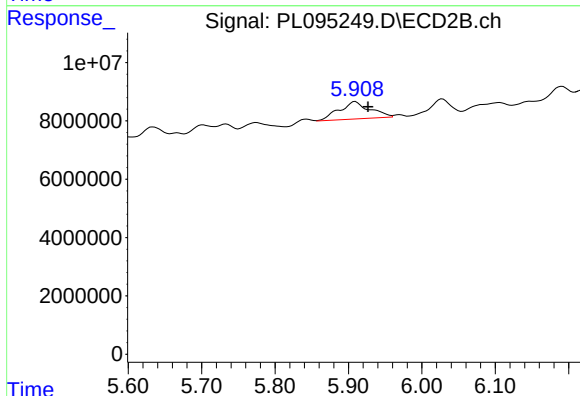


#27 Chlordane-5

R.T.: 5.909 min
Delta R.T.: -0.017 min
Response: 17177974
Conc: 91.94 ng/ml

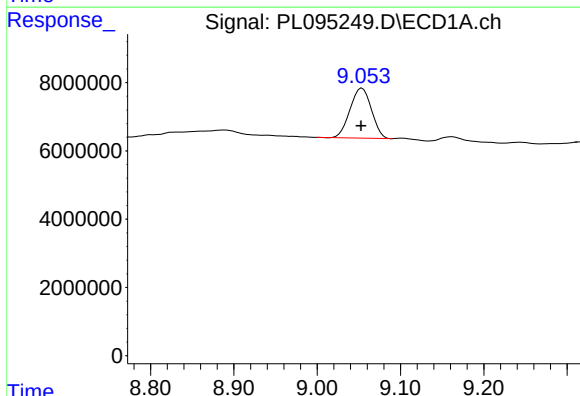

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.001 min
Response: 26154024
Conc: 10.86 ng/ml

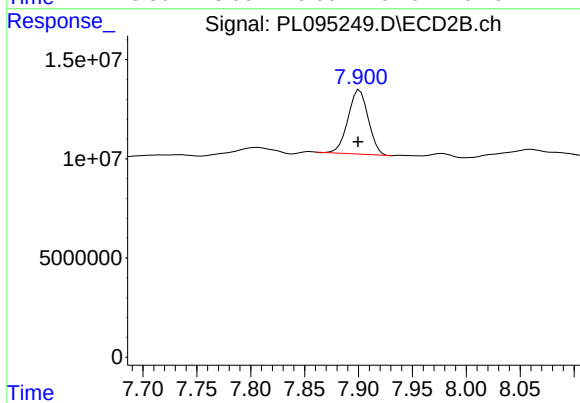

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: 0.001 min
Response: 42349093
Conc: 9.63 ng/ml