

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041525\
 Data File : PL095245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2025 17:16
 Operator : AR\AJ
 Sample : Q1807-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-041425

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/16/2025
 Supervised By : mohammad ahmed 04/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:25:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 14 19:12:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.534	2.768	57209239	71229132	20.854m	19.141
28) SA Decachlor...	9.055	7.901	36842991	55997095	15.302	12.729

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041525\
Data File : PL095245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2025 17:16
Operator : AR\AJ
Sample : Q1807-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-02-041425


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/16/2025
Supervised By : mohammad ahmed 04/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:25:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041425.M
Quant Title : GC Extractables
QLast Update : Mon Apr 14 19:12:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

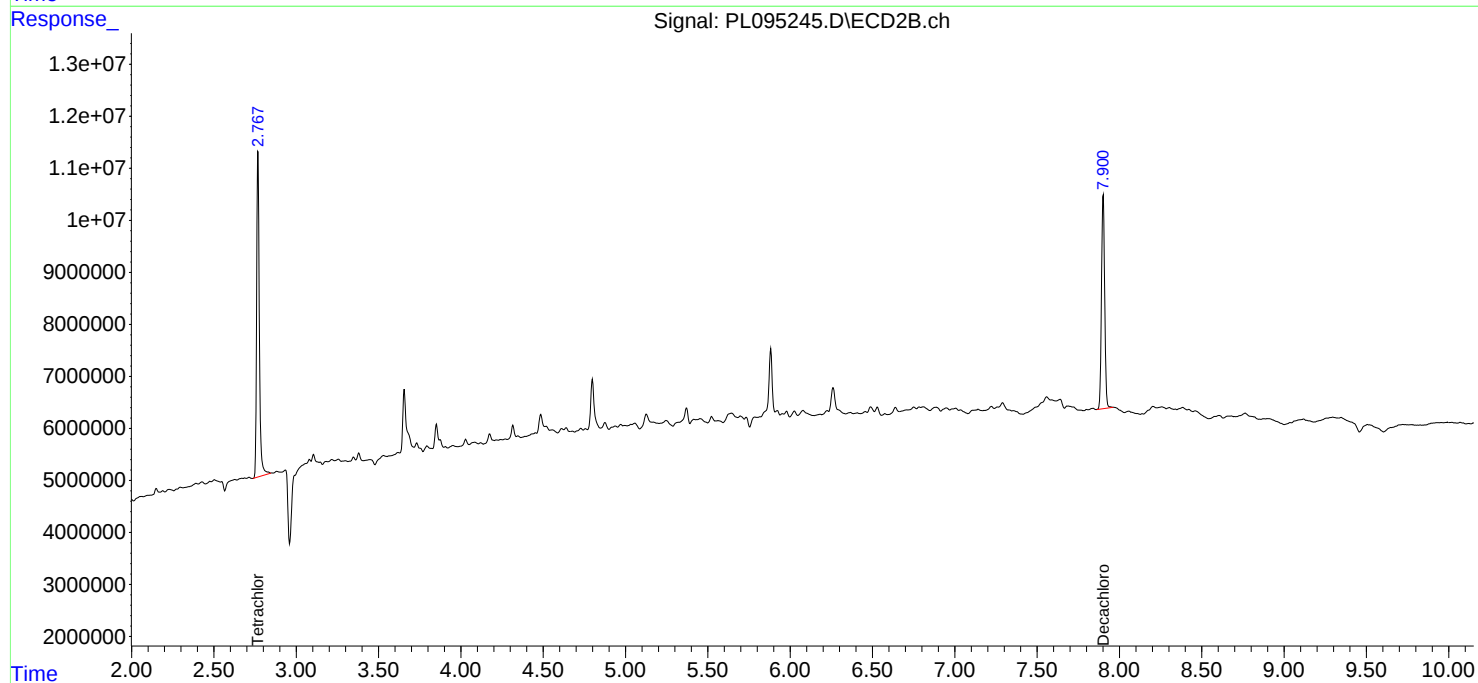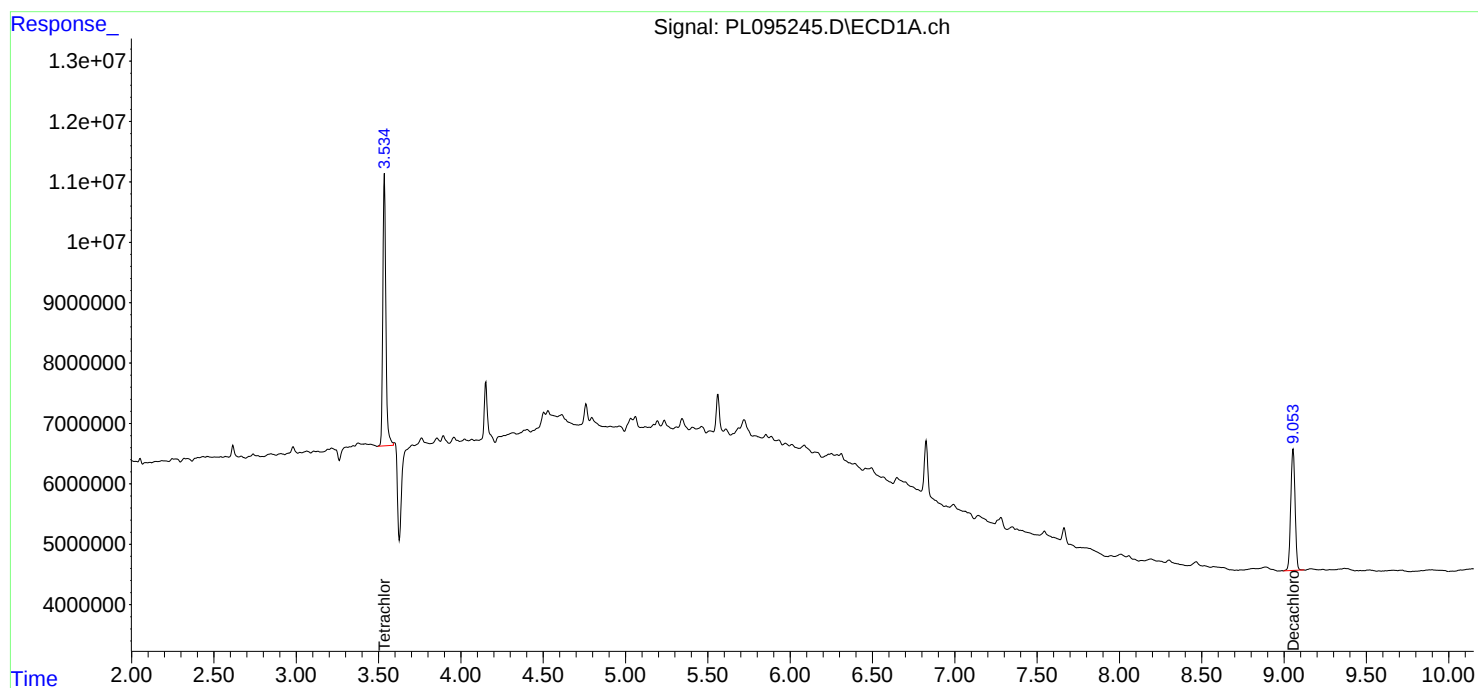

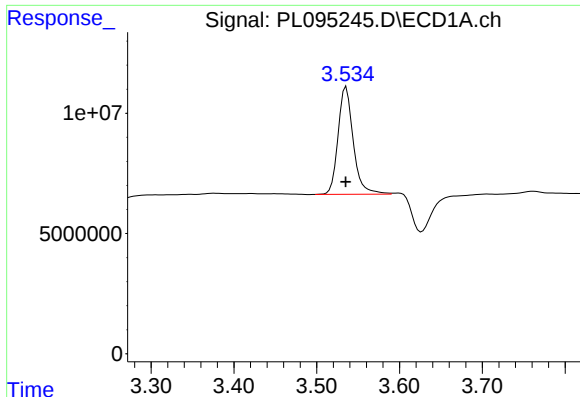


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: 0.000 min
Response: 57209239
Conc: 20.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-041425


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/16/2025
Supervised By :mohammad ahmed 04/16/2025

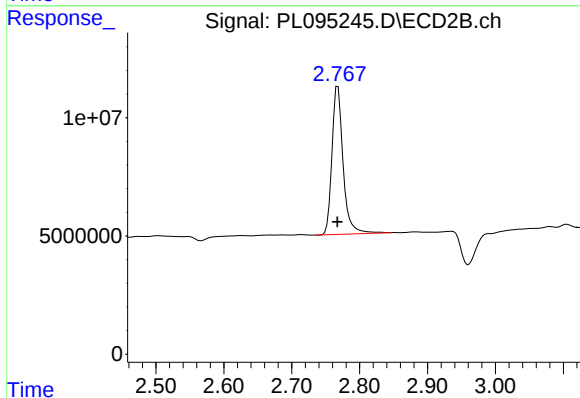


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 71229132
Conc: 19.14 ng/ml

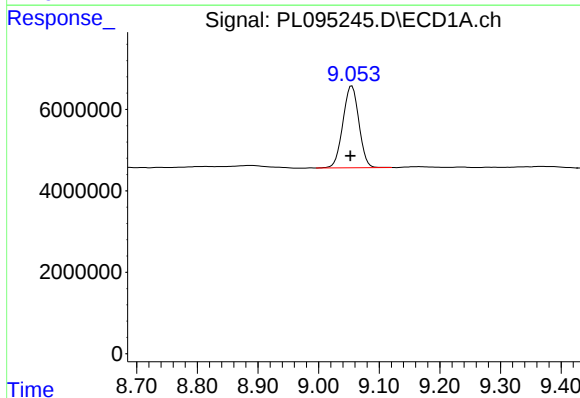

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.002 min
Response: 36842991
Conc: 15.30 ng/ml

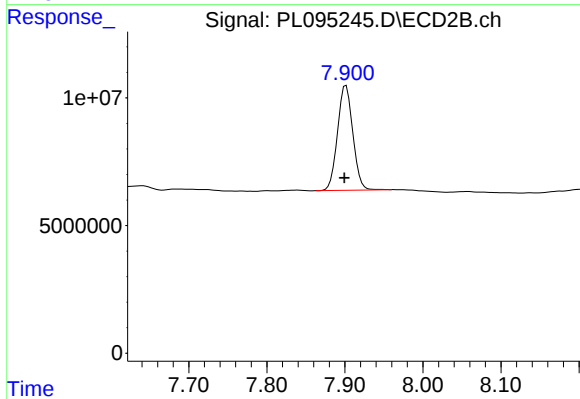

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: 0.002 min
Response: 55997095
Conc: 12.73 ng/ml