

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
 Data File : PL047442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2019 16:45
 Operator : AJ\SJ
 Sample : K2417-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-045

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 02:05:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	3.976	51698666	17997298	7.107	7.860
28)	SA Decachlor...	8.035	9.031	44657387	14248583	5.309	6.146
Target Compounds							
10)	B gamma-Chl...	5.270	0.000	4141920	0	0.403	N.D. #
11)	B alpha-Chl...	0.000	6.155	0	2895108	N.D.	1.021 #
25)	Chlordane-3	5.270	0.000	4141920	0	3.719	N.D. #
26)	Chlordane-4	0.000	6.155	0	2895108	N.D.	6.274 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
Data File : PL047442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2019 16:45
Operator : AJ\SJ
Sample : K2417-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-045

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 02:05:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

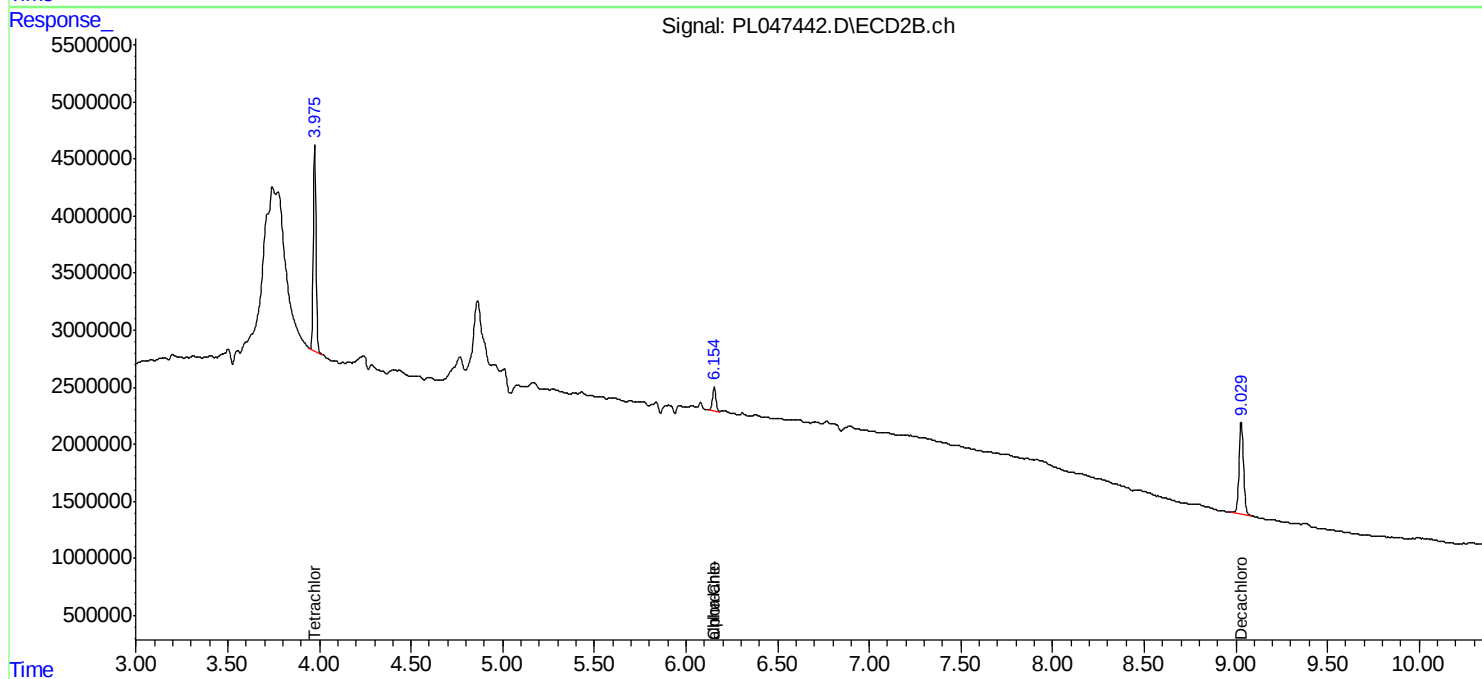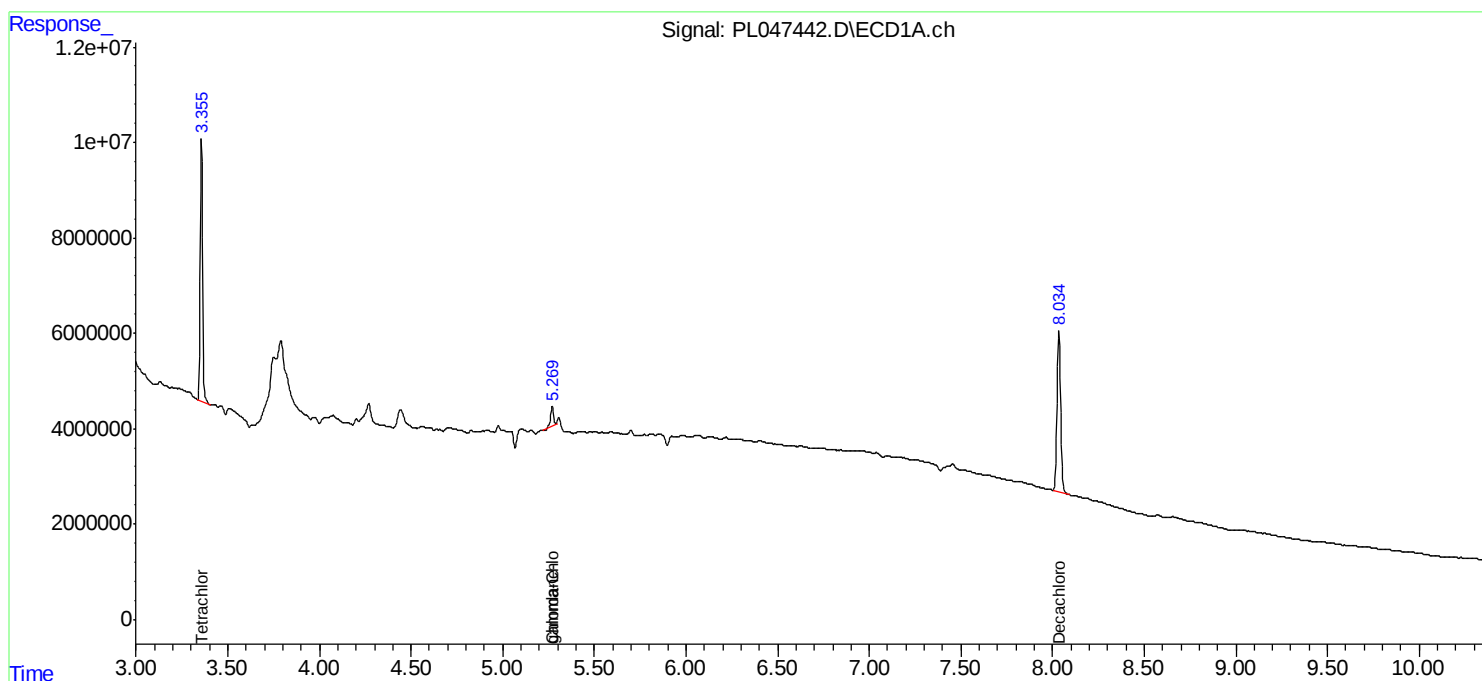


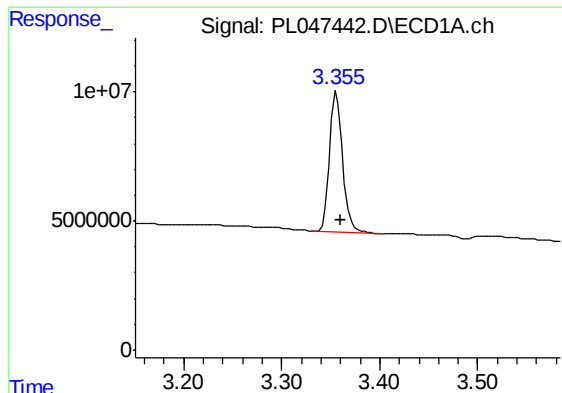

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 51698666
Conc: 7.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-045

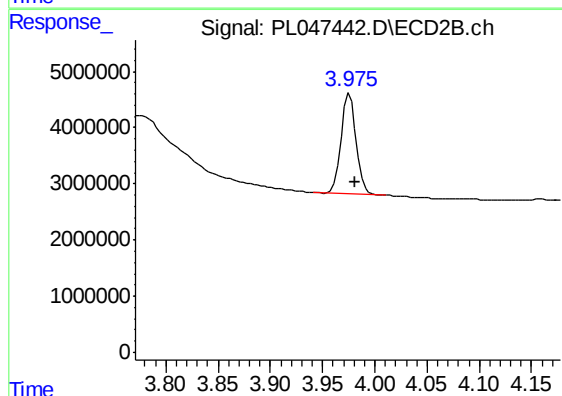


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 17997298
Conc: 7.86 ng/ml

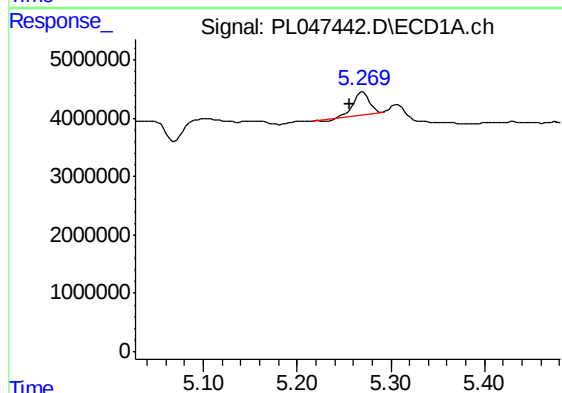


#10 gamma-Chlordane

R.T.: 5.270 min
Delta R.T.: 0.013 min
Response: 4141920
Conc: 0.40 ng/ml

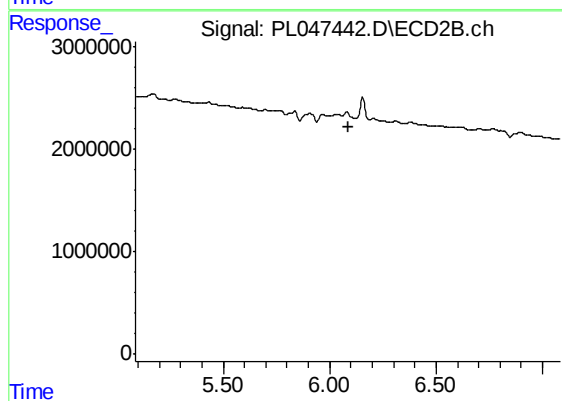

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

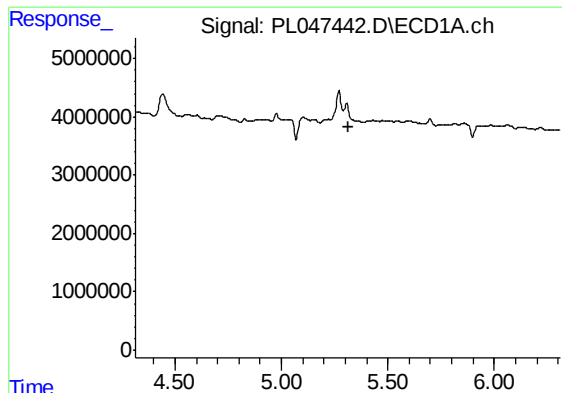

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-045

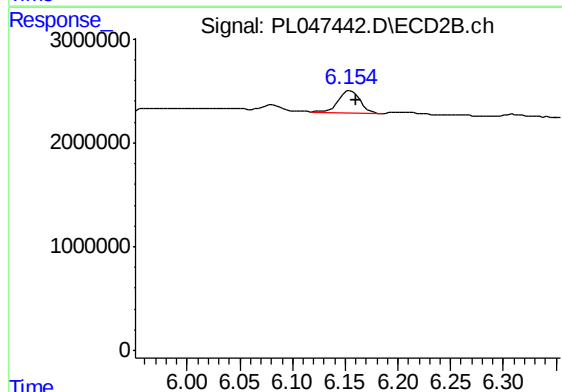


#11 alpha-Chlordane

R.T.: 6.155 min
Delta R.T.: -0.005 min
Response: 2895108
Conc: 1.02 ng/ml

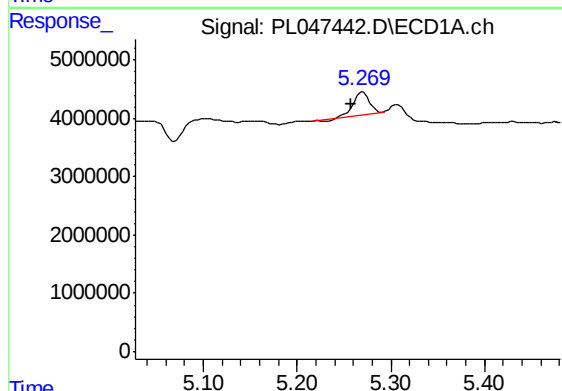


#25 Chlordane-3

R.T.: 5.270 min
Delta R.T.: 0.012 min
Response: 4141920
Conc: 3.72 ng/ml

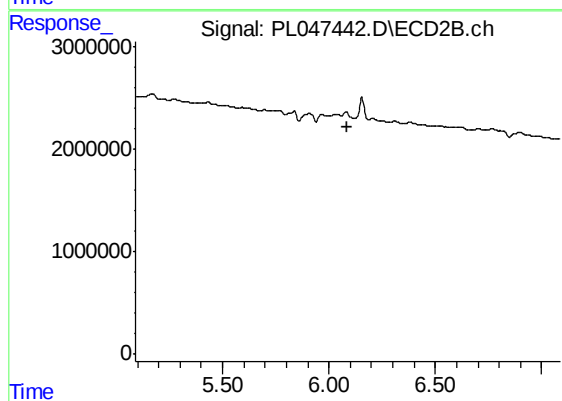

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.089 min
Response: 0
Conc: N.D.

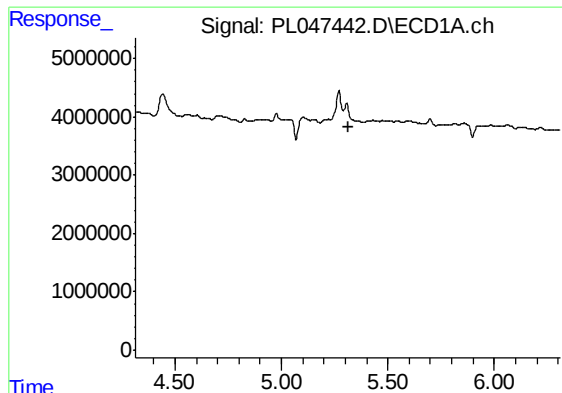

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-045

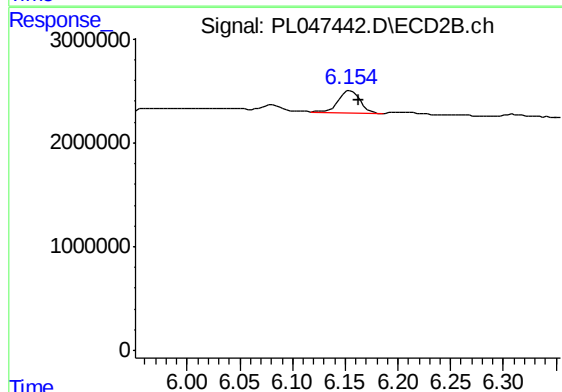


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: -0.008 min
Response: 2895108
Conc: 6.27 ng/ml

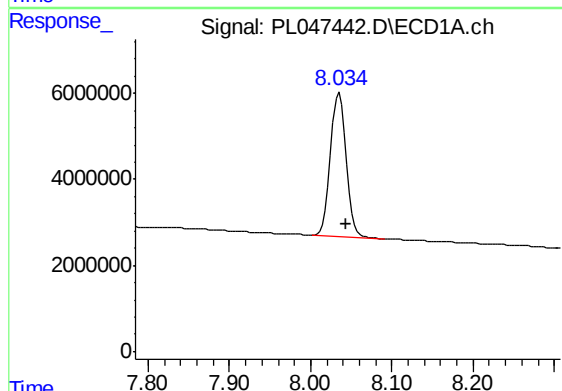

#28 Decachlorobiphenyl

R.T.: 8.035 min
Delta R.T.: -0.009 min
Response: 44657387
Conc: 5.31 ng/ml

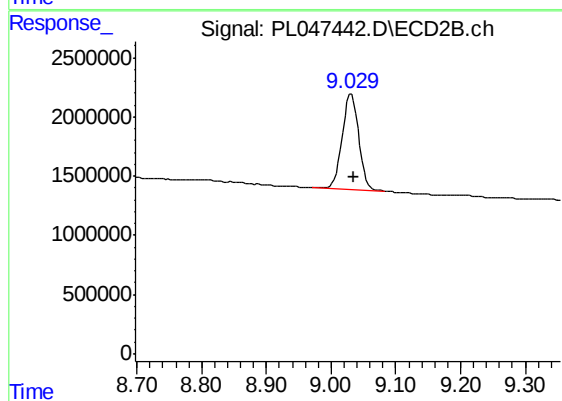

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: -0.004 min
Response: 14248583
Conc: 6.15 ng/ml