

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
 Data File : PL047445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2019 17:28
 Operator : AJ\SJ
 Sample : K2423-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP2-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 02:06:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	3.976	145.8E6	46915035	20.041	20.490
28)	SA Decachlor...	8.033	9.030	133.3E6	41515816	15.854	17.907
Target Compounds							
2)	A alpha-BHC	3.789	0.000	10077890	0	0.864	N.D. #
6)	B beta-BHC	4.320	0.000	6122466	0	1.360	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
Data File : PL047445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2019 17:28
Operator : AJ\SJ
Sample : K2423-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP2-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 02:06:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

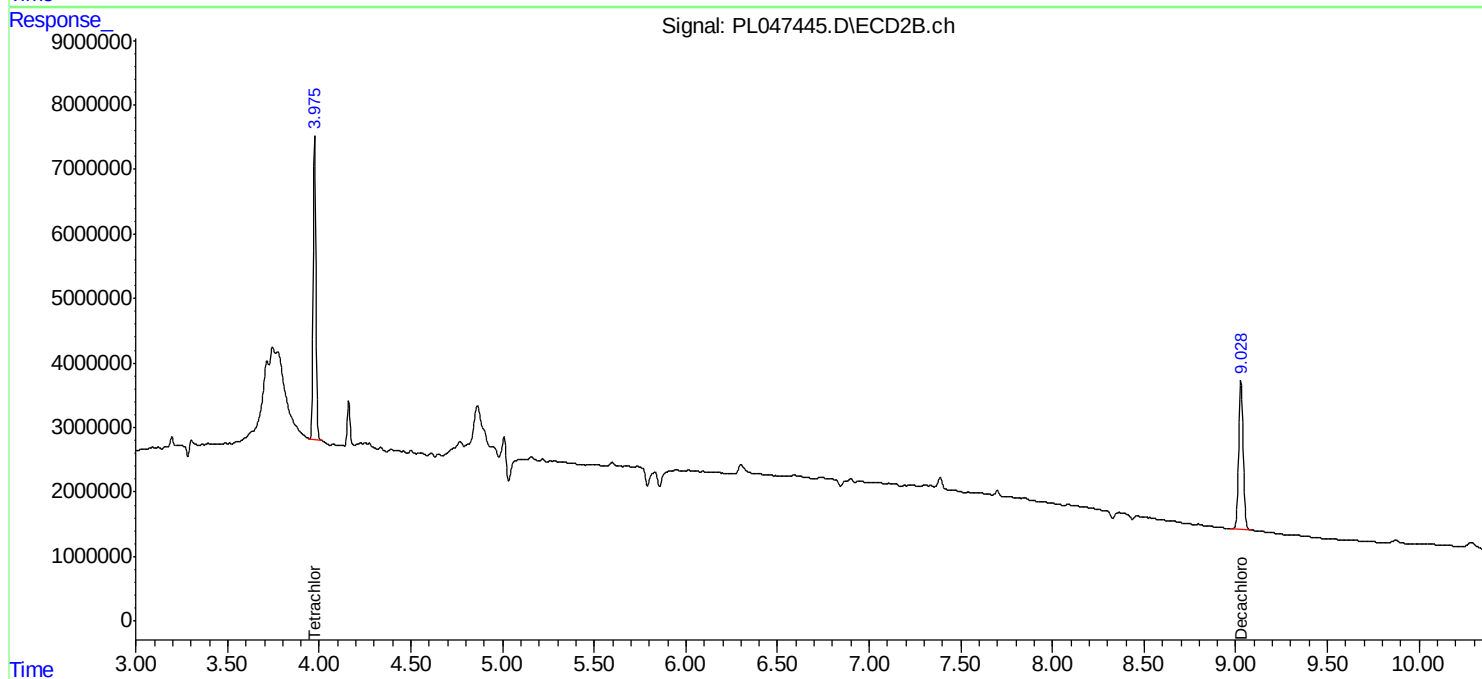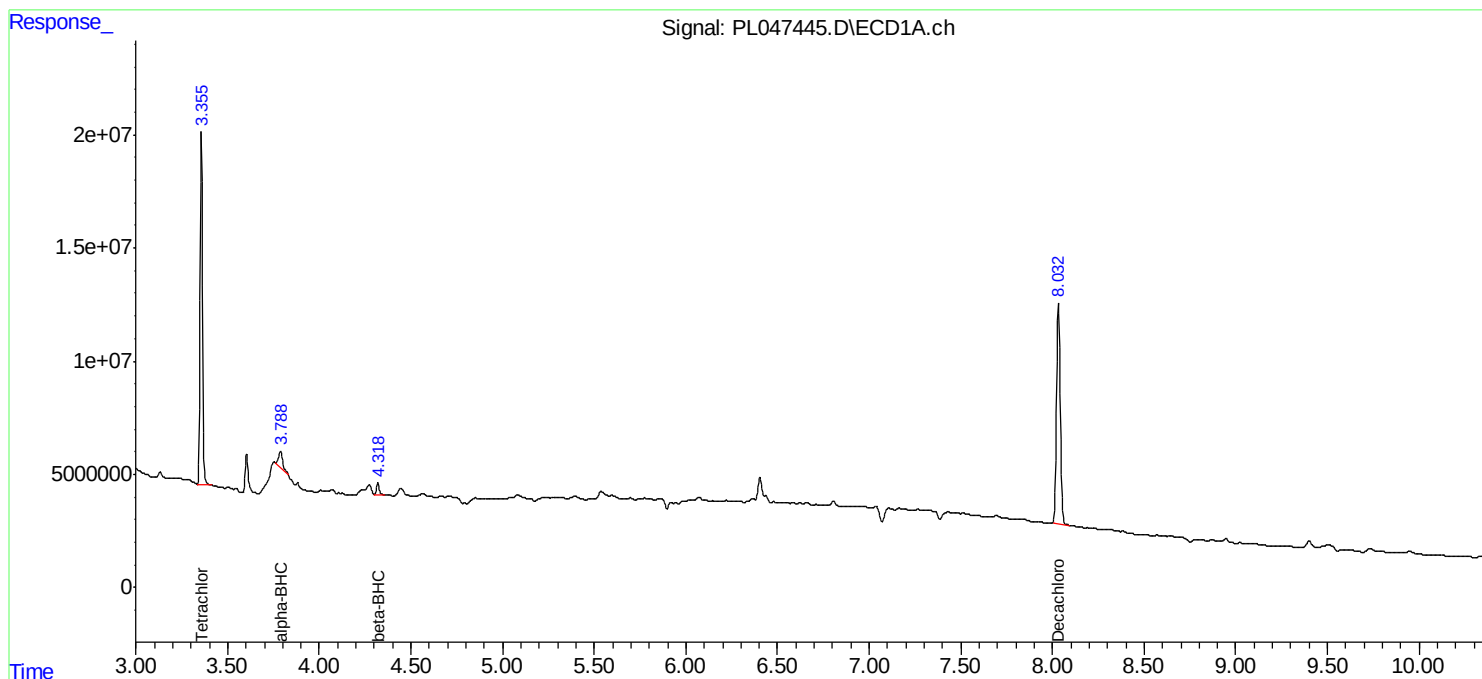


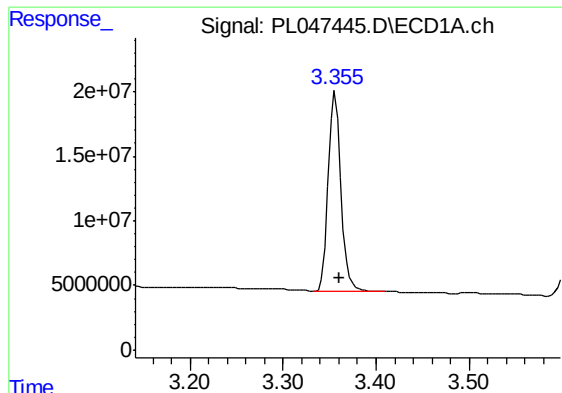

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 145792834
Conc: 20.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP2-A

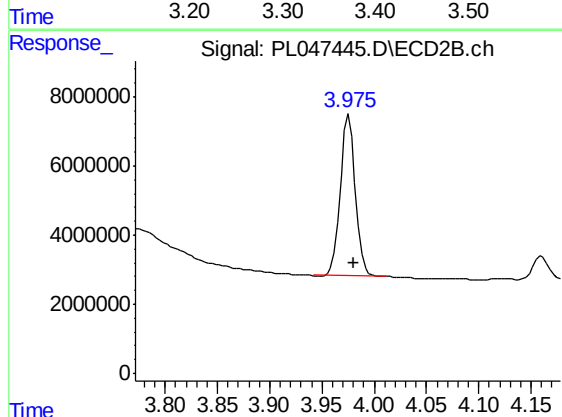


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 46915035
Conc: 20.49 ng/ml

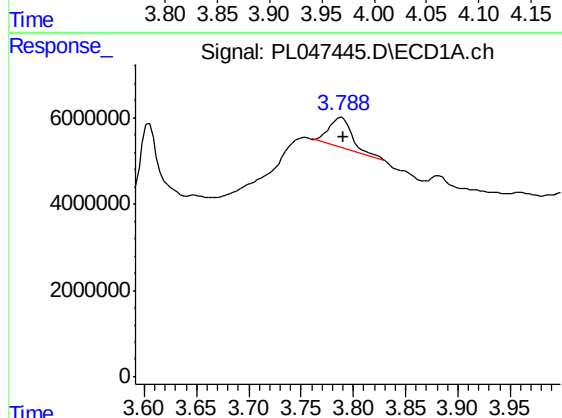


#2 alpha-BHC

R.T.: 3.789 min
Delta R.T.: -0.002 min
Response: 10077890
Conc: 0.86 ng/ml

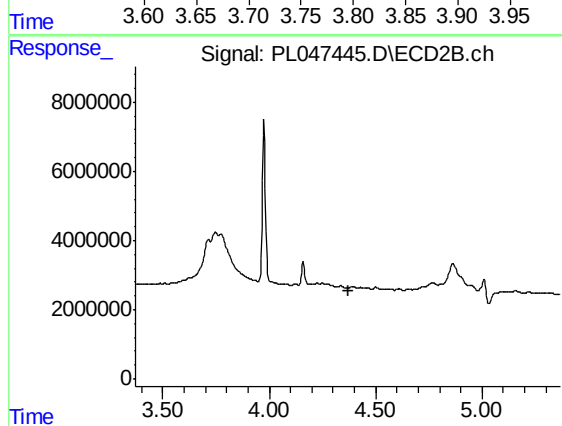

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

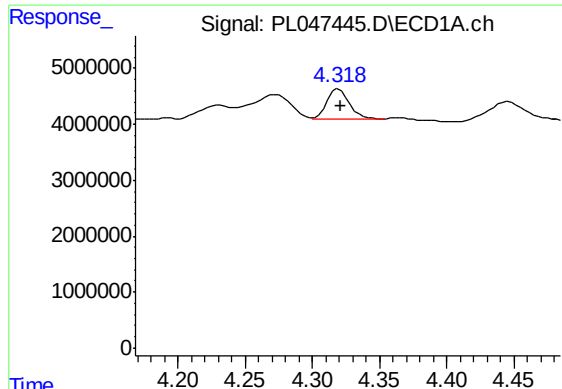

#6 beta-BHC


R.T.: 4.320 min
Delta R.T.: -0.001 min
Response: 6122466
Conc: 1.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP2-A

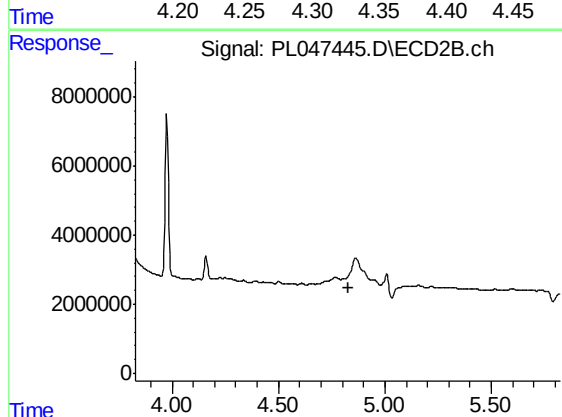


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.828 min
Response: 0
Conc: N.D.

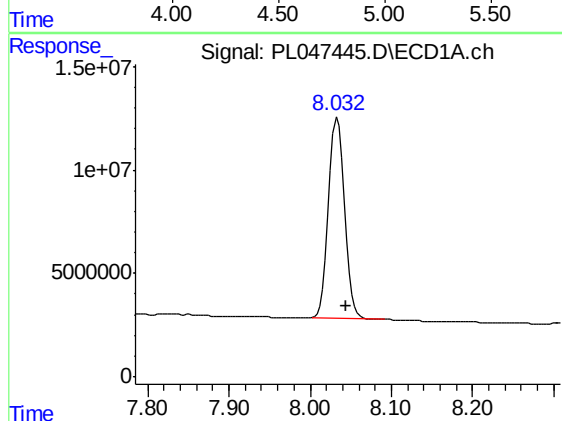

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 133349740
Conc: 15.85 ng/ml

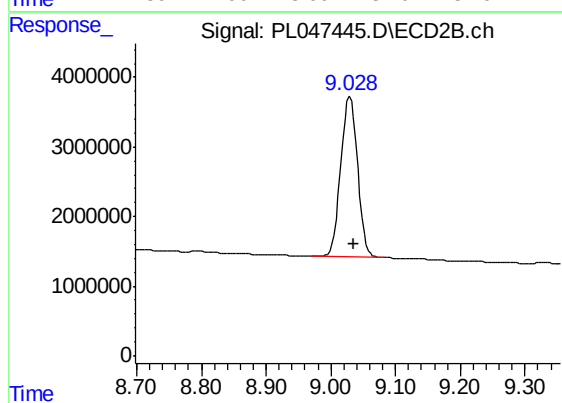

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.005 min
Response: 41515816
Conc: 17.91 ng/ml