

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
 Data File : PL047478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2019 01:23
 Operator : AJ\SJ
 Sample : K2411-08
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-14-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 02:15:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.356	3.975	136.0E6	44585116	18.694	19.473
28) SA Decachlor...	8.031	9.025	143.3E6	43133765	17.035	18.604
Target Compounds						
14) MA Endrin	5.859	0.000	9712505	0	1.031	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
Data File : PL047478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2019 01:23
Operator : AJ\SJ
Sample : K2411-08
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-14-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 02:15:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

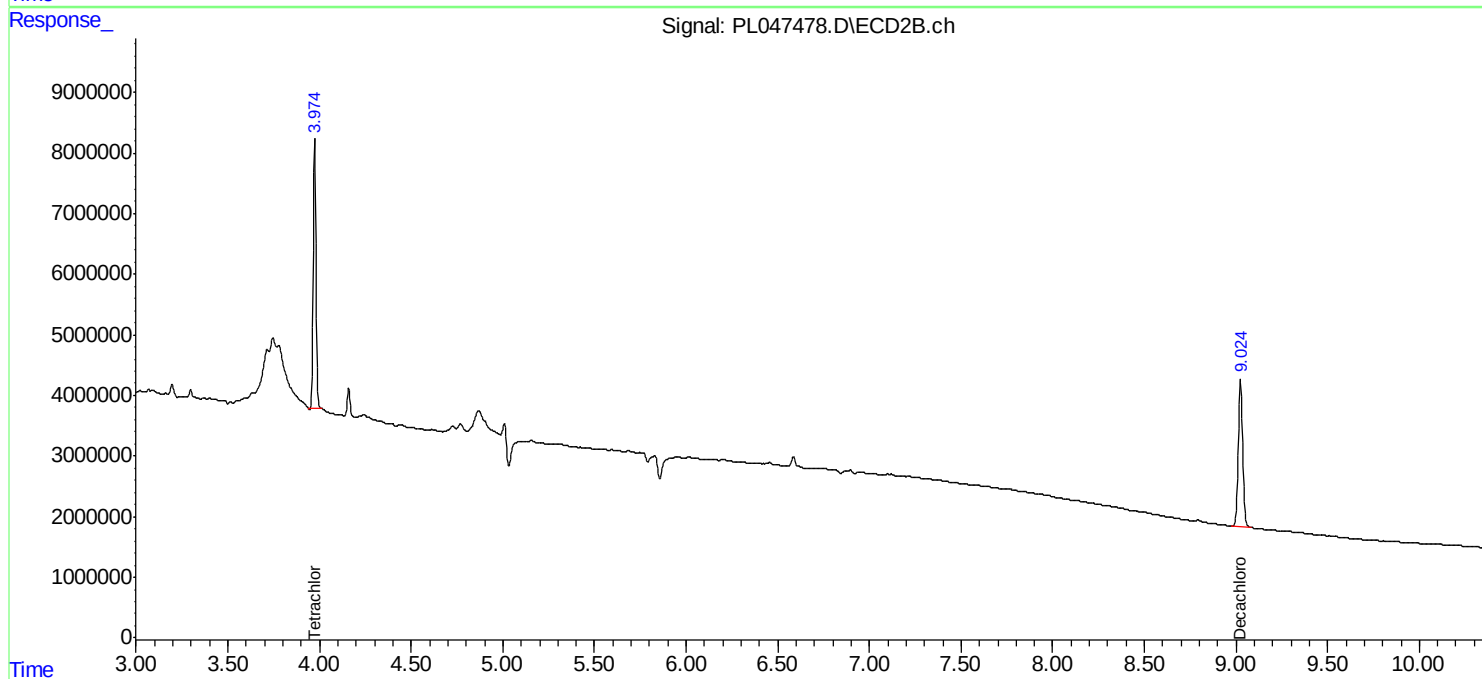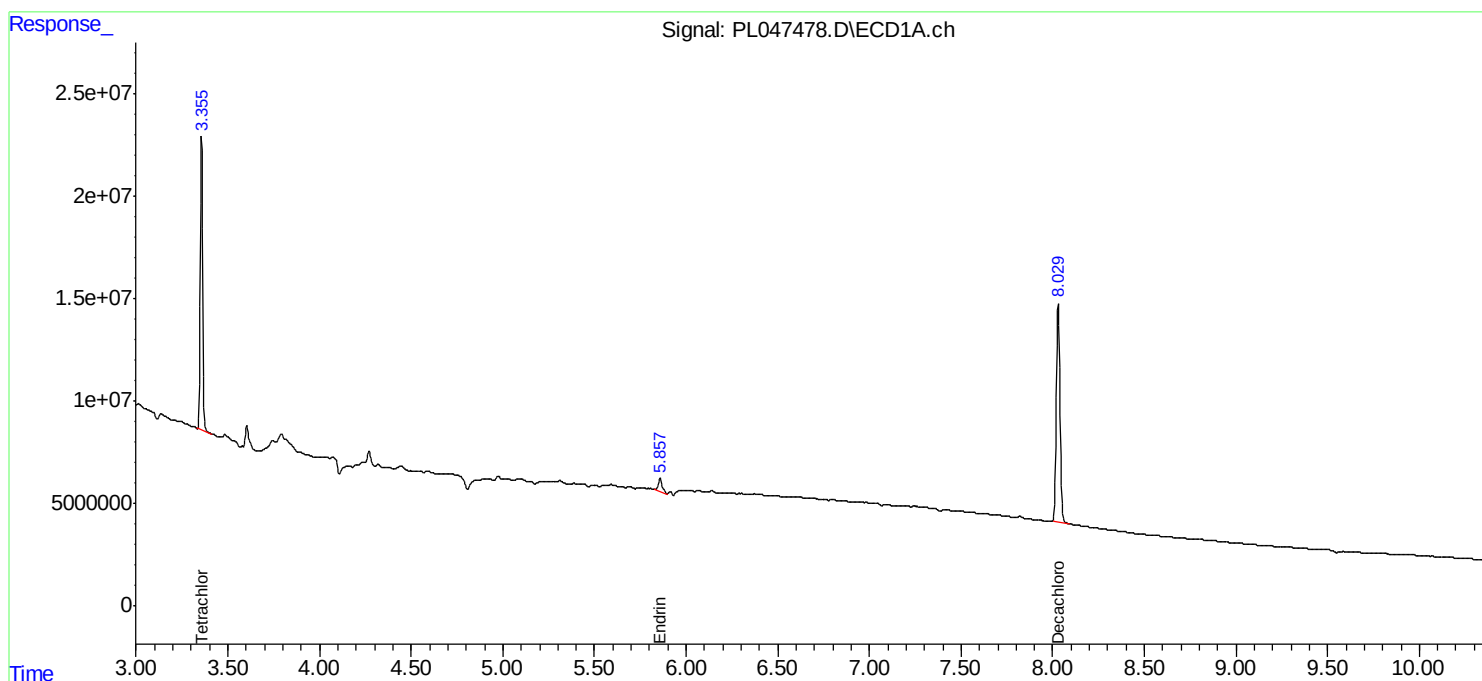


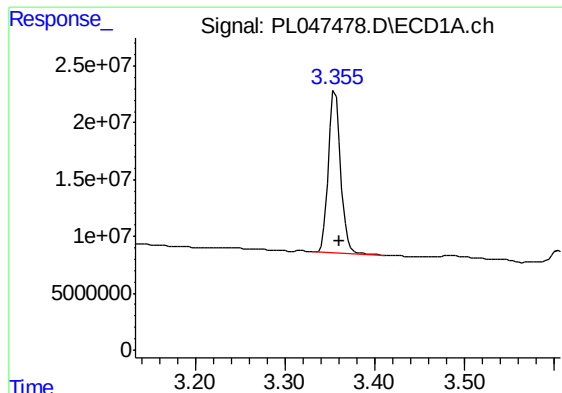

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 135995898
Conc: 18.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

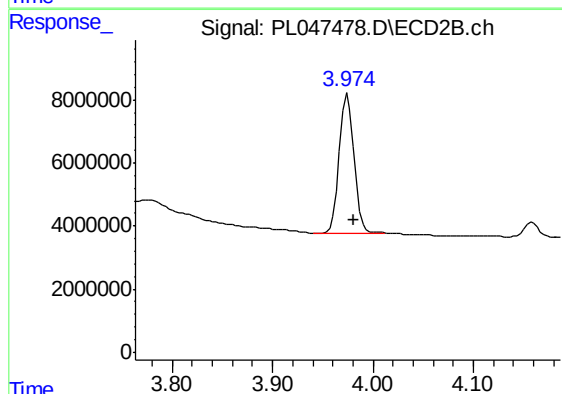


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.006 min
Response: 44585116
Conc: 19.47 ng/ml

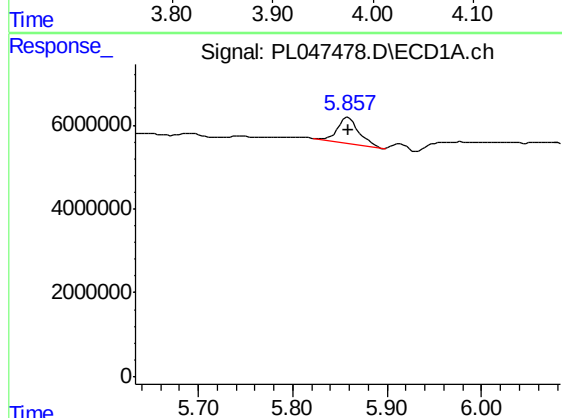


#14 Endrin

R.T.: 5.859 min
Delta R.T.: 0.000 min
Response: 9712505
Conc: 1.03 ng/ml

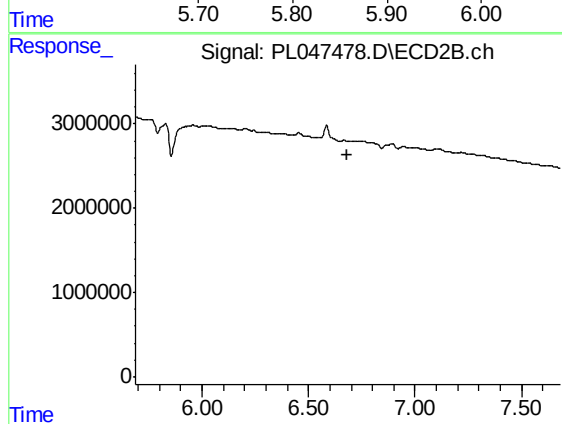

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.684 min
Response: 0
Conc: N.D.

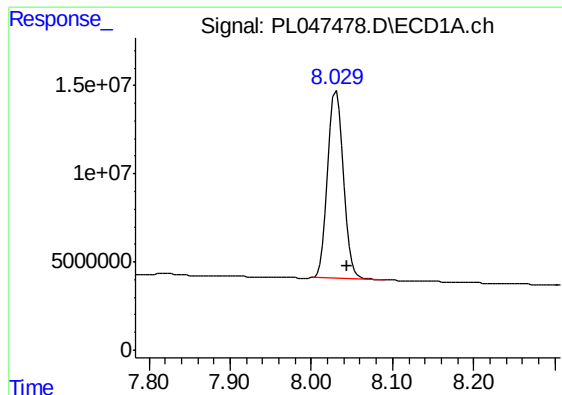

#28 Decachlorobiphenyl

R.T.: 8.031 min
Delta R.T.: -0.013 min
Response: 143285138
Conc: 17.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

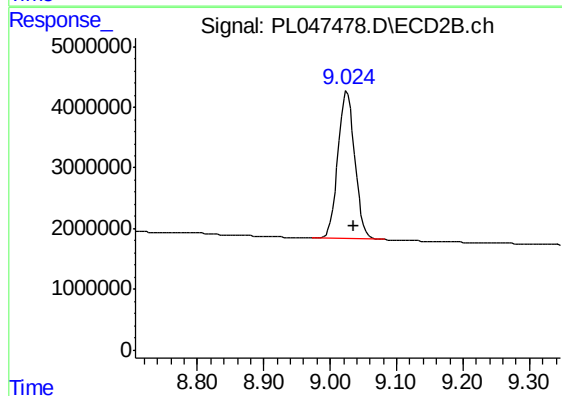

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: -0.010 min
Response: 43133765
Conc: 18.60 ng/ml