

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
 Data File : PL047484.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2019 02:49
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 04:52:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.355	3.975	147.5E6	46860979	20.280	20.467
28)	SA Decachlor...	8.030	9.026	182.7E6	53965055	21.721	23.276
Target Compounds							
2)	A alpha-BHC	3.792	0.000	7601843	0	0.652	N.D. #
8)	B Heptachlo...	0.000	5.840	0	8622784	N.D.	3.270 #
10)	B gamma-Chl...	0.000	6.086	0	5238295	N.D.	1.846 #
12)	B 4,4'-DDE	5.503f	0.000	176675	0	0.019	N.D. #
14)	MA Endrin	0.000	6.679	0	10343022	N.D.	4.328 #
25)	Chlordane-3	0.000	6.086	0	5238295	N.D.	13.739 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
Data File : PL047484.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2019 02:49
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 04:52:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

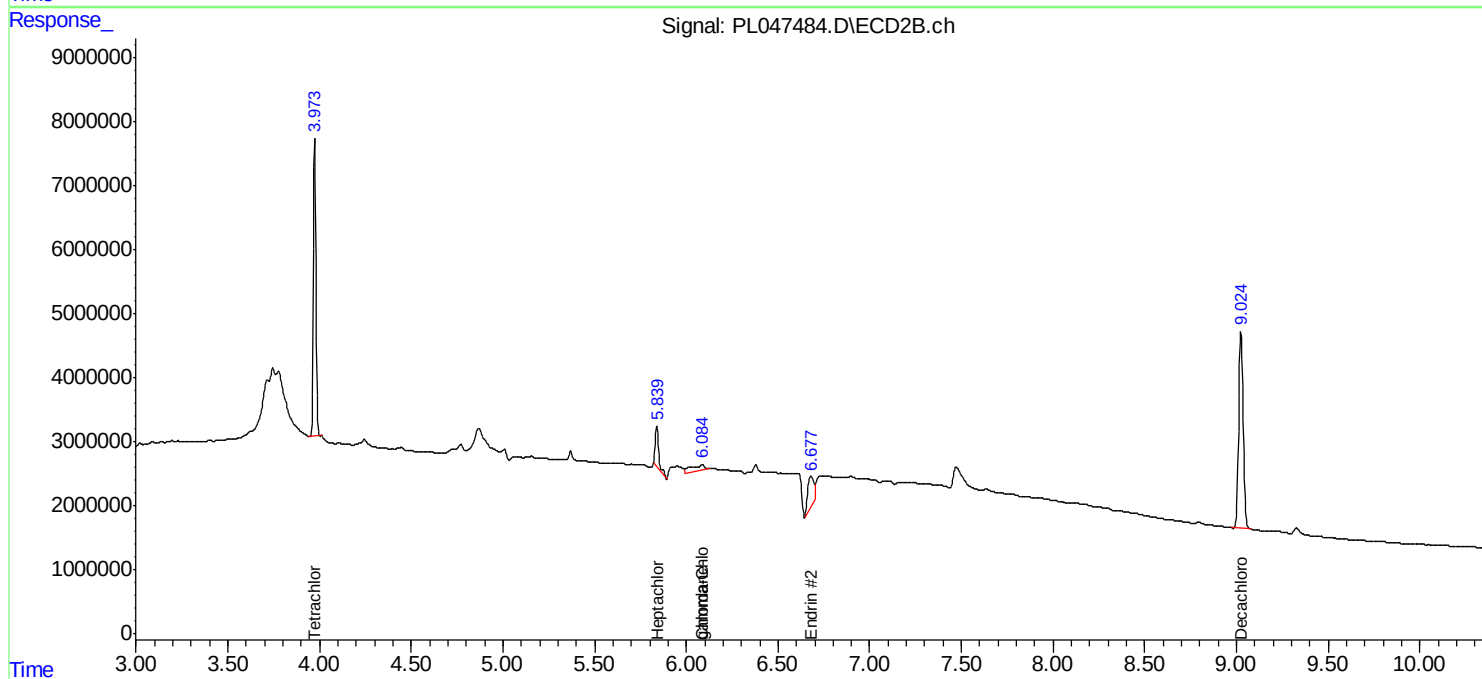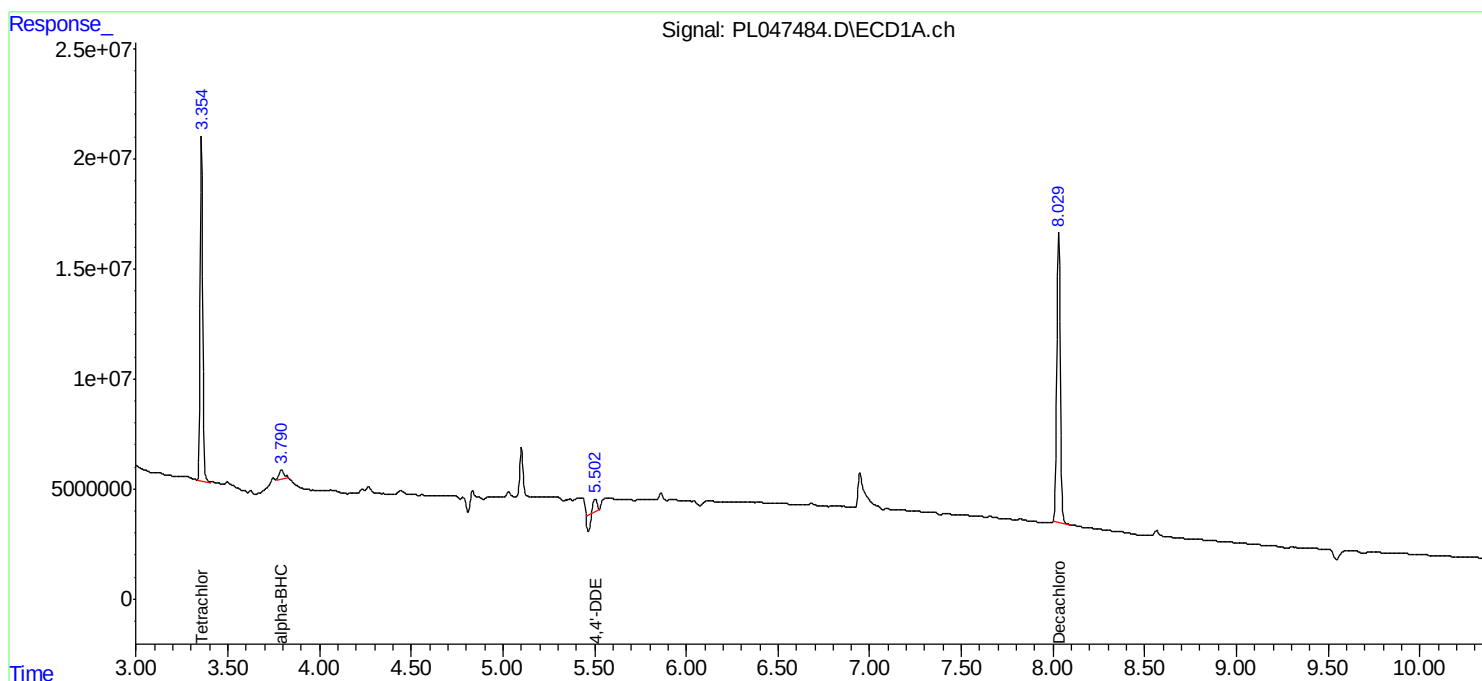


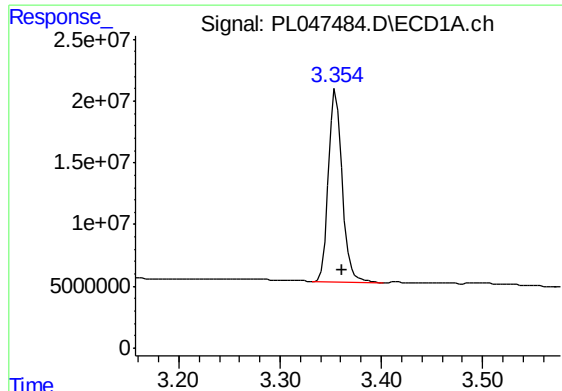

#1 Tetrachloro-m-xylene


R.T.: 3.355 min
Delta R.T.: -0.006 min
Response: 147531494
Conc: 20.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

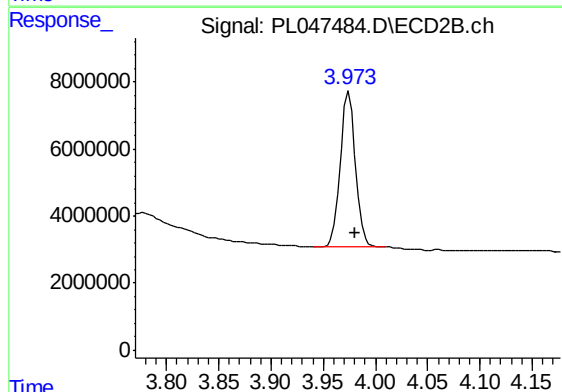


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.006 min
Response: 46860979
Conc: 20.47 ng/ml

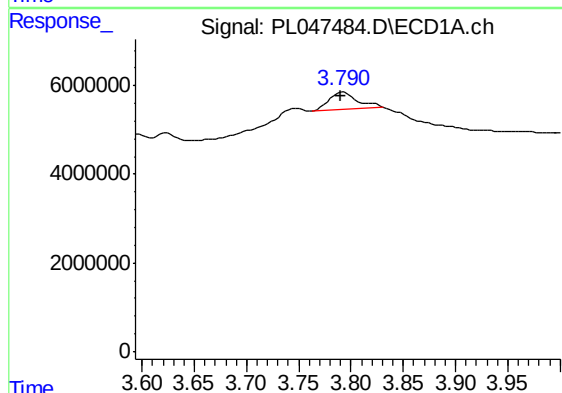


#2 alpha-BHC

R.T.: 3.792 min
Delta R.T.: 0.002 min
Response: 7601843
Conc: 0.65 ng/ml

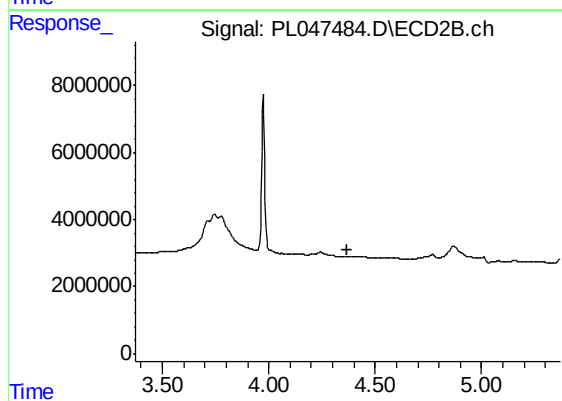

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

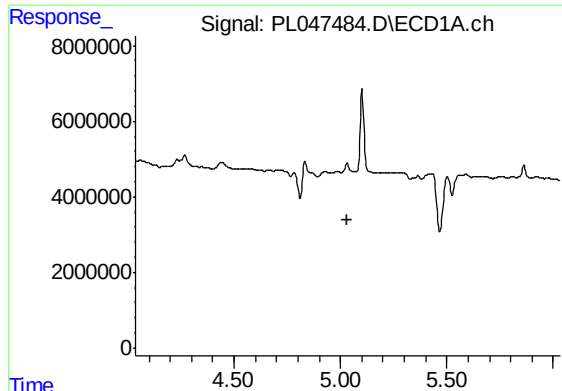

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

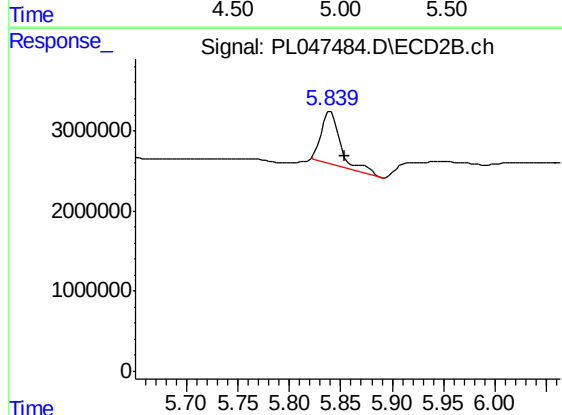


#8 Heptachlor epoxide

R.T.: 5.840 min
Delta R.T.: -0.013 min
Response: 8622784
Conc: 3.27 ng/ml

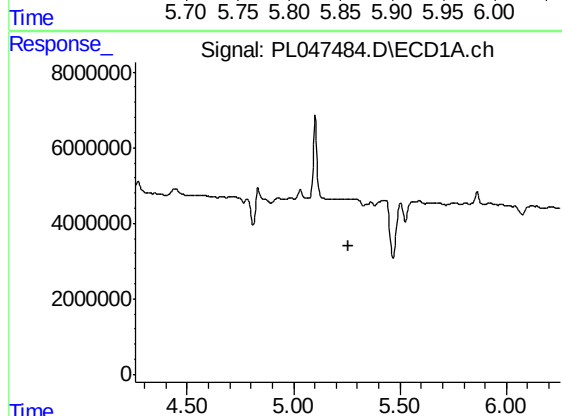


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

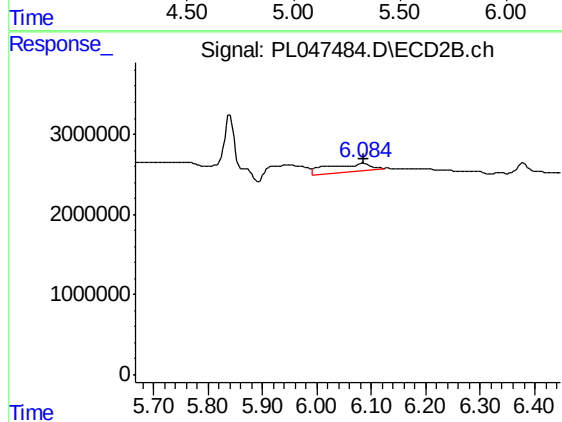

#10 gamma-Chlordane


R.T.: 6.086 min
Delta R.T.: -0.002 min
Response: 5238295
Conc: 1.85 ng/ml

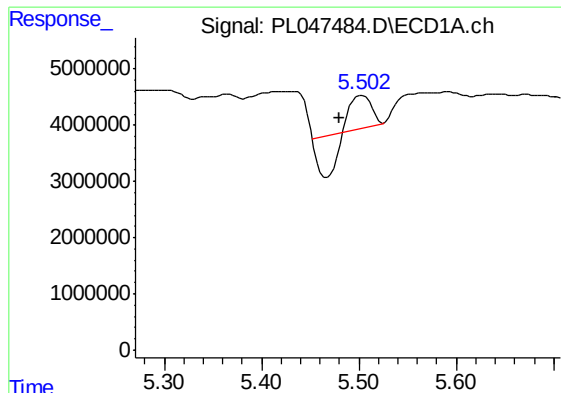

#12 4,4'-DDE


R.T.: 5.503 min
Delta R.T.: 0.023 min
Response: 176675
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

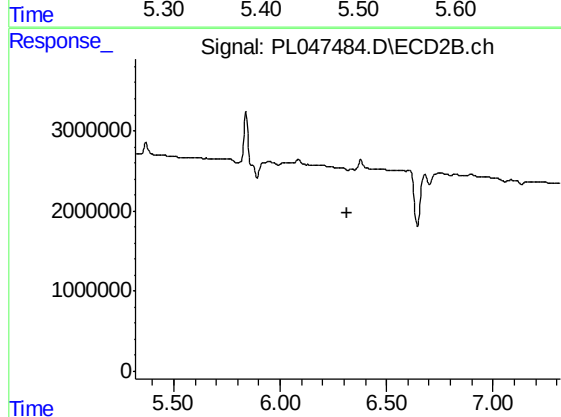


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.318 min
Response: 0
Conc: N.D.

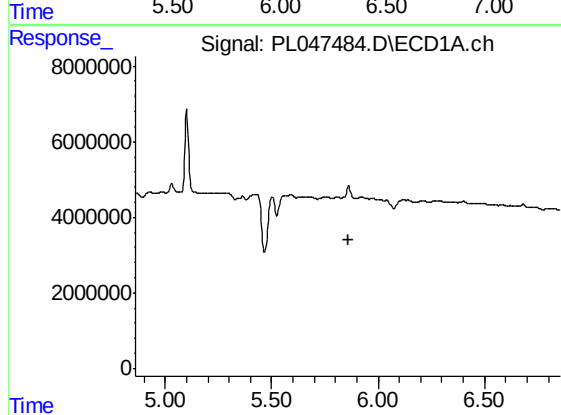


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.860 min
Response: 0
Conc: N.D.

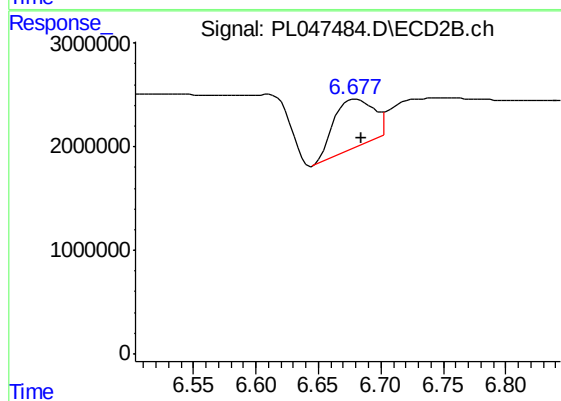

#14 Endrin


R.T.: 6.679 min
Delta R.T.: -0.005 min
Response: 10343022
Conc: 4.33 ng/ml

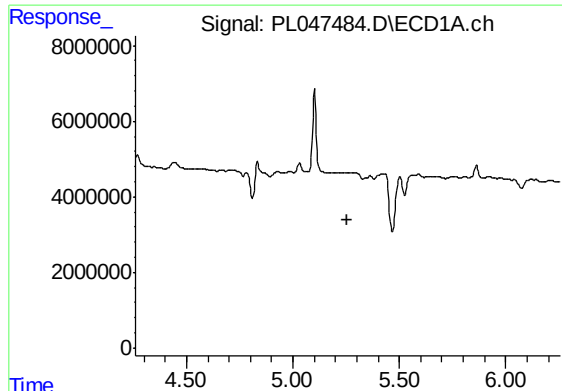

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

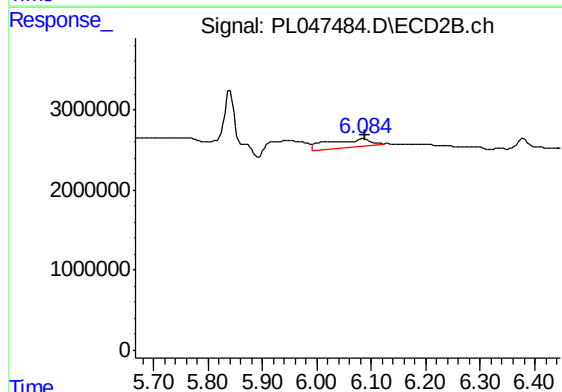


#25 Chlordane-3

R.T.: 6.086 min
Delta R.T.: -0.003 min
Response: 5238295
Conc: 13.74 ng/ml

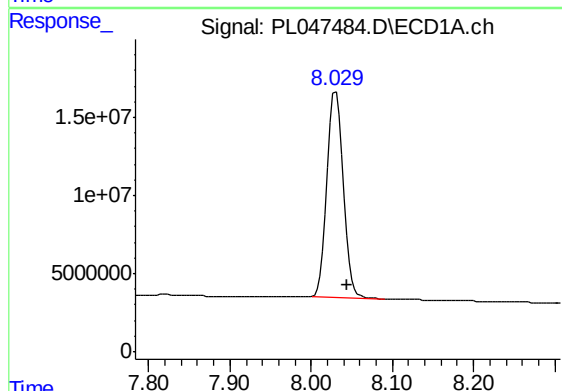

#28 Decachlorobiphenyl

R.T.: 8.030 min
Delta R.T.: -0.014 min
Response: 182695169
Conc: 21.72 ng/ml

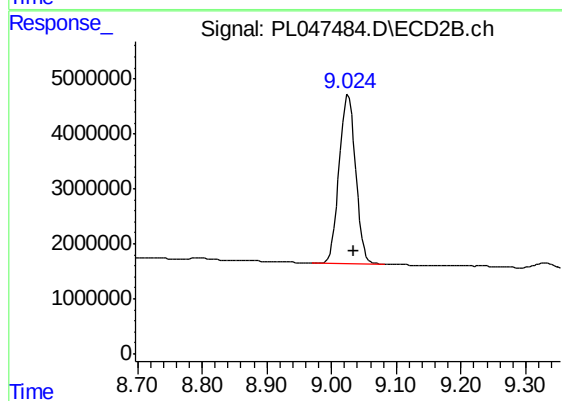

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.009 min
Response: 53965055
Conc: 23.28 ng/ml