

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
 Data File : PL047441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2019 16:31
 Operator : AJ\SJ
 Sample : K2414-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-044

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 02:05:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.356	3.975	70758407	24679581	9.727	10.779
28) SA Decachlor...	8.033	9.030	82243278	25790821	9.778	11.124
Target Compounds						
17) MA 4,4'-DDT	6.219	7.099	10434041	3649407	1.378	1.740 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
Data File : PL047441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2019 16:31
Operator : AJ\SJ
Sample : K2414-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-044

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 02:05:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

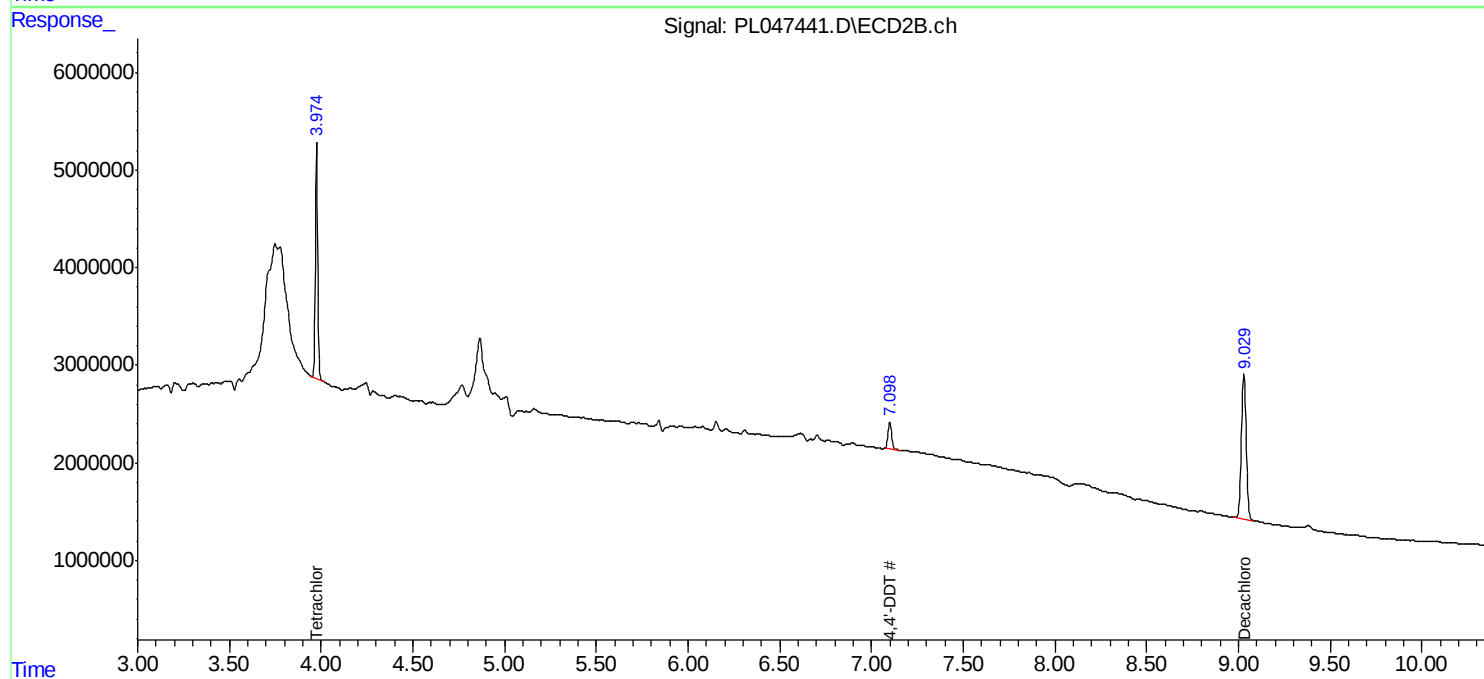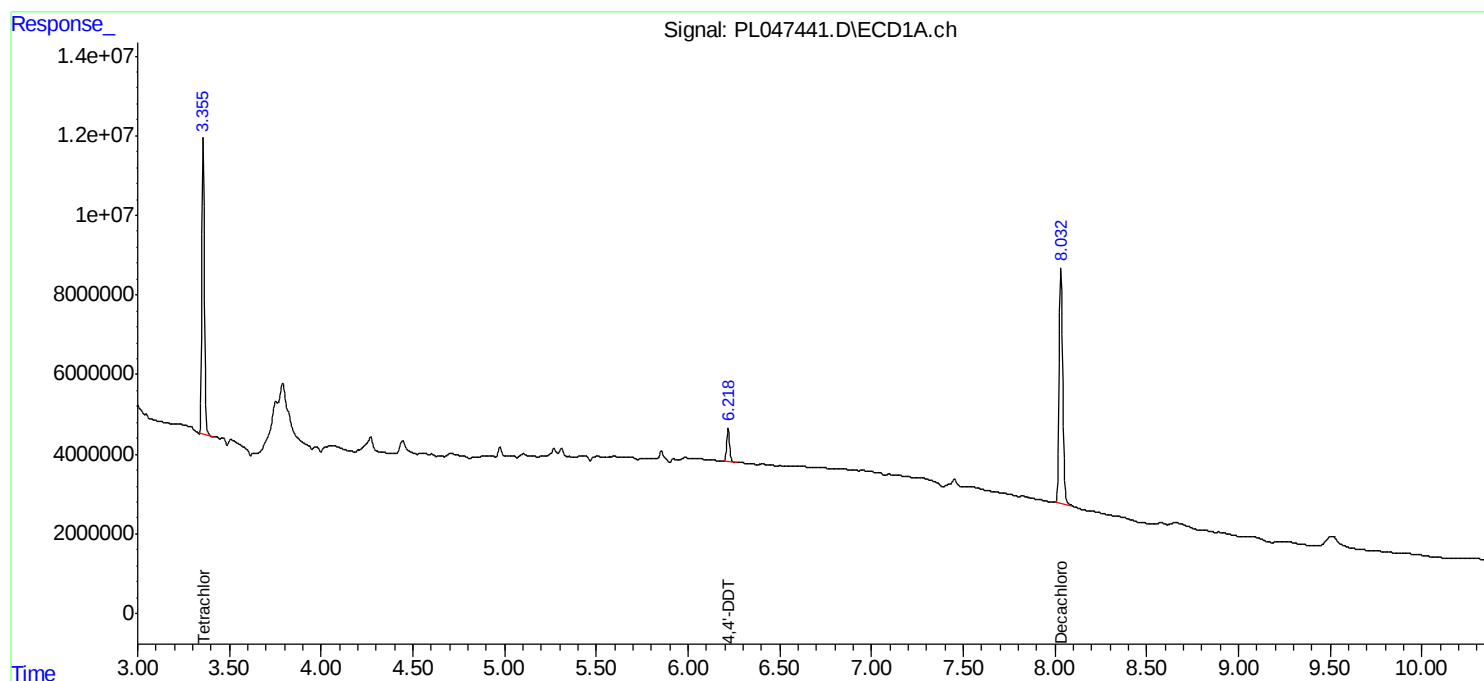


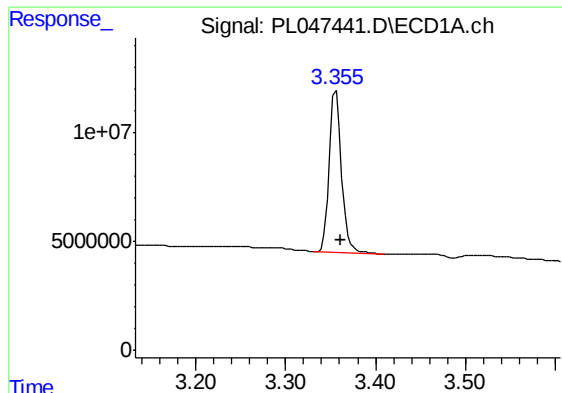

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 70758407
Conc: 9.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-044

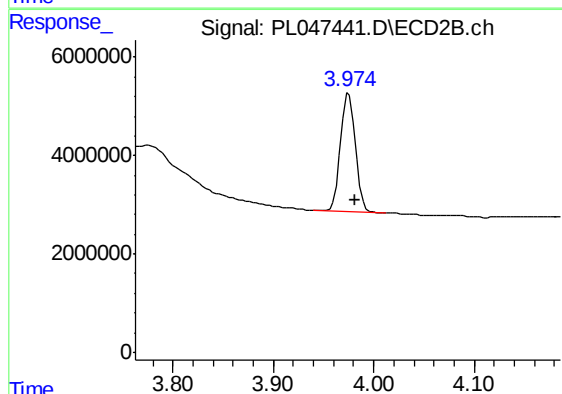


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.005 min
Response: 24679581
Conc: 10.78 ng/ml

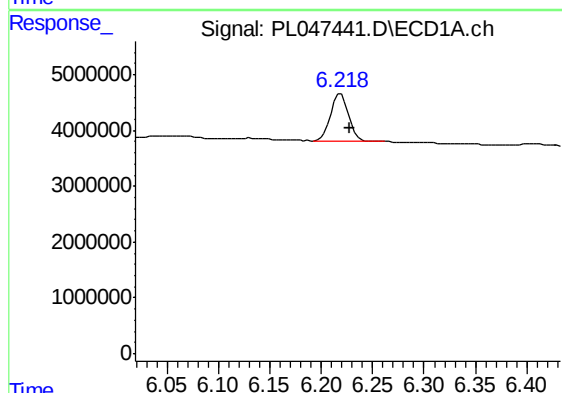


#17 4,4'-DDT

R.T.: 6.219 min
Delta R.T.: -0.009 min
Response: 10434041
Conc: 1.38 ng/ml

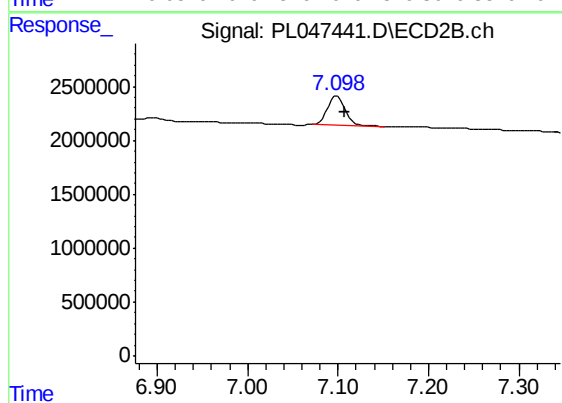

#17 4,4'-DDT


R.T.: 7.099 min
Delta R.T.: -0.008 min
Response: 3649407
Conc: 1.74 ng/ml

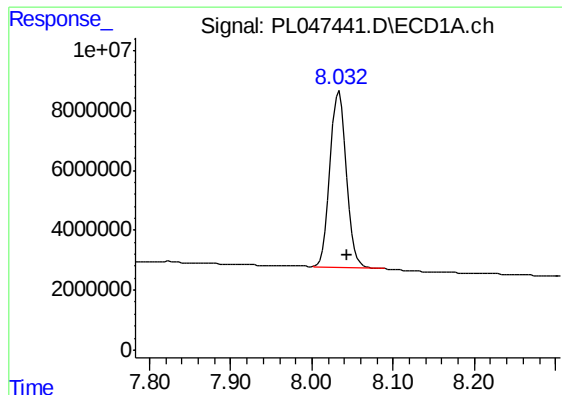

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 82243278
Conc: 9.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-044

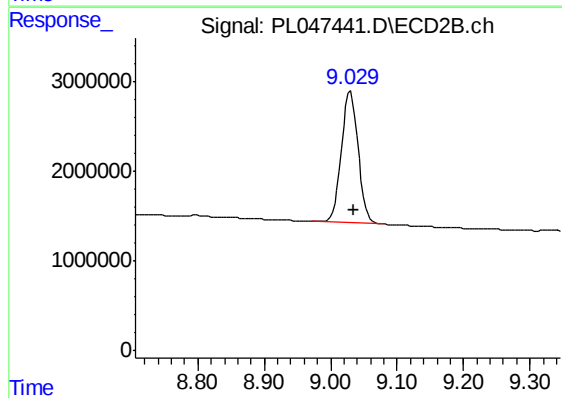

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.005 min
Response: 25790821
Conc: 11.12 ng/ml