

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
 Data File : PL047465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2019 22:16
 Operator : AJ\SJ
 Sample : K2411-07
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-14-S

Manual Integrations
 APPROVED

Sohil
 4/17/2019 4:53:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 02:11:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.356	3.975	67387185	22813235	9.263	9.964
28) SA Decachlor...	8.032	9.026	125.8E6	38606863	14.959	16.652
Target Compounds						
12) B 4,4'-DDE	5.470	6.309	33872712	10005894	3.679m	4.031
17) MA 4,4'-DDT	6.217	7.095	12648375	3770073	1.670	1.798m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
Data File : PL047465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2019 22:16
Operator : AJ\SJ
Sample : K2411-07
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-14-S


Manual Integrations
APPROVED

Sohil
4/17/2019 4:53:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 02:11:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

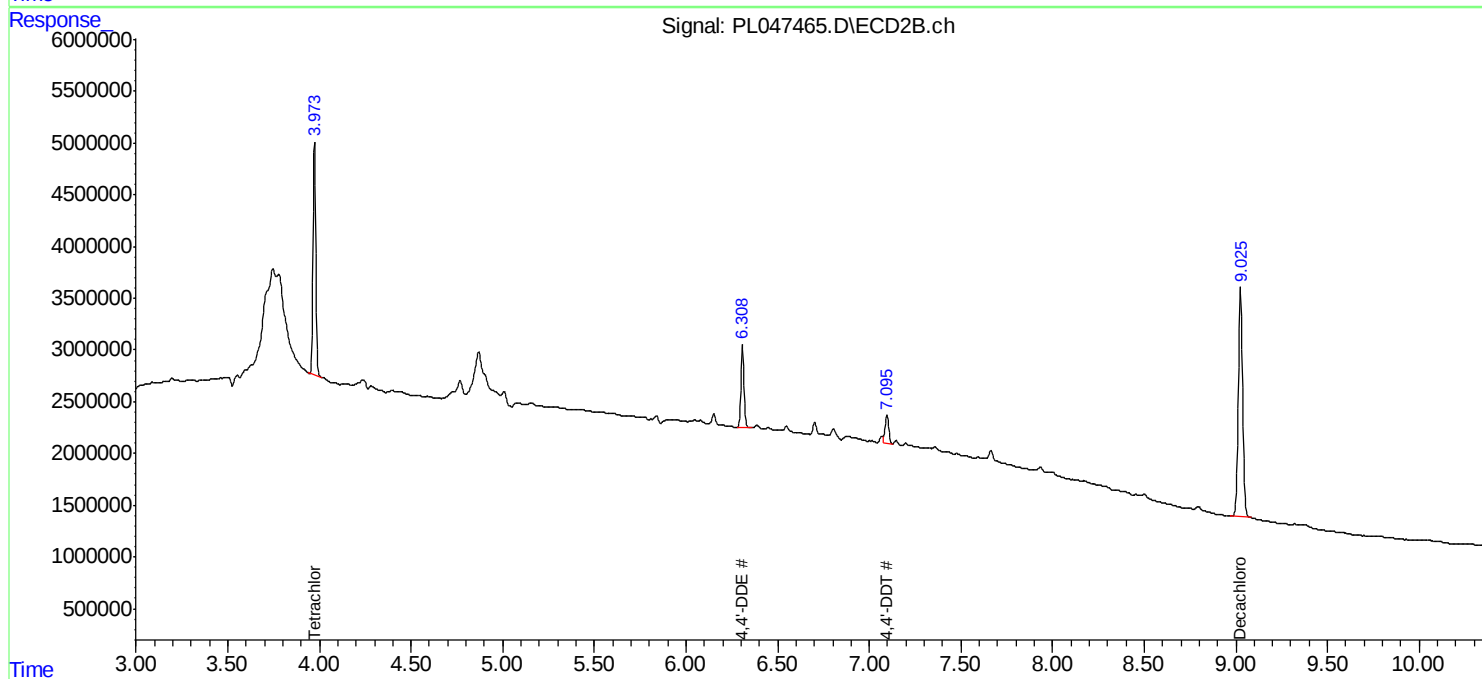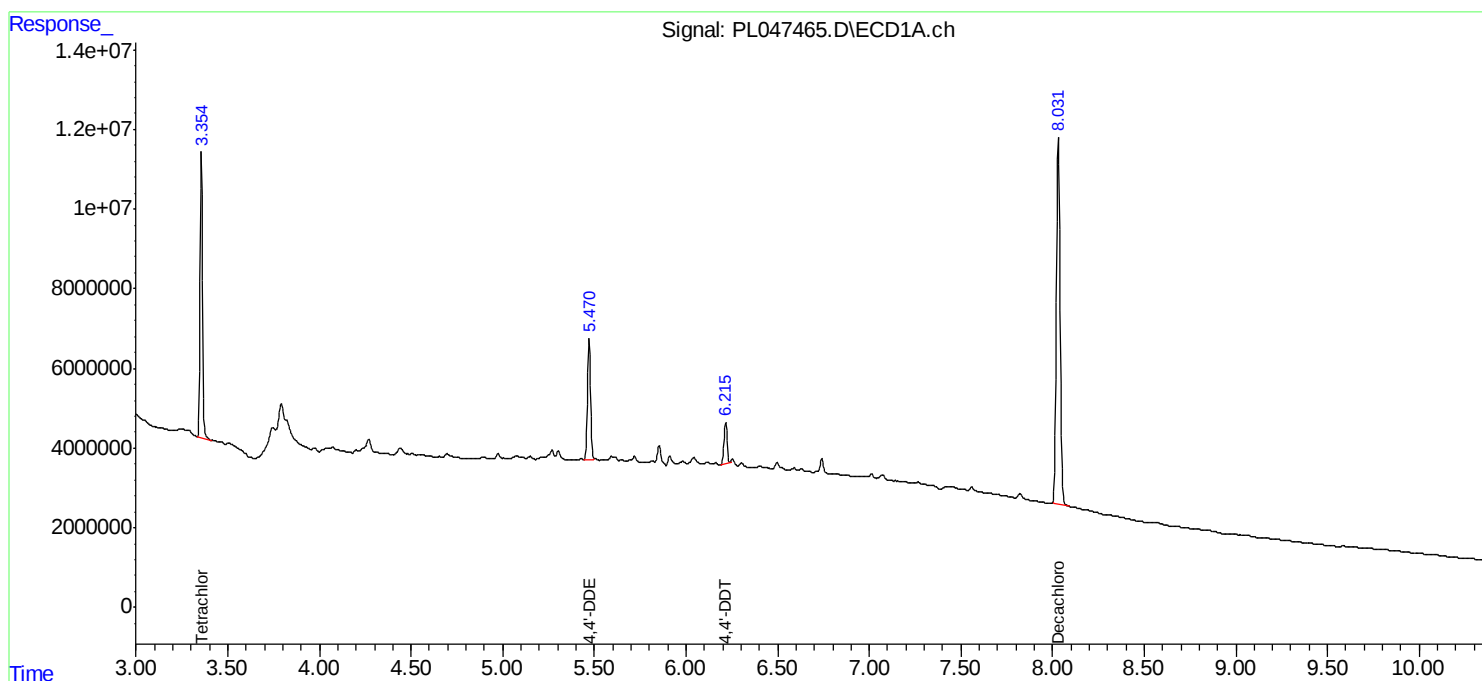

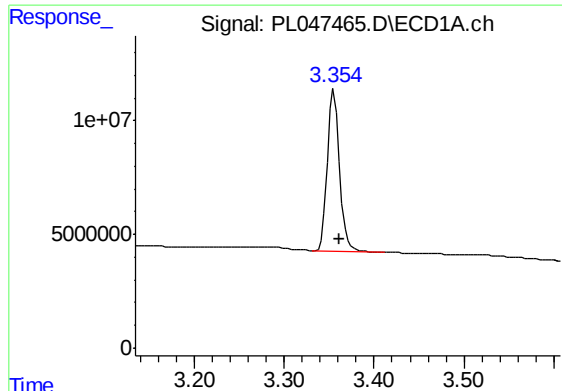


#1 Tetrachloro-m-xylene

R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 67387185
Conc: 9.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S


Manual Integrations
APPROVED

Sohil
4/17/2019 4:53:15 PM

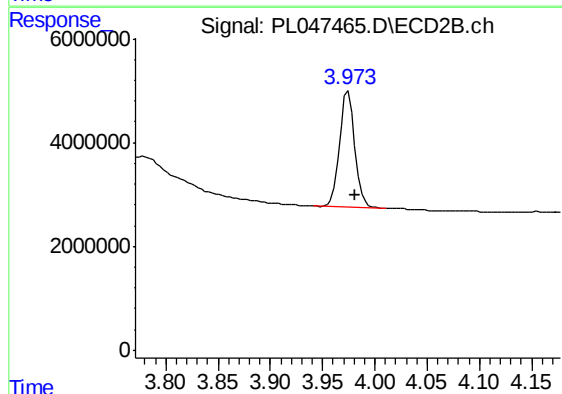


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.006 min
Response: 22813235
Conc: 9.96 ng/ml

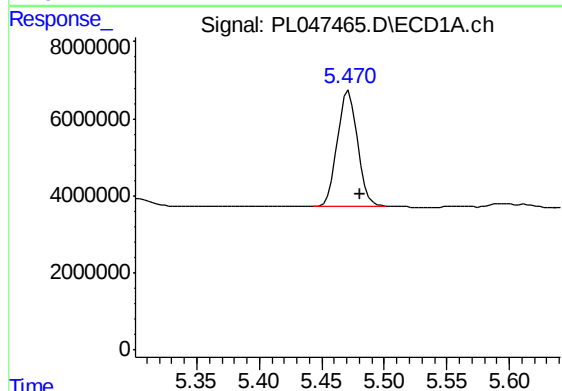


#12 4,4'-DDE

R.T.: 5.470 min
Delta R.T.: -0.010 min
Response: 33872712
Conc: 3.68 ng/ml m

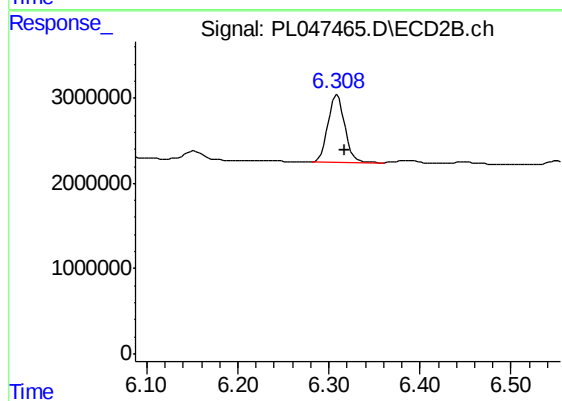

#12 4,4'-DDE

R.T.: 6.309 min
Delta R.T.: -0.009 min
Response: 10005894
Conc: 4.03 ng/ml

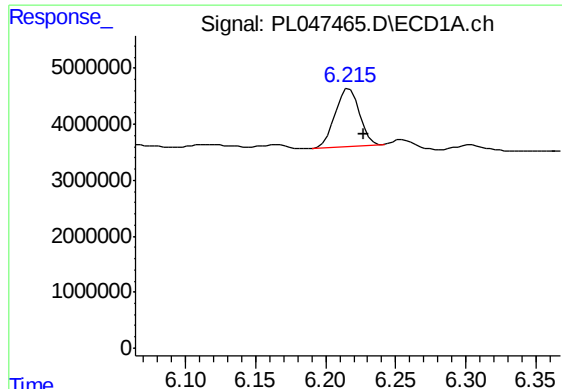


#17 4,4'-DDT

R.T.: 6.217 min
Delta R.T.: -0.011 min
Response: 12648375
Conc: 1.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S


Manual Integrations
APPROVED

Sohil
4/17/2019 4:53:15 PM

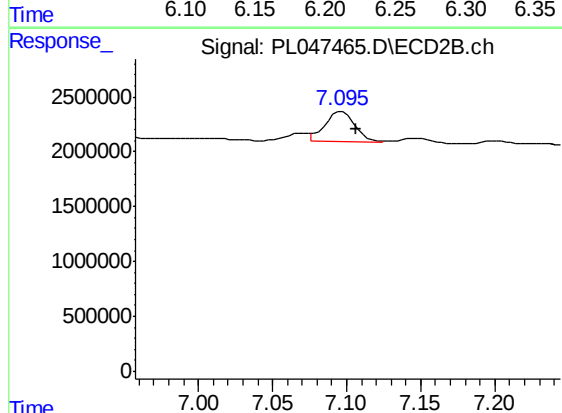


#17 4,4'-DDT

R.T.: 7.095 min
Delta R.T.: -0.012 min
Response: 3770073
Conc: 1.80 ng/ml m

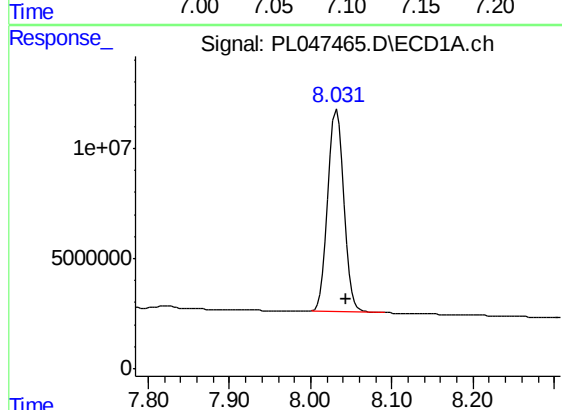

#28 Decachlorobiphenyl

R.T.: 8.032 min
Delta R.T.: -0.012 min
Response: 125823440
Conc: 14.96 ng/ml

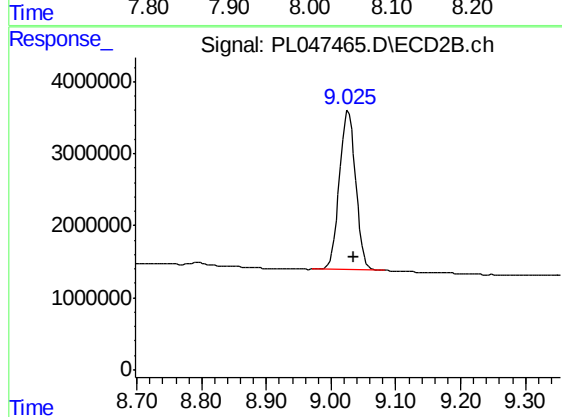

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.009 min
Response: 38606863
Conc: 16.65 ng/ml