

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
 Data File : PL047482.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2019 02:20
 Operator : AJ\SJ
 Sample : K2422-08
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP1-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 04:51:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	3.975	144.8E6	46800575	19.906	20.440
28)	SA Decachlor...	8.032	9.026	162.4E6	48689998	19.314	21.001
Target Compounds							
20)	A Methoxychlor	6.762	7.556	66224431	21529616	15.583	16.889



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
Data File : PL047482.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2019 02:20
Operator : AJ\SJ
Sample : K2422-08
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP1-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 04:51:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

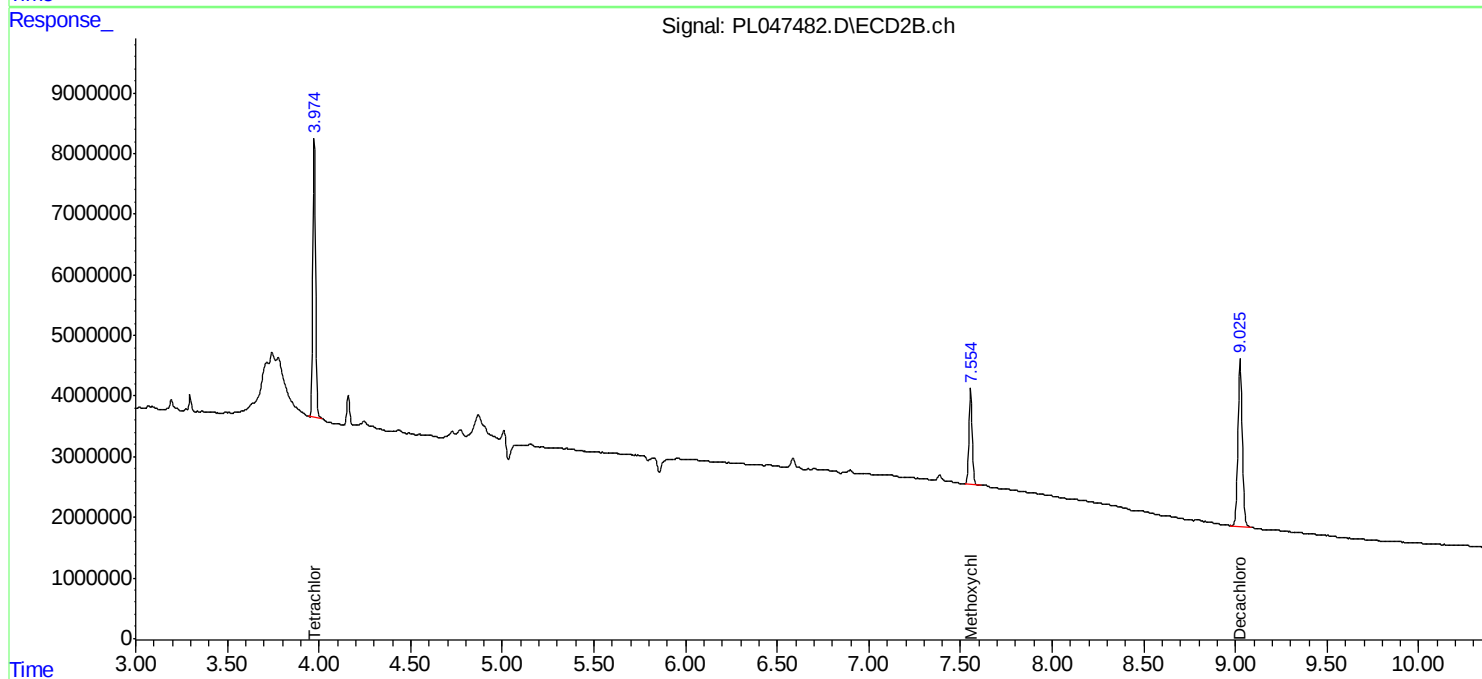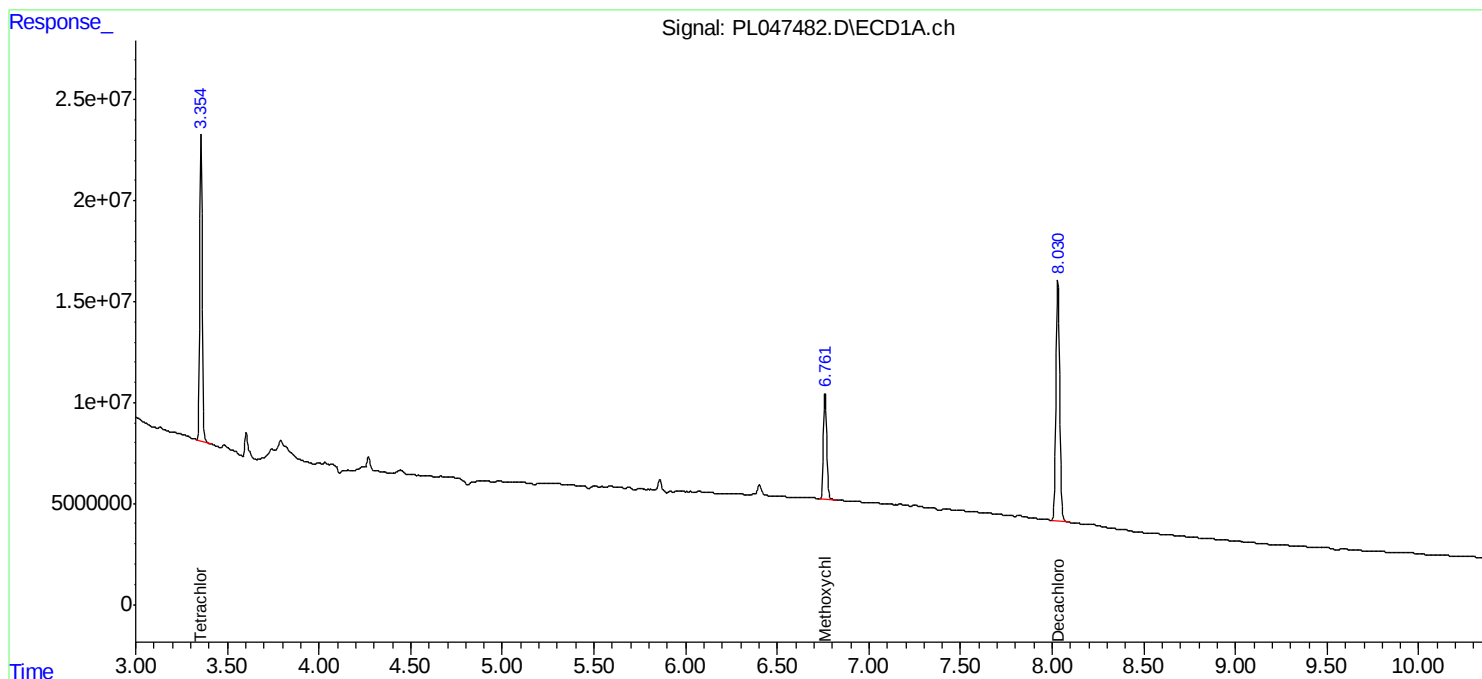


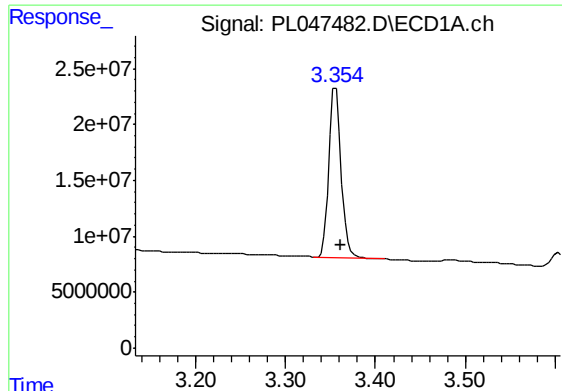

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 144806157
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-D

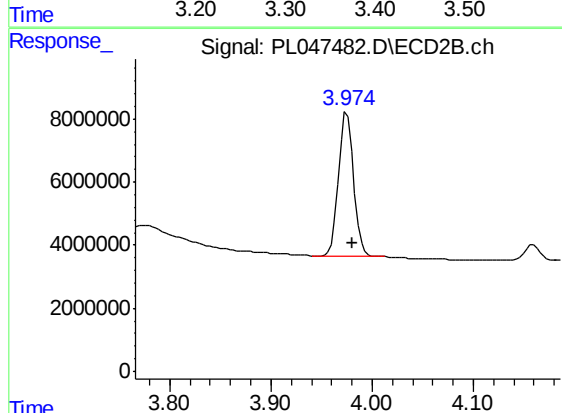


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.005 min
Response: 46800575
Conc: 20.44 ng/ml

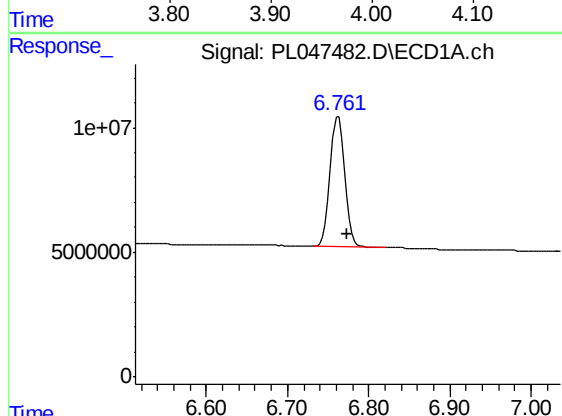


#20 Methoxychlor

R.T.: 6.762 min
Delta R.T.: -0.011 min
Response: 66224431
Conc: 15.58 ng/ml

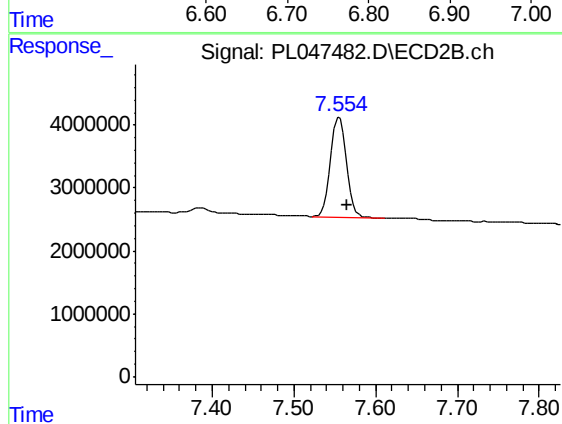

#20 Methoxychlor


R.T.: 7.556 min
Delta R.T.: -0.010 min
Response: 21529616
Conc: 16.89 ng/ml

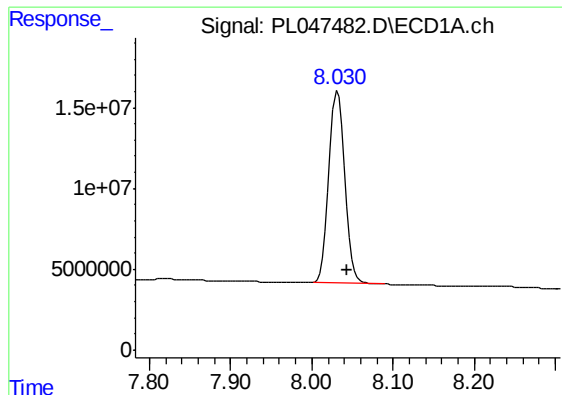

#28 Decachlorobiphenyl

R.T.: 8.032 min
Delta R.T.: -0.012 min
Response: 162447348
Conc: 19.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-D

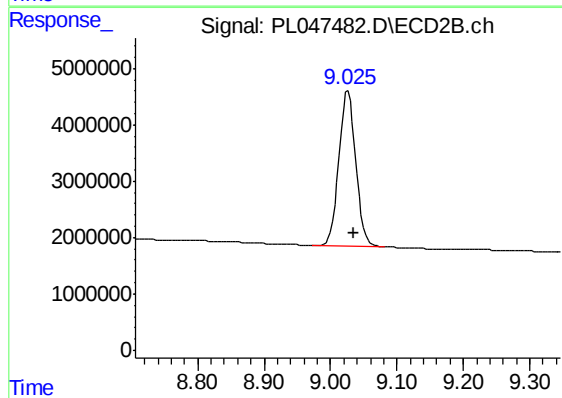

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.009 min
Response: 48689998
Conc: 21.00 ng/ml