

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
 Data File : PL047483.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2019 02:35
 Operator : AJ\SJ
 Sample : K2422-12
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP3-S

Manual Integrations
 APPROVED

Sohil
 4/17/2019 4:53:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 04:52:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.355	3.974	134.7E6	43211580	18.513	18.873
28) SA Decachlor...	8.031	9.025	148.8E6	44203159	17.694	19.066
Target Compounds						
20) A Methoxychlor	6.761	7.553	5019859	1715638	1.181m	1.346m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041619\
Data File : PL047483.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2019 02:35
Operator : AJ\SJ
Sample : K2422-12
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP3-S


Manual Integrations
APPROVED

Sohil
4/17/2019 4:53:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 04:52:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

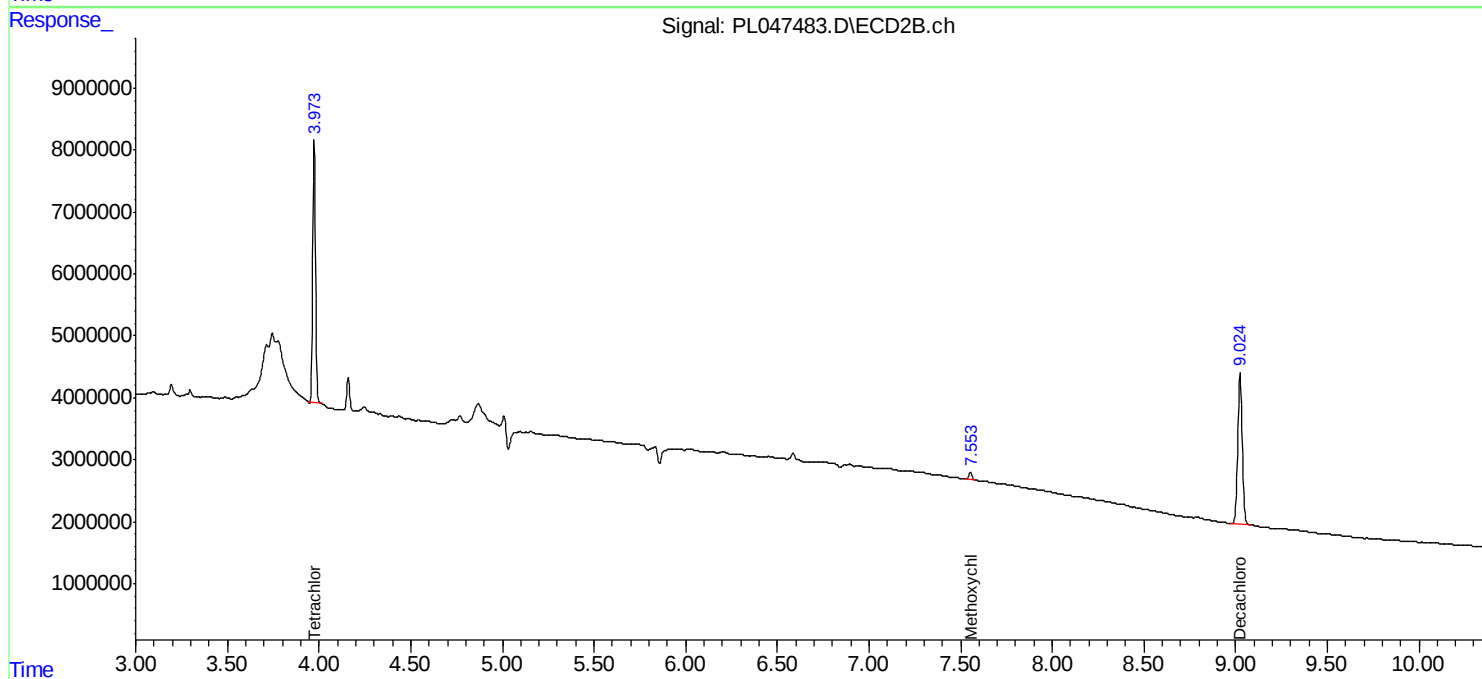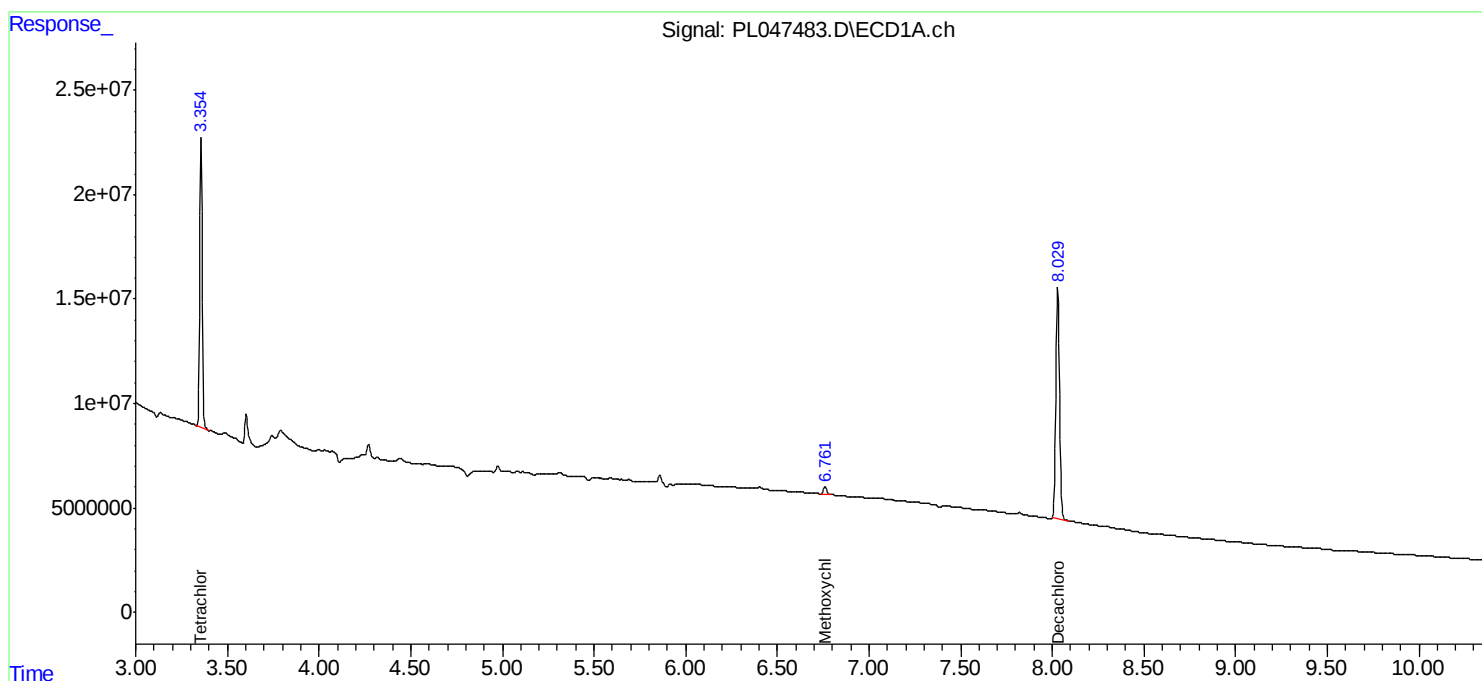

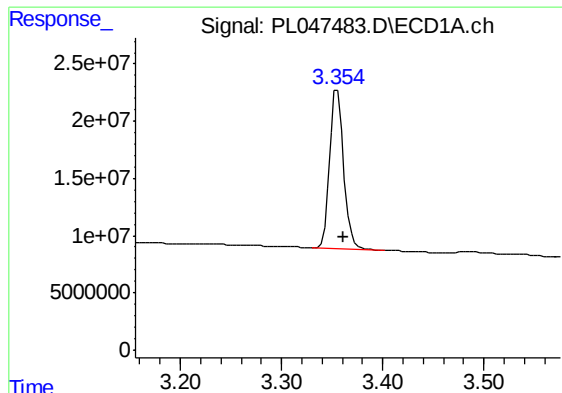


#1 Tetrachloro-m-xylene

R.T.: 3.355 min
Delta R.T.: -0.006 min
Response: 134679010
Conc: 18.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP3-S


Manual Integrations
APPROVED

Sohil
4/17/2019 4:53:24 PM

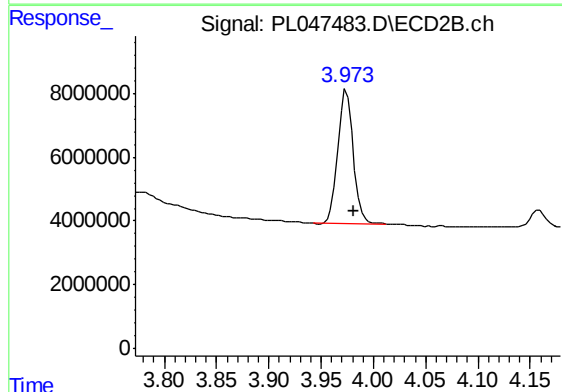


#1 Tetrachloro-m-xylene

R.T.: 3.974 min
Delta R.T.: -0.006 min
Response: 43211580
Conc: 18.87 ng/ml

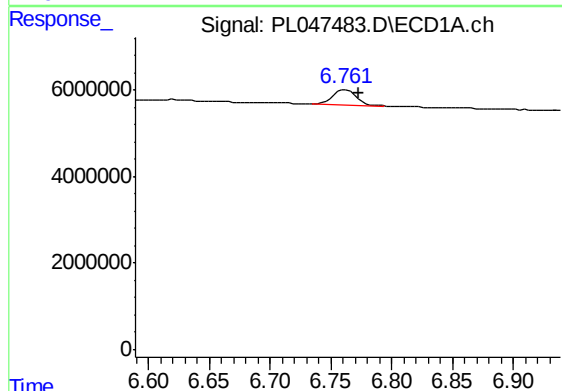


#20 Methoxychlor

R.T.: 6.761 min
Delta R.T.: -0.013 min
Response: 5019859
Conc: 1.18 ng/ml m

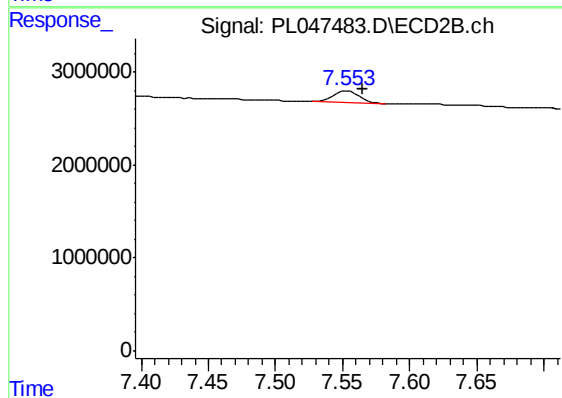

#20 Methoxychlor

R.T.: 7.553 min
Delta R.T.: -0.013 min
Response: 1715638
Conc: 1.35 ng/ml m

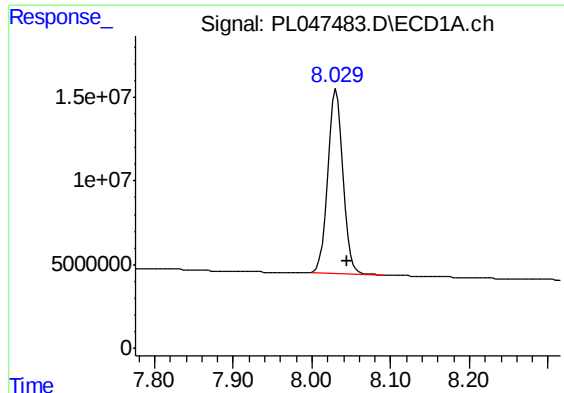


#28 Decachlorobiphenyl

R.T.: 8.031 min
Delta R.T.: -0.014 min
Response: 148821744
Conc: 17.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP3-S

Manual Integrations
APPROVED

Sohil
4/17/2019 4:53:24 PM

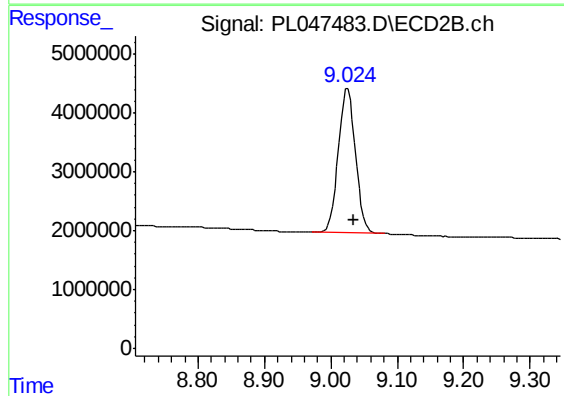

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: -0.010 min
Response: 44203159
Conc: 19.07 ng/ml