

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041620\
 Data File : PL058082.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2020 20:18
 Operator : AJ\MA
 Sample : L2284-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-11-SA

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 01:09:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.955	200.6E6	41026778	19.896	18.905
28)	SA Decachlor...	8.202	8.975	226.2E6	51349058	21.946	22.988
Target Compounds							
2)	A alpha-BHC	3.888	4.348	5259485	-207299	0.303	N.D. #
4)	MA Heptachlor	4.491	5.131	57107	2057267	0.004	0.613 #
5)	MB Aldrin	0.000	5.406f	0	138144	N.D.	0.043 #
6)	B beta-BHC	4.432	0.000	2456337	0	0.389	N.D. #
7)	B delta-BHC	4.640	0.000	9277824	0	0.611	N.D. #
8)	B Heptachlo...	0.000	5.797f	0	9009231	N.D.	3.336 #
13)	MA Dieldrin	0.000	6.442f	0	310165	N.D.	0.102 #
15)	B Endosulfa...	0.000	6.867	0	746234	N.D.	0.288 #
24)	Chlordane-2	4.847f	5.406	1523828	138144	3.775	1.324 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041620\
Data File : PL058082.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2020 20:18
Operator : AJ\MA
Sample : L2284-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-11-SA

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 01:09:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

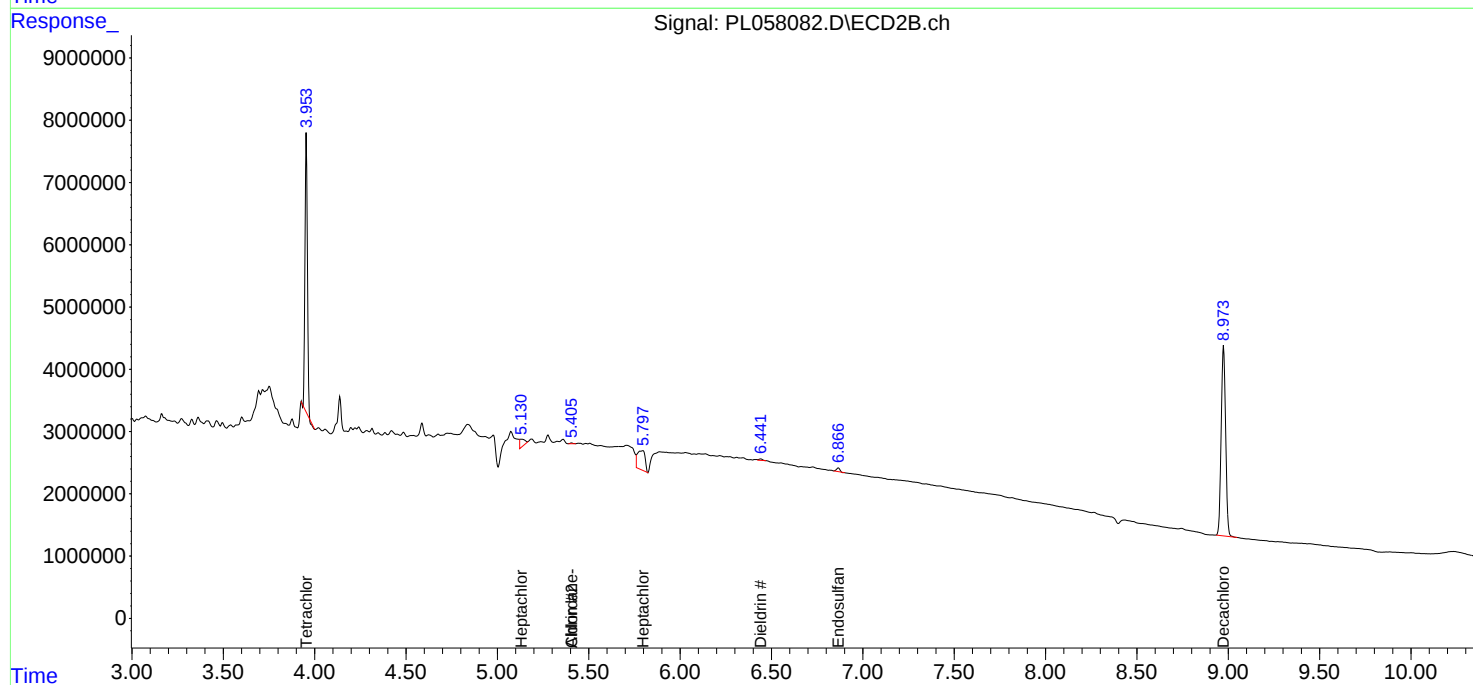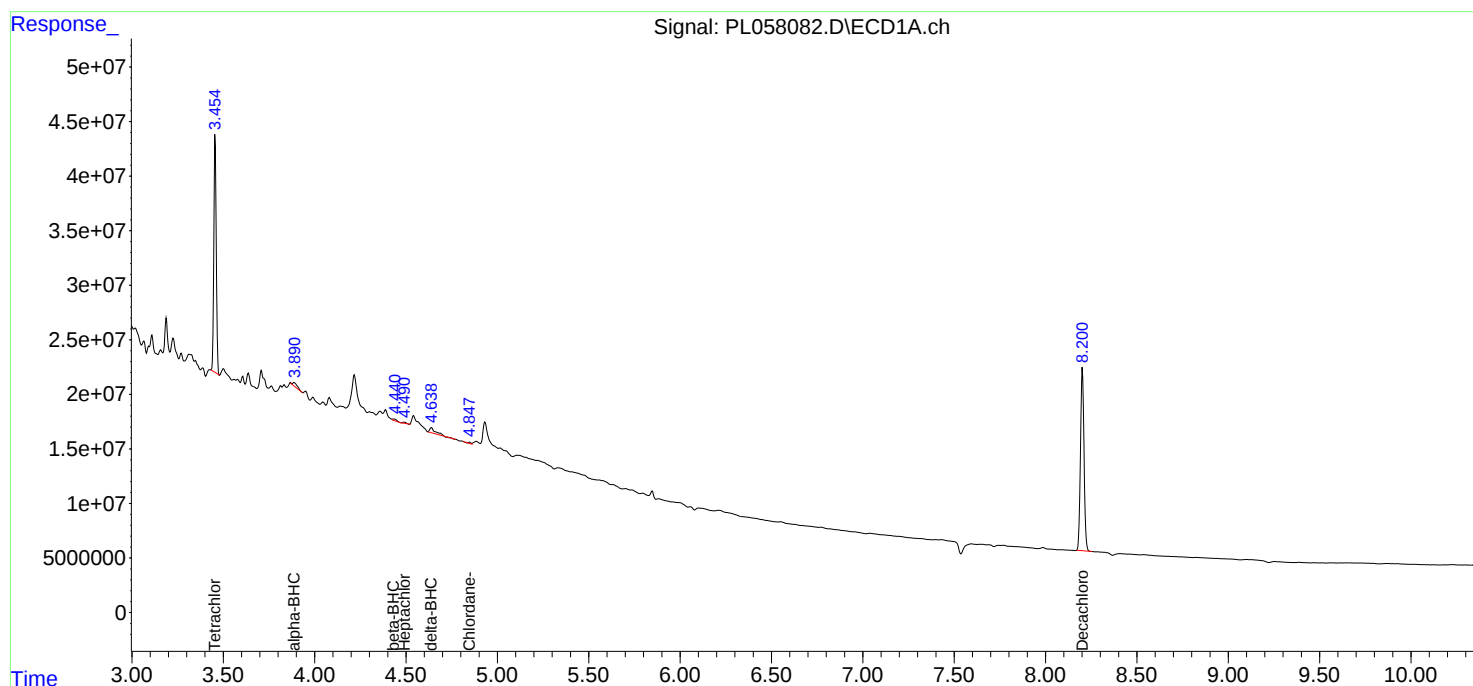


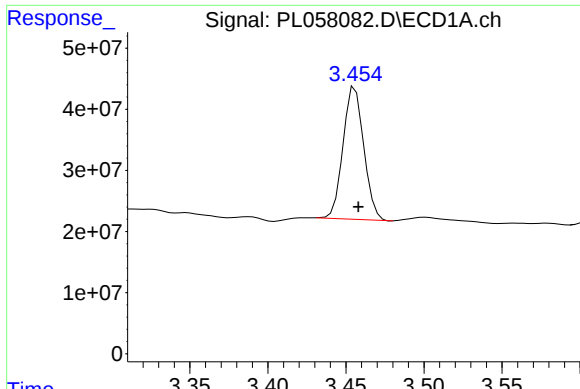

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 200576500
Conc: 19.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-11-SA

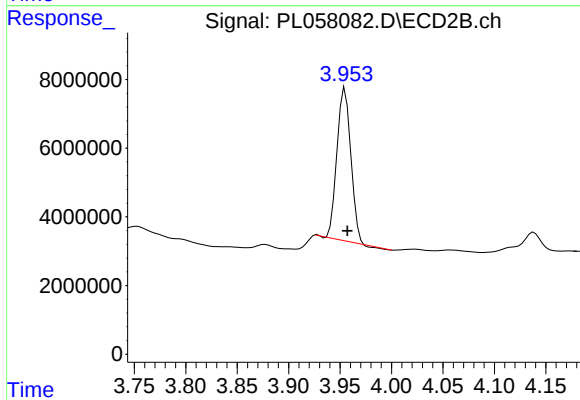


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 41026778
Conc: 18.91 ng/ml

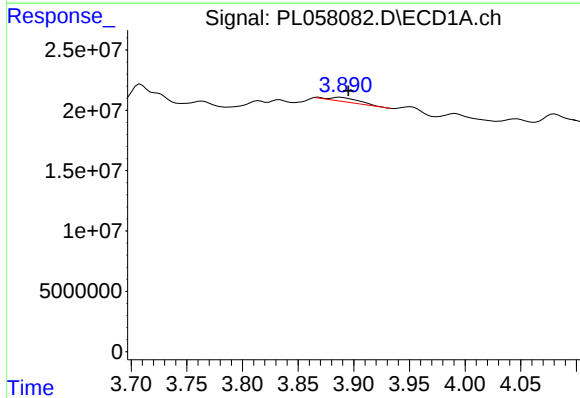


#2 alpha-BHC

R.T.: 3.888 min
Delta R.T.: -0.007 min
Response: 5259485
Conc: 0.30 ng/ml

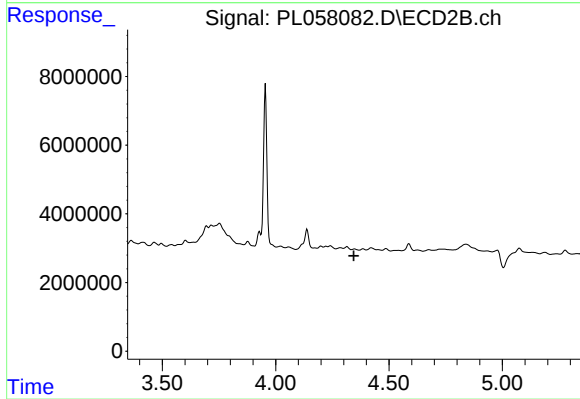

#2 alpha-BHC


R.T.: 4.348 min
Delta R.T.: 0.003 min
Response: -207299
Conc: N.D.

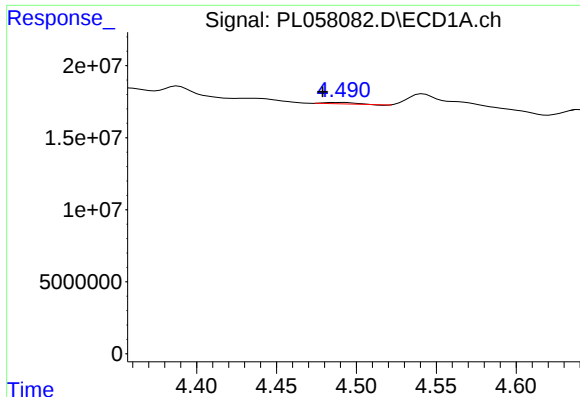

#4 Heptachlor


R.T.: 4.491 min
Delta R.T.: 0.012 min
Response: 57107
Conc: 0.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-11-SA

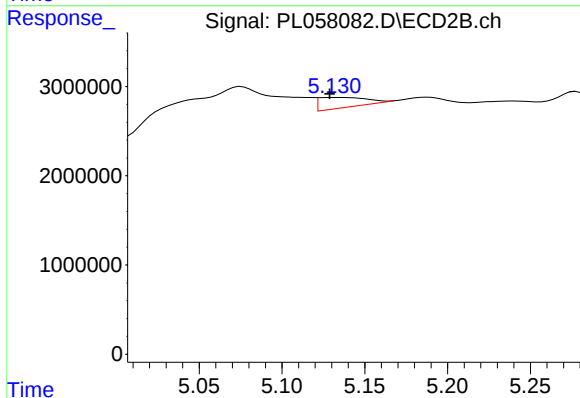


#4 Heptachlor

R.T.: 5.131 min
Delta R.T.: 0.003 min
Response: 2057267
Conc: 0.61 ng/ml

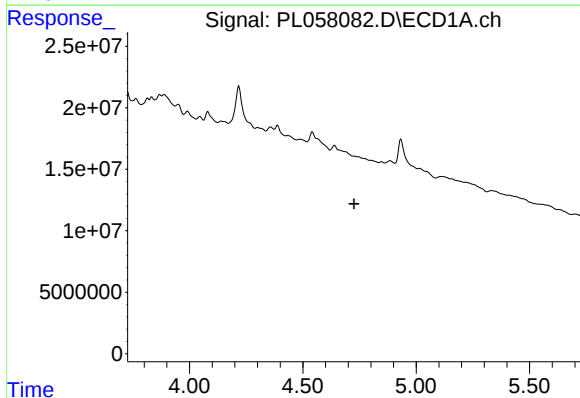


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.727 min
Response: 0
Conc: N.D.

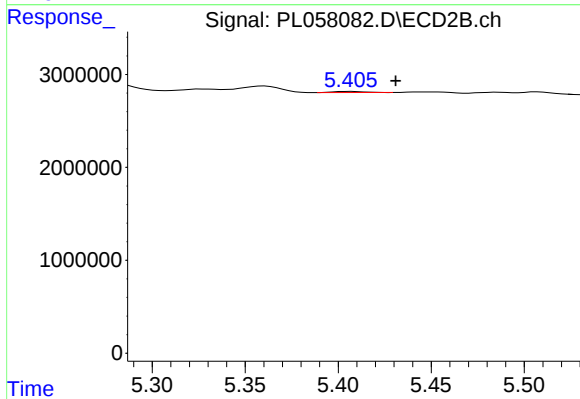

#5 Aldrin


R.T.: 5.406 min
Delta R.T.: -0.025 min
Response: 138144
Conc: 0.04 ng/ml

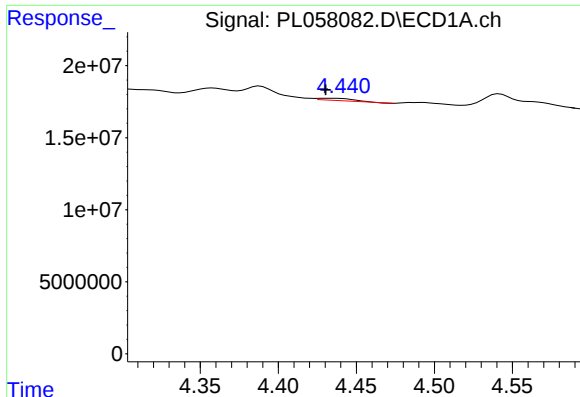

#6 beta-BHC


R.T.: 4.432 min
Delta R.T.: 0.002 min
Response: 2456337
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-11-SA

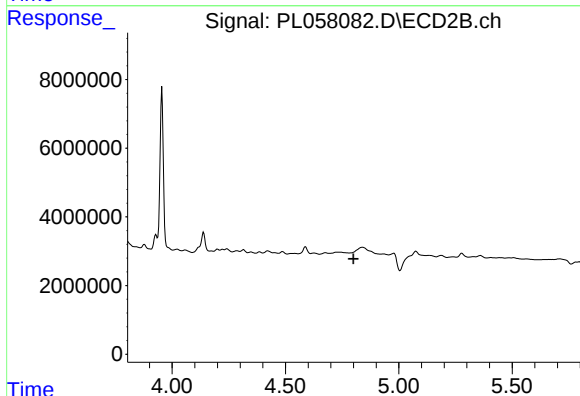


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

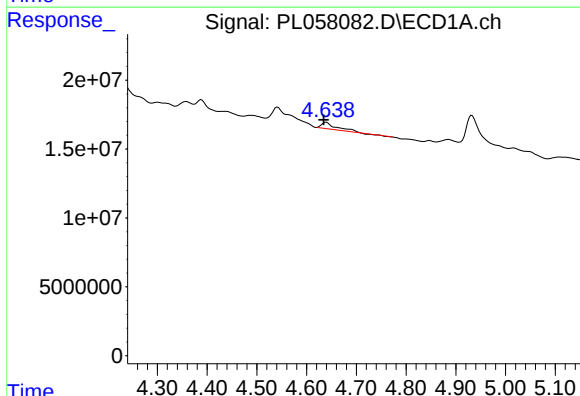


#7 delta-BHC

R.T.: 4.640 min
Delta R.T.: 0.005 min
Response: 9277824
Conc: 0.61 ng/ml

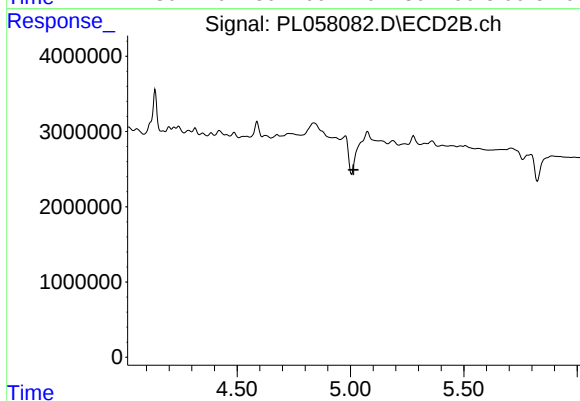

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 5.014 min
Response: 0
Conc: N.D.

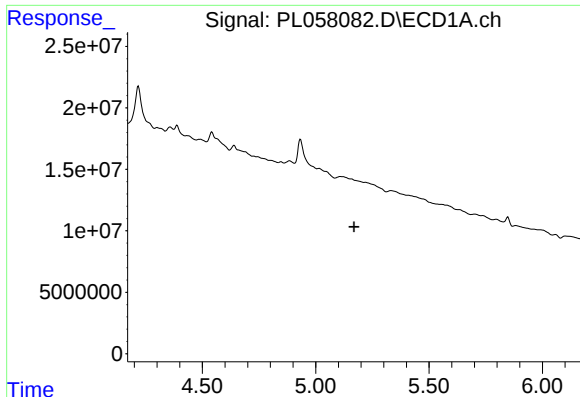

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-11-SA

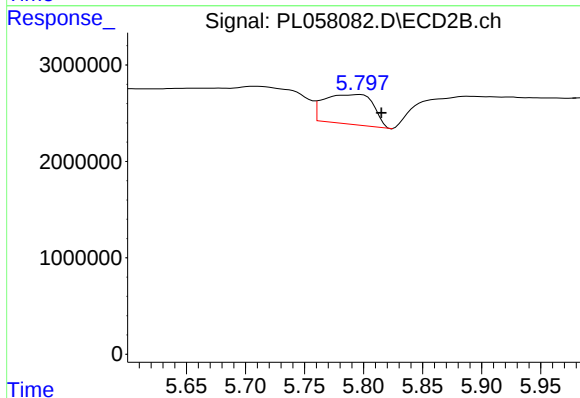


#8 Heptachlor epoxide

R.T.: 5.797 min
Delta R.T.: -0.018 min
Response: 9009231
Conc: 3.34 ng/ml

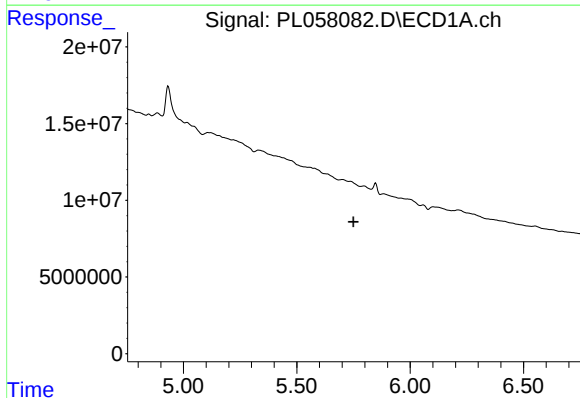


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

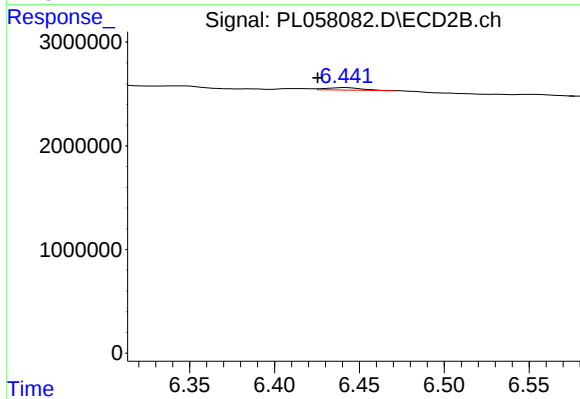

#13 Dieldrin


R.T.: 6.442 min
Delta R.T.: 0.017 min
Response: 310165
Conc: 0.10 ng/ml

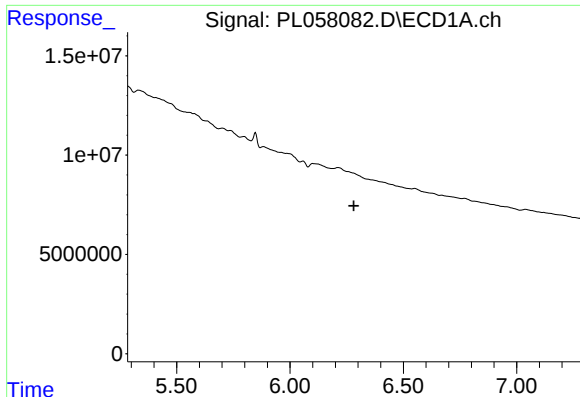

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-11-SA

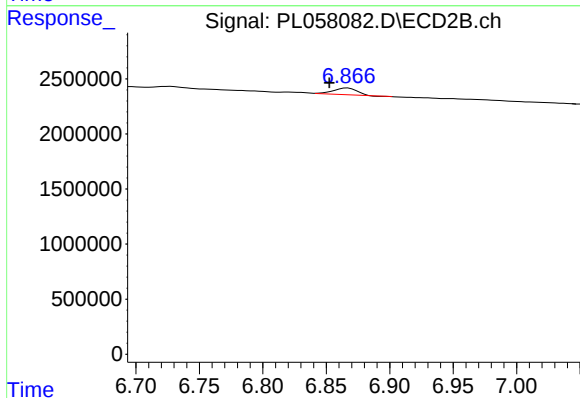


#15 Endosulfan II

R.T.: 6.867 min
Delta R.T.: 0.015 min
Response: 746234
Conc: 0.29 ng/ml

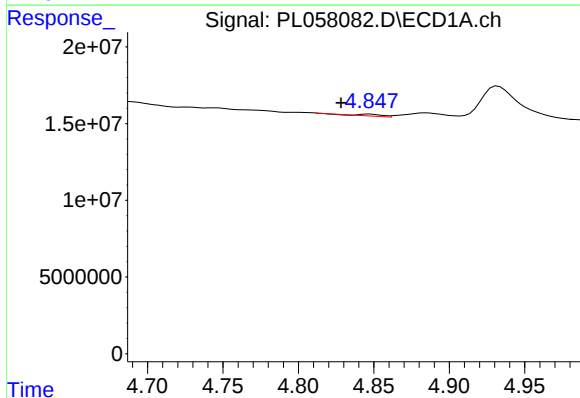


#24 Chlordane-2

R.T.: 4.847 min
Delta R.T.: 0.019 min
Response: 1523828
Conc: 3.77 ng/ml

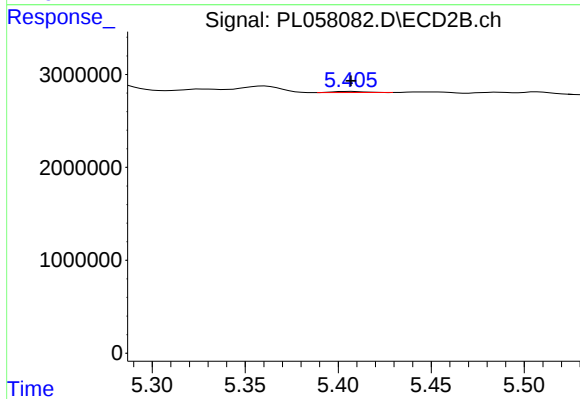

#24 Chlordane-2


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 138144
Conc: 1.32 ng/ml

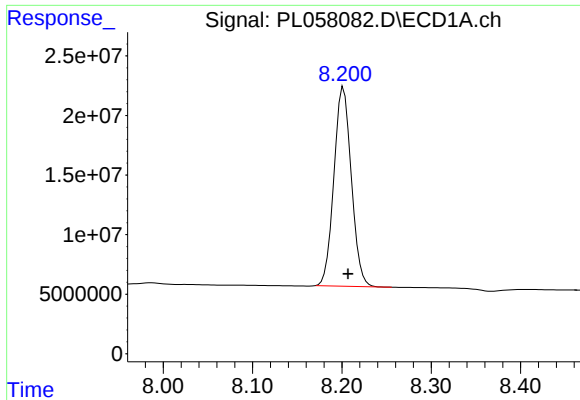

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.005 min
Response: 226228512
Conc: 21.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-11-SA

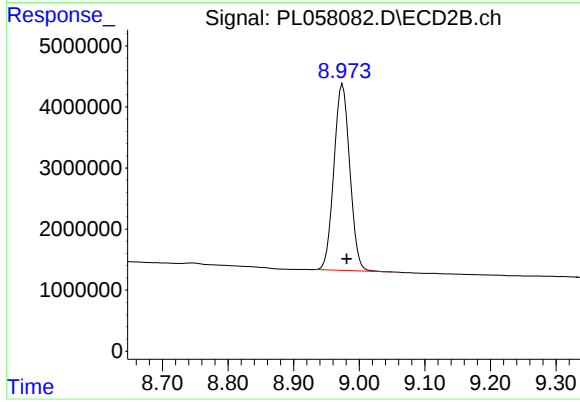

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: -0.006 min
Response: 51349058
Conc: 22.99 ng/ml