

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041620\
 Data File : PL058083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2020 20:33
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 01:09:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.955	243.4E6	48153446	24.147	22.189
28)	SA Decachlor...	8.202	8.974	238.9E6	53020451	23.180	23.736
Target Compounds							
2)	A alpha-BHC	3.897	0.000	5436811	0	0.313	N.D. #
4)	MA Heptachlor	0.000	5.133	0	9993495	N.D.	2.978 #
8)	B Heptachlo...	0.000	5.799f	0	5100489	N.D.	1.889 #
11)	B alpha-Chl...	5.447	0.000	4864804	0	0.365	N.D. #
15)	B Endosulfa...	0.000	6.866	0	612772	N.D.	0.236 #
16)	A 4,4'-DDD	6.109f	0.000	1722965	0	0.172	N.D. #
23)	Chlordane-1	4.351f	0.000	1326095	0	3.585	N.D. #
26)	Chlordane-4	5.447	0.000	4864804	0	4.677	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041620\
Data File : PL058083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2020 20:33
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 01:09:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

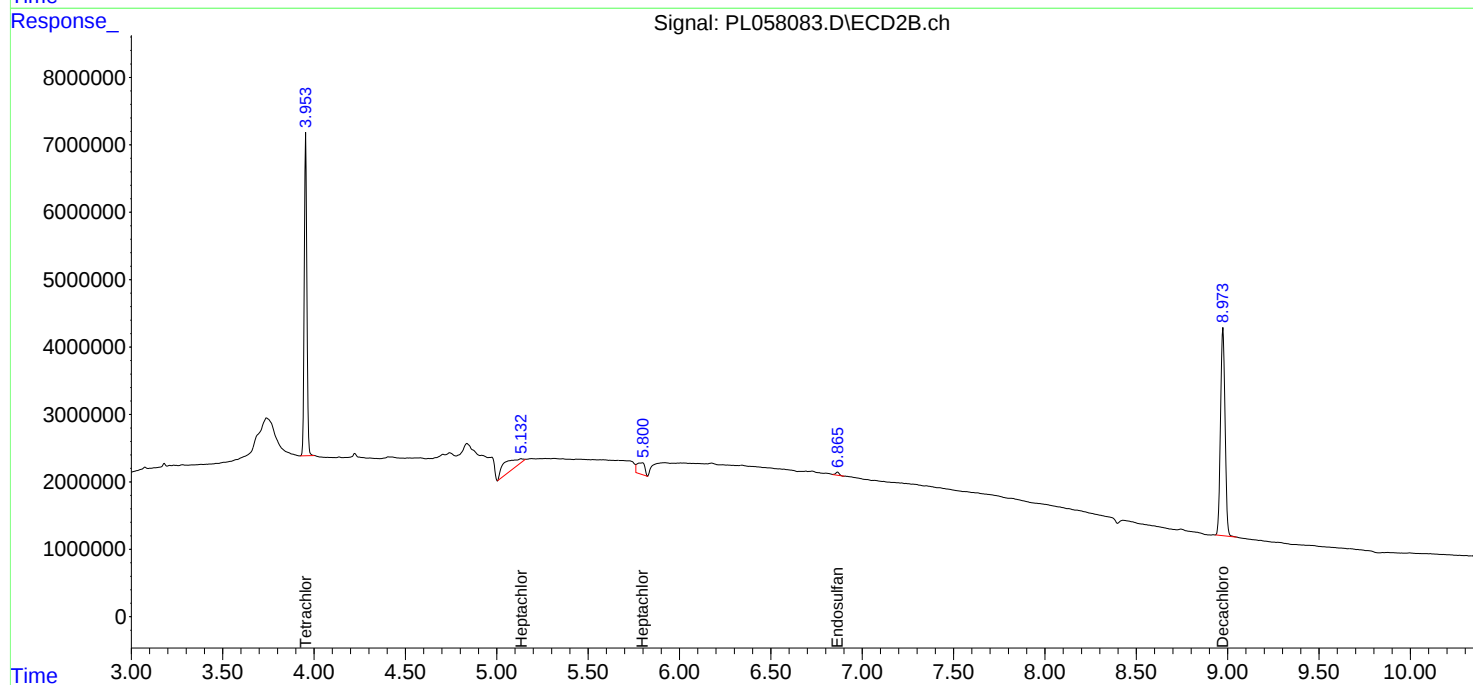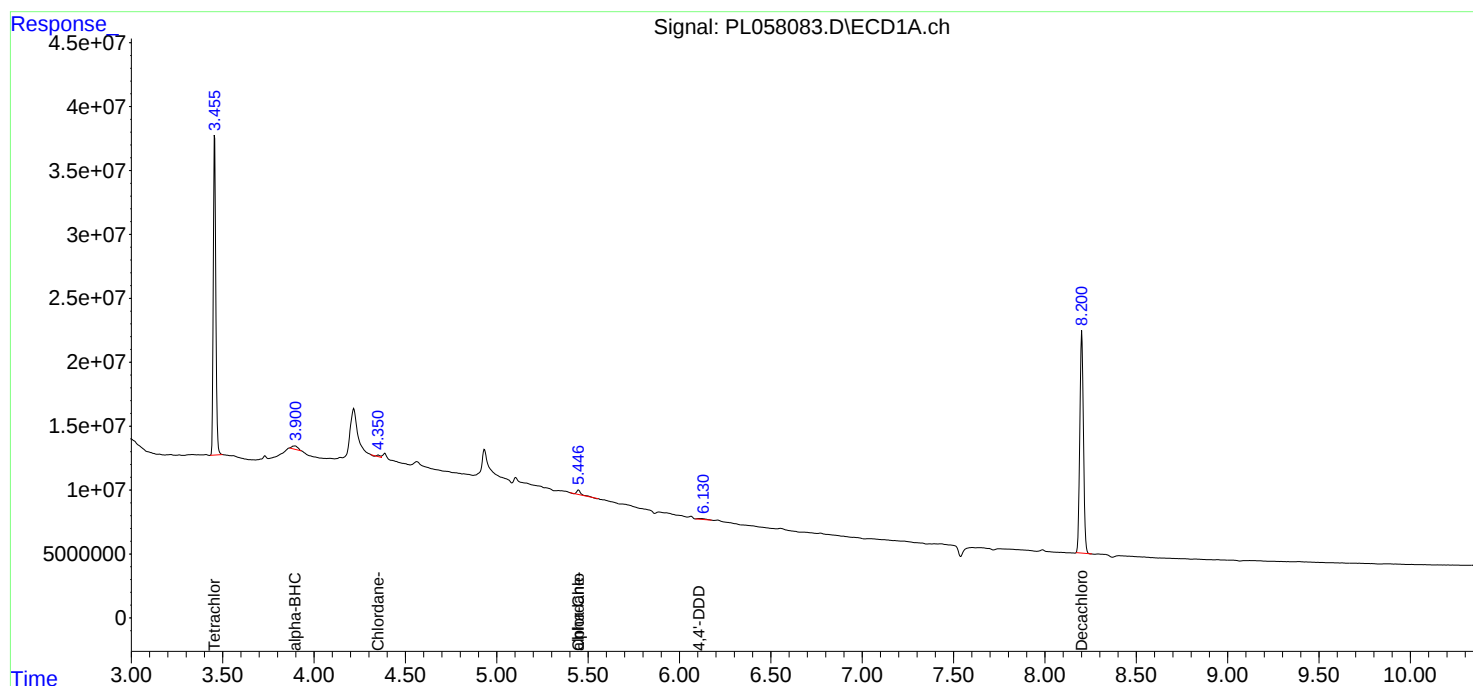


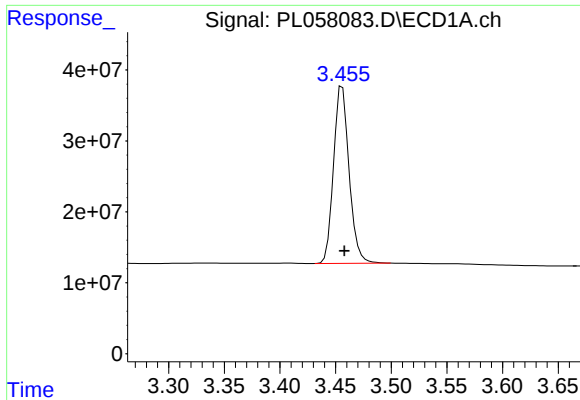

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 243427374
Conc: 24.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

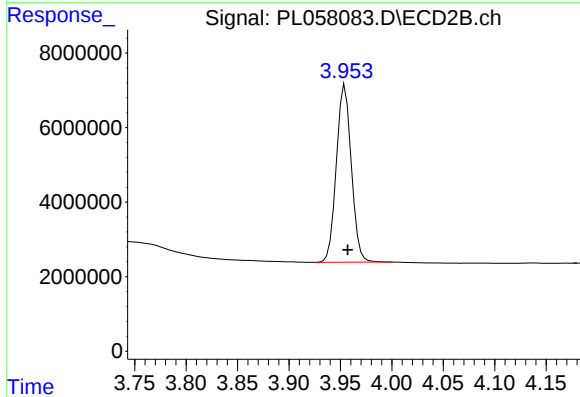


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.003 min
Response: 48153446
Conc: 22.19 ng/ml

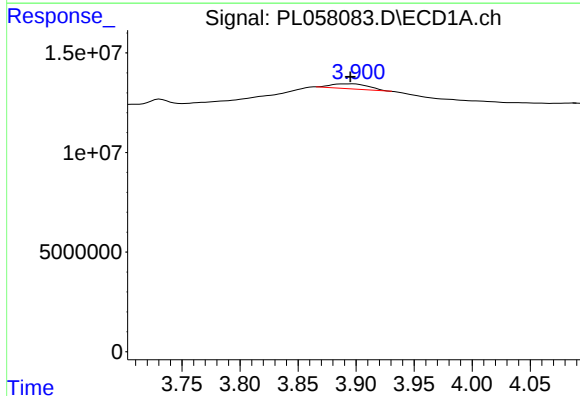


#2 alpha-BHC

R.T.: 3.897 min
Delta R.T.: 0.002 min
Response: 5436811
Conc: 0.31 ng/ml

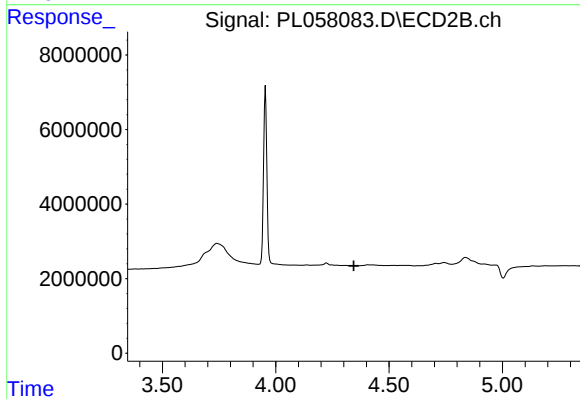

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

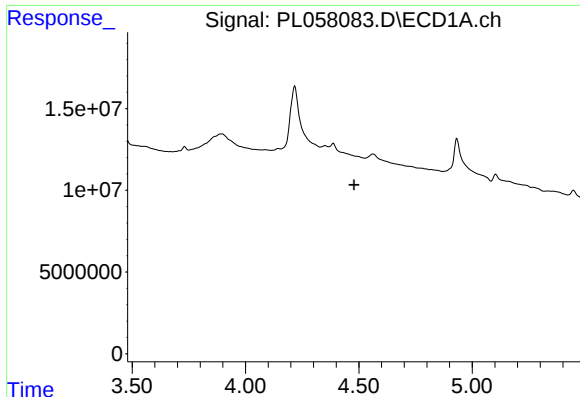

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

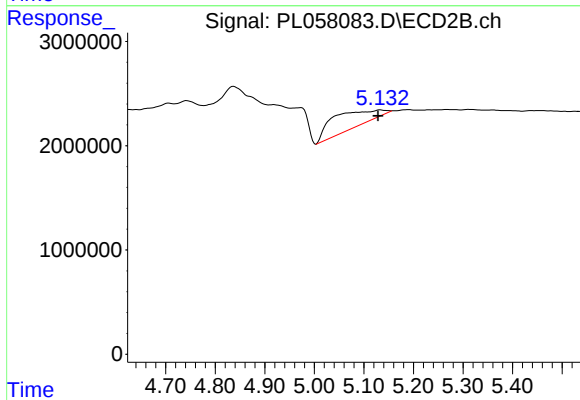


#4 Heptachlor

R.T.: 5.133 min
Delta R.T.: 0.004 min
Response: 9993495
Conc: 2.98 ng/ml

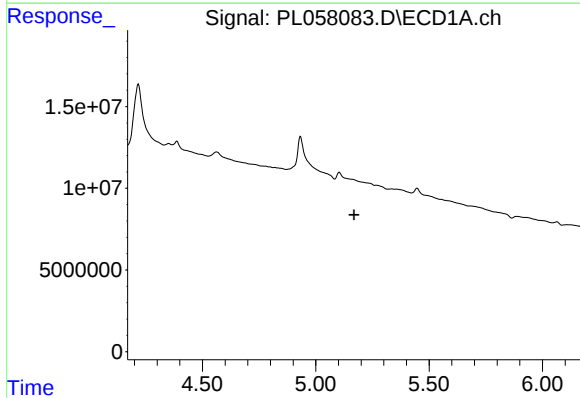


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

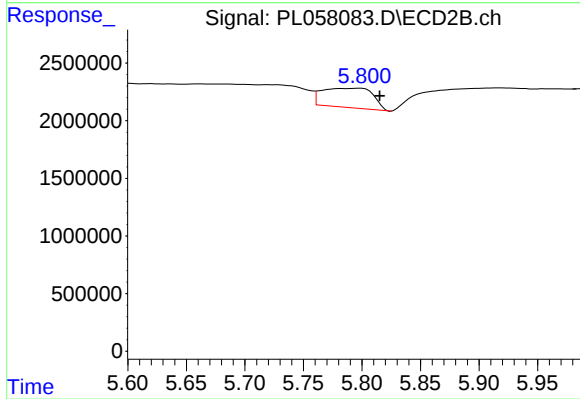

#8 Heptachlor epoxide


R.T.: 5.799 min
Delta R.T.: -0.016 min
Response: 5100489
Conc: 1.89 ng/ml

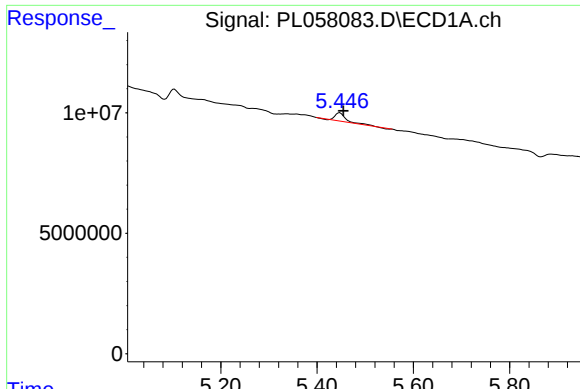

#11 alpha-Chlordane


R.T.: 5.447 min
Delta R.T.: -0.007 min
Response: 4864804
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

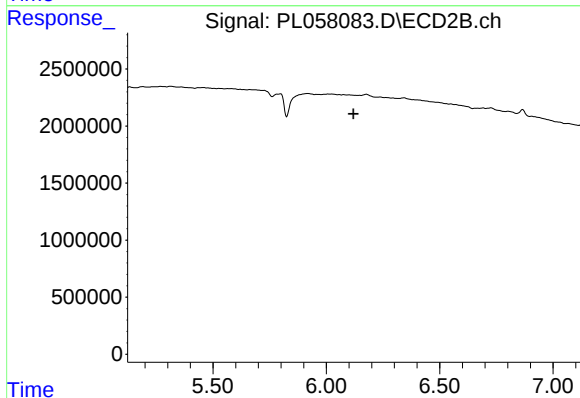


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

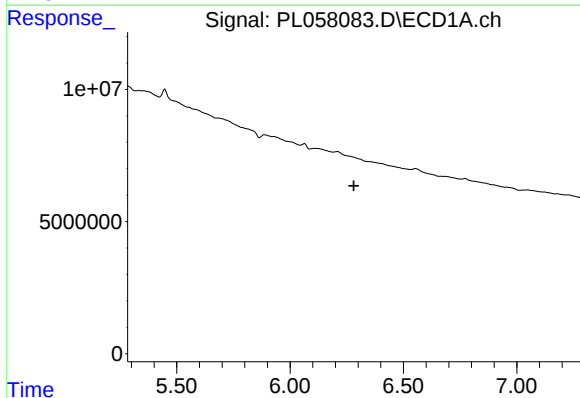


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

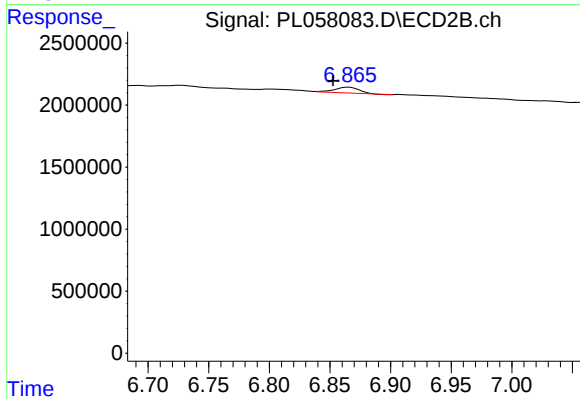

#15 Endosulfan II


R.T.: 6.866 min
Delta R.T.: 0.013 min
Response: 612772
Conc: 0.24 ng/ml

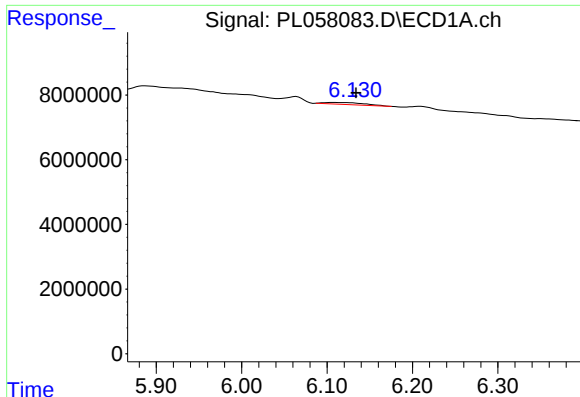

#16 4,4'-DDD


R.T.: 6.109 min
Delta R.T.: -0.025 min
Response: 1722965
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

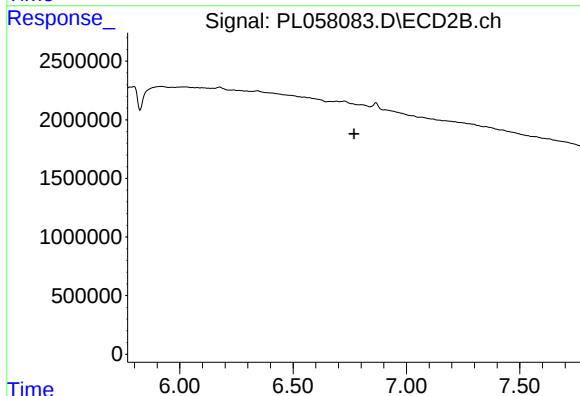


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.769 min
Response: 0
Conc: N.D.

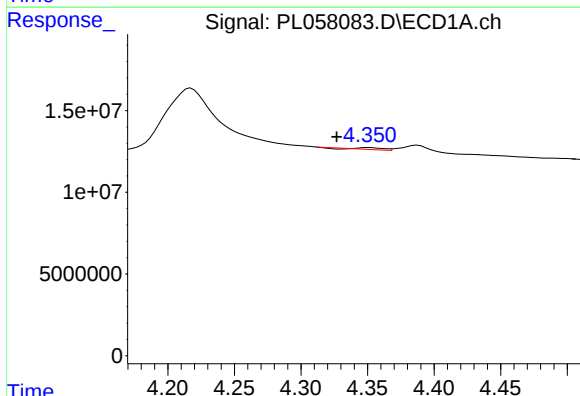


#23 Chlordane-1

R.T.: 4.351 min
Delta R.T.: 0.024 min
Response: 1326095
Conc: 3.59 ng/ml

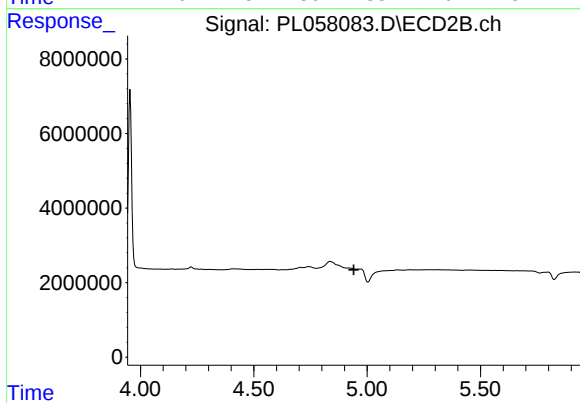

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

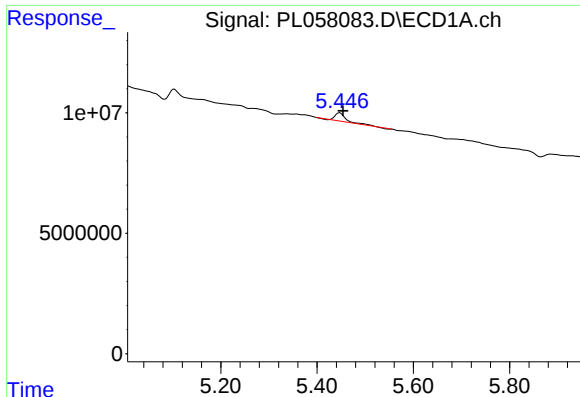

#26 Chlordane-4


R.T.: 5.447 min
Delta R.T.: -0.007 min
Response: 4864804
Conc: 4.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

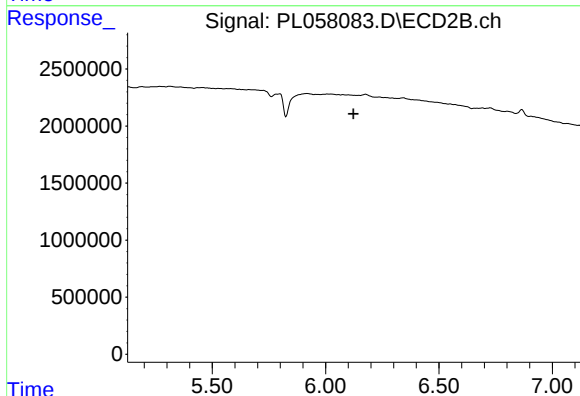


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

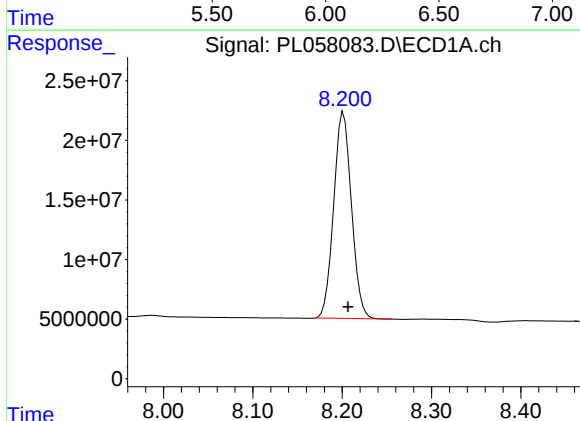

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.005 min
Response: 238946006
Conc: 23.18 ng/ml

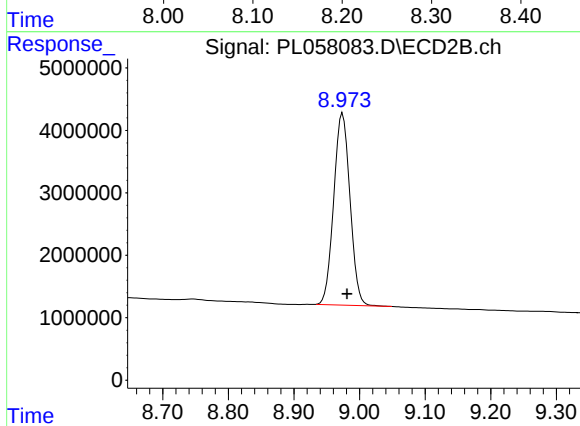

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.007 min
Response: 53020451
Conc: 23.74 ng/ml