

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041620\
 Data File : PL058118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 04:49
 Operator : AJ\MA
 Sample : L2307-03
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 05:22:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.955	220.9E6	49113636	21.914	22.632
28)	SA Decachlor...	8.201	8.973	174.7E6	39006471	16.948	17.462
Target Compounds							
4)	MA Heptachlor	4.469	5.135	5431466	1281672	0.339	0.382
8)	B Heptachlo...	0.000	5.796f	0	6909512	N.D.	2.559 #
15)	B Endosulfa...	6.312f	6.866	4435070	503409	0.401	0.194 #
19)	B Endosulfa...	6.674	0.000	872256	0	0.086	N.D. #
23)	Chlordane-1	4.305f	0.000	2785826	0	7.532	N.D. #
27)	Chlordane-5	6.312f	0.000	4435070	0	11.724	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041620\
Data File : PL058118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 04:49
Operator : AJ\MA
Sample : L2307-03
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 05:22:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

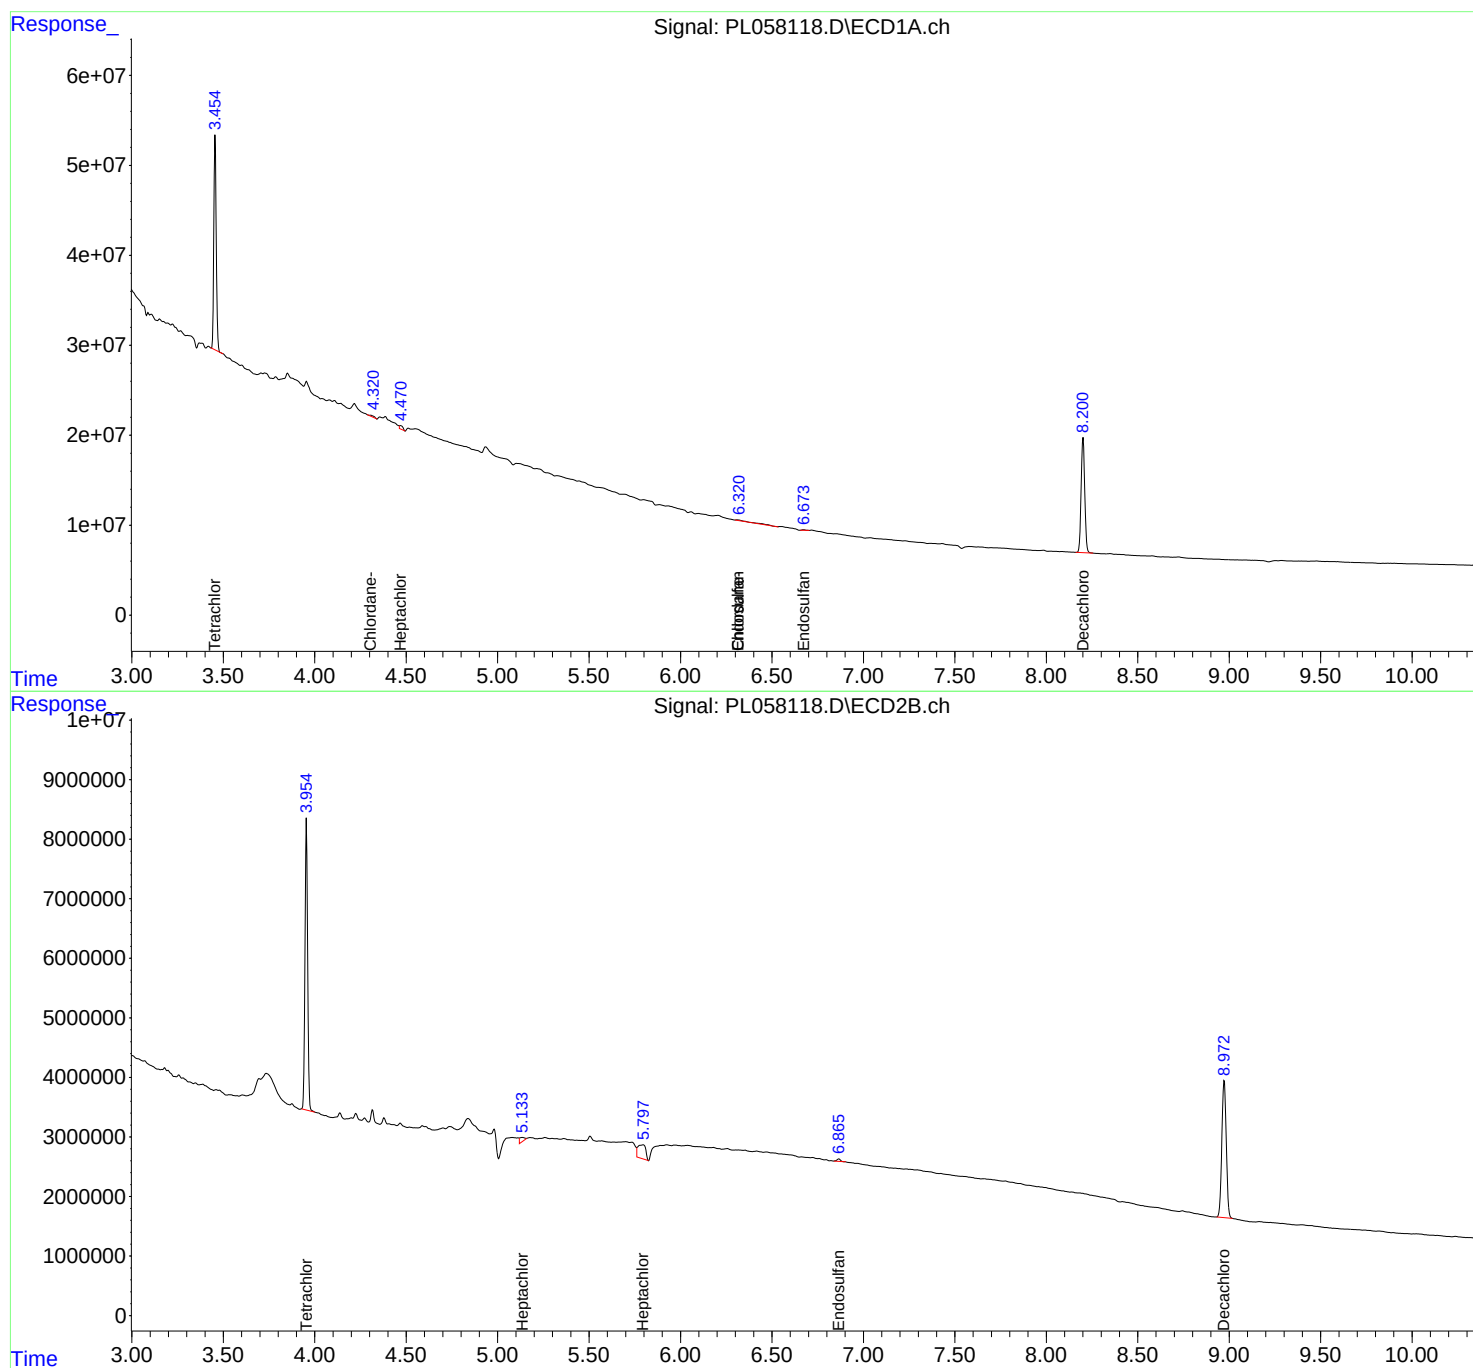


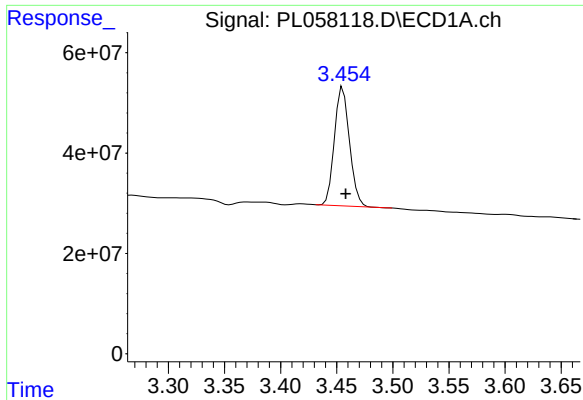

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 220918625
Conc: 21.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

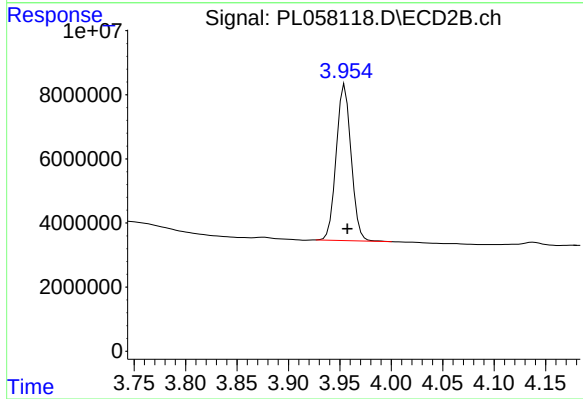


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 49113636
Conc: 22.63 ng/ml

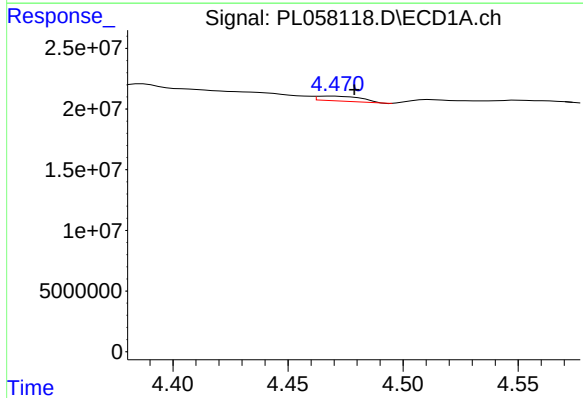


#4 Heptachlor

R.T.: 4.469 min
Delta R.T.: -0.010 min
Response: 5431466
Conc: 0.34 ng/ml

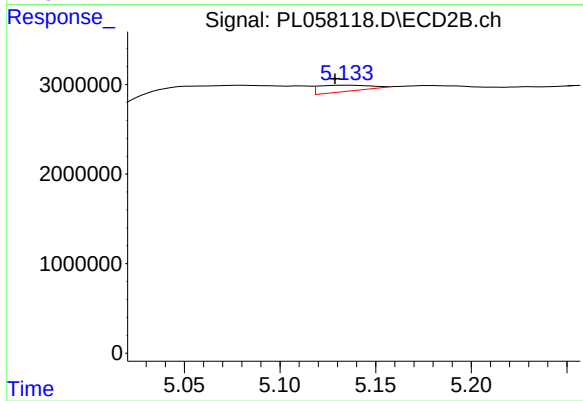

#4 Heptachlor


R.T.: 5.135 min
Delta R.T.: 0.006 min
Response: 1281672
Conc: 0.38 ng/ml

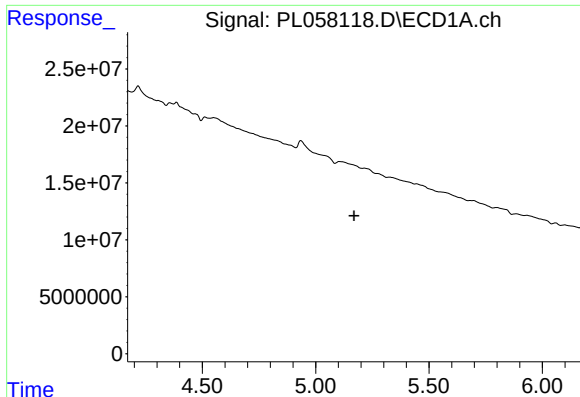

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

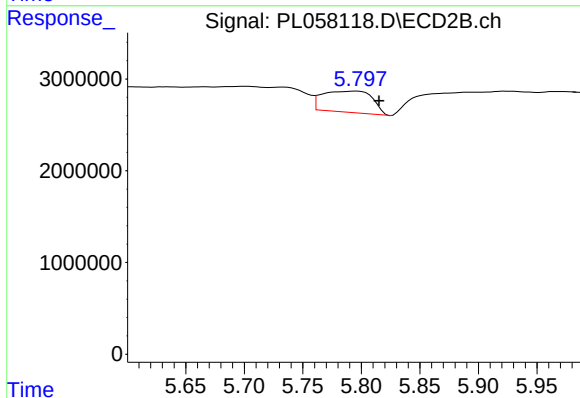


#8 Heptachlor epoxide

R.T.: 5.796 min
Delta R.T.: -0.019 min
Response: 6909512
Conc: 2.56 ng/ml

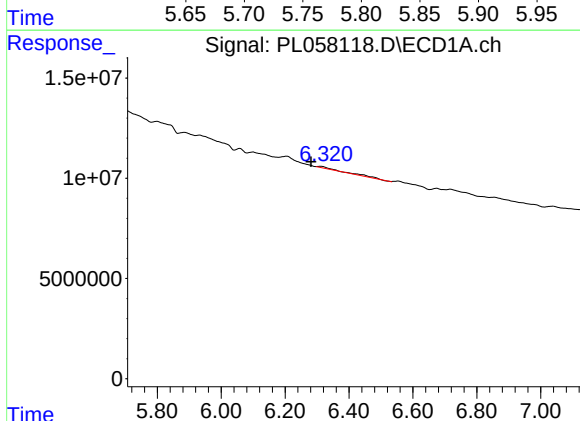


#15 Endosulfan II

R.T.: 6.312 min
Delta R.T.: 0.030 min
Response: 4435070
Conc: 0.40 ng/ml

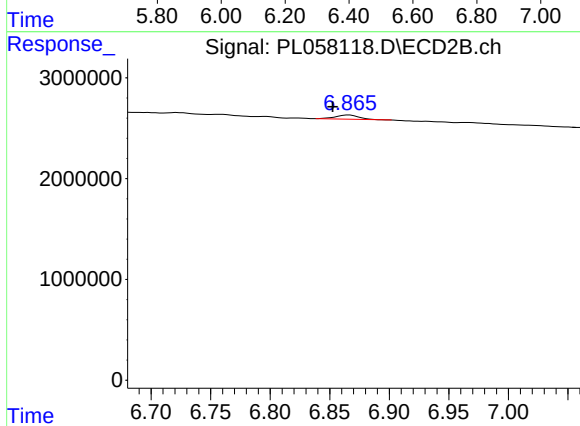

#15 Endosulfan II


R.T.: 6.866 min
Delta R.T.: 0.014 min
Response: 503409
Conc: 0.19 ng/ml

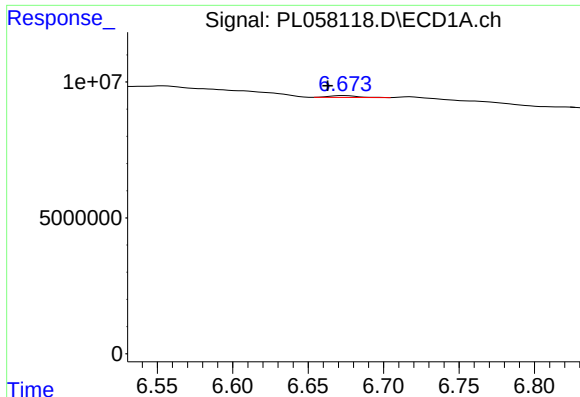

#19 Endosulfan Sulfate


R.T.: 6.674 min
Delta R.T.: 0.011 min
Response: 872256
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

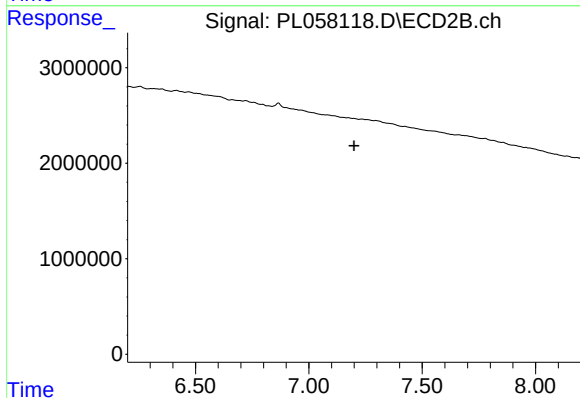


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

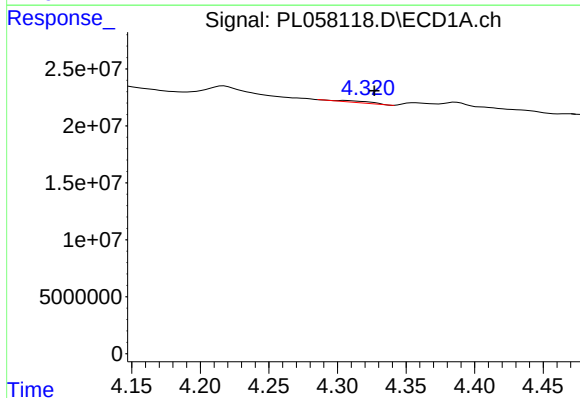


#23 Chlordane-1

R.T.: 4.305 min
Delta R.T.: -0.022 min
Response: 2785826
Conc: 7.53 ng/ml

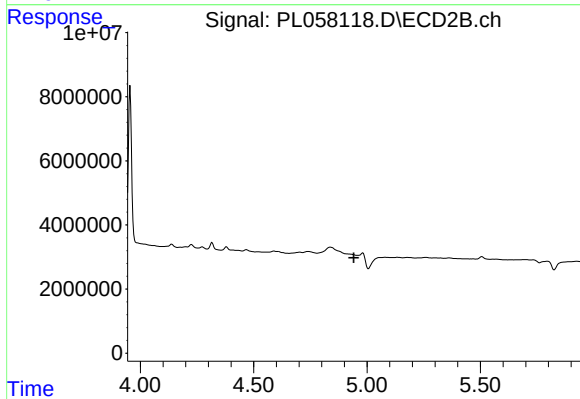

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

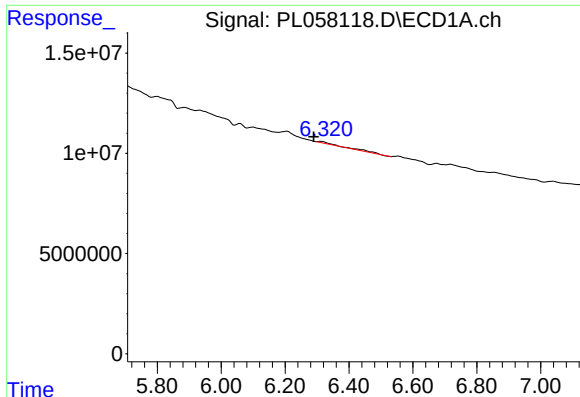

#27 Chlordane-5


R.T.: 6.312 min
Delta R.T.: 0.021 min
Response: 4435070
Conc: 11.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

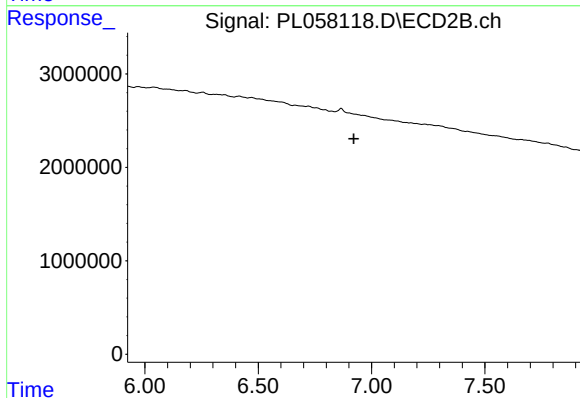


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

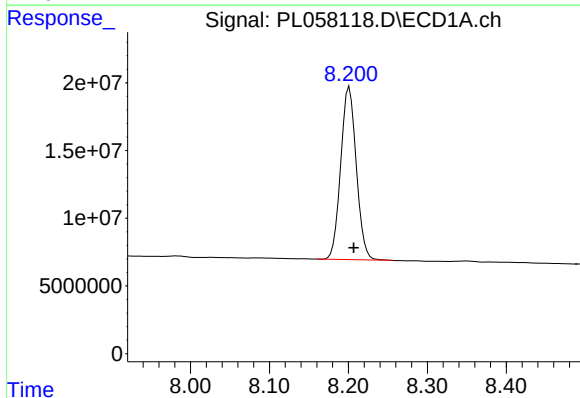

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: -0.005 min
Response: 174708788
Conc: 16.95 ng/ml

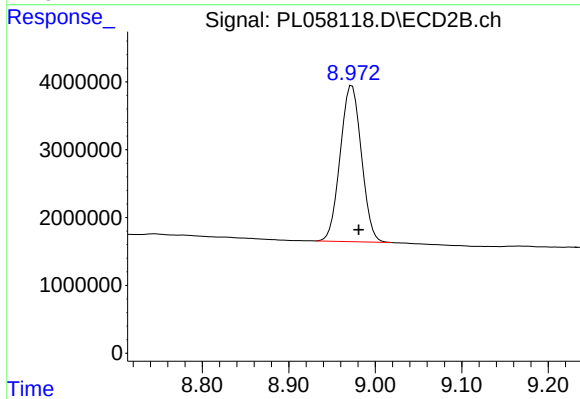

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: -0.008 min
Response: 39006471
Conc: 17.46 ng/ml