

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041620\
 Data File : PL058108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 02:27
 Operator : AJ\MA
 Sample : L2245-14
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-23A

Manual Integrations
 APPROVED

mohammad
 4/20/2020 11:00:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 02:35:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.454	3.954	107.8E6	20099816	10.695m	9.262
28)	SA Decachlor...	8.202	8.975	244.2E6	54653762	23.691	24.467
Target Compounds							
11)	B alpha-Chl...	5.449	6.117	17241233	8372077	1.295m	2.558m#
12)	B 4,4'-DDE	5.614	6.274	68764062	15412550	5.249m	5.206

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041620\
Data File : PL058108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 02:27
Operator : AJ\MA
Sample : L2245-14
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-23A


Manual Integrations
APPROVED

mohammad
4/20/2020 11:00:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 02:35:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

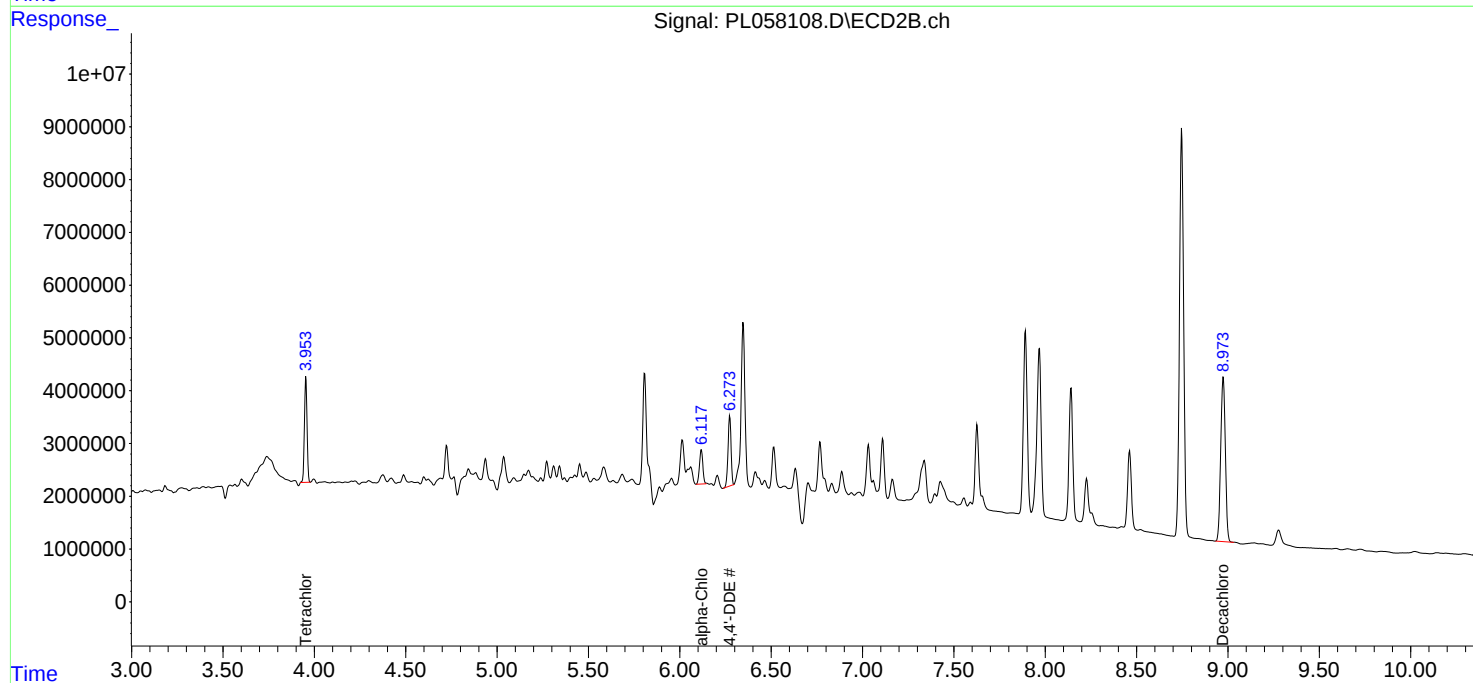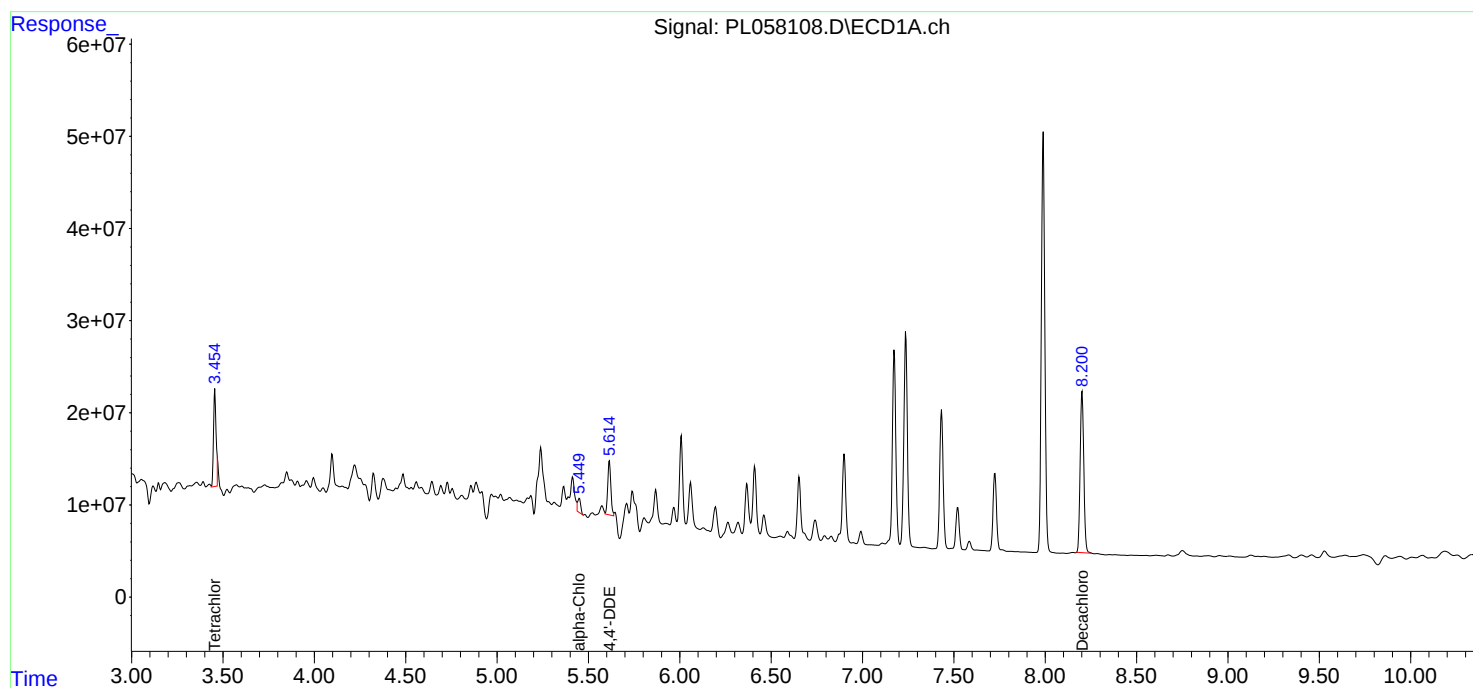

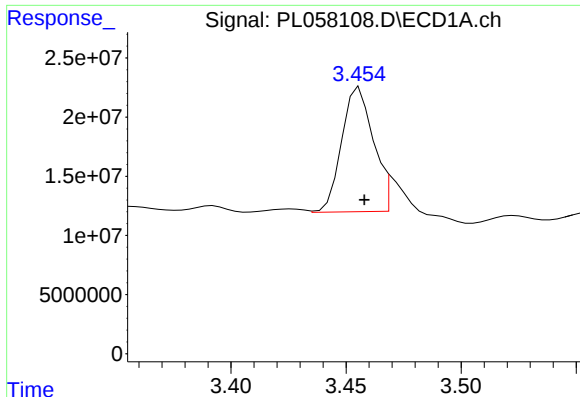


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: -0.004 min
Response: 107819064
Conc: 10.70 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-23A


Manual Integrations
APPROVED

mohammad
4/20/2020 11:00:35 AM

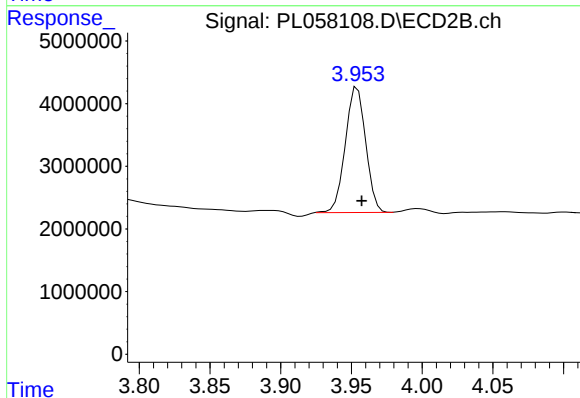


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.003 min
Response: 20099816
Conc: 9.26 ng/ml

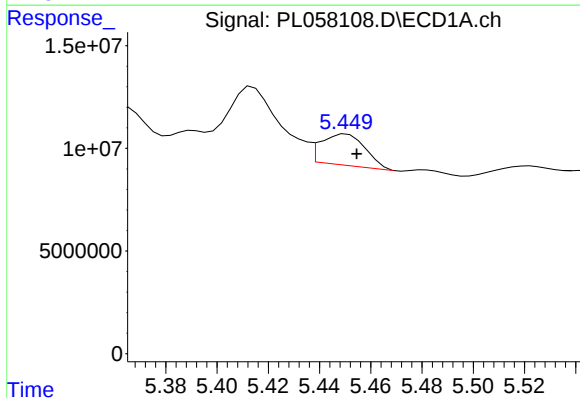


#11 alpha-Chlordane

R.T.: 5.449 min
Delta R.T.: -0.005 min
Response: 17241233
Conc: 1.29 ng/ml m

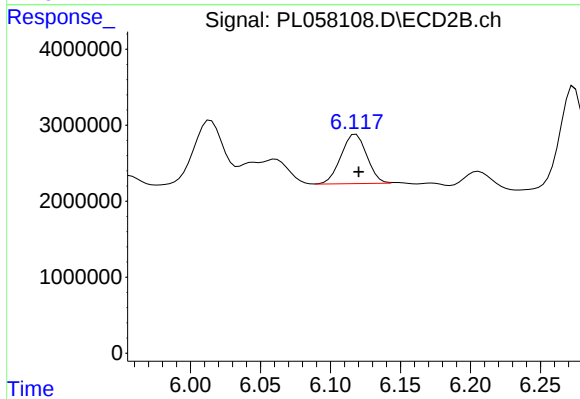

#11 alpha-Chlordane

R.T.: 6.117 min
Delta R.T.: -0.003 min
Response: 8372077
Conc: 2.56 ng/ml m

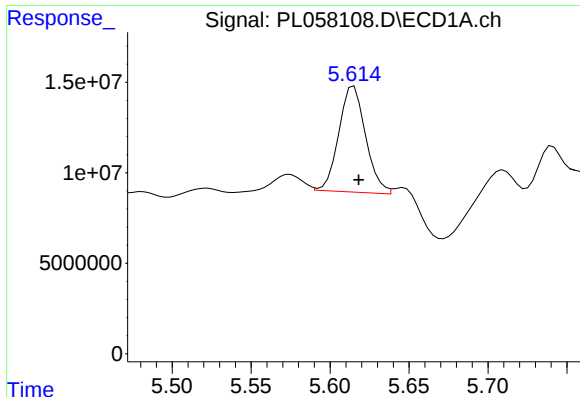


#12 4,4'-DDE

R.T.: 5.614 min
Delta R.T.: -0.005 min
Response: 68764062
Conc: 5.25 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-23A


Manual Integrations
APPROVED

mohammad
4/20/2020 11:00:35 AM

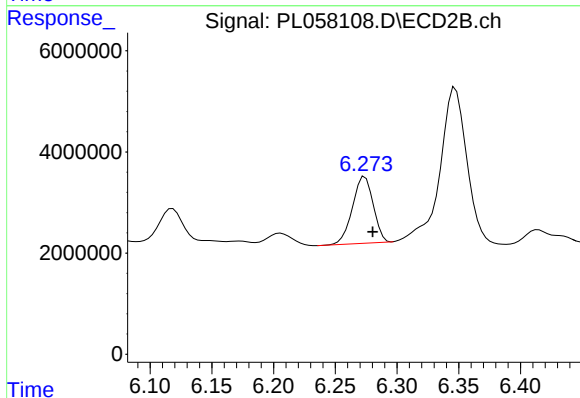


#12 4,4'-DDE

R.T.: 6.274 min
Delta R.T.: -0.006 min
Response: 15412550
Conc: 5.21 ng/ml

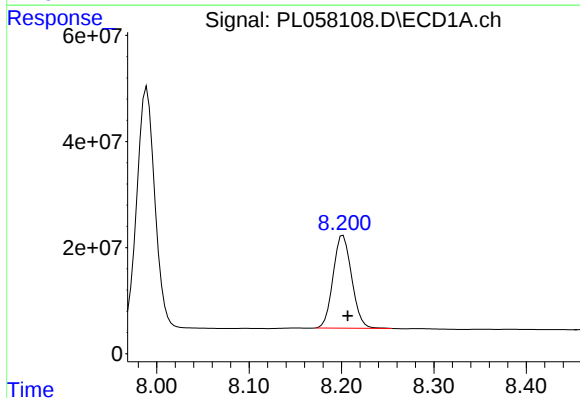

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.005 min
Response: 244214078
Conc: 23.69 ng/ml

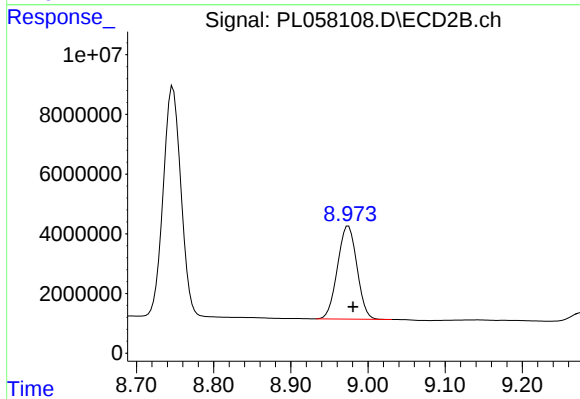

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: -0.006 min
Response: 54653762
Conc: 24.47 ng/ml