

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041620\
 Data File : PL058119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 05:04
 Operator : AJ\MA
 Sample : L2300-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WATER-RECLAIM-SYSTEM-SEDIM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 05:23:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.954	169.8E6	35877683	16.847	16.532
28)	SA Decachlor...	8.201	8.974	159.5E6	35702593	15.473	15.983

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041620\
Data File : PL058119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 05:04
Operator : AJ\MA
Sample : L2300-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WATER-RECLAIM-SYSTEM-SEDIM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 05:23:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

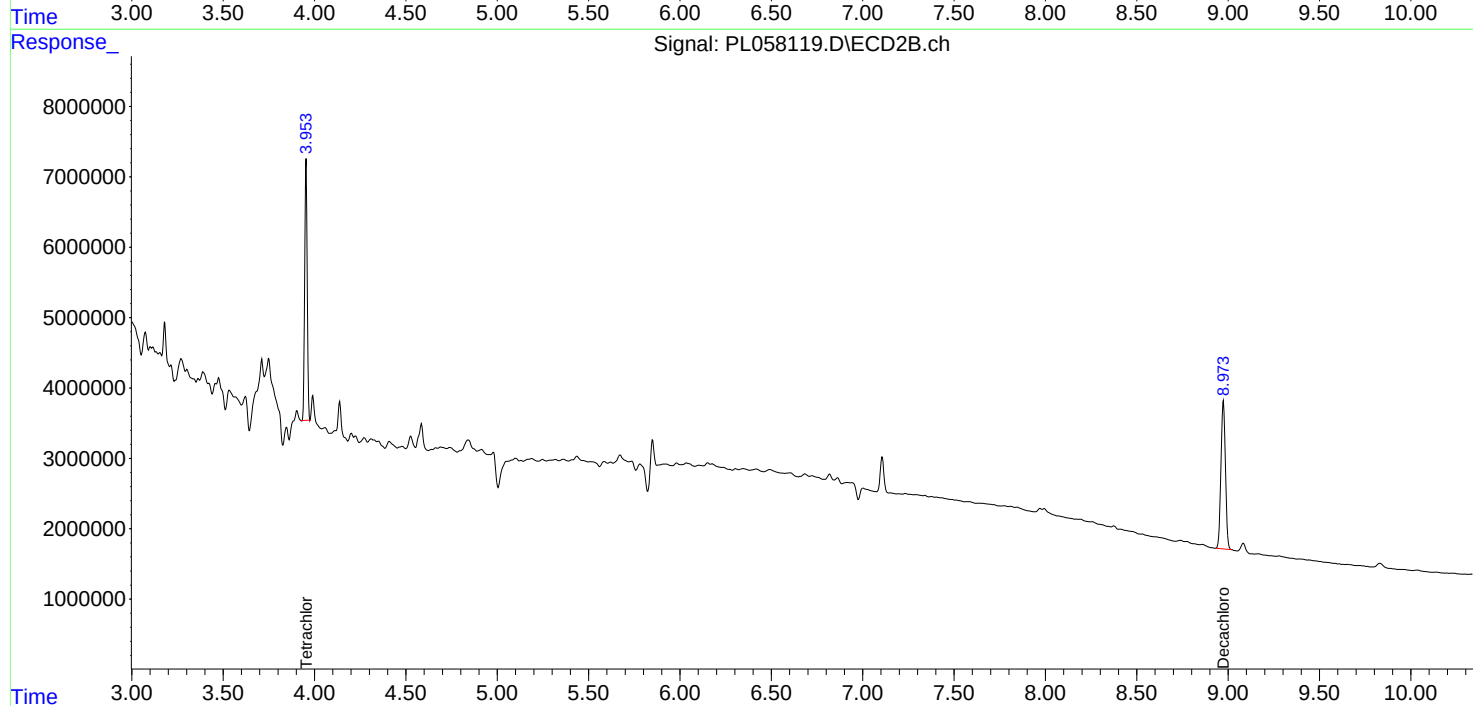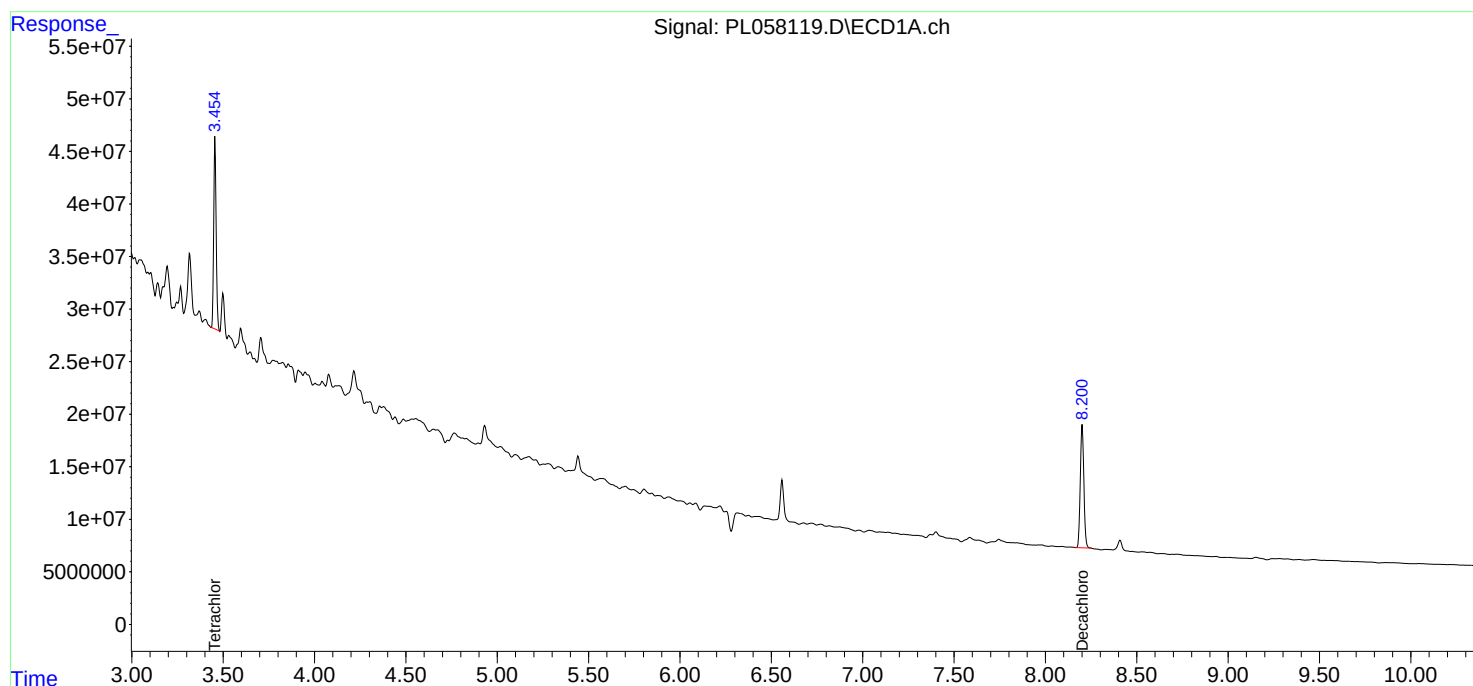


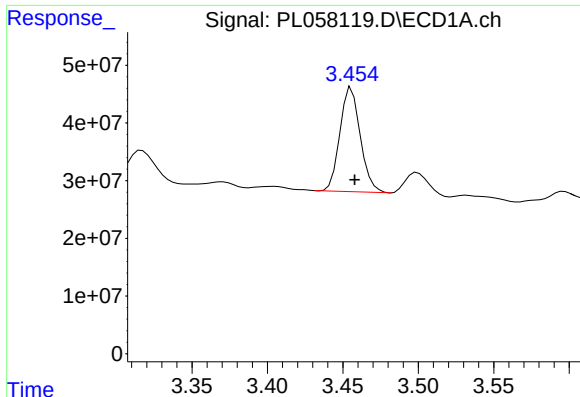

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 169839569
Conc: 16.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
WATER-RECLAIM-SYSTEM-SEDIM

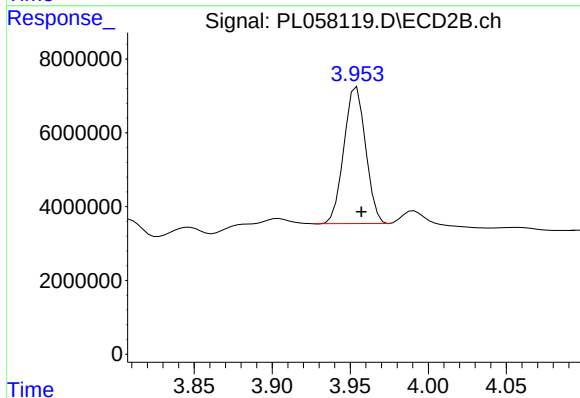


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.003 min
Response: 35877683
Conc: 16.53 ng/ml

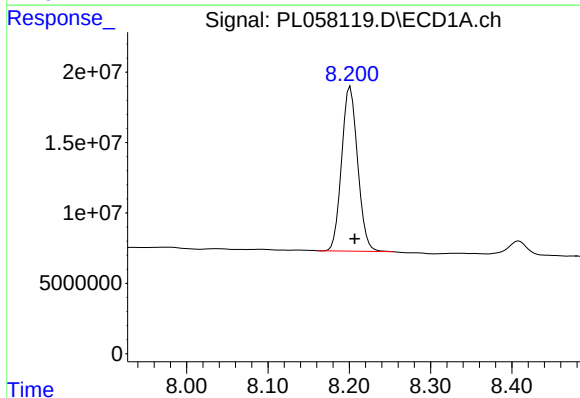

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: -0.005 min
Response: 159502540
Conc: 15.47 ng/ml

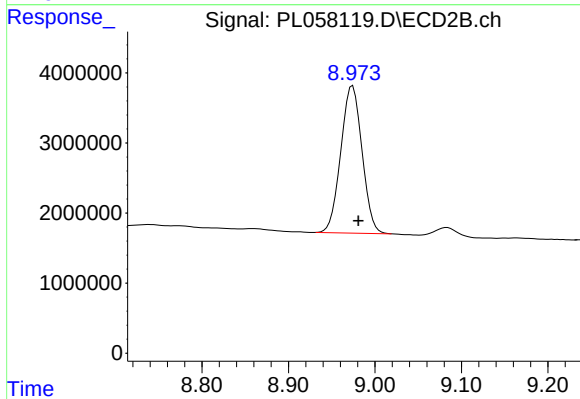

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.007 min
Response: 35702593
Conc: 15.98 ng/ml