

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
 Data File : PL066263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 21:42
 Operator : AR\AJ
 Sample : PB135778BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 23:15:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.155	51617305	88335706	20.280	21.960
28)	SA Decachlor...	8.170	9.355	54434392	70819973	22.821	21.685
Target Compounds							
4)	MA Heptachlor	0.000	5.355	0	3755103	N.D.	0.675 #
5)	MB Aldrin	0.000	5.674	0	354515	N.D.	0.071 #
14)	MA Endrin	5.975	0.000	2832526	0	0.812	N.D. #
15)	B Endosulfa...	0.000	7.125	0	2698082	N.D.	0.774 #
17)	MA 4,4'-DDT	0.000	7.362f	0	1995943	N.D.	0.588 #
18)	B Endrin al...	0.000	7.255	0	3071616	N.D.	1.098 #
21)	B Endrin ke...	0.000	7.976	0	2333919	N.D.	0.634 #
23)	Chlordane-1	4.333f	0.000	2768405	0	24.216	N.D. #
24)	Chlordane-2	0.000	5.674f	0	354515	N.D.	2.015 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
Data File : PL066263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 21:42
Operator : AR\AJ
Sample : PB135778BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 23:15:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

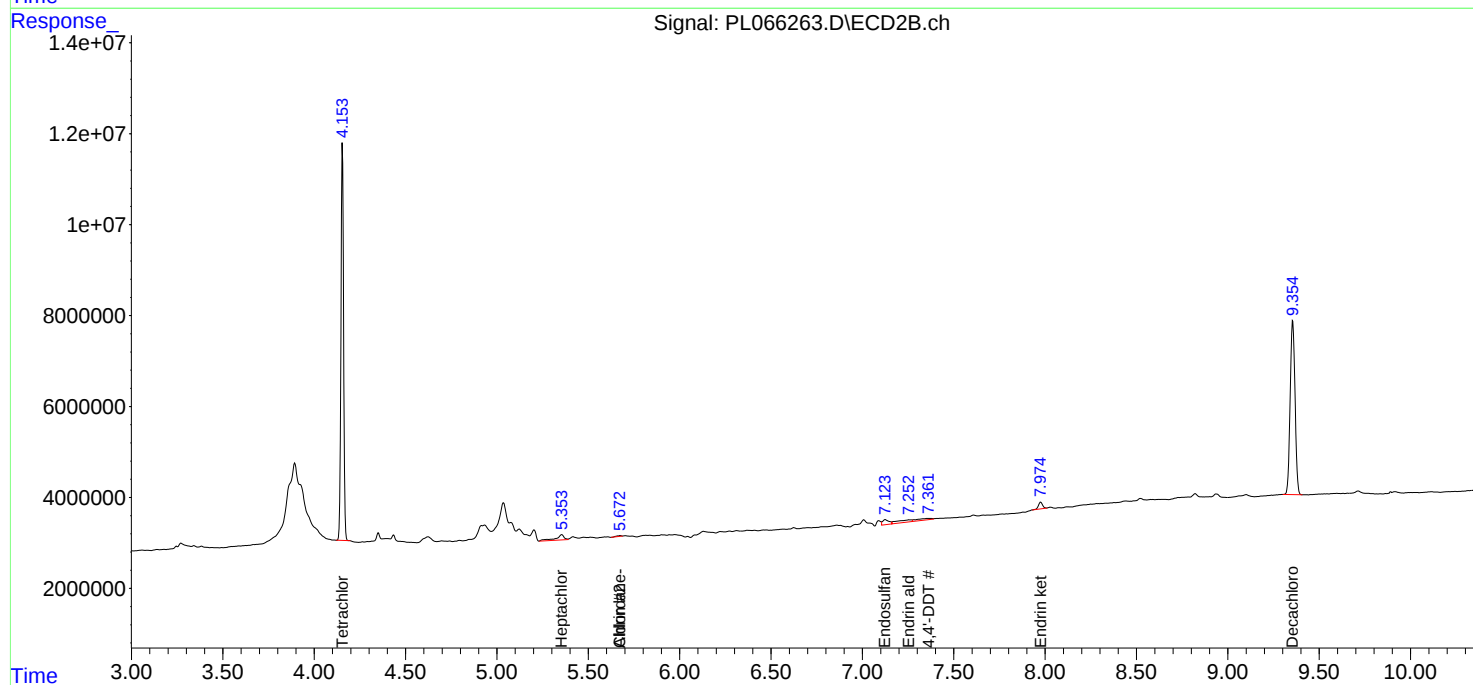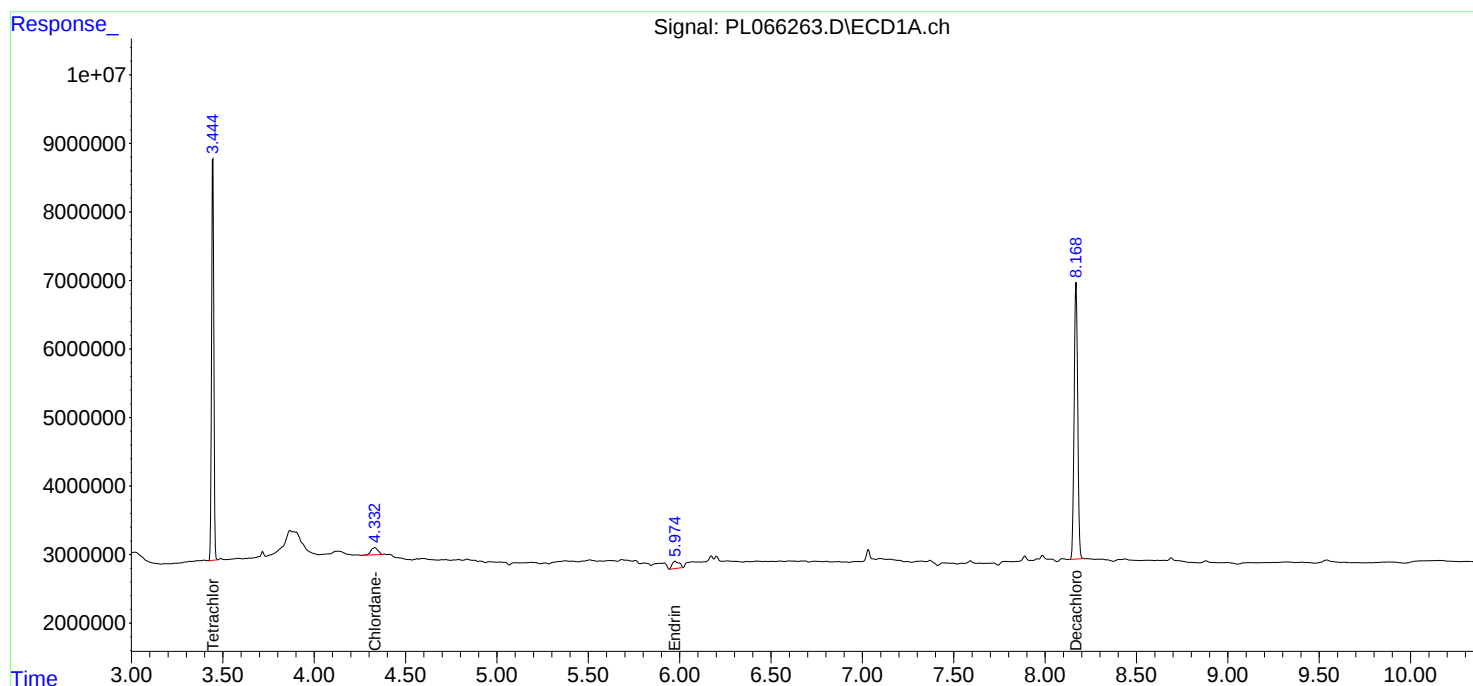


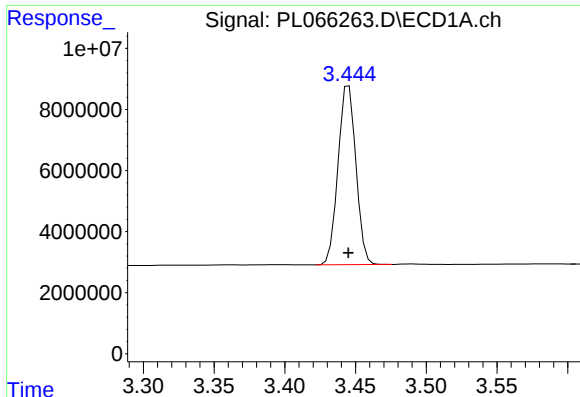

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 51617305
Conc: 20.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

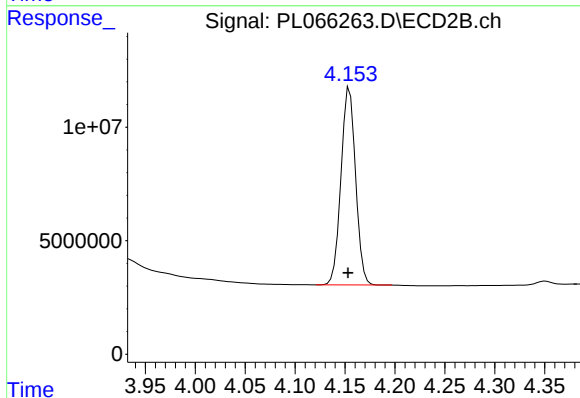


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 88335706
Conc: 21.96 ng/ml

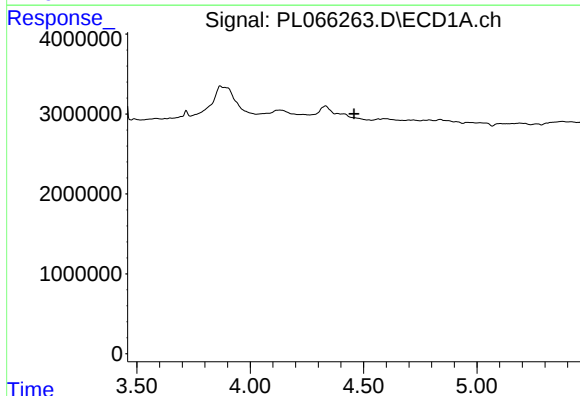


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.459 min
Response: 0
Conc: N.D.

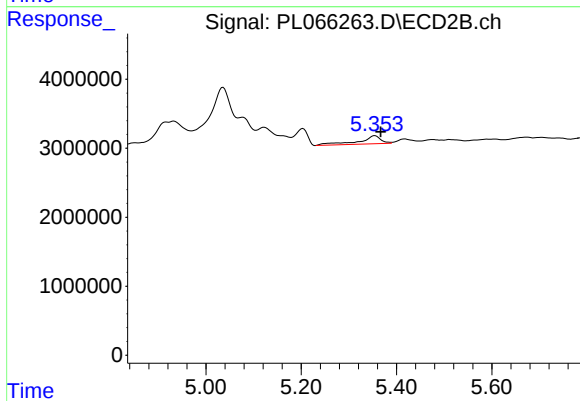

#4 Heptachlor


R.T.: 5.355 min
Delta R.T.: -0.012 min
Response: 3755103
Conc: 0.67 ng/ml

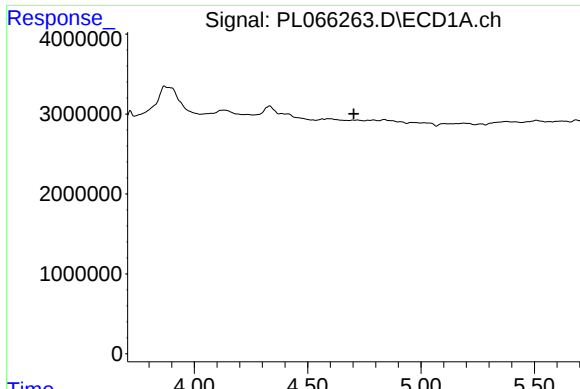

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.704 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

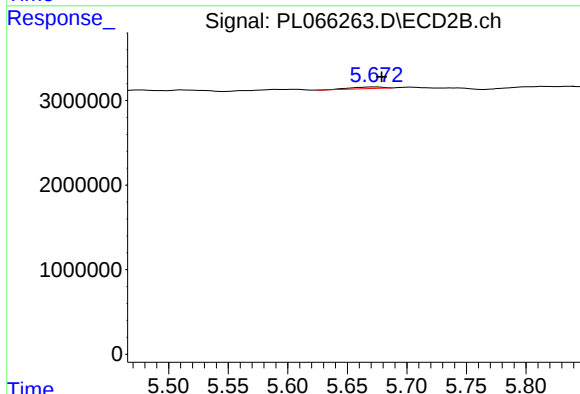


#5 Aldrin

R.T.: 5.674 min
Delta R.T.: -0.005 min
Response: 354515
Conc: 0.07 ng/ml

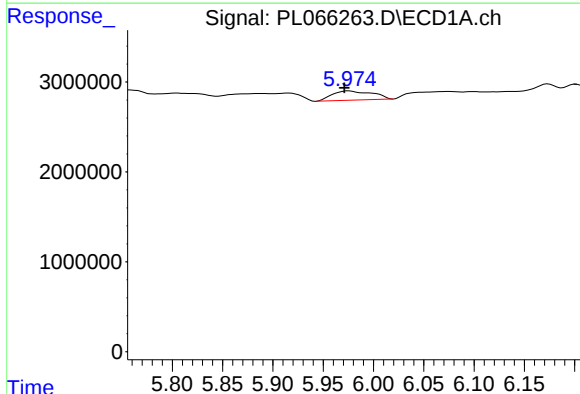


#14 Endrin

R.T.: 5.975 min
Delta R.T.: 0.004 min
Response: 2832526
Conc: 0.81 ng/ml

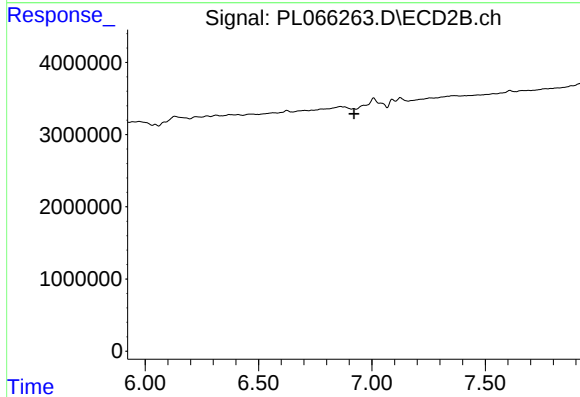

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

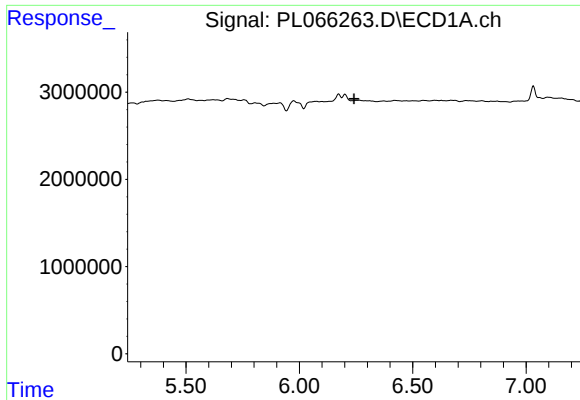

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

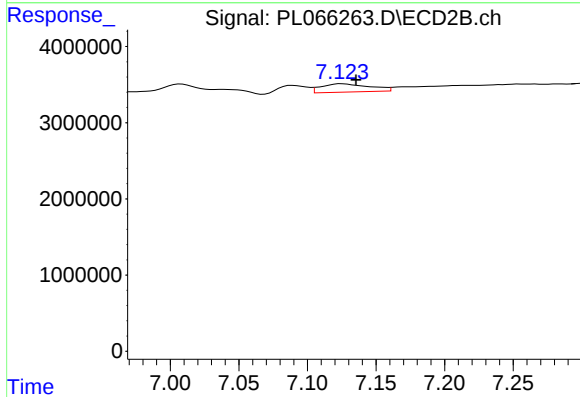


#15 Endosulfan II

R.T.: 7.125 min
Delta R.T.: -0.011 min
Response: 2698082
Conc: 0.77 ng/ml

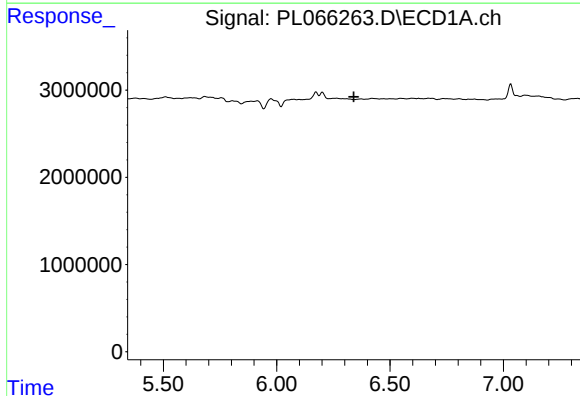


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.341 min
Response: 0
Conc: N.D.

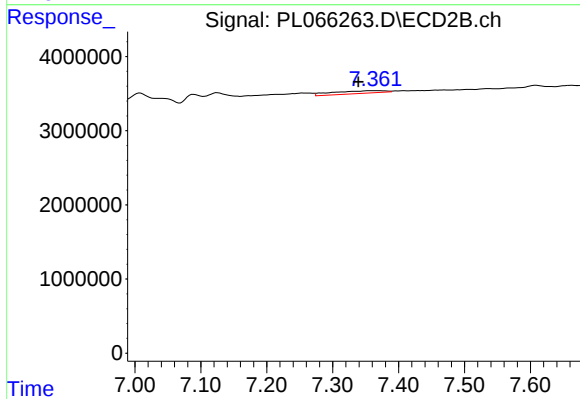

#17 4,4'-DDT


R.T.: 7.362 min
Delta R.T.: 0.023 min
Response: 1995943
Conc: 0.59 ng/ml

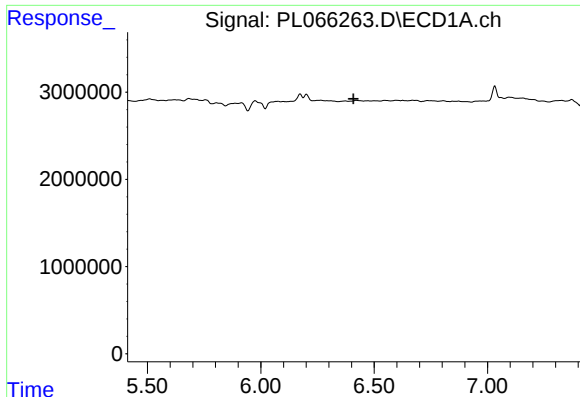

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

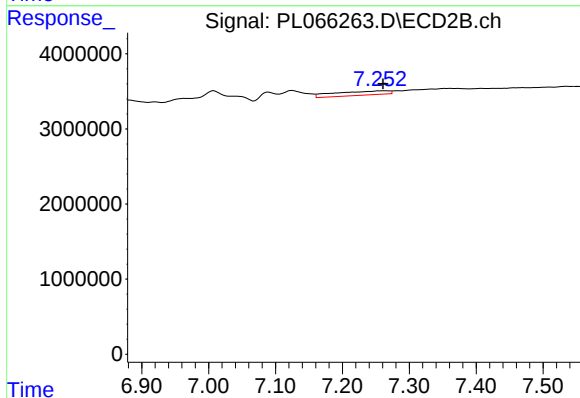


#18 Endrin aldehyde

R.T.: 7.255 min
Delta R.T.: -0.006 min
Response: 3071616
Conc: 1.10 ng/ml

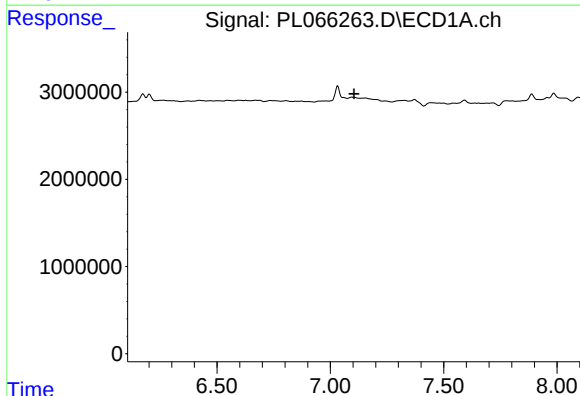


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

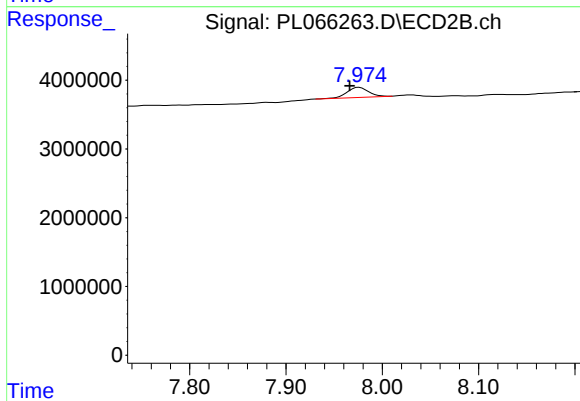

#21 Endrin ketone


R.T.: 7.976 min
Delta R.T.: 0.010 min
Response: 2333919
Conc: 0.63 ng/ml

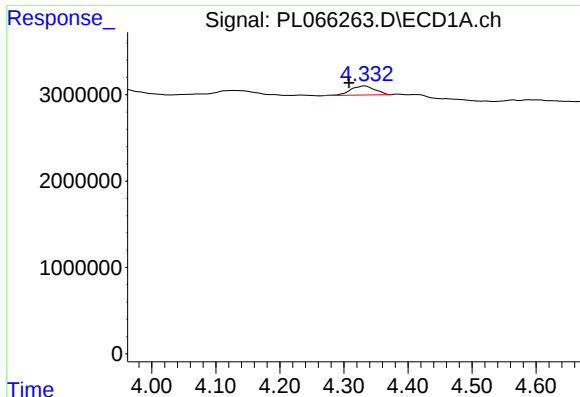

#23 Chlordane-1


R.T.: 4.333 min
Delta R.T.: 0.024 min
Response: 2768405
Conc: 24.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

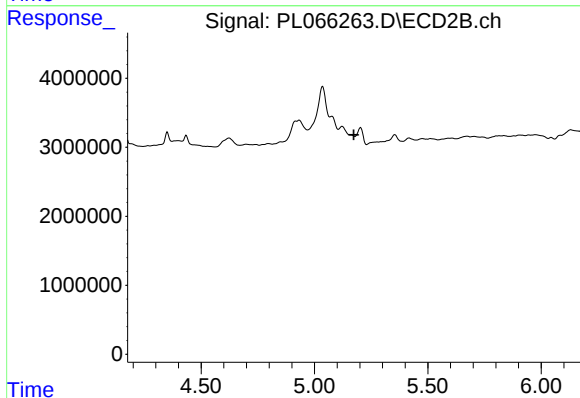


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.173 min
Response: 0
Conc: N.D.

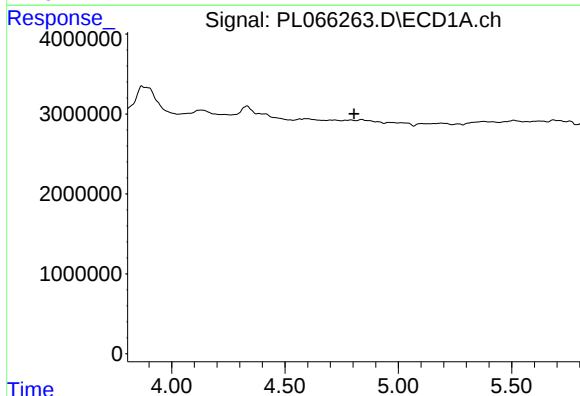


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.805 min
Response: 0
Conc: N.D.

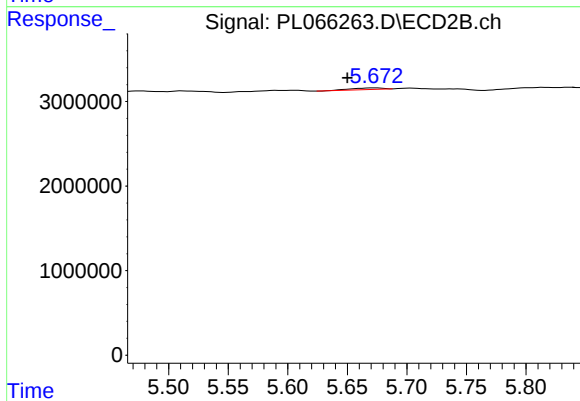

#24 Chlordane-2


R.T.: 5.674 min
Delta R.T.: 0.024 min
Response: 354515
Conc: 2.02 ng/ml

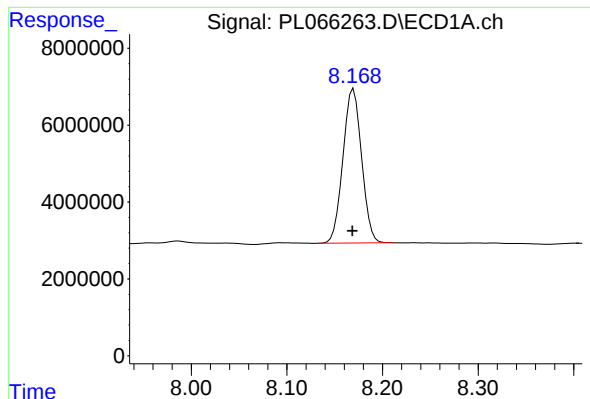

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.001 min
Response: 54434392
Conc: 22.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

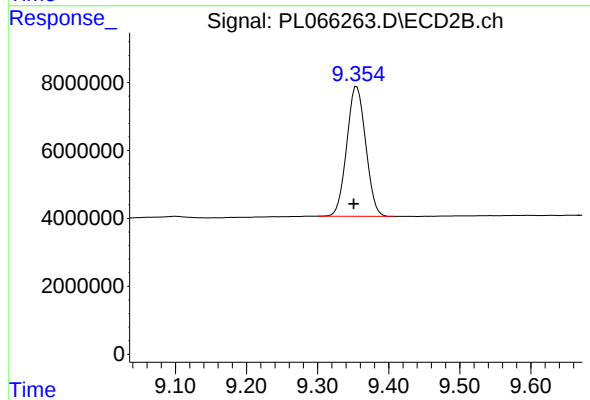

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.004 min
Response: 70819973
Conc: 21.68 ng/ml